

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
 Data File : VX025006.D
 Acq On : 28 Oct 2021 15:04
 Operator : JC/MD
 Sample : VX1028MBL02
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK619

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M

Title : VOC Analysis

Signal : TIC: VX025006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	78137	80289	11.85%	1.562%
2	1.618	84	87	91	rBV4	1237	1803	0.27%	0.035%
3	1.672	91	96	102	rVV	54831	67881	10.02%	1.320%
4	2.185	177	180	183	rBV2	660	555	0.08%	0.011%
5	2.306	193	200	215	rBV	144972	233814	34.50%	4.548%
6	2.447	221	223	226	rVB2	821	737	0.11%	0.014%
7	2.477	226	228	231	rBV2	727	607	0.09%	0.012%
8	2.569	240	243	247	rBV	820	1209	0.18%	0.024%
9	2.678	258	261	264	rVB	601	775	0.11%	0.015%
10	2.721	264	268	271	rBV3	792	1242	0.18%	0.024%
11	2.794	275	280	285	rVB4	2178	3518	0.52%	0.068%
12	3.386	374	377	378	rVB2	608	617	0.09%	0.012%
13	3.422	378	383	385	rBV2	546	773	0.11%	0.015%
14	3.526	399	400	403	rVB2	681	538	0.08%	0.010%
15	3.562	403	406	409	rBV2	531	748	0.11%	0.015%
16	3.678	423	425	427	rVB2	641	670	0.10%	0.013%
17	3.855	450	454	456	rBV2	762	1175	0.17%	0.023%
18	3.916	459	464	466	rBV	584	844	0.12%	0.016%
19	3.934	466	467	470	rVB	854	544	0.08%	0.011%
20	4.074	488	490	497	rBV2	660	1109	0.16%	0.022%
21	4.172	504	506	512	rBV	804	1057	0.16%	0.021%
22	4.294	524	526	531	rVB	687	961	0.14%	0.019%
23	4.465	546	554	570	rVV	54449	168495	24.86%	3.277%
24	4.904	625	626	630	rBV	705	686	0.10%	0.013%
25	5.062	636	652	666	rBV	98605	304185	44.88%	5.917%
26	5.208	673	676	679	rVB3	792	755	0.11%	0.015%
27	5.300	687	691	694	rBV	810	1197	0.18%	0.023%
28	5.361	698	701	703	rBV	632	743	0.11%	0.014%
29	5.544	729	731	735	rBV3	631	958	0.14%	0.019%
30	5.653	744	749	754	rBV3	640	1299	0.19%	0.025%
31	5.977	790	802	814	rBV2	227542	677734	100.00%	13.182%
32	6.147	826	830	831	rBV2	645	785	0.12%	0.015%
33	6.263	847	849	851	rVV2	810	572	0.08%	0.011%
34	6.361	862	865	866	rBV2	525	602	0.09%	0.012%
35	6.769	922	932	943	rVV	168058	403026	59.47%	7.839%
36	6.867	946	948	952	rBV3	615	902	0.13%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
 Data File : VX025006.D
 Acq On : 28 Oct 2021 15:04
 Operator : JC/MD
 Sample : VX1028MBL02
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK619

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

37	7.117	982	989	997	rBV6	2897	7865	1.16%	0.153%
38	7.245	1009	1010	1013	rBV	526	557	0.08%	0.011%
39	7.312	1013	1021	1032	rVV	139569	310600	45.83%	6.041%
40	7.769	1092	1096	1097	rBV	587	649	0.10%	0.013%
41	8.330	1181	1188	1197	rBV	98865	160916	23.74%	3.130%
42	8.653	1231	1241	1249	rBV	333595	518080	76.44%	10.077%
43	8.726	1249	1253	1258	rVB3	4218	7349	1.08%	0.143%
44	8.805	1264	1266	1269	rBV	480	539	0.08%	0.010%
45	8.952	1285	1290	1300	rVB	79759	115201	17.00%	2.241%
46	9.391	1356	1362	1375	rVV	251606	372232	54.92%	7.240%
47	9.762	1421	1423	1428	rVB2	705	695	0.10%	0.014%
48	9.830	1432	1434	1437	rBV	542	633	0.09%	0.012%
49	9.958	1453	1455	1457	rBV2	712	613	0.09%	0.012%
50	10.055	1465	1471	1479	rBV	348342	464315	68.51%	9.031%
51	10.311	1509	1513	1515	rBV3	1059	1381	0.20%	0.027%
52	10.427	1529	1532	1534	rBV3	1187	1151	0.17%	0.022%
53	10.592	1558	1559	1561	rBV	868	656	0.10%	0.013%
54	10.640	1565	1567	1570	rVV3	807	1003	0.15%	0.020%
55	10.671	1570	1572	1575	rVB	664	644	0.10%	0.013%
56	10.860	1601	1603	1606	rVV	729	1012	0.15%	0.020%
57	10.896	1607	1609	1613	rVV2	850	964	0.14%	0.019%
58	10.957	1613	1619	1621	rVV3	818	1521	0.22%	0.030%
59	11.122	1641	1646	1652	rVB3	2574	4407	0.65%	0.086%
60	11.195	1652	1658	1664	rBV	255040	325809	48.07%	6.337%
61	11.280	1669	1672	1673	rBV2	911	732	0.11%	0.014%
62	11.427	1692	1696	1698	rBV3	767	822	0.12%	0.016%
63	11.463	1698	1702	1703	rBV2	1043	1353	0.20%	0.026%
64	11.561	1712	1718	1720	rVB3	653	1001	0.15%	0.019%
65	11.683	1733	1738	1741	rBV2	743	1432	0.21%	0.028%
66	11.750	1746	1749	1756	rVB4	2487	3830	0.57%	0.074%
67	11.933	1777	1779	1783	rVB3	1612	2037	0.30%	0.040%
68	11.975	1783	1786	1789	rBV	815	1081	0.16%	0.021%
69	12.024	1789	1794	1800	rVV	323238	404336	59.66%	7.865%
70	12.103	1804	1807	1808	rBV2	950	763	0.11%	0.015%
71	12.128	1808	1811	1813	rVV4	1159	1533	0.23%	0.030%
72	12.152	1813	1815	1818	rVB3	1576	1692	0.25%	0.033%
73	12.323	1837	1843	1851	rVB	346112	435839	64.31%	8.477%
74	12.421	1858	1859	1863	rVB2	1212	1284	0.19%	0.025%
75	12.488	1865	1870	1872	rBV3	849	1070	0.16%	0.021%
76	12.555	1879	1881	1883	rVB	727	690	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
 Data File : VX025006.D
 Acq On : 28 Oct 2021 15:04
 Operator : JC/MD
 Sample : VX1028MBL02
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK619

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

77	12.579	1883	1885	1887	rBV	867	834	0.12%	0.016%
78	12.603	1887	1889	1892	rVB3	735	733	0.11%	0.014%
79	12.658	1896	1898	1900	rBV	593	535	0.08%	0.010%
80	12.731	1909	1910	1913	rBV	561	588	0.09%	0.011%
81	13.292	1998	2002	2005	rBV	899	1109	0.16%	0.022%
82	13.469	2027	2031	2032	rBV2	615	690	0.10%	0.013%
83	13.689	2062	2067	2071	rBV2	826	1209	0.18%	0.024%
84	13.975	2111	2114	2116	rVB	727	892	0.13%	0.017%
85	14.170	2143	2146	2148	rVB	576	558	0.08%	0.011%
86	14.646	2221	2224	2226	rBV3	716	786	0.12%	0.015%
87	14.786	2244	2247	2248	rBV	672	699	0.10%	0.014%
88	15.024	2285	2286	2289	rBV3	445	548	0.08%	0.011%
89	15.298	2329	2331	2335	rVB2	935	1460	0.22%	0.028%
90	15.335	2335	2337	2338	rBV	649	561	0.08%	0.011%
91	15.371	2341	2343	2344	rVV2	1035	694	0.10%	0.013%
92	15.408	2348	2349	2354	rVV	1008	1183	0.17%	0.023%
93	15.639	2382	2387	2388	rBV2	926	1229	0.18%	0.024%
94	15.731	2398	2402	2403	rBV2	783	697	0.10%	0.014%
95	15.780	2407	2410	2411	rBV2	474	552	0.08%	0.011%
96	16.048	2453	2454	2456	rBV	645	589	0.09%	0.011%
97	16.243	2484	2486	2489	rVV3	739	767	0.11%	0.015%
98	16.298	2493	2495	2499	rBV2	584	744	0.11%	0.014%
99	16.347	2501	2503	2505	rVB2	627	557	0.08%	0.011%
100	16.469	2519	2523	2527	rBV3	824	1280	0.19%	0.025%

Sum of corrected areas: 5141186




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
Data File : VX025006.D
Acq On : 28 Oct 2021 15:04
Operator : JC/MD
Sample : VX1028MBL02
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK619

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

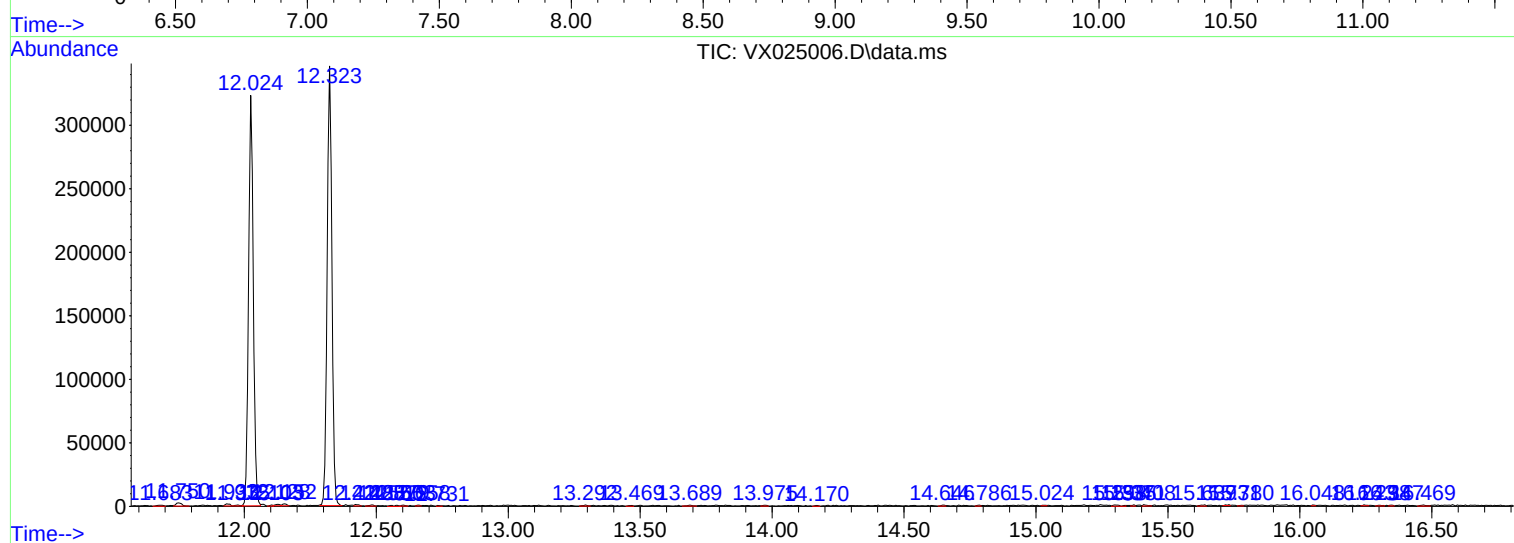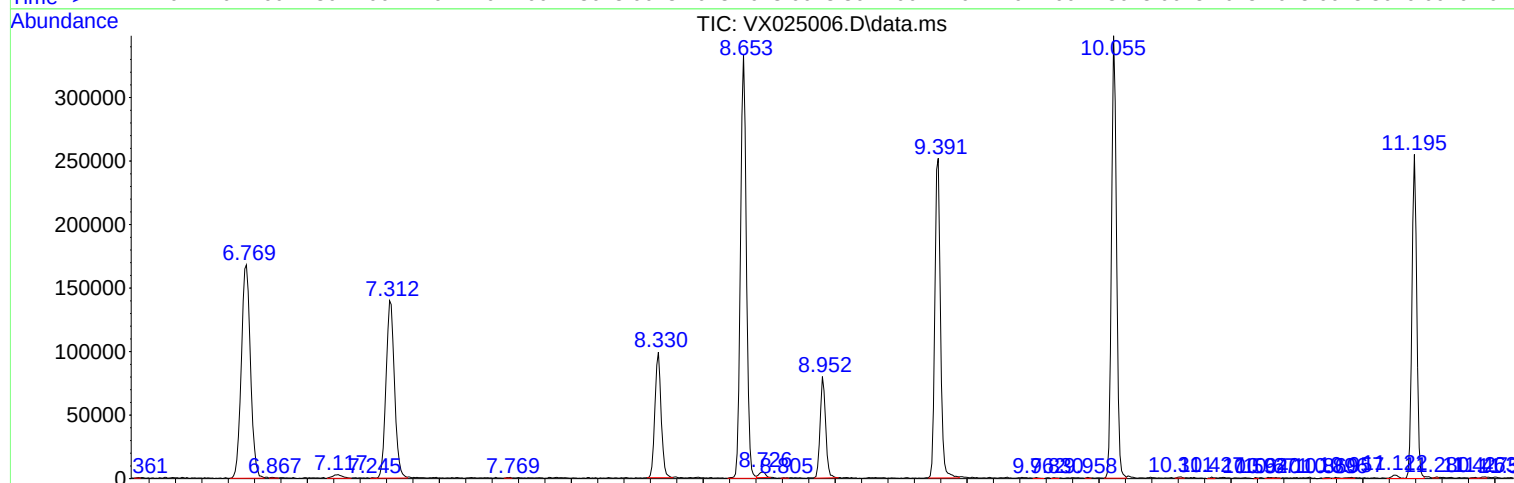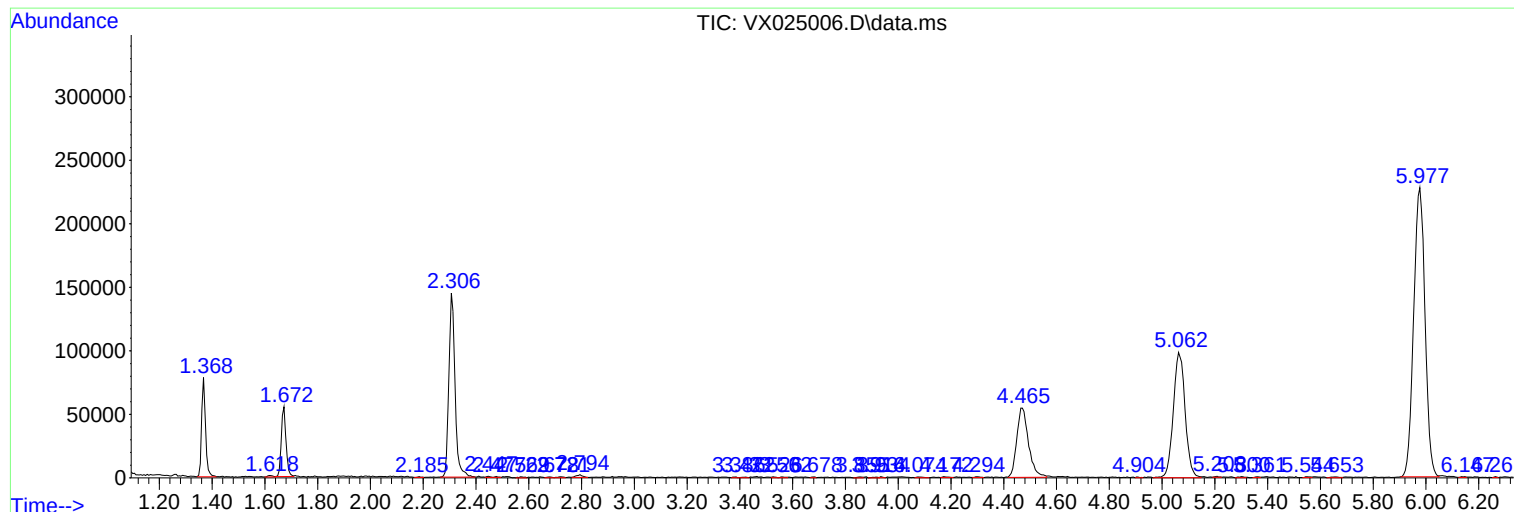

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
Data File : VX025006.D
Acq On : 28 Oct 2021 15:04
Operator : JC/MD
Sample : VX1028MBL02
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK619

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
Data File : VX025006.D
Acq On : 28 Oct 2021 15:04
Operator : JC/MD
Sample : VX1028MBL02
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK619

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
