
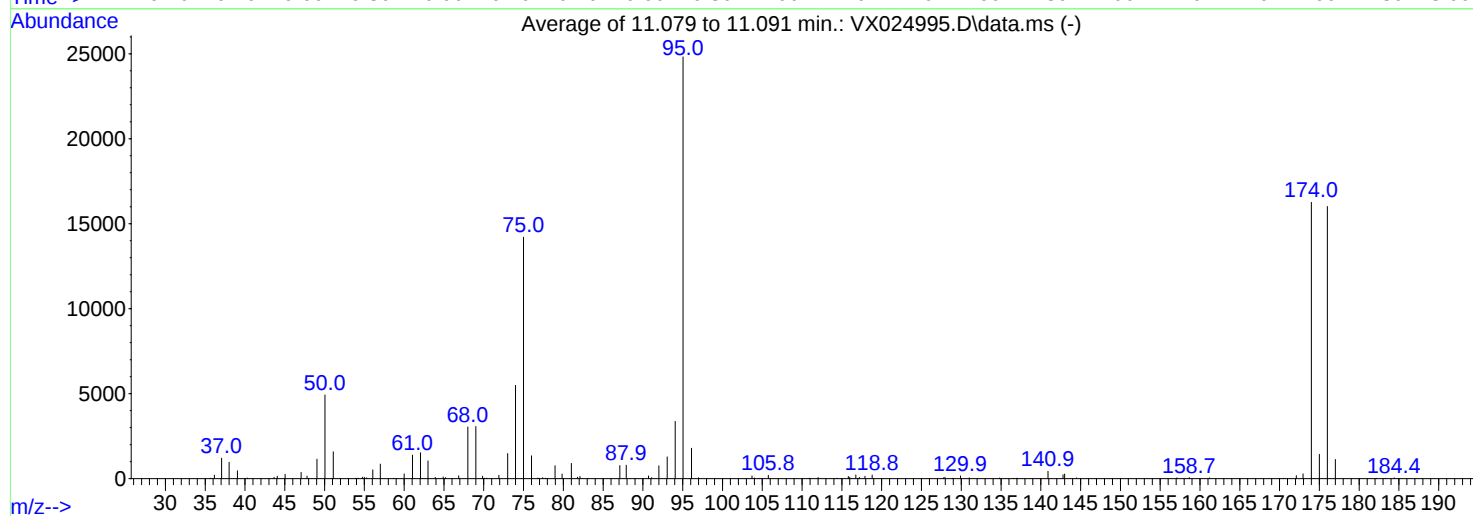


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102821\
 Data File : VX024995.D
 Acq On : 28 Oct 2021 09:57
 Operator : JC/MD
 Sample : BFB607
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB607

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
 Title : VOC Analysis
 Last Update : Sat Oct 30 01:06:24 2021

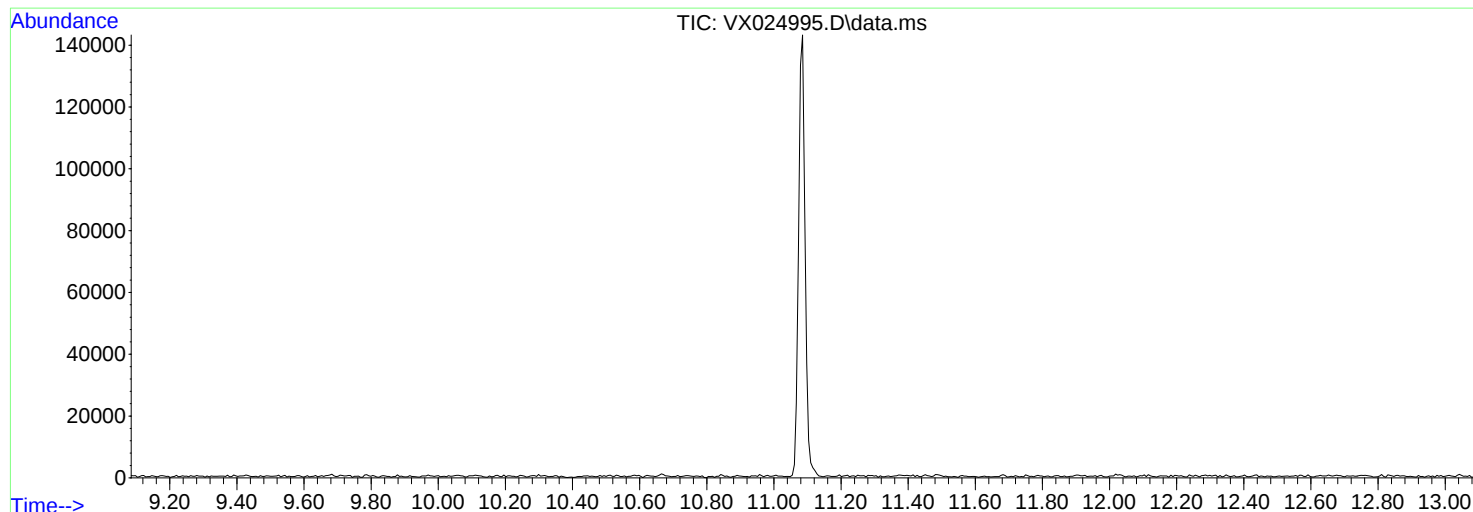

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1634

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	4928	PASS
75	95	30	80	57.2	14205	PASS
95	95	100	100	100.0	24821	PASS
96	95	5	9	7.2	1791	PASS
173	174	0.00	2	1.7	283	PASS
174	95	50	120	65.5	16263	PASS
175	174	5	9	8.8	1436	PASS
176	174	95	101	98.5	16013	PASS
177	176	5	9	7.1	1129	PASS

m/z	Abundance
36.20	174.0
37.00	739.0
38.00	840.0
38.90	146.0
39.20	222.0
43.60	76.0
45.10	235.0
47.00	348.0
47.70	125.0
49.10	858.0
50.00	3356.0
51.10	924.0
54.20	96.0
55.00	247.0
56.00	322.0
57.00	313.0
59.90	163.0
61.10	859.0
62.00	1243.0
62.90	764.0
64.90	104.0
67.90	1575.0
68.90	2028.0
70.10	77.0
72.00	138.0
73.00	1034.0
74.00	3950.0
75.00	8999.0
76.00	764.0
77.40	57.0
79.00	495.0
79.70	125.0
80.90	582.0
82.10	107.0
83.10	66.0
87.20	549.0
87.80	435.0
90.70	162.0
92.00	773.0
93.00	1032.0
94.00	2740.0
95.00	17896.0
96.10	1081.0
104.00	105.0
104.70	52.0
105.80	178.0
116.00	216.0
116.80	196.0
118.00	97.0
118.70	123.0
127.90	116.0
128.90	60.0
129.80	142.0
131.00	87.0
134.80	54.0
136.60	52.0
140.90	409.0
142.80	319.0
144.50	76.0
157.10	53.0
161.20	141.0
172.20	106.0
172.90	250.0
174.00	13716.0
175.00	1254.0
176.00	13003.0
177.00	740.0

Instrument :
MSVOA_X
ClientSampleId :
BFB607

m/z	Abundance
37.80	53.0
38.20	96.0
39.90	104.0
43.90	52.0
126.40	96.0

Instrument :
MSVOA_X
ClientSampleId :
BFB607

m/z	Abundance
35.70	93.0
36.10	108.0
37.10	1629.0
38.00	1183.0
39.00	513.0
40.30	101.0
43.70	147.0
44.10	228.0
45.00	263.0
47.10	391.0
47.90	87.0
49.10	1503.0
50.10	5434.0
51.10	1954.0
53.90	68.0
54.80	117.0
55.30	131.0
56.00	603.0
57.00	885.0
58.70	69.0
60.00	362.0
61.00	1622.0
62.10	1642.0
63.00	1203.0
63.90	168.0
64.90	212.0
66.80	336.0
68.00	3779.0
69.00	3520.0
70.00	131.0
72.00	141.0
73.00	1685.0
74.00	6341.0
75.00	16824.0
76.00	1909.0
76.80	109.0
77.40	112.0
79.00	995.0
80.00	284.0
81.00	972.0
82.10	291.0
87.10	916.0
87.90	924.0
90.70	134.0
91.10	162.0
92.10	808.0
93.10	1610.0
94.10	3403.0
95.10	27920.0
96.10	1959.0
97.00	81.0
103.70	214.0
105.70	129.0
112.00	85.0
114.40	76.0
114.90	54.0
115.80	201.0
116.70	132.0
117.20	231.0
117.90	169.0
118.90	261.0
127.80	170.0
130.00	175.0
131.00	53.0
137.00	73.0
140.90	373.0
142.80	363.0
158.60	90.0
170.50	70.0
172.20	174.0
173.00	139.0
174.00	16512.0
175.00	1257.0
176.00	15108.0
177.00	1145.0
182.20	54.0
184.40	71.0

Instrument :
MSVOA_X
ClientSampleId :
BFB607

m/z	Abundance
36.10	355.0
37.00	1240.0
38.00	1317.0
39.10	505.0
39.90	71.0
44.10	354.0
45.10	275.0
47.00	373.0
47.80	233.0
49.00	1095.0
50.00	5993.0
51.10	1878.0
54.70	147.0
56.10	620.0
57.00	1385.0
60.10	327.0
61.10	1671.0
62.00	1680.0
63.10	1167.0
64.00	53.0
65.20	199.0
66.90	179.0
68.00	3771.0
69.10	3666.0
69.80	288.0
70.40	98.0
71.00	67.0
71.80	321.0
73.00	1723.0
74.00	6176.0
75.00	16792.0
76.00	1354.0
77.80	89.0
78.90	801.0
79.80	405.0
81.00	1128.0
81.80	255.0
87.00	852.0
88.00	1012.0
90.70	198.0
91.90	678.0
93.00	1202.0
94.00	3982.0
95.00	28648.0
96.10	2334.0
97.00	71.0
103.70	264.0
105.80	277.0
110.90	77.0
112.00	121.0
115.80	199.0
116.70	319.0
117.90	155.0
118.70	263.0
128.00	126.0
129.90	175.0
134.80	54.0
140.90	511.0
143.00	806.0
144.50	58.0
157.10	94.0
158.70	113.0
172.00	270.0
173.00	460.0
174.00	18560.0
175.00	1797.0
176.00	19928.0
177.00	1503.0
183.30	55.0
184.40	69.0

Instrument :
MSVOA_X
ClientSampleId :
BFB607