

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102822\
 Data File : VX032465.D
 Acq On : 28 Oct 2022 17:22
 Operator : JC/MD
 Sample : N5313-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TCLP-VOC-GRAB-7-SW-QUARTER

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Title : SW846 8260

Signal : TIC: VX032465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	25	34	51	rBV	8693	29434	2.29%	0.349%
2	2.380	205	212	223	rBV	9322	15883	1.24%	0.188%
3	2.788	272	279	297	rBV	121479	245139	19.06%	2.909%
4	4.721	586	596	608	rBV2	8583	26068	2.03%	0.309%
5	5.385	693	705	720	rBV	74050	217720	16.93%	2.584%
6	5.556	722	733	749	rVB	127817	361966	28.15%	4.295%
7	5.958	789	799	816	rBV	81195	214909	16.71%	2.550%
8	6.342	852	862	875	rBV	53545	138789	10.79%	1.647%
9	6.763	919	931	942	rBV	207172	539564	41.96%	6.403%
10	7.641	1062	1075	1080	rBV	27866	53781	4.18%	0.638%
11	7.696	1080	1084	1091	rVB	9829	18084	1.41%	0.215%
12	7.799	1094	1101	1122	rVV	753526	1285911	100.00%	15.259%
13	8.549	1217	1224	1234	rBV	176672	269240	20.94%	3.195%
14	8.653	1234	1241	1250	rBV	392029	635537	49.42%	7.542%
15	8.952	1284	1290	1302	rBV	217666	320390	24.92%	3.802%
16	9.244	1332	1338	1344	rBV	247939	343984	26.75%	4.082%
17	9.311	1344	1349	1351	rVV	20534	29689	2.31%	0.352%
18	9.348	1351	1355	1357	rVV	35347	55526	4.32%	0.659%
19	9.378	1357	1360	1366	rVB	98846	131185	10.20%	1.557%
20	9.482	1372	1377	1388	rBV	407434	523981	40.75%	6.218%
21	9.579	1388	1393	1408	rVB	272185	347474	27.02%	4.123%
22	9.915	1442	1448	1458	rBV	776431	978056	76.06%	11.606%
23	10.055	1463	1471	1477	rBV	426246	567274	44.11%	6.732%
24	10.281	1504	1508	1519	rBV	9243	13708	1.07%	0.163%
25	10.506	1538	1545	1554	rBV	11194	14822	1.15%	0.176%
26	10.640	1562	1567	1571	rBV	65825	78922	6.14%	0.937%
27	11.079	1634	1639	1651	rBV	348971	460021	35.77%	5.459%
28	12.024	1788	1794	1804	rBV	408589	510076	39.67%	6.053%




Sum of corrected areas: 8427133

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102822\
Data File : VX032465.D
Acq On : 28 Oct 2022 17:22
Operator : JC/MD
Sample : N5313-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TCLP-VOC-GRAB-7-SW-QUARTER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

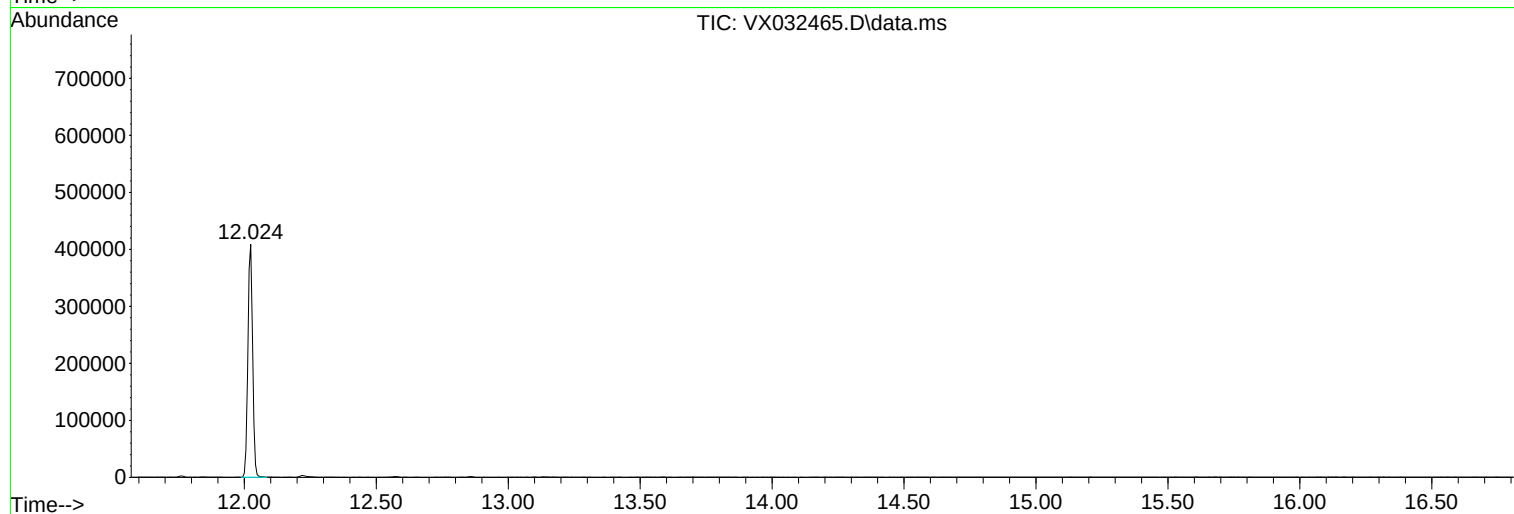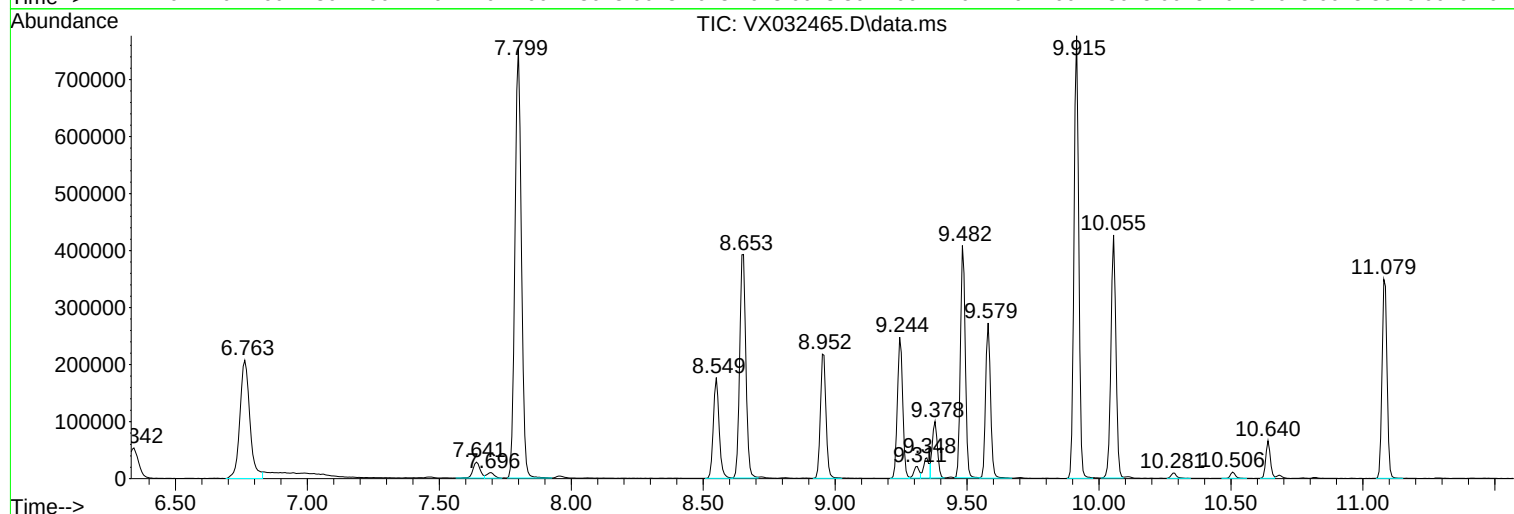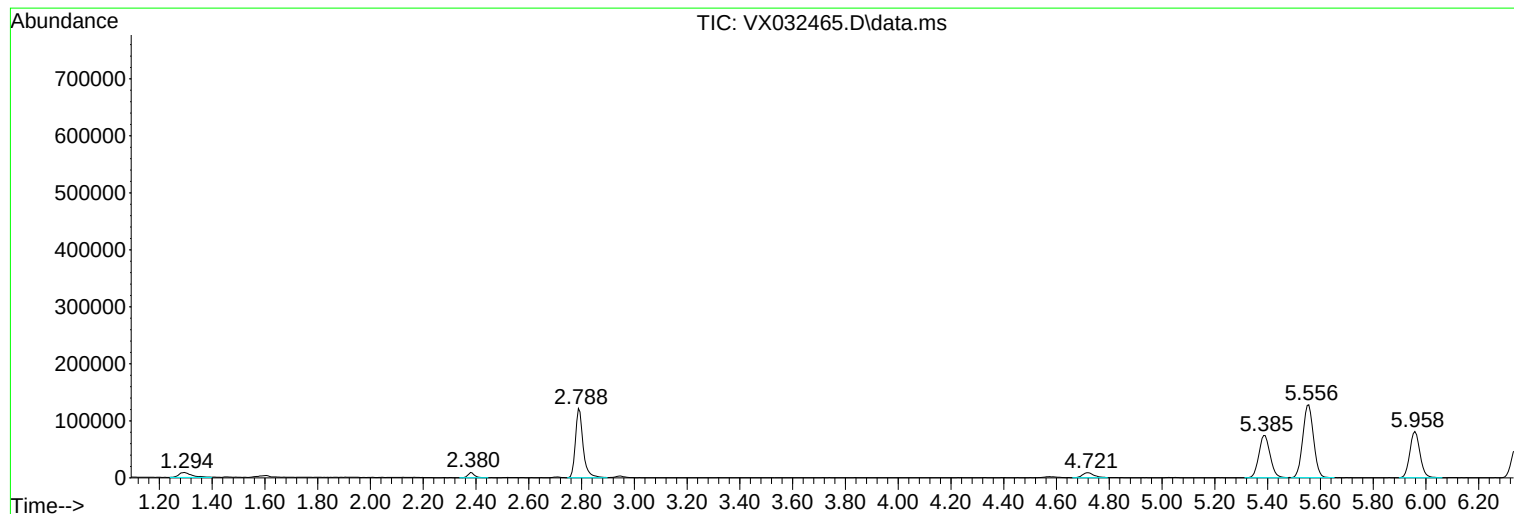

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102822\
Data File : VX032465.D
Acq On : 28 Oct 2022 17:22
Operator : JC/MD
Sample : N5313-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TCLP-VOC-GRAB-7-SW-QUARTER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102822\
Data File : VX032465.D
Acq On : 28 Oct 2022 17:22
Operator : JC/MD
Sample : N5313-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TCLP-VOC-GRAB-7-SW-QUARTER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------