
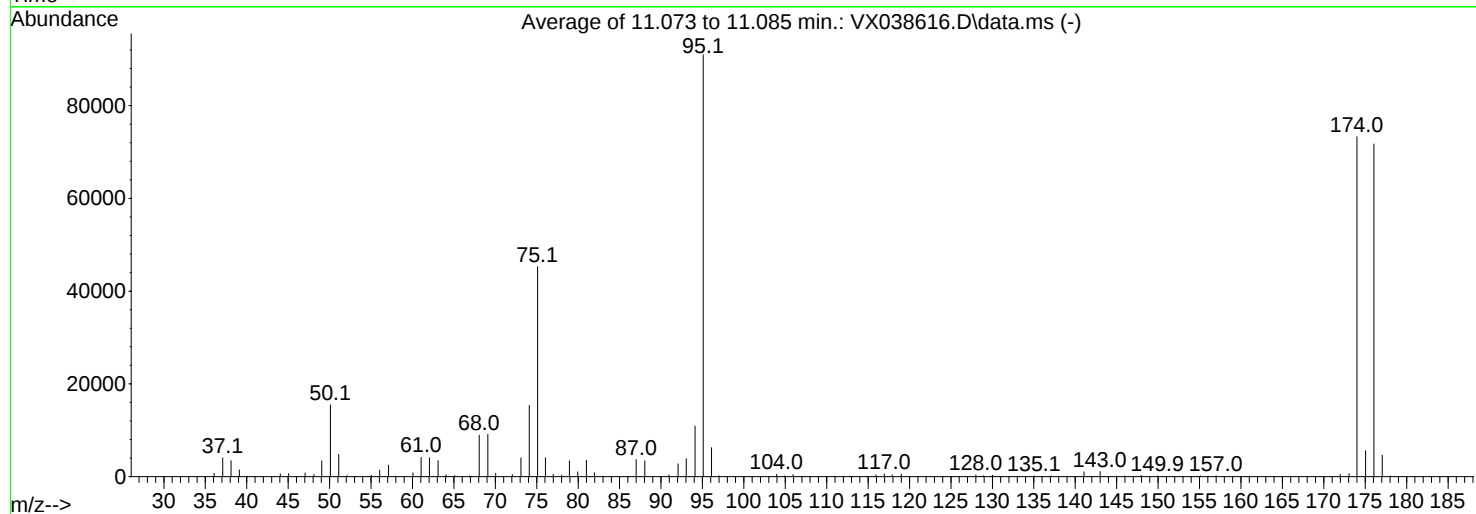


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX102823\
Data File : VX038616.D
Acq On : 27 Oct 2023 21:13
Operator : JC/MD
Sample : BFB651
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB651

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102823WMA.M
Title : VOC Analysis
Last Update : Sat Oct 28 02:45:59 2023

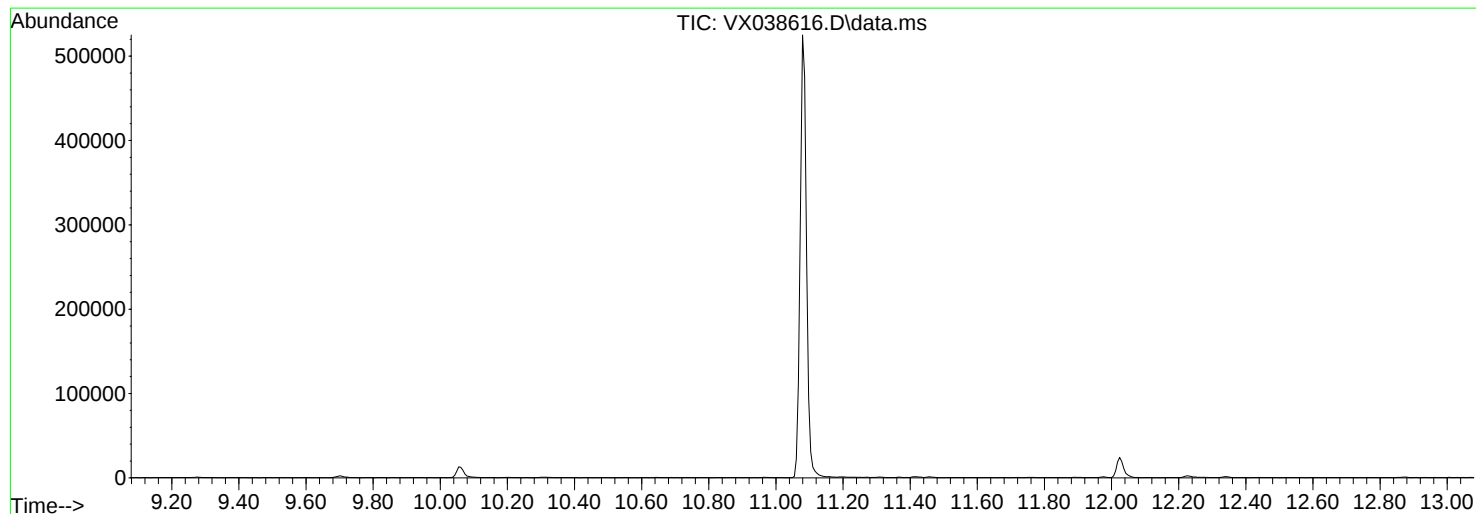

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	15455	PASS
75	95	30	80	49.8	45277	PASS
95	95	100	100	100.0	90952	PASS
96	95	5	9	6.9	6254	PASS
173	174	0.00	2	0.8	610	PASS
174	95	50	120	80.6	73307	PASS
175	174	5	9	7.6	5594	PASS
176	174	95	101	97.8	71720	PASS
177	176	5	9	6.4	4610	PASS

m/z	Abundance
40.10	156.0
44.00	214.0

Instrument :
MSVOA_X
ClientSampleId :
BFB651

m/z	Abundance
36.10	681.0
37.10	3730.0
38.10	2926.0
39.10	1151.0
40.10	217.0
44.10	870.0
45.00	652.0
47.00	687.0
48.10	484.0
49.10	2957.0
50.10	12740.0
51.10	3730.0
52.00	140.0
55.10	253.0
56.10	1018.0
57.10	1767.0
58.00	105.0
60.10	608.0
61.00	3469.0
62.10	2994.0
63.10	2767.0
64.00	286.0
65.10	167.0
66.90	186.0
68.00	6875.0
69.10	6892.0
70.10	601.0
72.00	318.0
73.10	3262.0
74.10	12432.0
75.10	35624.0
76.10	3328.0
77.10	531.0
78.10	269.0
78.90	2785.0
80.00	791.0
81.00	2615.0
81.90	574.0
82.90	71.0
85.90	107.0
87.00	2751.0
88.10	2514.0
91.00	240.0
92.00	1884.0
93.00	2830.0
94.10	8311.0
95.10	68728.0
96.10	4683.0
97.00	126.0
104.00	335.0
104.90	121.0
106.00	324.0
109.80	51.0
111.00	98.0
112.00	56.0
112.80	72.0
113.10	86.0
114.80	86.0
116.00	284.0
117.00	472.0
117.90	243.0
119.00	369.0
123.90	58.0
128.00	356.0
129.10	103.0
129.80	203.0
130.80	96.0
135.00	114.0
136.80	65.0
137.20	98.0
141.10	616.0
141.80	176.0
143.00	811.0
145.00	119.0
146.00	141.0
148.00	173.0
150.00	107.0
154.80	86.0
155.30	75.0
157.00	113.0
158.90	52.0
160.80	87.0
172.00	407.0
173.00	360.0
174.00	46264.0
175.00	3695.0
176.00	45576.0
177.10	3008.0
178.20	91.0

Instrument :
MSVOA_X
ClientSampleId :
BFB651

m/z	Abundance
36.00	891.0
37.10	4791.0
38.10	3868.0
39.10	1762.0
40.00	286.0
44.10	860.0
45.10	801.0
46.20	107.0
47.10	926.0
48.10	483.0
49.10	4258.0
50.10	18320.0
51.10	5878.0
52.10	352.0
55.00	309.0
56.10	1698.0
57.10	3217.0
57.90	151.0
60.10	1013.0
61.10	4878.0
62.10	5084.0
63.10	4138.0
64.10	452.0
65.00	333.0
66.90	349.0
68.10	11006.0
69.10	11269.0
70.00	762.0
72.10	584.0
73.10	4620.0
74.10	18304.0
75.10	55456.0
76.00	4784.0
76.90	537.0
78.00	378.0
79.00	4058.0
80.00	1356.0
81.00	4346.0
82.00	1099.0
83.00	97.0
86.10	158.0
87.00	4786.0
88.00	4141.0
90.90	431.0
92.10	3688.0
93.10	4488.0
94.10	12830.0
95.10	109968.0
96.10	8006.0
97.00	250.0
103.90	665.0
104.90	212.0
106.00	587.0
107.10	106.0
109.90	58.0
110.80	146.0
112.10	89.0
112.90	90.0
115.00	83.0
115.90	340.0
116.90	740.0
117.90	548.0
119.00	705.0
128.00	320.0
128.90	289.0
130.00	438.0
131.10	139.0
135.00	220.0
137.00	232.0
141.00	1219.0
142.00	154.0
143.00	1337.0
144.00	114.0
144.90	168.0
146.00	118.0
147.90	301.0
150.00	136.0
154.00	86.0
155.10	213.0
156.90	199.0
159.00	106.0
161.00	112.0
170.90	70.0
172.00	536.0
173.00	678.0
174.00	86000.0
175.10	6499.0
176.00	82800.0
177.00	5424.0
178.10	198.0

Instrument :
MSVOA_X
ClientSampleId :
BFB651

m/z	Abundance
36.00	592.0
37.10	3659.0
38.10	3560.0
39.10	1409.0
40.10	300.0
44.10	720.0
45.00	552.0
46.10	74.0
47.00	760.0
48.10	513.0
49.00	3063.0
50.10	15306.0
51.10	4774.0
52.20	201.0
55.00	308.0
56.00	1464.0
57.10	2465.0
58.00	112.0
60.00	876.0
61.10	4092.0
62.00	4094.0
63.10	3430.0
64.00	371.0
65.20	248.0
67.10	232.0
68.10	8932.0
69.10	9241.0
70.10	816.0
72.00	438.0
73.10	4246.0
74.10	15311.0
75.10	44752.0
76.10	4146.0
77.00	410.0
77.90	397.0
79.00	3366.0
79.90	1008.0
81.00	3533.0
81.90	902.0
83.10	107.0
86.00	191.0
87.00	3526.0
88.00	3583.0
90.90	414.0
92.10	2682.0
93.10	4286.0
94.10	11619.0
95.10	94160.0
96.10	6072.0
97.00	120.0
103.90	452.0
104.90	164.0
105.90	448.0
107.10	111.0
109.90	56.0
110.90	103.0
112.00	116.0
112.90	116.0
114.80	117.0
115.90	514.0
116.90	668.0
117.90	347.0
119.00	598.0
128.00	361.0
128.90	243.0
130.00	534.0
130.90	160.0
135.10	227.0
137.00	187.0
141.00	1228.0
142.00	214.0
143.00	1212.0
143.90	119.0
144.90	109.0
145.90	113.0
147.90	362.0
149.90	136.0
154.00	121.0
155.00	264.0
157.10	255.0
159.00	138.0
161.10	161.0
170.80	86.0
172.00	546.0
173.10	793.0
174.00	87656.0
175.00	6588.0
176.10	86784.0
177.00	5398.0
178.00	176.0

Instrument :
MSVOA_X
ClientSampleId :
BFB651