


Data Path : \\74.0.250.170\terastorage\voasrv\HPCHEM1\MSVOA_X\Data\VX102919\
Data File : VX013260.D
Acq On : 29 Oct 2019 09:58
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102419W.M
Title : SW846 8260
Last Update : Thu Oct 24 03:56:38 2019

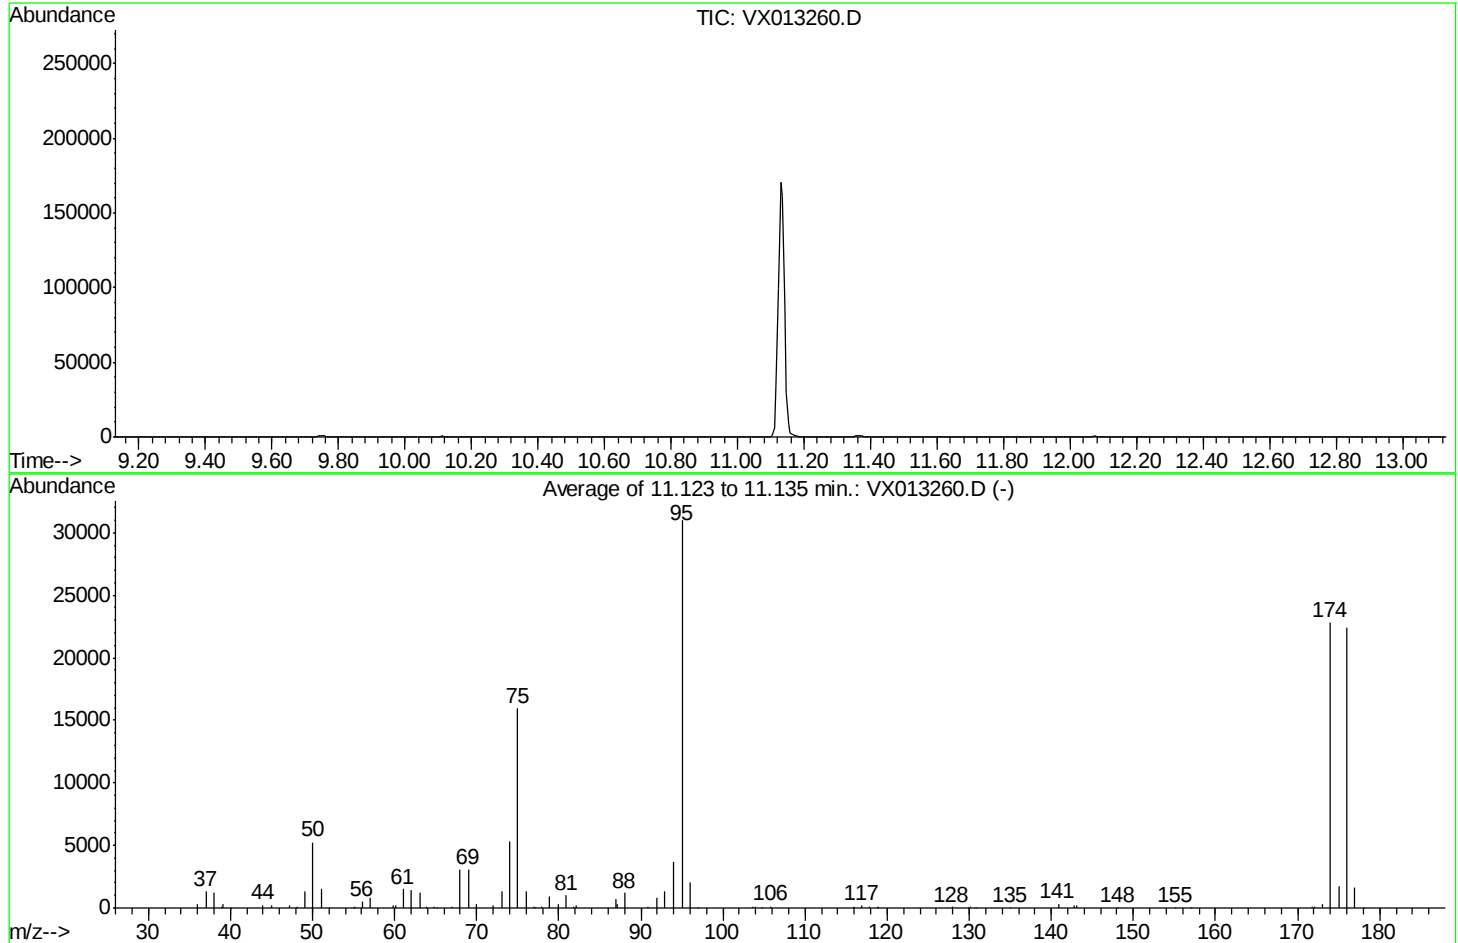

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	5230	PASS
75	95	30	60	51.4	15931	PASS
95	95	100	100	100.0	30986	PASS
96	95	5	9	6.5	2002	PASS
173	174	0.00	2	1.3	304	PASS
174	95	50	100	73.6	22813	PASS
175	174	5	9	7.7	1763	PASS
176	174	95	101	98.2	22403	PASS
177	176	5	9	7.2	1613	PASS