

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102920\
 Data File : VX019177.D
 Acq On : 28 Oct 2020 21:15
 Operator : JC/MD
 Sample : L4485-09
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MDL-WATER-02

Quant Time: Oct 29 06:34:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 29 06:24:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	186800	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	166482	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.06	152	76167	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	63033	5.22	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.40%
7) Chloroethane-d5	1.70	69	52095	5.17	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.40%
11) 1,1-Dichloroethene-d2	2.34	63	92750	3.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.60%
20) 2-Butanone-d5	4.56	46	143668	54.40	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.80%
24) Chloroform-d	5.14	84	114581	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
26) 1,2-Dichloroethane-d4	6.03	65	62961	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.20%
32) Benzene-d6	6.05	84	237537	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.80%
36) 1,2-Dichloropropane-d6	7.37	67	68913	5.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.20%
41) Toluene-d8	8.70	98	221153	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
43) trans-1,3-Dichloropropene-	8.99	79	28321	5.12	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.40%
46) 2-Hexanone-d5	9.43	63	131107	54.11	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.22%
56) 1,1,2,2-Tetrachloroethane-	11.23	84	50890	5.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.20%
66) 1,2-Dichlorobenzene-d4	12.36	152	76371	5.40	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.00%

Target Compounds

					Ovalue
2) Dichlorodifluoromethane	1.18	85	3582	0.232 ug/L	100
3) Chloromethane	1.31	50	3417	0.256 ug/L	96
5) Vinyl chloride	1.39	62	3525	0.235 ug/L #	70
6) Bromomethane	1.64	94	2527	0.261 ug/L	99
8) Chloroethane	1.72	64	2336	0.257 ug/L	98
9) Trichlorofluoromethane	1.92	101	5138	0.237 ug/L	90
10) 1,1,2-Trichloro-1,2,2-trif	2.37	101	3790	0.308 ug/L #	78
12) 1,1-Dichloroethene	2.36	96	3789	0.316 ug/L #	1
13) Acetone	2.46	43	3598	2.389 ug/L	65
14) Carbon disulfide	2.55	76	8966	0.241 ug/L	96
15) Methyl Acetate	2.76	43	1098	0.273 ug/L	92
16) Methylene chloride	2.83	84	5377	0.376 ug/L	96
17) Methyl tert-butyl Ether	3.17	73	6609	0.230 ug/L	97
18) trans-1,2-Dichloroethene	3.14	96	2978	0.236 ug/L	98
19) 1,1-Dichloroethane	3.67	63	4898	0.227 ug/L	96
21) 2-Butanone	4.67	43	5548	2.098 ug/L	94
22) cis-1,2-Dichloroethene	4.56	96	3131	0.233 ug/L	94

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102920\
 Data File : VX019177.D
 Acq On : 28 Oct 2020 21:15
 Operator : JC/MD
 Sample : L4485-09
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MDL-WATER-02

Quant Time: Oct 29 06:34:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 29 06:24:00 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
23) Bromochloromethane	4.98	128	1183	0.212	ug/L	84
25) Chloroform	5.18	83	6109	0.272	ug/L	92
27) 1,2-Dichloroethane	6.17	62	3482	0.248	ug/L	96
29) 1,1,1-Trichloroethane	5.46	97	4657	0.227	ug/L	97
30) Cyclohexane	5.55	56	4676	0.228	ug/L	96
31) Carbon tetrachloride	5.74	117	3757	0.215	ug/L	95
33) Benzene	6.10	78	11632	0.235	ug/L	100
34) Trichloroethene	7.19	95	3177	0.234	ug/L	97
35) Methylcyclohexane	7.44	83	4850	0.221	ug/L	97
37) 1,2-Dichloropropane	7.49	63	2818	0.241	ug/L #	86
38) Bromodichloromethane	7.87	83	3412	0.224	ug/L	92
39) cis-1,3-Dichloropropene	8.42	75	3748	0.209	ug/L	97
40) 4-Methyl-2-pentanone	8.62	43	14072	2.254	ug/L #	87
42) Toluene	8.76	91	12232	0.228	ug/L	100
44) trans-1,3-Dichloropropene	9.02	75	4624	0.308	ug/L	89
45) 1,1,2-Trichloroethane	9.20	97	1889	0.221	ug/L	98
47) Tetrachloroethene	9.31	164	2310	0.223	ug/L	91
48) 2-Hexanone	9.48	43	11282	2.584	ug/L	99
49) Dibromochloromethane	9.57	129	2071	0.210	ug/L	96
50) 1,2-Dibromoethane	9.66	107	1806	0.228	ug/L #	98
51) Chlorobenzene	10.12	112	7589	0.224	ug/L	94
52) Ethylbenzene	10.23	91	13033	0.217	ug/L	99
53) m,p-xylene	10.34	106	5120	0.223	ug/L	97
54) o-xylene	10.68	106	4910	0.223	ug/L	96
55) Styrene	10.70	104	7462	0.207	ug/L	95
57) 1,1,2,2-Tetrachloroethane	11.25	83	2426	0.250	ug/L #	90
59) Bromoform	10.84	173	1047	0.209	ug/L #	94
60) Isopropylbenzene	11.00	105	12608	0.225	ug/L	99
61) 1,2,3-Trichloropropane	11.28	75	1603	0.235	ug/L	95
62) 1,3,5-Trimethylbenzene	11.49	105	10133	0.216	ug/L	99
63) 1,2,4-Trimethylbenzene	11.79	105	10147	0.214	ug/L	99
64) 1,3-Dichlorobenzene	12.01	146	5735	0.231	ug/L	97
65) 1,4-Dichlorobenzene	12.08	146	6064	0.244	ug/L	98
67) 1,2-Dichlorobenzene	12.38	146	5498	0.241	ug/L	92
68) 1,2-Dibromo-3-chloropropan	12.98	75	397	0.254	ug/L #	71
69) 1,3,5-Trichlorobenzene	13.15	180	4086	0.224	ug/L	98
70) 1,2,4-trichlorobenzene	13.63	180	3435	0.216	ug/L	99
71) Naphthalene	13.82	128	5833	0.204	ug/L	99
72) 1,2,3-Trichlorobenzene	14.00	180	3089	0.220	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX102920\
Data File : VX019177.D
Acq On : 28 Oct 2020 21:15
Operator : JC/MD
Sample : L4485-09
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-02

Quant Time: Oct 29 06:34:52 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 29 06:24:00 2020
Response via : Initial Calibration

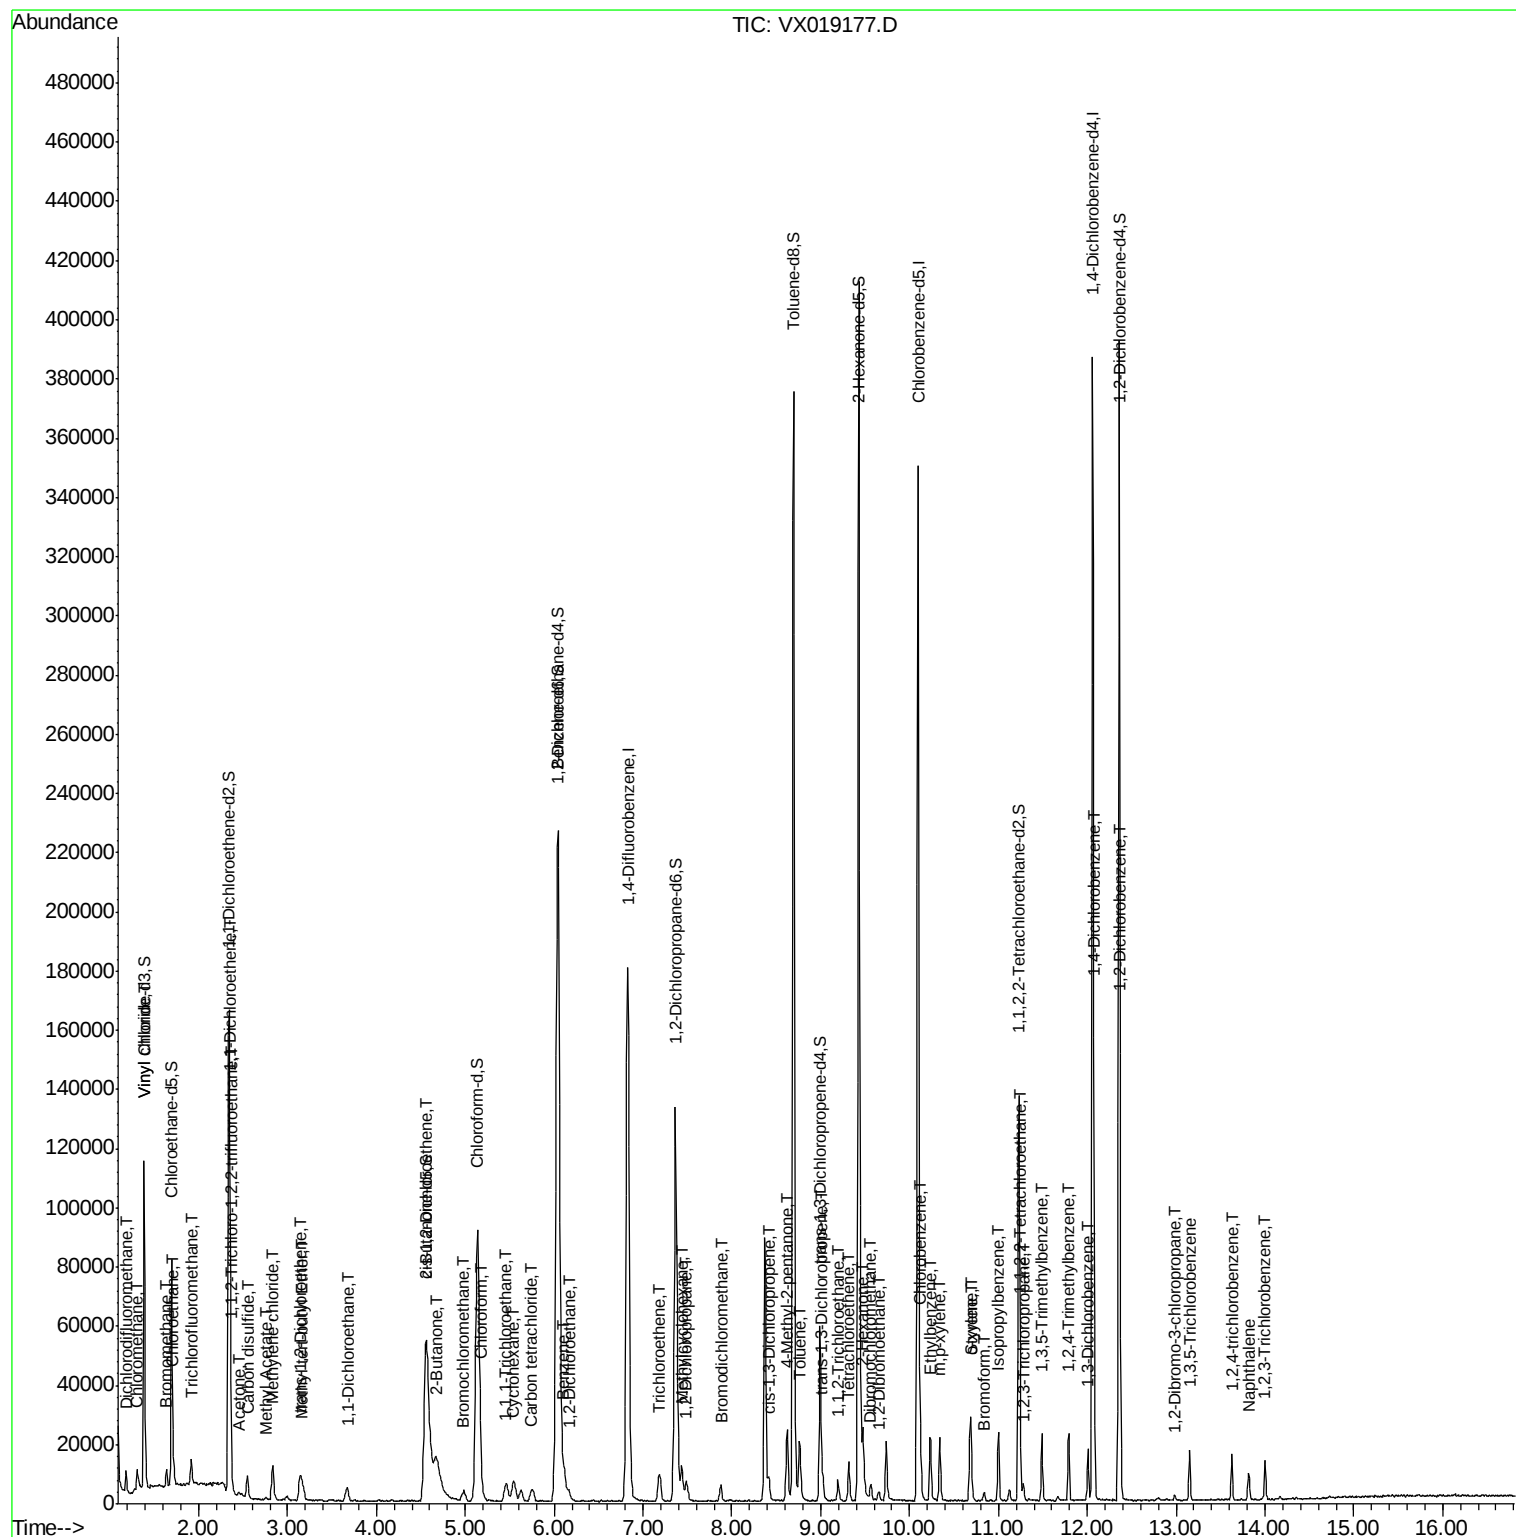



#2

Dichlorodifluoromethane

Concen: 0.232 ug/L

RT: 1.18 min Scan# 16

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :


MDL-WATER-02

Tot Ion: 85 Resp: 3582

Ion Ratio Lower Upper




85 100

87 32.4 26.1 39.1

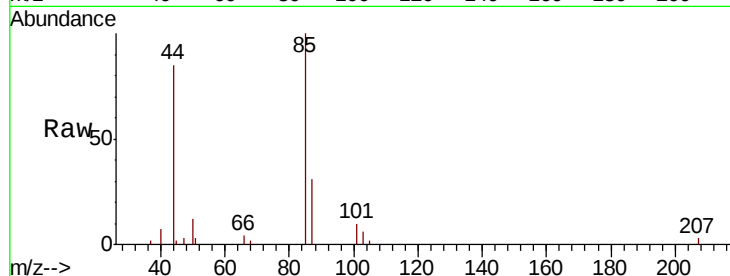

Abundance Ion 85.00 (84.70 to 85.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

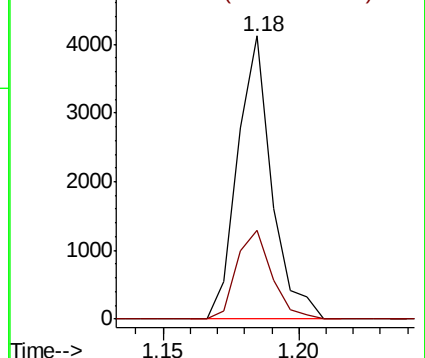

#3

Chloromethane

Concen: 0.256 ug/L

RT: 1.31 min Scan# 36

Delta R.T. -0.00 min

Lab File: VX019177.D


Acq: 28 Oct 2020 21:15

Tgt Ion: 50 Resp: 3417

Ion Ratio Lower Upper



50 100


52 31.2 23.4 43.6



Abundance Ion 50.05 (49.75 to 50.75): VX0

Ion 52.05 (51.75 to 52.75): VX0

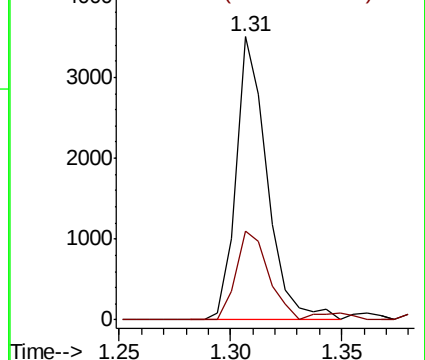



#5

Vinyl chloride

Concen: 0.235 ug/L

RT: 1.39 min Scan# 50

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :


MDL-WATER-02

Tot Ion: 62 Resp: 3525

Ion Ratio Lower Upper

62 100

64 50.5 23.5 43.7#

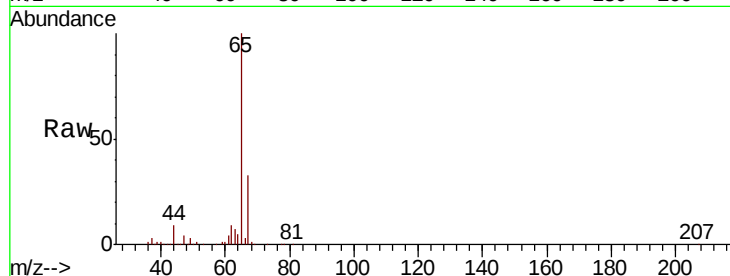

Abundance Ion 62.00 (61.70 to 62.70): VX0

Ion 64.10 (63.80 to 64.80): VX0

1.39

4000

3000

2000

1000



0

1.35

1.40

1.45

Time-->



#6

Bromomethane

Concen: 0.261 ug/L

RT: 1.64 min Scan# 90

Delta R.T. -0.00 min

Lab File: VX019177.D


Acq: 28 Oct 2020 21:15

Tgt Ion: 94 Resp: 2527

Ion Ratio Lower Upper

94 100

96 98.4 67.9 126.1



Abundance Ion 94.00 (93.70 to 94.70): VX0

Ion 96.00 (95.70 to 96.70): VX0

1.64

2000

1500

1000

500


0


1.60

1.65

1.70

Time-->









#8
Chloroethane
Concen: 0.257 ug/L
RT: 1.72 min Scan# 103
Delta R.T. -0.00 min
Lab File: VX019177.D
Acq: 28 Oct 2020 21:15




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-02


Tot Ion: 64 Resp: 2336
Ion Ratio Lower Upper
64 100
66 31.5 22.7 42.1

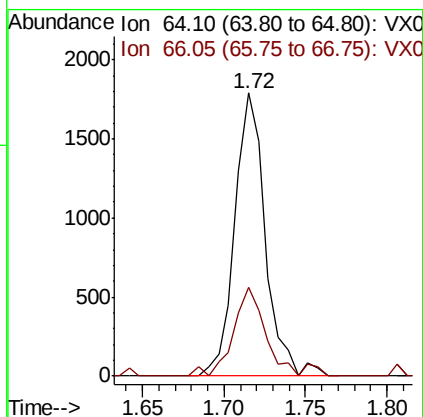

#9
Trichlorofluoromethane
Concen: 0.237 ug/L
RT: 1.92 min Scan# 136
Delta R.T. -0.00 min
Lab File: VX019177.D
Acq: 28 Oct 2020 21:15

Tgt Ion: 101 Resp: 5138
Ion Ratio Lower Upper
101 100
103 72.5 51.9 77.9

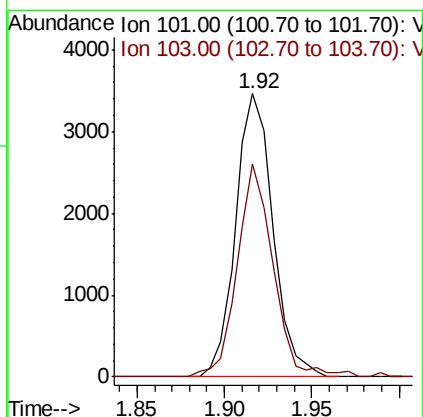

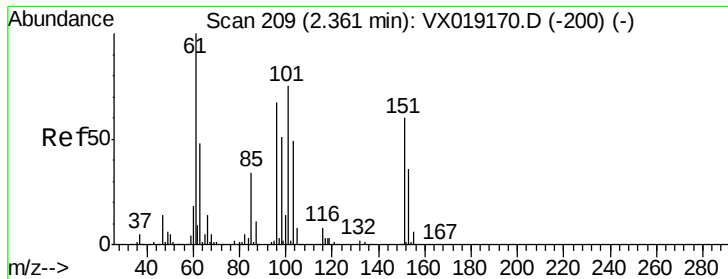

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.308 ug/L

RT: 2.37 min Scan# 210

Delta R.T. 0.01 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :

MDL-WATER-02


Tot Ion:101 Resp: 3790

Ion Ratio Lower Upper

101 100

85 36.1 35.3 52.9




151 52.2 60.9 91.3#

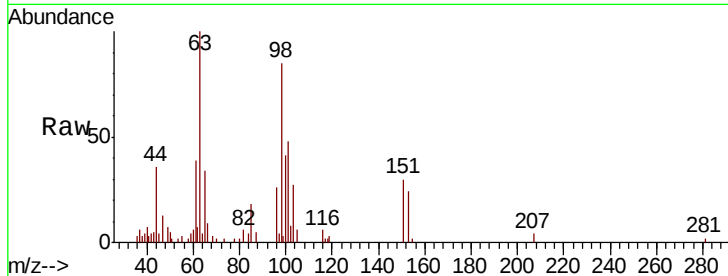

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VX0

Ion 151.00 (150.70 to 151.70): V

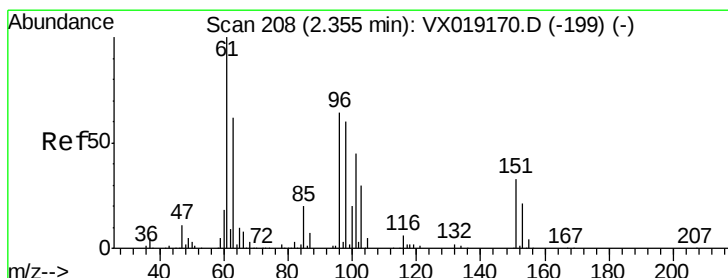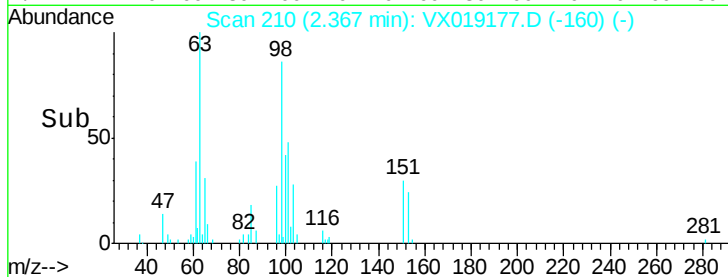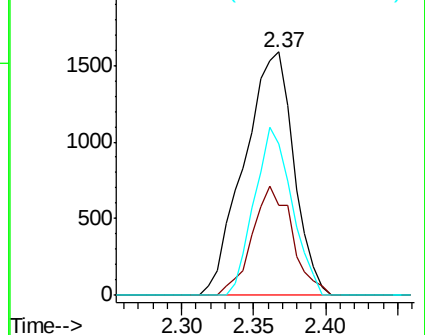

#12

1,1-Dichloroethene

Concen: 0.316 ug/L

RT: 2.36 min Scan# 208

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15


Tgt Ion: 96 Resp: 3789

Ion Ratio Lower Upper

96 100

61 268.9 109.5 203.3#



63 1088.5 68.3 126.9#

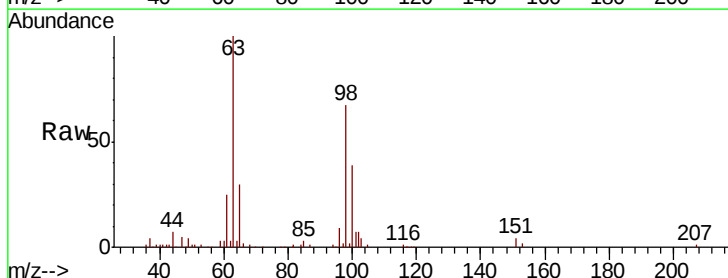


Abundance Ion 96.00 (95.70 to 96.70): VX0

Ion 61.05 (60.75 to 61.75): VX0

Ion 63.00 (62.70 to 63.70): VX0

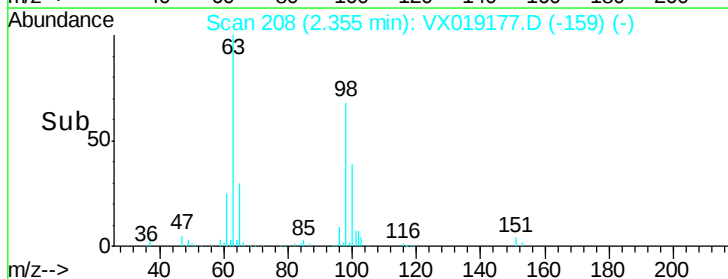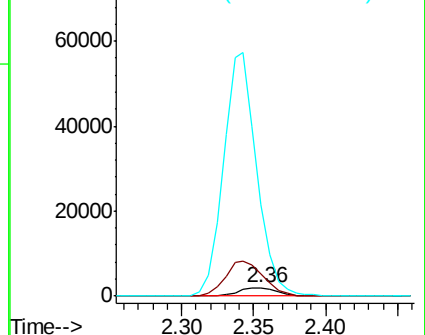



#13

Acetone

Concen: 2.389 ug/L

RT: 2.46 min Scan# 225

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :


MDL-WATER-02

Tot Ion: 43 Resp: 3598

Ion Ratio Lower Upper




43 100

58 13.2 0.0 65.4



Abundance Ion 43.05 (42.75 to 43.75): VX0

Ion 58.05 (57.75 to 58.75): VX0

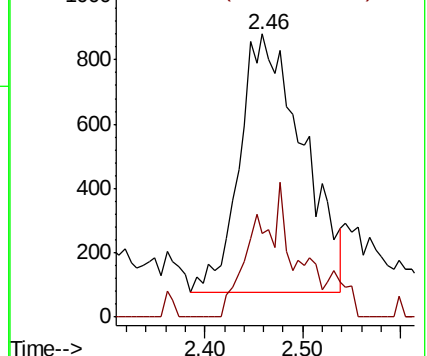

#14

Carbon disulfide

Concen: 0.241 ug/L

RT: 2.55 min Scan# 240

Delta R.T. -0.00 min

Lab File: VX019177.D


Acq: 28 Oct 2020 21:15

Tgt Ion: 76 Resp: 8966

Ion Ratio Lower Upper



76 100


78 7.9 7.4 11.0



Abundance Ion 76.05 (75.75 to 76.75): VX0

Ion 78.00 (77.70 to 78.70): VX0




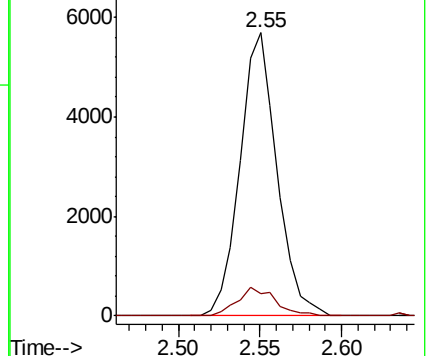




#15
Methyl Acetate
Concen: 0.273 ug/L
RT: 2.76 min Scan# 274
Delta R.T. -0.00 min
Lab File: VX019177.D
Acq: 28 Oct 2020 21:15




Instrument :
MSVOA_X
ClientSampled :
MDL-WATER-02


Tot Ion: 43 Resp: 1098
Ion Ratio Lower Upper
43 100
74 32.3 22.3 33.5

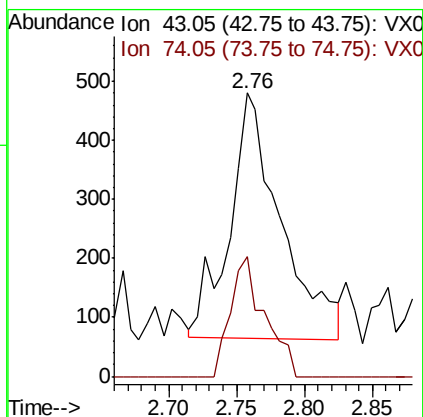

#16
Methylene chloride
Concen: 0.376 ug/L
RT: 2.83 min Scan# 286
Delta R.T. -0.00 min
Lab File: VX019177.D
Acq: 28 Oct 2020 21:15

Tgt Ion: 84 Resp: 5377
Ion Ratio Lower Upper
84 100
86 67.5 42.2 78.4
49 109.7 77.5 143.9



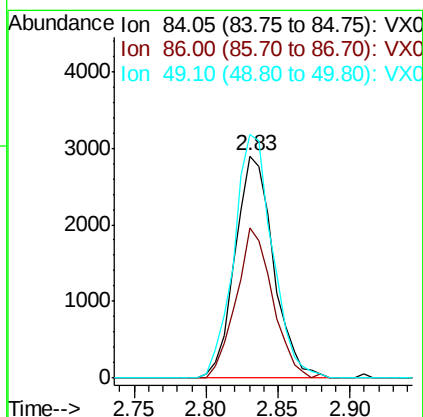





#17
Methvl tert-butvl Ether
Concen: 0.230 ug/L
RT: 3.17 min Scan# 342
Delta R.T. 0.01 min
Lab File: VX019177.D
Acq: 28 Oct 2020 21:15




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-02


Tot Ion: 73 Resp: 6609
Ion Ratio Lower Upper
73 100
43 17.1 16.1 24.1
57 21.1 16.8 25.2

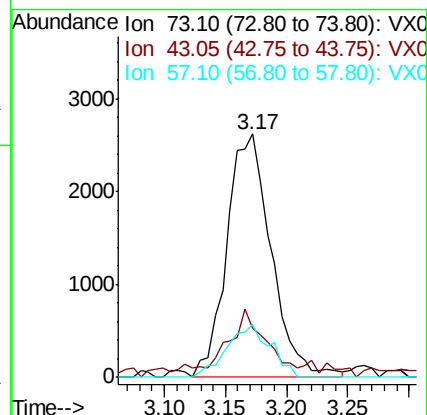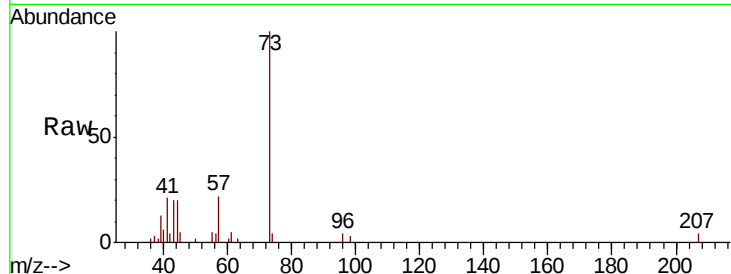

#18
trans-1,2-Dichloroethene
Concen: 0.236 ug/L
RT: 3.14 min Scan# 337
Delta R.T. 0.01 min
Lab File: VX019177.D
Acq: 28 Oct 2020 21:15

Tgt Ion: 96 Resp: 2978
Ion Ratio Lower Upper
96 100
61 135.0 93.7 173.9
98 63.7 42.8 79.6



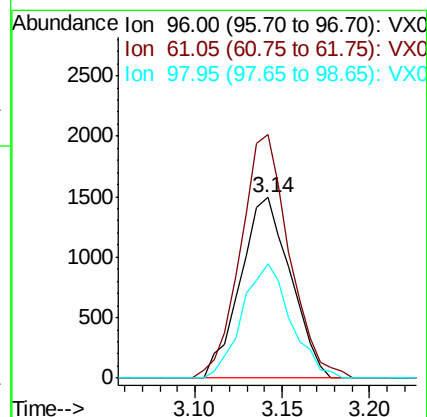





#19
 1,1-Dichloroethane
 Concen: 0.227 ug/L
 RT: 3.67 min Scan# 424
 Delta R.T. 0.01 min
 Lab File: VX019177.D
 Acq: 28 Oct 2020 21:15




Instrument :
 MSVOA_X
 ClientSampleId :
 MDL-WATER-02


Tot Ion	Ratio	Lower	Upper
63	100		
65	34.2	22.5	41.9
83	15.6	9.7	17.9

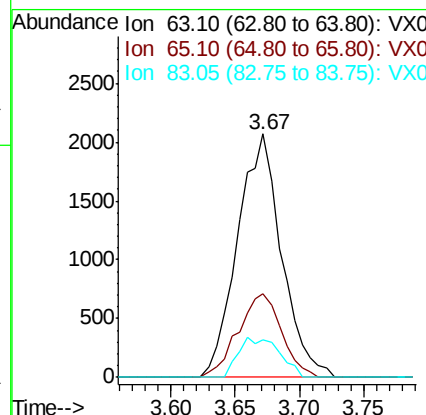

#21
 2-Butanone
 Concen: 2.098 ug/L
 RT: 4.67 min Scan# 587
 Delta R.T. 0.01 min
 Lab File: VX019177.D
 Acq: 28 Oct 2020 21:15

Tgt Ion	Ratio	Lower	Upper
43	100		
72	25.6	14.4	43.4

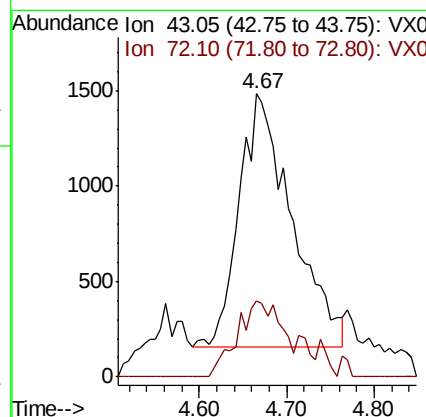







#22

cis-1,2-Dichloroethene
 Concen: 0.233 ug/L
 RT: 4.56 min Scan# 570
 Delta R.T. -0.00 min
 Lab File: VX019177.D
 Acq: 28 Oct 2020 21:15

Instrument :
 MSVOA_X
 ClientSampleId :
 MDL-WATER-02




Tot Ion	Ratio	Lower	Upper
96	100		
61	115.6	85.7	159.1
68	0.0	0.0	0.0

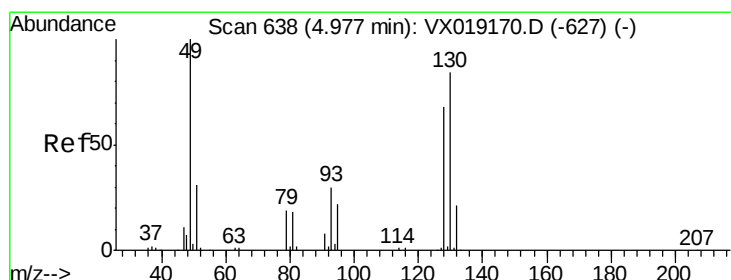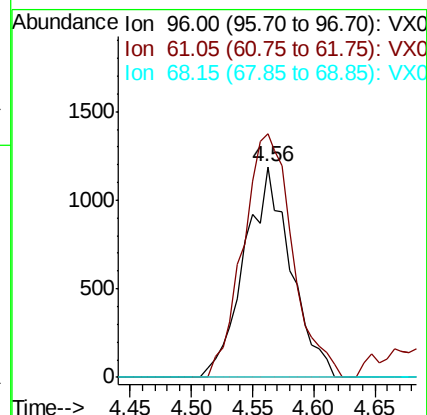


#23

Bromochloromethane
 Concen: 0.212 ug/L
 RT: 4.98 min Scan# 638
 Delta R.T. -0.00 min
 Lab File: VX019177.D
 Acq: 28 Oct 2020 21:15

Tgt Ion	Ratio	Lower	Upper
128	100		
49	167.2	102.8	191.0
130	146.1	86.3	160.3
51	42.5	36.5	54.7

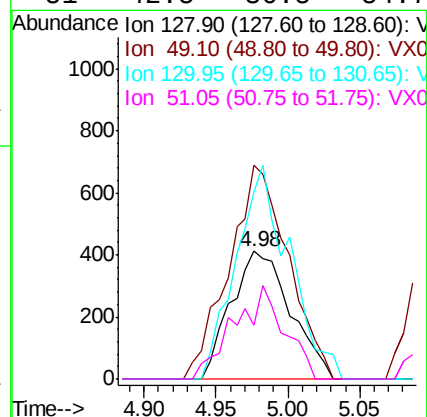



#25

Chloroform

Concen: 0.272 ug/L

RT: 5.18 min Scan# 671

Delta R.T. 0.01 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :


MDL-WATER-02

Tot Ion: 83 Resp: 6109

Ion Ratio Lower Upper




83 100

85 61.5 47.6 88.4



Abundance Ion 83.05 (82.75 to 83.75): VX0

Ion 85.00 (84.70 to 85.70): VX0

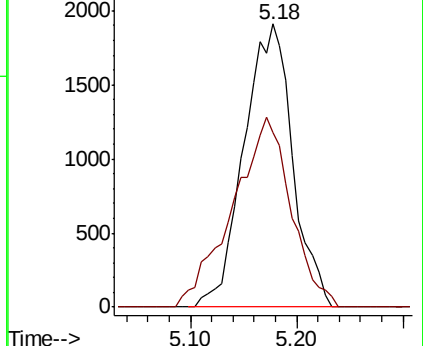

#27

1,2-Dichloroethane

Concen: 0.248 ug/L

RT: 6.17 min Scan# 833

Delta R.T. 0.01 min

Lab File: VX019177.D


Acq: 28 Oct 2020 21:15

Tgt Ion: 62 Resp: 3482

Ion Ratio Lower Upper



62 100


98 10.8 7.4 11.0



Abundance Ion 62.00 (61.70 to 62.70): VX0

Ion 98.05 (97.75 to 98.75): VX0

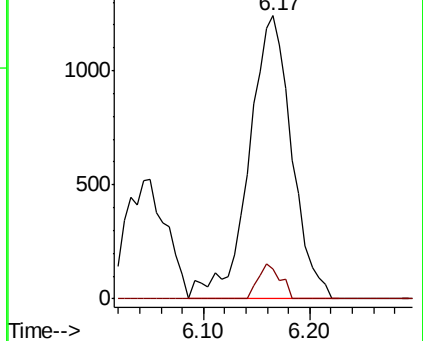

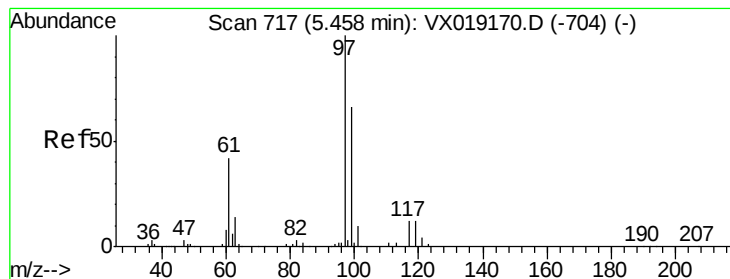

#29

1,1,1-Trichloroethane

Concen: 0.227 ug/L

RT: 5.46 min Scan# 717

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :

MDL-WATER-02


Tot Ion: 97 Resp: 4657

Ion Ratio Lower Upper

97 100

99 61.3 51.8 77.8




61 42.6 34.5 51.7

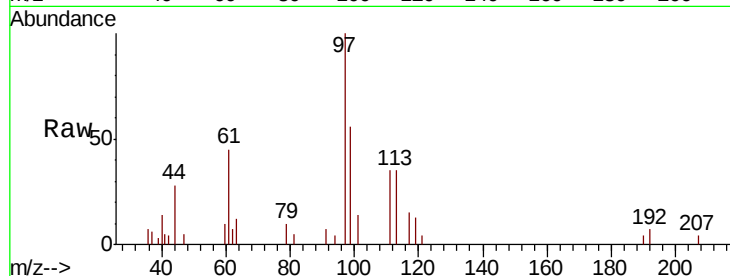

Abundance Ion 96.95 (96.65 to 97.65): VX0

Ion 99.05 (98.75 to 99.75): VX0

Ion 61.05 (60.75 to 61.75): VX0

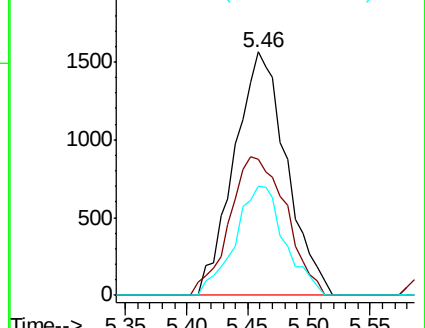

#30

Cyclohexane

Concen: 0.228 ug/L

RT: 5.55 min Scan# 732

Delta R.T. 0.01 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15


Tgt Ion: 56 Resp: 4676

Ion Ratio Lower Upper

56 100

69 34.2 26.2 39.2



84 97.3 74.5 111.7




Abundance Ion 56.10 (55.80 to 56.80): VX0

Ion 69.15 (68.85 to 69.85): VX0

Ion 84.15 (83.85 to 84.85): VX0

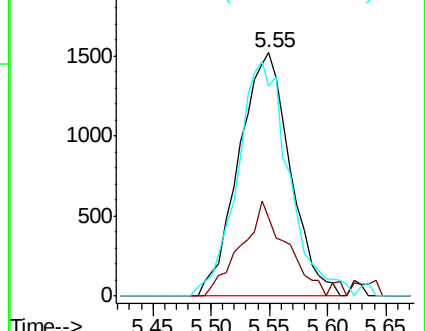



#31

Carbon tetrachloride

Concen: 0.215 ug/L

RT: 5.74 min Scan# 764

Delta R.T. -0.01 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :


MDL-WATER-02

Tot Ion:117 Resp: 3757

Ion Ratio Lower Upper




117 100

119 101.5 77.3 115.9



Abundance Ion 116.90 (116.60 to 117.60): V

Ion 118.90 (118.60 to 119.60): V

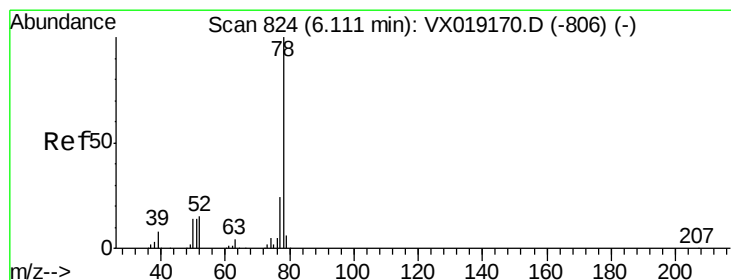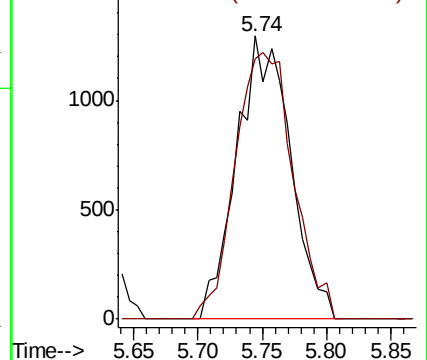

#33

Benzene

Concen: 0.235 ug/L


RT: 6.10 min Scan# 823

Delta R.T. -0.01 min



Lab File: VX019177.D


Acq: 28 Oct 2020 21:15

Tgt Ion: 78 Resp: 11632



Abundance Ion 78.10 (77.80 to 78.80): VX0

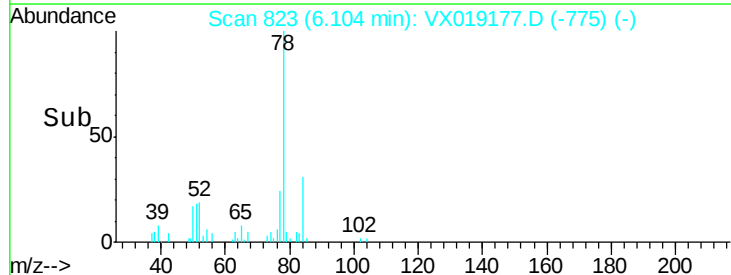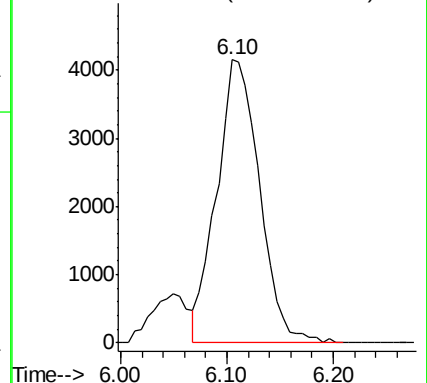



#34

Trichloroethene

Concen: 0.234 ug/L

RT: 7.19 min Scan# 1001

Delta R.T. 0.01 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :

MDL-WATER-02

Tot Ion: 95 Resp: 3177


Ion Ratio Lower Upper

95 100

97 68.3 45.2 84.0

132 89.8 65.3 121.3

130 99.3 70.6 131.0






Abundance Ion 95.00 (94.70 to 95.70): VX0

Ion 96.95 (96.65 to 97.65): VX0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

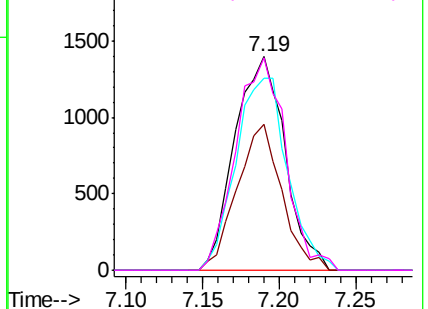

#35

Methylcyclohexane

Concen: 0.221 ug/L

RT: 7.44 min Scan# 1042

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15


Tgt Ion: 83 Resp: 4850

Ion Ratio Lower Upper

83 100

55 75.8 58.5 87.7



98 48.2 40.1 60.1




Abundance Ion 83.15 (82.85 to 83.85): VX0

Ion 55.10 (54.80 to 55.80): VX0

Ion 98.15 (97.85 to 98.85): VX0

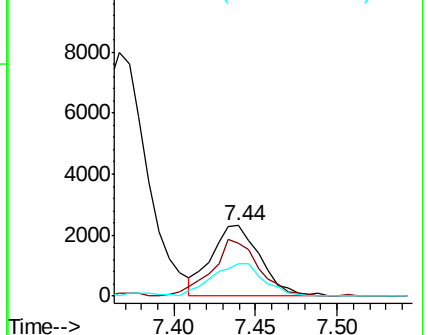



#37

1,2-Dichloropropane

Concen: 0.241 ug/L

RT: 7.49 min Scan# 1051

Delta R.T. 0.01 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :


MDL-WATER-02

Tot Ion: 63 Resp: 2818

Ion Ratio Lower Upper




63 100

112 0.0 3.8 5.6#



Abundance Ion 63.10 (62.80 to 63.80): VX0

Ion 112.10 (111.80 to 112.80): V

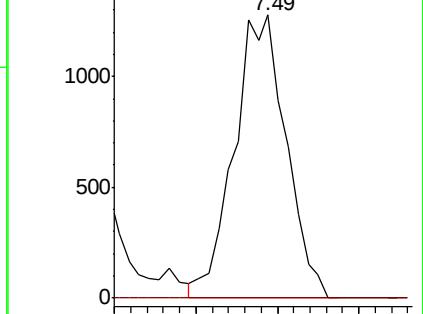

#38

Bromodichloromethane

Concen: 0.224 ug/L

RT: 7.87 min Scan# 1113

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15


Tgt Ion: 83 Resp: 3412

Ion Ratio Lower Upper

83 100

85 56.7 44.4 82.5



127 10.1 7.2 10.8




Abundance Ion 82.95 (82.65 to 83.65): VX0

Ion 85.00 (84.70 to 85.70): VX0

Ion 126.90 (126.60 to 127.60): V

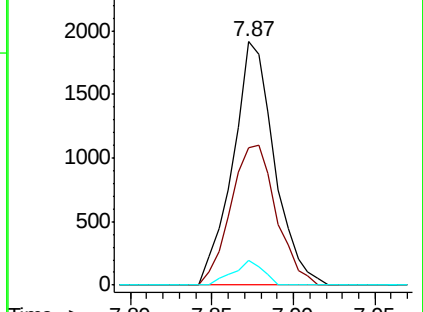



#39

cis-1,3-Dichloropropene

Concen: 0.209 ug/L

RT: 8.42 min Scan# 1202

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :





MDL-WATER-02

Tot Ion: 75 Resp: 3748

Ion Ratio Lower Upper

75 100

77 32.8 21.8 40.6

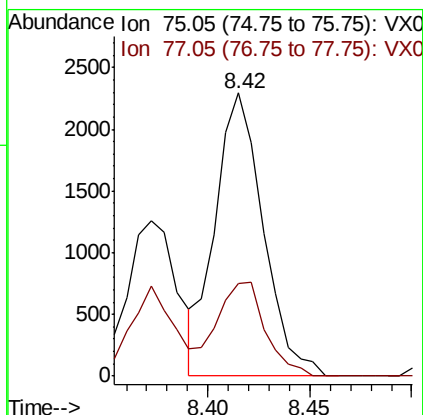

#40

4-Methyl-2-pentanone

Concen: 2.254 ug/L

RT: 8.62 min Scan# 1236

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15




Tgt Ion: 43 Resp: 14072


Ion Ratio Lower Upper

43 100

58 42.5 34.1 51.1

100 0.0 15.0 22.4#

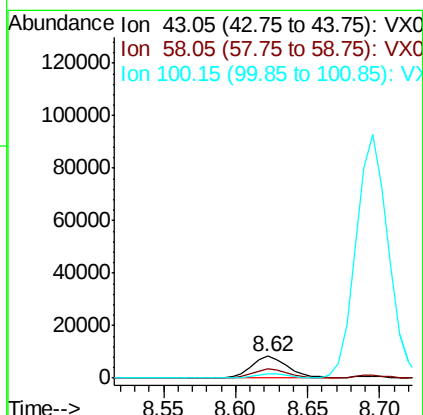

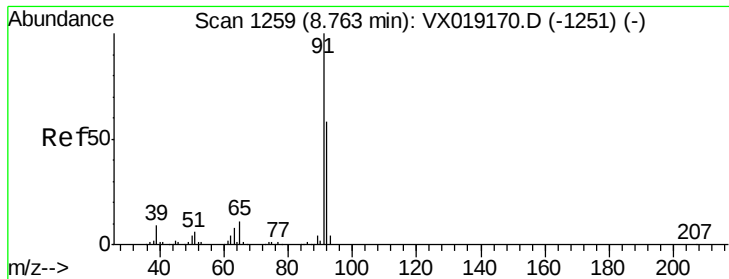

#42

Toluene

Concen: 0.228 ug/L

RT: 8.76 min Scan# 1259

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :


MDL-WATER-02

Tot Ion: 91 Resp: 12232

Ion Ratio Lower Upper




91 100

92 58.5 40.7 75.7

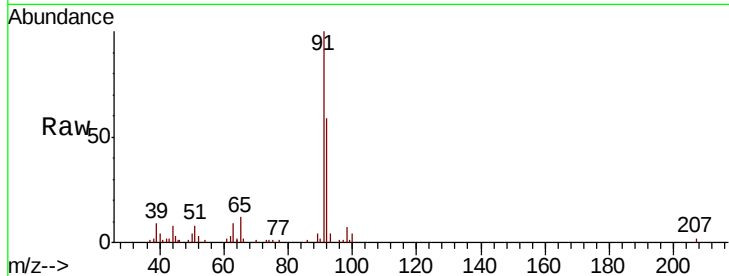

Abundance Ion 91.15 (90.85 to 91.85): VX0

Ion 92.15 (91.85 to 92.85): VX0

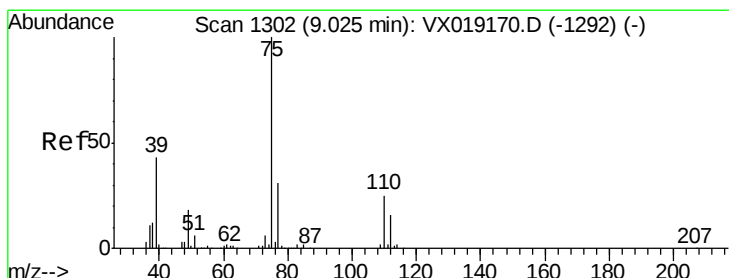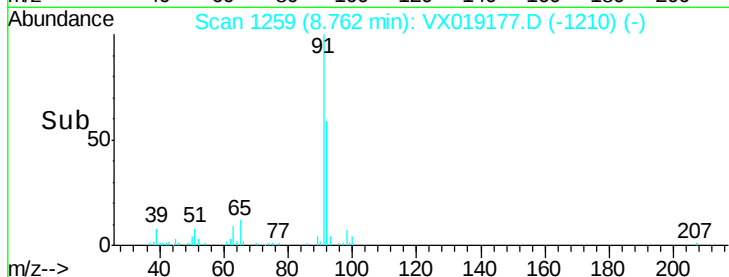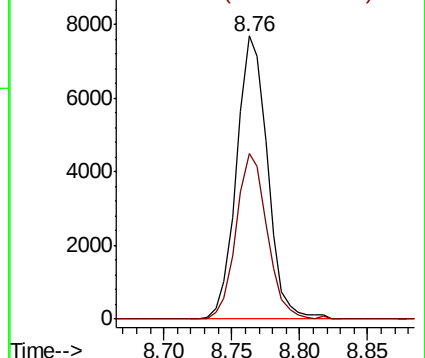

#44

trans-1,3-Dichloropropene

Concen: 0.308 ug/L

RT: 9.02 min Scan# 1301

Delta R.T. -0.01 min

Lab File: VX019177.D


Acq: 28 Oct 2020 21:15

Tgt Ion: 75 Resp: 4624

Ion Ratio Lower Upper



75 100


77 37.0 21.7 40.3

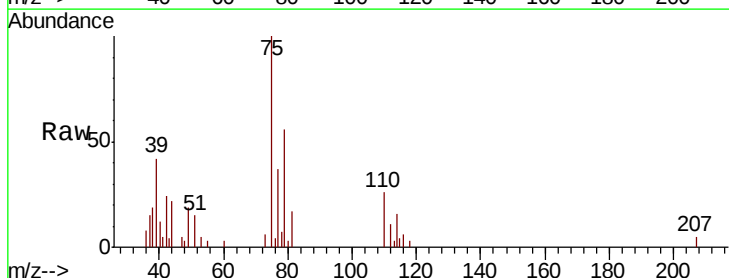

Abundance Ion 75.05 (74.75 to 75.75): VX0

Ion 77.05 (76.75 to 77.75): VX0

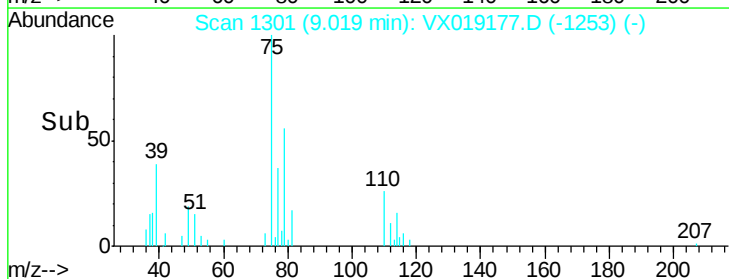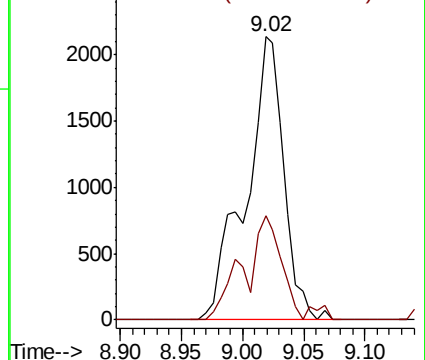



#45

1,1,2-Trichloroethane

Concen: 0.221 ug/L

RT: 9.20 min Scan# 1330

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :

MDL-WATER-02

Tot Ion: 97 Resp: 1889


Ion Ratio Lower Upper

97 100

99 61.3 44.8 83.2

83 83.9 59.1 109.7

85 55.8 37.4 69.4






Abundance Ion 96.95 (96.65 to 97.65): VX019177.D (-1281) (-)

Ion 99.05 (98.75 to 99.75): VX019177.D (-1281) (-)

Ion 82.95 (82.65 to 83.65): VX019177.D (-1281) (-)

Ion 85.00 (84.70 to 85.70): VX019177.D (-1281) (-)

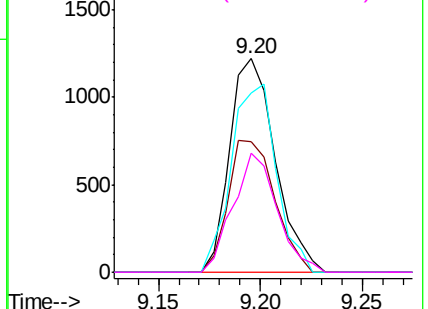

#47

Tetrachloroethene

Concen: 0.223 ug/L

RT: 9.31 min Scan# 1349

Delta R.T. -0.01 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Tgt Ion: 164 Resp: 2310


Ion Ratio Lower Upper

164 100

129 88.0 64.2 119.2

131 83.0 63.8 118.4

166 112.3 88.3 164.1






Abundance Ion 163.90 (163.60 to 164.60): VX019177.D (-1301) (-)

Ion 128.95 (128.65 to 129.65): VX019177.D (-1301) (-)

Ion 130.95 (130.65 to 131.65): VX019177.D (-1301) (-)

Ion 165.90 (165.60 to 166.60): VX019177.D (-1301) (-)



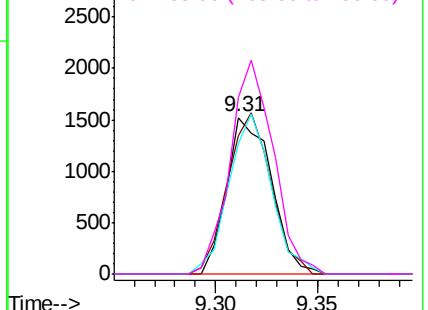



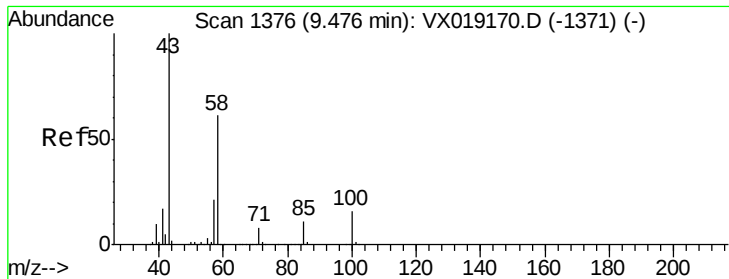

#48
2-Hexanone
Concen: 2.584 ug/L
RT: 9.48 min Scan# 1376
Delta R.T. -0.00 min
Lab File: VX019177.D
Acq: 28 Oct 2020 21:15




Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-02


Tot Ion:	43	Resp:	11282
Ion	Ratio	Lower	Upper
43	100		
58	61.3	49.3	73.9
57	22.6	17.2	25.8
100	14.2	11.8	17.8

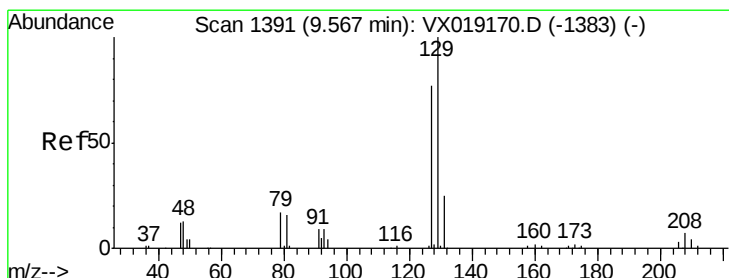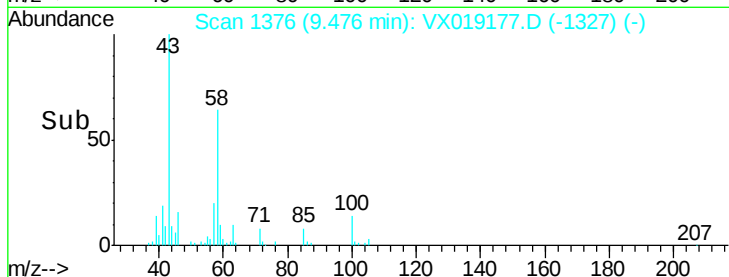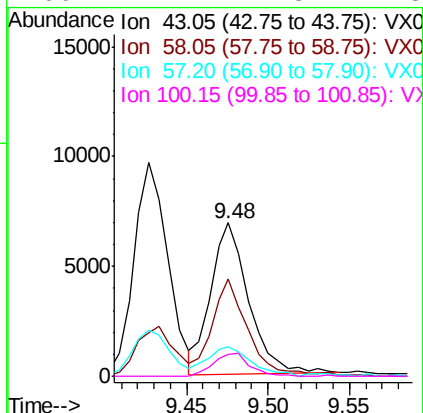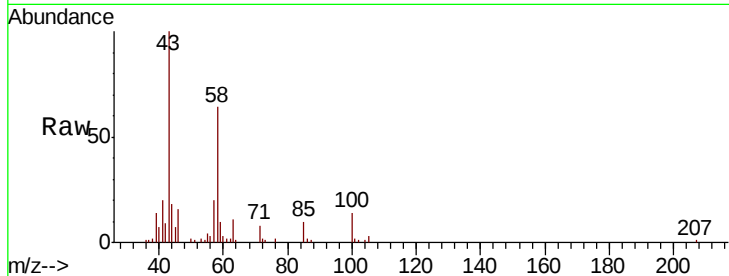

#49
Dibromochloromethane
Concen: 0.210 ug/L
RT: 9.57 min Scan# 1391
Delta R.T. -0.00 min
Lab File: VX019177.D
Acq: 28 Oct 2020 21:15

Tgt Ion:	129	Resp:	2071
Ion	Ratio	Lower	Upper
129	100		
127	80.4	53.6	99.6

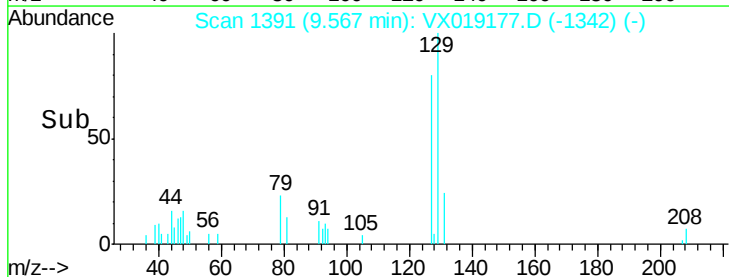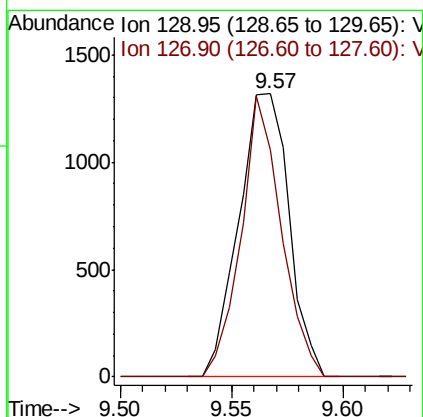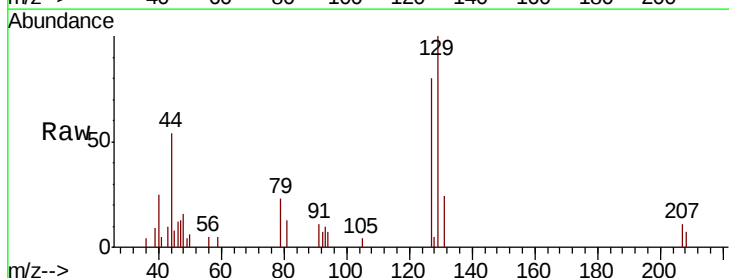



#50

1,2-Dibromoethane

Concen: 0.228 ug/L

RT: 9.66 min Scan# 1406

Delta R.T. 0.01 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :

MDL-WATER-02


Tot Ion:107 Resp: 1806

Ion Ratio Lower Upper

107 100

109 88.7 62.9 116.9




188 0.0 3.0 4.4#

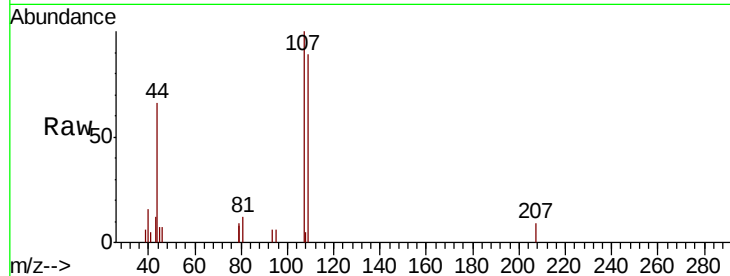

Abundance Ion 106.95 (106.65 to 107.65): V

Ion 109.00 (108.70 to 109.70): V

Ion 187.90 (187.60 to 188.60): V

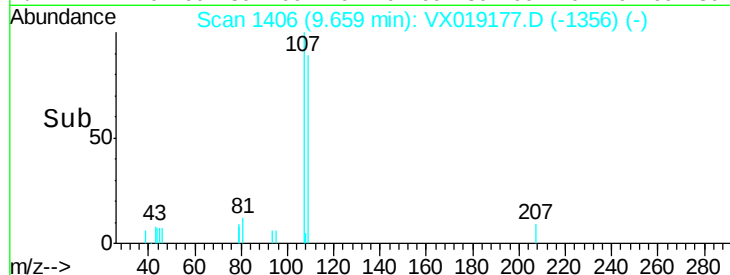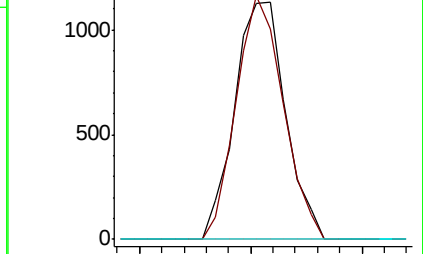

#51

Chlorobenzene

Concen: 0.224 ug/L

RT: 10.12 min Scan# 1482

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15


Tgt Ion:112 Resp: 7589

Ion Ratio Lower Upper

112 100

114 29.2 22.5 41.9



77 53.1 46.2 69.2

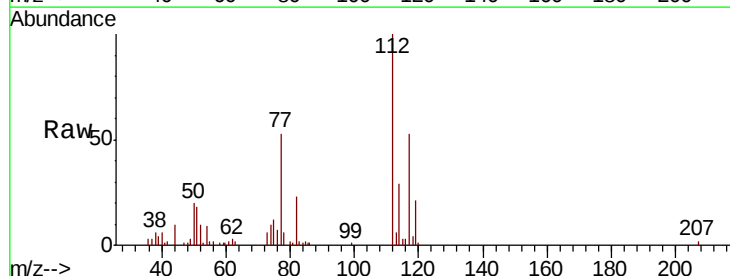


Abundance Ion 112.10 (111.80 to 112.80): V

Ion 114.05 (113.75 to 114.75): V

Ion 77.10 (76.80 to 77.80): V

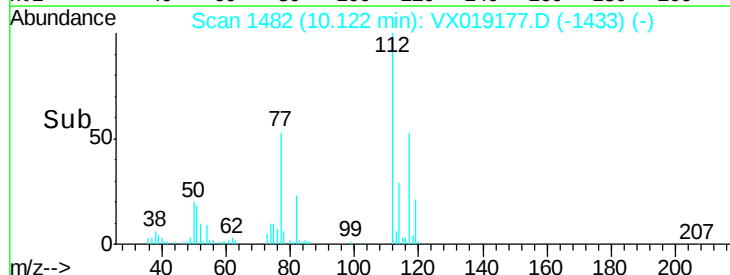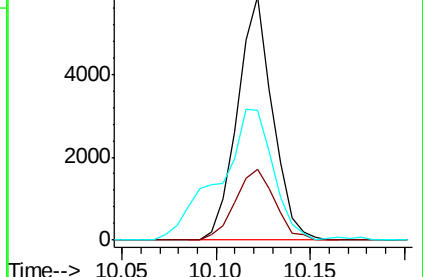



#52

Ethylbenzene

Concen: 0.217 ug/L

RT: 10.23 min Scan# 1500

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampled :


MDL-WATER-02

Tot Ion: 91 Resp: 13033

Ion Ratio Lower Upper




91 100

106 30.7 21.1 39.1



Abundance Ion 91.15 (90.85 to 91.85): VX0

Ion 106.15 (105.85 to 106.85): V

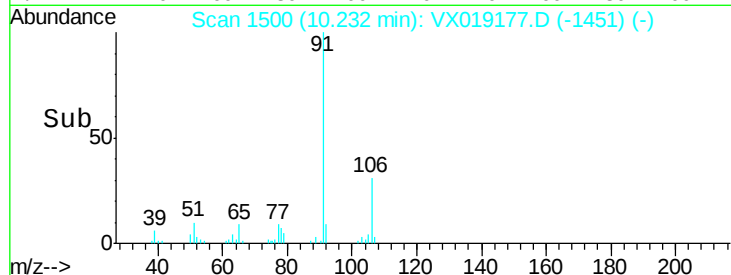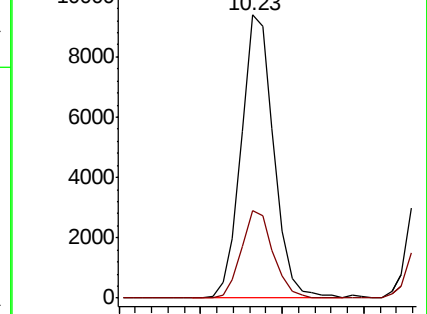

#53

m,p-xylene

Concen: 0.223 ug/L

RT: 10.34 min Scan# 1518

Delta R.T. -0.00 min

Lab File: VX019177.D


Acq: 28 Oct 2020 21:15

Tgt Ion: 106 Resp: 5120

Ion Ratio Lower Upper



106 100


91 206.8 141.5 262.7



Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VX0

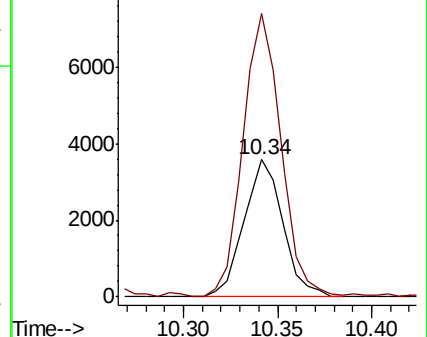



#54

o-xylene

Concen: 0.223 ug/L

RT: 10.68 min Scan# 1574

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampled :


MDL-WATER-02

Tot Ion:106 Resp: 4910

Ion Ratio Lower Upper




106 100

91 202.8 145.9 271.1



Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VX0

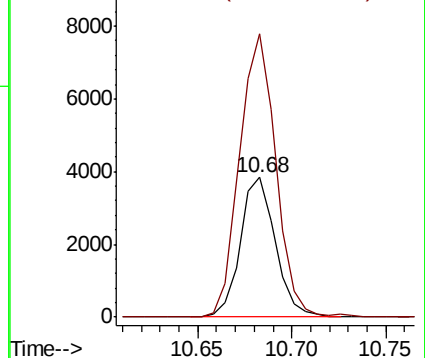

#55

Styrene

Concen: 0.207 ug/L

RT: 10.70 min Scan# 1576

Delta R.T. -0.00 min

Lab File: VX019177.D


Acq: 28 Oct 2020 21:15

Tgt Ion:104 Resp: 7462

Ion Ratio Lower Upper



104 100


78 48.7 31.7 58.9



Abundance Ion 104.10 (103.80 to 104.80): V

Ion 78.10 (77.80 to 78.80): VX0

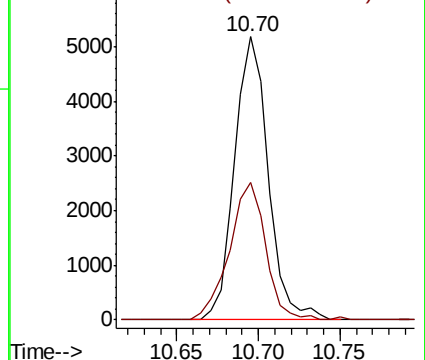

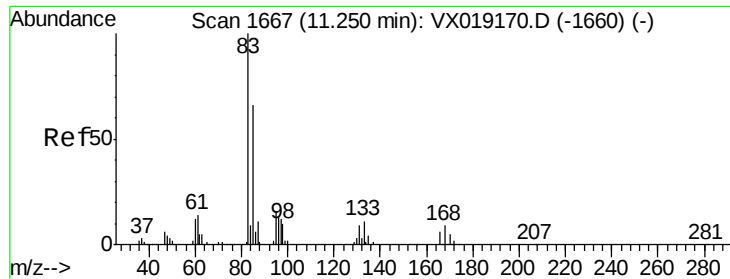

#57

1,1,2,2-Tetrachloroethane

Concen: 0.250 ug/L

RT: 11.25 min Scan# 1667

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :

MDL-WATER-02


Tot Ion: 83 Resp: 2426

Ion Ratio Lower Upper

83 100

85 58.3 46.0 85.4




131 14.6 7.7 11.5#

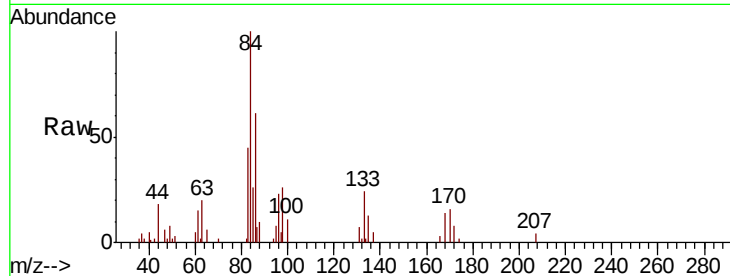

Abundance Ion 82.95 (82.65 to 83.65): VX019177.D (-1618) (-)

Ion 85.00 (84.70 to 85.70): VX019177.D (-1618) (-)

Ion 130.95 (130.65 to 131.65): VX019177.D (-1618) (-)

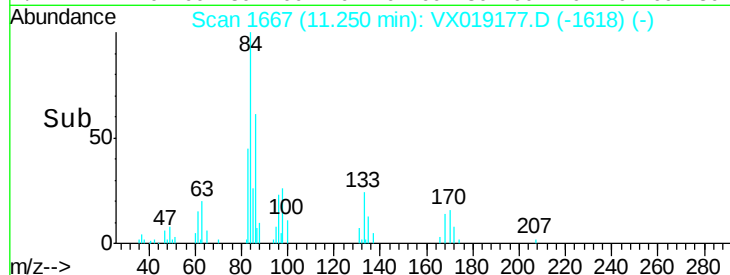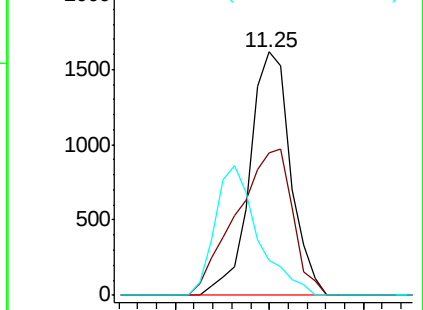

#59

Bromoform

Concen: 0.209 ug/L

RT: 10.84 min Scan# 1600

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15


Tgt Ion: 173 Resp: 1047

Ion Ratio Lower Upper

173 100

175 50.5 38.6 57.8



254 2.5 7.4 11.0#




Abundance Ion 172.90 (172.60 to 173.60): VX019177.D (-1551) (-)

Ion 174.90 (174.60 to 175.60): VX019177.D (-1551) (-)

Ion 253.75 (253.45 to 254.45): VX019177.D (-1551) (-)

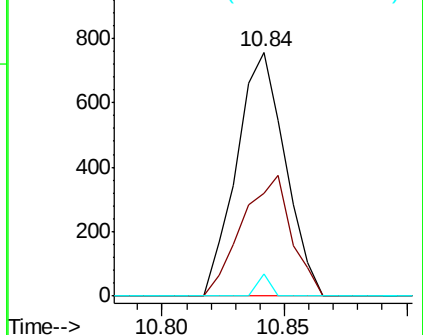



#60

Isopropylbenzene

Concen: 0.225 ug/L

RT: 11.00 min Scan# 1626

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :

MDL-WATER-02


Tot Ion:105 Resp: 12608

Ion Ratio Lower Upper

105 100

120 27.8 21.4 32.2




77 16.1 12.9 19.3



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

Ion 77.00 (76.70 to 77.70): V

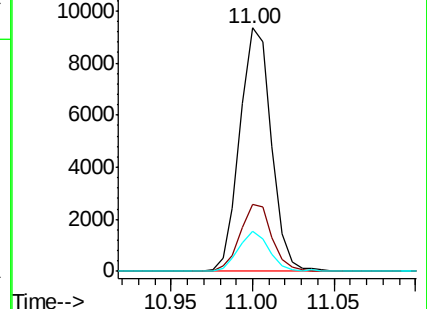

#61

1,2,3-Trichloropropane

Concen: 0.235 ug/L

RT: 11.28 min Scan# 1672

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15


Tgt Ion: 75 Resp: 1603

Ion Ratio Lower Upper

75 100

77 35.8 25.6 38.4



110 42.9 32.4 48.6




Abundance Ion 75.00 (74.70 to 75.70): VX0

Ion 77.00 (76.70 to 77.70): VX0

Ion 110.00 (109.70 to 110.70): V

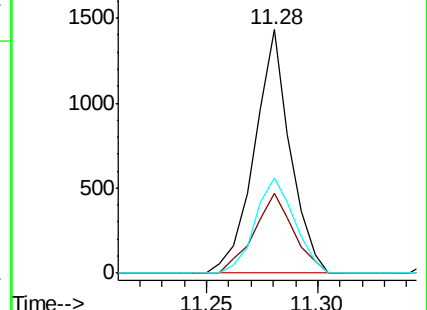



#62

1,3,5-Trimethylbenzene

Concen: 0.216 ug/L

RT: 11.49 min Scan# 1707

Delta R.T. 0.01 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampled :


MDL-WATER-02

Tot Ion:105 Resp: 10133

Ion Ratio Lower Upper




105 100

120 49.4 38.9 58.3



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

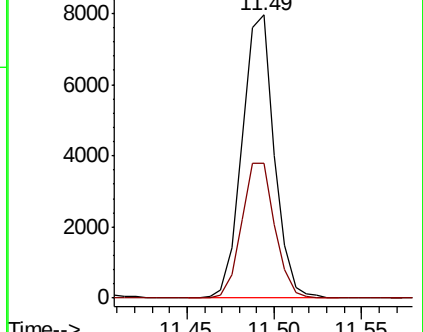

#63

1,2,4-Trimethylbenzene

Concen: 0.214 ug/L

RT: 11.79 min Scan# 1756

Delta R.T. -0.00 min

Lab File: VX019177.D


Acq: 28 Oct 2020 21:15

Tgt Ion:105 Resp: 10147

Ion Ratio Lower Upper



105 100


120 45.6 36.1 54.1



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

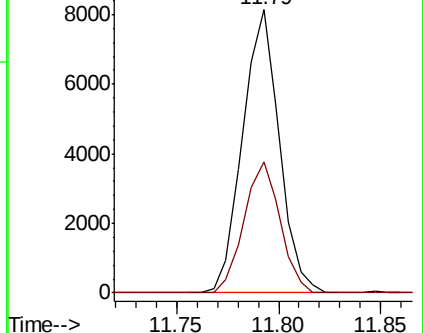



#64

1,3-Dichlorobenzene

Concen: 0.231 ug/L

RT: 12.01 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15

Instrument :

MSVOA_X

ClientSampleId :

MDL-WATER-02


Tot Ion:146 Resp: 5735

Ion Ratio Lower Upper

146 100

111 43.1 27.3 50.7




148 64.6 45.4 84.2



Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

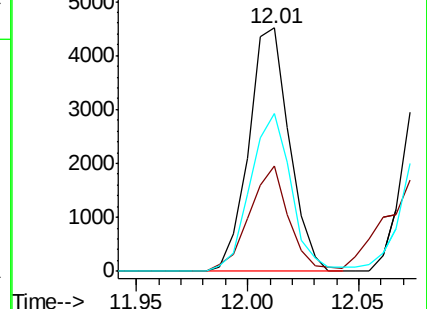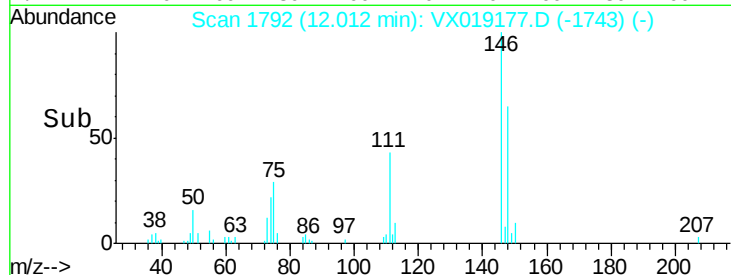

#65

1,4-Dichlorobenzene

Concen: 0.244 ug/L

RT: 12.08 min Scan# 1803

Delta R.T. -0.00 min

Lab File: VX019177.D

Acq: 28 Oct 2020 21:15


Tgt Ion:146 Resp: 6064

Ion Ratio Lower Upper

146 100

111 40.4 28.1 52.3



148 65.6 44.5 82.7




Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V



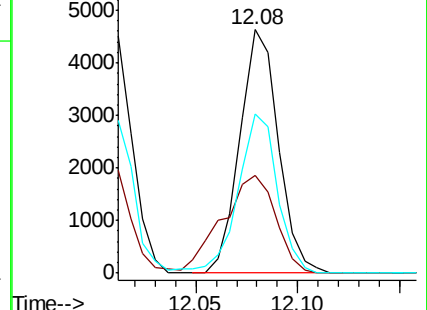





#67
 1,2-Dichlorobenzene
 Concen: 0.241 ug/L
 RT: 12.38 min Scan# 1852
 Delta R.T. -0.00 min
 Lab File: VX019177.D
 Acq: 28 Oct 2020 21:15




Instrument :
 MSVOA_X
 ClientSampleId :
 MDL-WATER-02


Tot Ion:146 Resp: 5498
 Ion Ratio Lower Upper
 146 100
 111 37.6 32.6 49.0
 148 54.5 49.4 74.2

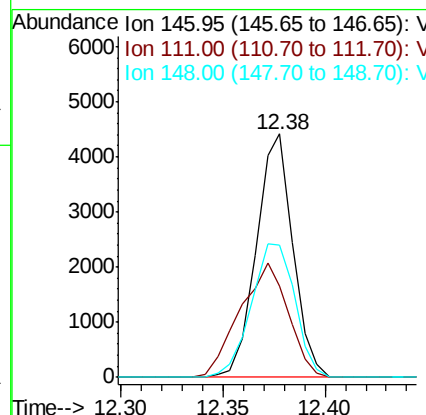

#68
 1,2-Dibromo-3-chloropropane
 Concen: 0.254 ug/L
 RT: 12.98 min Scan# 1951
 Delta R.T. -0.00 min
 Lab File: VX019177.D
 Acq: 28 Oct 2020 21:15

Tgt Ion: 75 Resp: 397
 Ion Ratio Lower Upper
 75 100
 155 44.9 62.9 94.3#
 157 75.7 77.5 116.3#

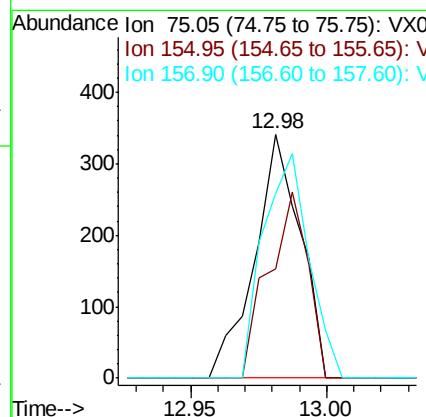




#69
 1,3,5-Trichlorobenzene
 Concen: 0.224 ug/L
 RT: 13.15 min Scan# 1979
 Delta R.T. -0.00 min
 Lab File: VX019177.D
 Acq: 28 Oct 2020 21:15

Instrument :
 MSVOA_X
 ClientSampleId :
 MDL-WATER-02

Tot Ion:180	Resp:	4086	
Ion Ratio	Lower	Upper	
180 100			
182 93.7	74.1	111.1	
184 31.8	24.4	36.6	
145 32.3	24.9	37.3	






Abundance Ion 180.00 (179.70 to 180.70): V

Ion 182.00 (181.70 to 182.70): V


Ion 184.00 (183.70 to 184.70): V

Ion 145.00 (144.70 to 145.70): V

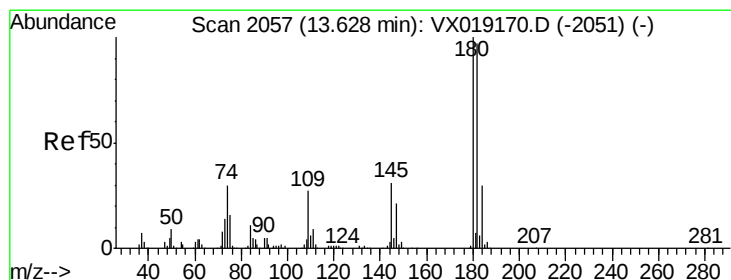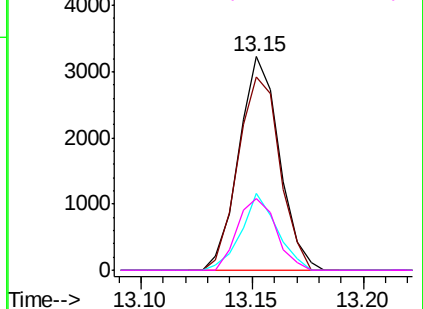

#70
 1,2,4-trichlorobenzene
 Concen: 0.216 ug/L
 RT: 13.63 min Scan# 2057
 Delta R.T. -0.00 min
 Lab File: VX019177.D
 Acq: 28 Oct 2020 21:15



Tgt Ion	180	Resp:	3435
	Ratio	Lower	Upper
180	100		
182	97.4	77.8	116.6
145	33.0	25.0	37.4




Abundance Ion 179.90 (179.60 to 180.60): V

Ion 182.00 (181.70 to 182.70): V

Ion 144.95 (144.65 to 145.65): V



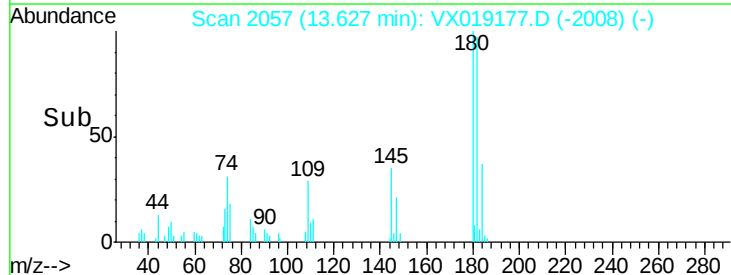
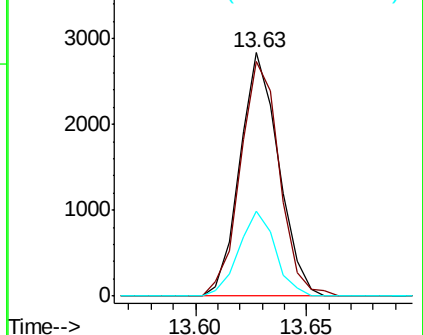




#71
Naphthalene
Concen: 0.204 ug/L
RT: 13.82 min Scan# 2088
Delta R.T. -0.00 min
Lab File: VX019177.D
Acq: 28 Oct 2020 21:15

Instrument :
MSVOA_X
ClientSampleId :
MDL-WATER-02

Tot Ion:128 Resp: 5833
Ion Ratio Lower Upper
128 100
129 10.2 8.6 13.0
127 12.1 10.1 15.1

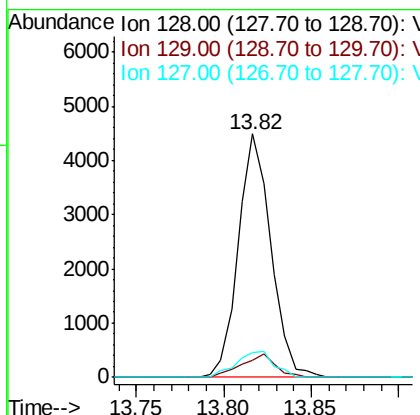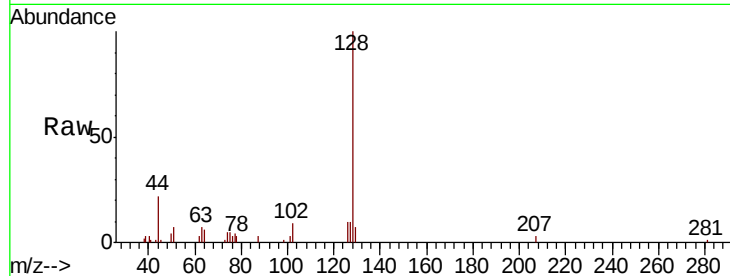

#72
1,2,3-Trichlorobenzene
Concen: 0.220 ug/L
RT: 14.00 min Scan# 2118
Delta R.T. -0.00 min
Lab File: VX019177.D
Acq: 28 Oct 2020 21:15

Tgt Ion:180 Resp: 3089
Ion Ratio Lower Upper
180 100
182 93.9 77.0 115.4
145 33.0 27.8 41.6

