

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102920\
 Data File : VX019173.D
 Acq On : 28 Oct 2020 19:34
 Operator : JC/MD
 Sample : VX1028WBL01
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK301

Quant Time: Oct 29 06:46:41 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 29 06:24:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	198588	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	177391	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.06	152	80997	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	62087	4.83	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.60%
7) Chloroethane-d5	1.70	69	52004	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.20%
11) 1,1-Dichloroethene-d2	2.34	63	90019	3.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.80%
20) 2-Butanone-d5	4.56	46	136880	48.75	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.50%
24) Chloroform-d	5.14	84	114426	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
26) 1,2-Dichloroethane-d4	6.03	65	62981	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
32) Benzene-d6	6.05	84	238613	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
36) 1,2-Dichloropropane-d6	7.37	67	68505	5.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.00%
41) Toluene-d8	8.70	98	222357	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.40%
43) trans-1,3-Dichloropropene-	8.99	79	27813	4.72	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.40%
46) 2-Hexanone-d5	9.43	63	128685	49.84	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.68%
56) 1,1,2,2-Tetrachloroethane-	11.23	84	50744	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.60%
66) 1,2-Dichlorobenzene-d4	12.36	152	74362	4.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.00%


Target Compounds					Ovalue
16) Methylene chloride	2.83	84	2478	0.163 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX102920\
Data File : VX019173.D
Acq On : 28 Oct 2020 19:34
Operator : JC/MD
Sample : VX1028WBL01
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK301

Quant Time: Oct 29 06:46:41 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 29 06:24:00 2020
Response via : Initial Calibration

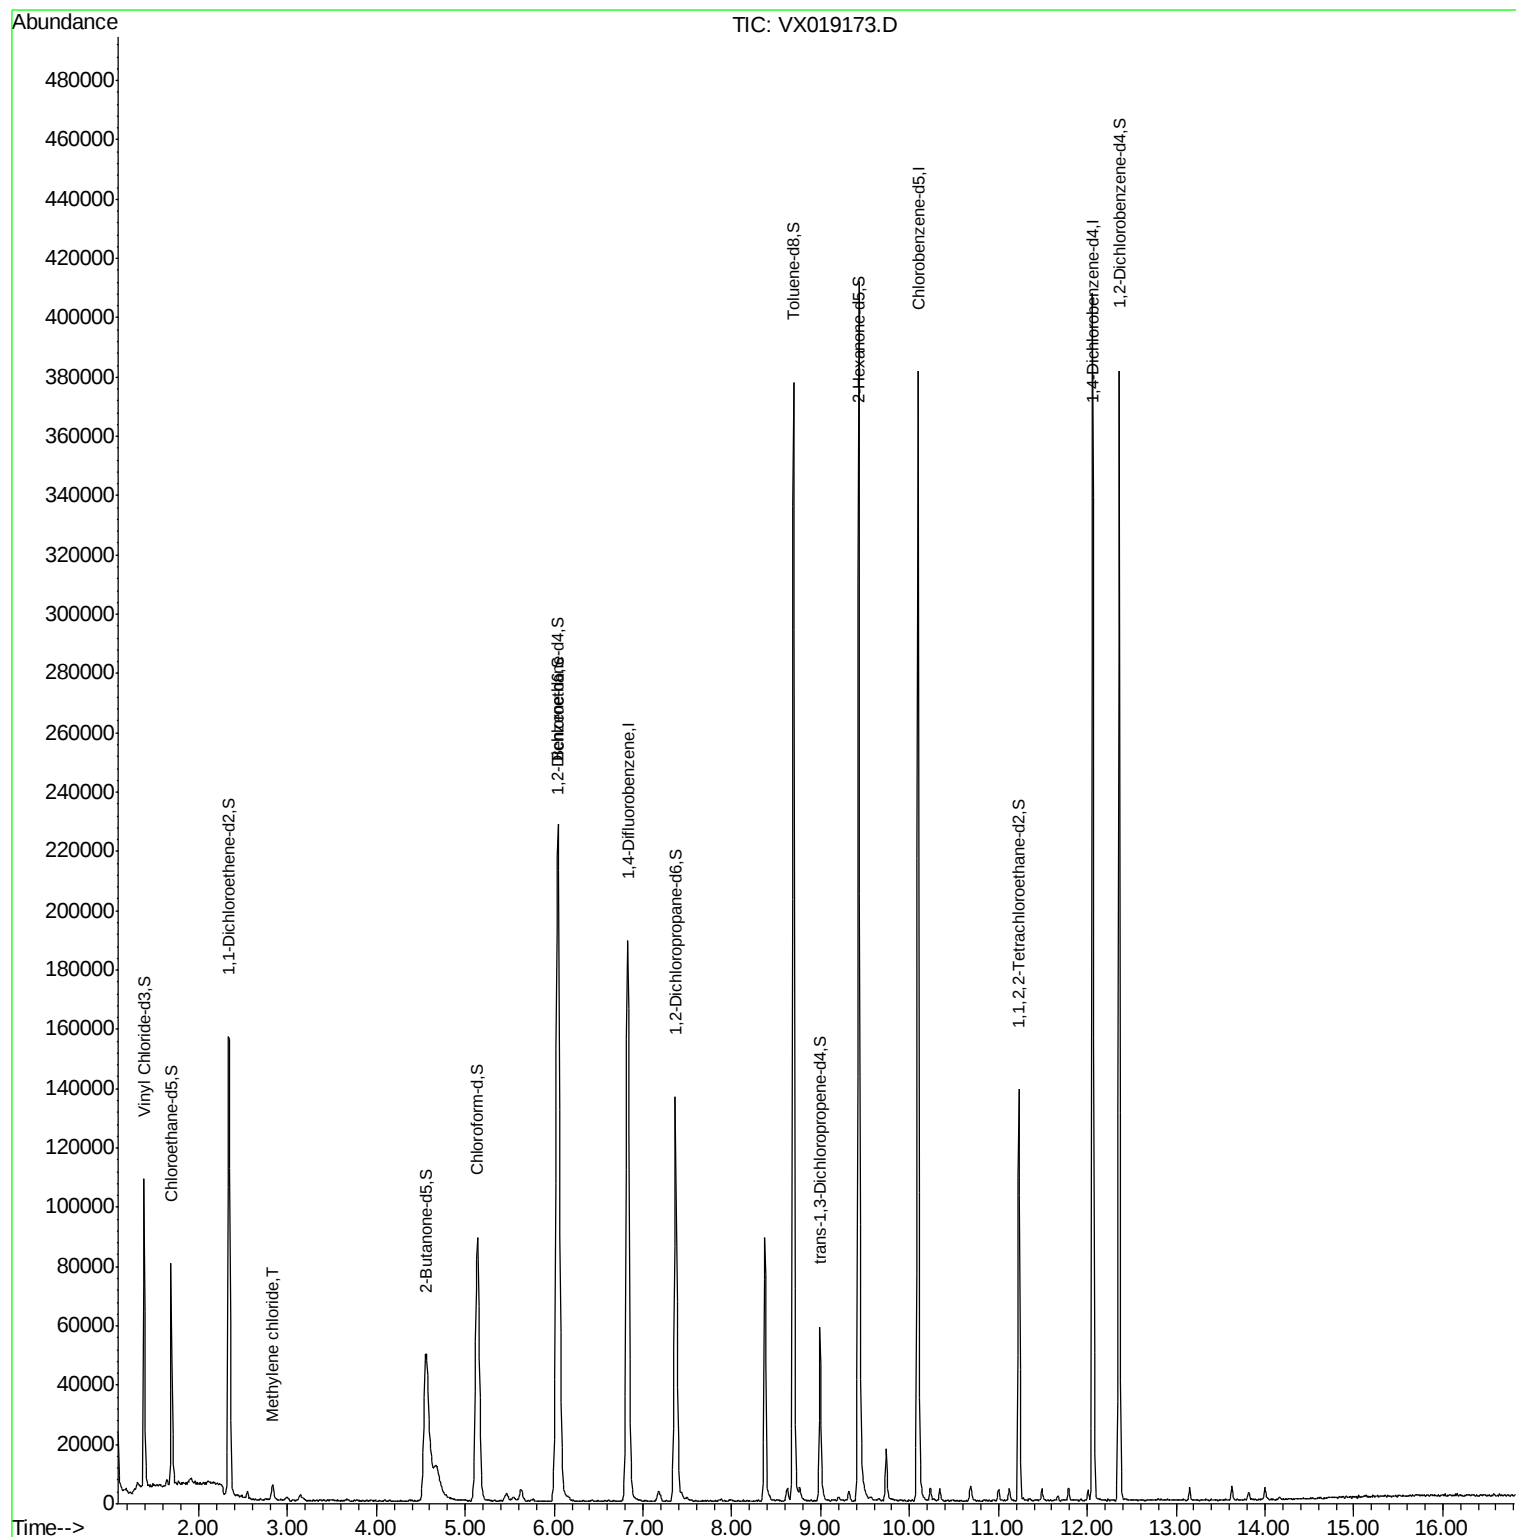

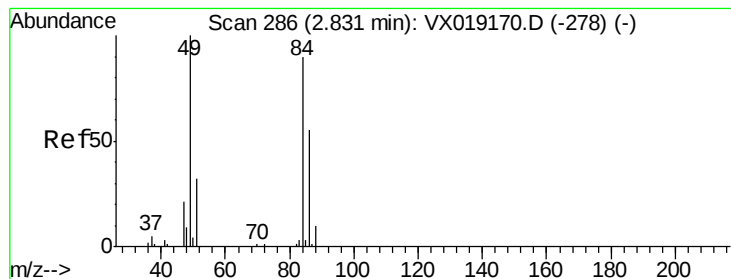

#16
 Methvlene chloride
 Concen: 0.163 ug/L
 RT: 2.83 min Scan# 286
 Delta R.T. 0.00 min
 Lab File: VX019173.D
 Acq: 28 Oct 2020 19:34

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK301

Tot Ion: 84 Resp: 2478
 Ion Ratio Lower Upper
 84 100
 86 56.9 42.2 78.4
 49 111.6 77.5 143.9

