

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX102920\
 Data File : VX019175.D
 Acq On : 28 Oct 2020 20:25
 Operator : JC/MD
 Sample : VX1028WBL03
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK303

Quant Time: Oct 29 06:52:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 29 06:24:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	197579	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	176138	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.06	152	80128	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	64540	5.05	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.00%
7) Chloroethane-d5	1.70	69	53744	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.80%
11) 1,1-Dichloroethene-d2	2.34	63	93182	3.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.60%
20) 2-Butanone-d5	4.56	46	142444	50.99	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.98%
24) Chloroform-d	5.14	84	116726	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%
26) 1,2-Dichloroethane-d4	6.03	65	64416	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
32) Benzene-d6	6.04	84	243043	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
36) 1,2-Dichloropropane-d6	7.37	67	69422	5.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.20%
41) Toluene-d8	8.70	98	224980	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
43) trans-1,3-Dichloropropene-	8.99	79	28833	4.92	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.40%
46) 2-Hexanone-d5	9.43	63	132057	51.51	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.02%
56) 1,1,2,2-Tetrachloroethane-	11.23	84	51917	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.40%
66) 1,2-Dichlorobenzene-d4	12.36	152	77149	5.19	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.80%


Target Compounds					Ovalue
16) Methylene chloride	2.83	84	2107	0.139 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX102920\
Data File : VX019175.D
Acq On : 28 Oct 2020 20:25
Operator : JC/MD
Sample : VX1028WBL03
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK303

Quant Time: Oct 29 06:52:24 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 29 06:24:00 2020
Response via : Initial Calibration

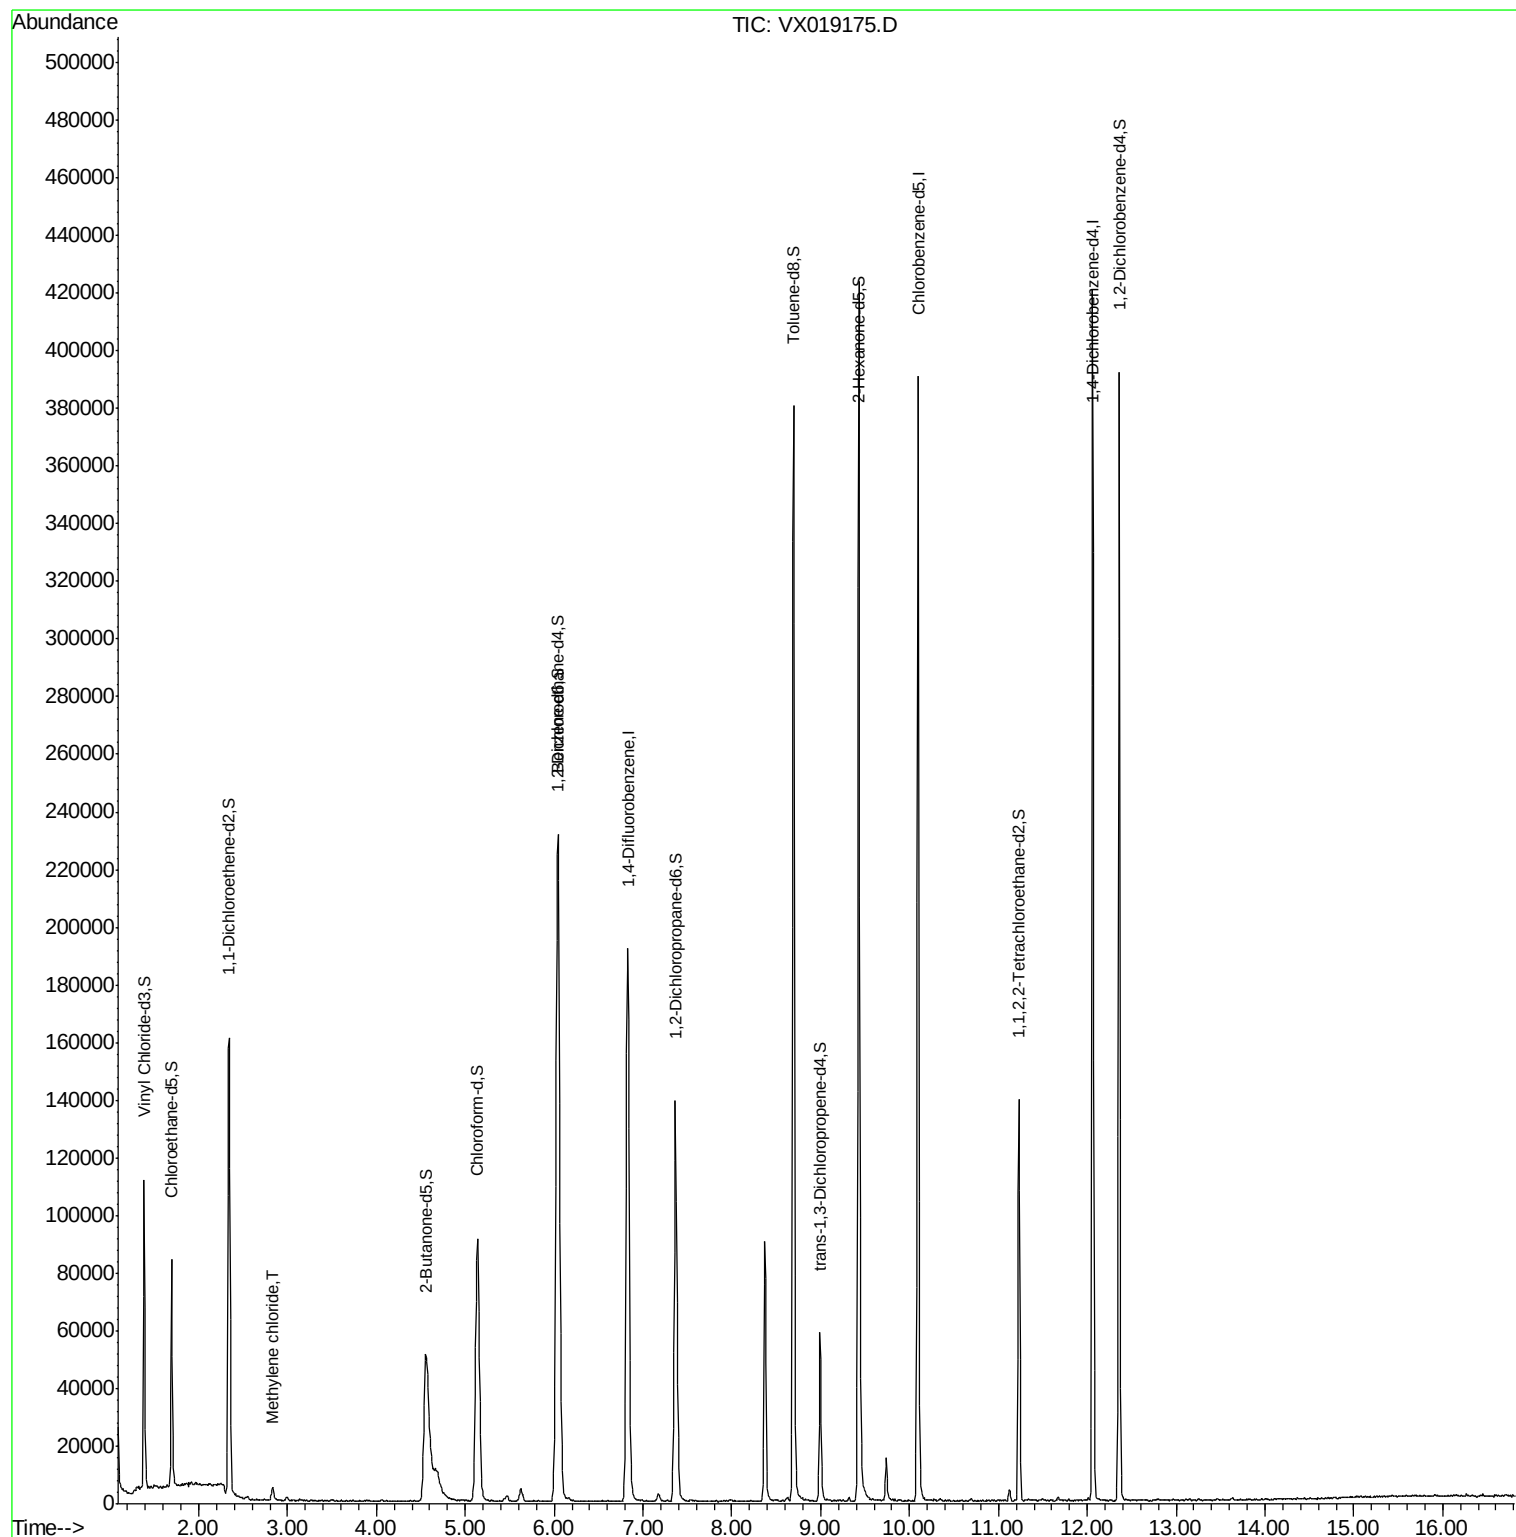

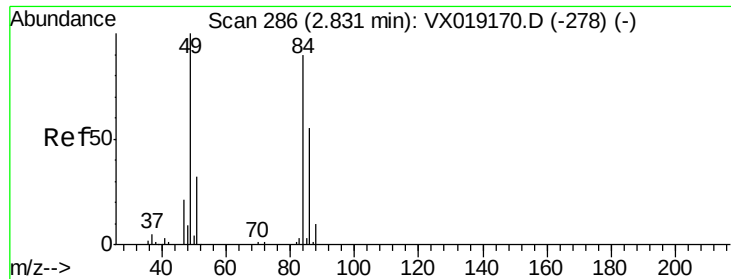

#16
 Methylene chloride
 Concen: 0.139 ug/L
 RT: 2.83 min Scan# 286
 Delta R.T. -0.00 min
 Lab File: VX019175.D
 Acq: 28 Oct 2020 20:25

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK303

Tot Ion: 84 Resp: 2107
 Ion Ratio Lower Upper
 84 100
 86 74.0 42.2 78.4
 49 105.9 77.5 143.9

