


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX102920\
Data File : VX019163.D
Acq On : 28 Oct 2020 14:40
Operator : JC/MD
Sample : BFB61
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB61

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Oct 29 06:24:00 2020

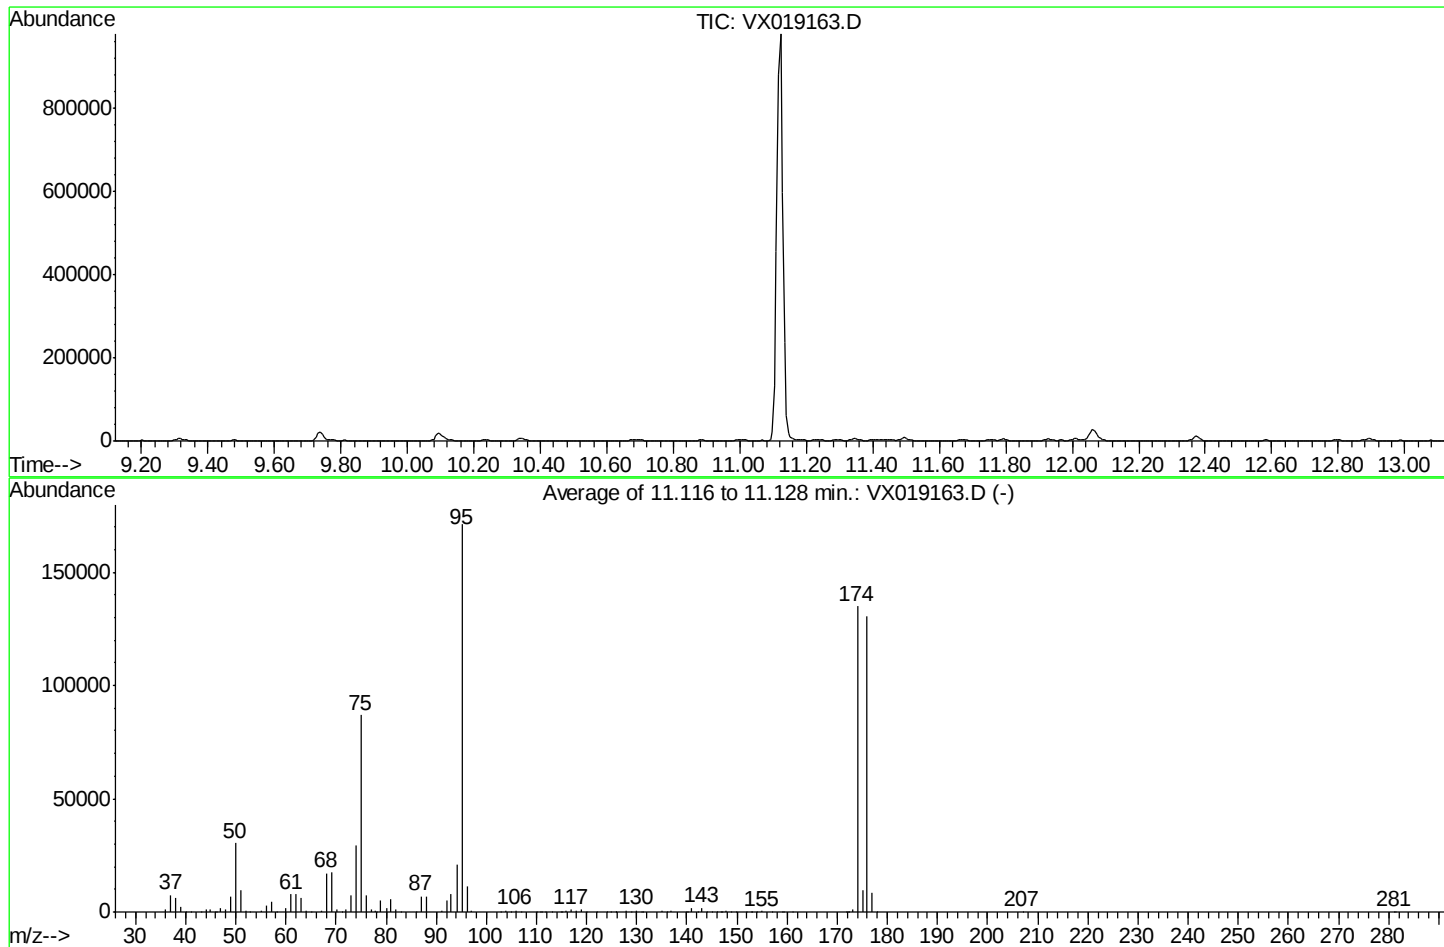

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	30416	PASS
75	95	30	80	50.8	86909	PASS
95	95	100	100	100.0	171181	PASS
96	95	5	9	6.6	11353	PASS
173	174	0.00	2	0.8	1061	PASS
174	95	50	120	78.9	134994	PASS
175	174	5	9	7.2	9747	PASS
176	174	95	105	96.8	130677	PASS
177	176	5	10	6.4	8427	PASS

m/z	Abundance
36.00	1487.0
37.00	8957.0
38.10	7778.0
39.00	3075.0
40.00	226.0
43.00	167.0
44.00	1819.0
45.00	1732.0
46.00	120.0
47.00	2197.0
48.00	1054.0
49.00	7848.0
50.00	36168.0
51.00	11600.0
52.00	528.0
52.90	73.0
55.00	466.0
56.10	3130.0
57.10	5337.0
58.00	271.0
60.00	1916.0
61.10	9031.0
62.10	9629.0
63.00	7035.0
64.10	765.0
65.10	143.0
67.10	571.0
68.00	19856.0
69.00	20200.0
70.10	1608.0
71.10	79.0
72.00	1051.0
73.10	8552.0
74.00	33040.0
75.10	99456.0
76.10	8784.0
77.10	1000.0
77.90	776.0
78.90	6186.0
80.00	1841.0
81.00	6280.0
81.90	1489.0
83.10	120.0
86.00	224.0
87.00	7588.0
88.00	6983.0
91.00	800.0
92.00	5277.0
93.00	8665.0
94.10	22624.0
95.10	188032.0
96.10	12785.0
97.00	380.0
102.90	85.0
103.90	768.0
104.90	282.0
105.90	868.0
106.90	211.0
109.90	77.0
110.80	146.0
111.90	143.0
113.00	227.0
114.80	232.0
115.90	799.0
117.00	1178.0
117.90	810.0
119.00	1009.0
120.00	75.0
122.00	77.0
124.00	86.0
125.00	62.0
125.80	95.0
127.90	596.0
128.90	342.0
129.90	790.0
130.90	320.0
135.00	285.0
136.10	61.0
136.90	324.0
139.80	113.0
140.90	1805.0
142.00	220.0
142.90	2025.0
143.90	110.0
144.90	204.0
145.90	276.0
146.90	99.0
148.00	466.0
148.80	109.0
149.90	160.0
152.00	149.0
152.80	139.0

Instrument :
MSVOA_X
ClientSampleId :
BFB61

153.90	114.0
155.10	426.0
156.90	257.0
159.00	190.0
161.00	224.0
172.00	284.0
173.00	947.0
174.00	130016.0
175.00	9816.0
176.00	126960.0
177.00	8561.0
178.10	228.0
207.00	130.0

Instrument :
MSVOA_X
ClientSampleId :
BFB61

m/z	Abundance
36.00	1525.0
37.00	8868.0
38.00	7476.0
39.10	3156.0
40.10	278.0
43.00	154.0
44.00	1703.0
45.00	1557.0
46.20	168.0
47.10	1850.0
48.00	1094.0
49.10	7528.0
50.00	35568.0
51.10	11128.0
52.00	491.0
55.00	467.0
56.00	3004.0
57.00	5305.0
58.10	215.0
60.00	1783.0
61.10	9032.0
62.10	9016.0
63.10	7197.0
64.10	692.0
65.00	187.0
67.10	534.0
68.00	20432.0
69.10	20496.0
70.10	1740.0
71.10	72.0
72.00	1102.0
73.00	9173.0
74.00	34832.0
75.00	103600.0
76.10	8698.0
77.00	1066.0
77.90	752.0
78.90	5843.0
80.00	1932.0
81.00	6773.0
82.00	1371.0
83.10	154.0
86.00	202.0
87.00	8604.0
88.00	8104.0
91.00	705.0
92.00	6009.0
93.00	8782.0
94.10	24992.0
95.10	205504.0
96.10	13542.0
97.10	415.0
103.00	105.0
103.90	967.0
104.80	242.0
105.90	943.0
106.90	251.0
110.00	178.0
111.10	178.0
111.90	155.0
113.00	190.0
115.00	237.0
115.90	832.0
117.00	1348.0
117.90	853.0
118.90	1164.0
120.00	52.0
124.00	171.0
124.90	102.0
126.00	100.0
128.00	743.0
129.00	304.0
129.90	779.0
131.10	301.0
134.80	381.0
135.90	65.0
136.90	449.0
139.90	135.0
141.00	2270.0
142.10	263.0
143.00	2166.0
144.00	102.0
145.00	271.0
146.00	306.0
146.80	144.0
147.80	404.0
148.90	122.0
149.80	280.0
151.90	109.0
153.00	193.0
153.80	127.0
154.90	436.0

Instrument :
MSVOA_X
ClientSampleId :
BFB61

157.00	411.0
158.90	157.0
159.20	141.0
161.00	217.0
171.70	171.0
172.20	282.0
173.10	1285.0
174.00	163520.0
175.00	11622.0
176.00	157696.0
177.00	9923.0
177.90	313.0
207.00	121.0
281.10	69.0

Instrument :
MSVOA_X
ClientSampleId :
BFB61

m/z	Abundance
36.00	965.0
37.00	4657.0
38.10	4086.0
39.00	1391.0
40.00	225.0
41.00	62.0
43.00	95.0
44.00	1340.0
45.00	888.0
46.00	93.0
47.00	989.0
48.00	549.0
49.00	4410.0
50.00	19512.0
51.00	5885.0
52.10	191.0
55.10	287.0
56.00	1678.0
57.00	3021.0
58.10	97.0
60.00	1097.0
61.00	5467.0
62.00	5424.0
63.10	4159.0
64.10	408.0
65.20	84.0
67.00	333.0
68.00	11389.0
69.00	11470.0
70.00	895.0
72.00	535.0
73.10	5005.0
74.10	19592.0
75.10	57840.0
76.00	4853.0
77.00	738.0
78.10	690.0
78.90	3986.0
80.00	1057.0
80.90	3770.0
81.90	940.0
83.00	107.0
86.10	103.0
87.00	4992.0
88.00	4617.0
90.90	407.0
92.00	3453.0
93.00	5595.0
94.00	14499.0
95.10	120008.0
96.10	7732.0
97.10	226.0
103.90	502.0
104.90	149.0
106.00	537.0
107.00	101.0
109.90	106.0
111.00	113.0
112.00	82.0
112.90	104.0
115.00	188.0
116.00	453.0
117.00	855.0
117.90	476.0
119.00	699.0
124.00	96.0
124.80	62.0
125.90	102.0
128.00	421.0
129.00	241.0
130.00	526.0
130.90	184.0
135.00	274.0
135.90	55.0
136.90	252.0
140.10	55.0
141.00	1433.0
142.00	197.0
143.00	1381.0
143.90	107.0
144.90	123.0
145.90	201.0
147.10	101.0
147.90	306.0
148.80	94.0
149.80	177.0
151.90	78.0
153.00	111.0
153.90	113.0
154.90	320.0
157.00	215.0
158.80	124.0

Instrument :
MSVOA_X
ClientSampleId :
BFB61

161.10	117.0
171.80	148.0
173.10	951.0
174.00	111448.0
175.00	7803.0
176.00	107376.0
177.00	6799.0
178.00	242.0
206.90	109.0
281.30	97.0

Instrument :
MSVOA_X
ClientSampleId :
BFB61

Scan 1638 (11.073 min): VX019163.D
BFB61

m/z	Abundance
39.20	100.0
39.90	144.0
43.00	84.0
44.00	729.0
45.00	57.0
75.00	56.0
207.00	110.0

Instrument :
MSVOA_X
ClientSampleId :
BFB61