


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX103018\
Data File : VX005682.D
Acq On : 30 Oct 2018 10:25
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102418W.M
Title : SW846 8260
Last Update : Thu Oct 25 02:52:45 2018

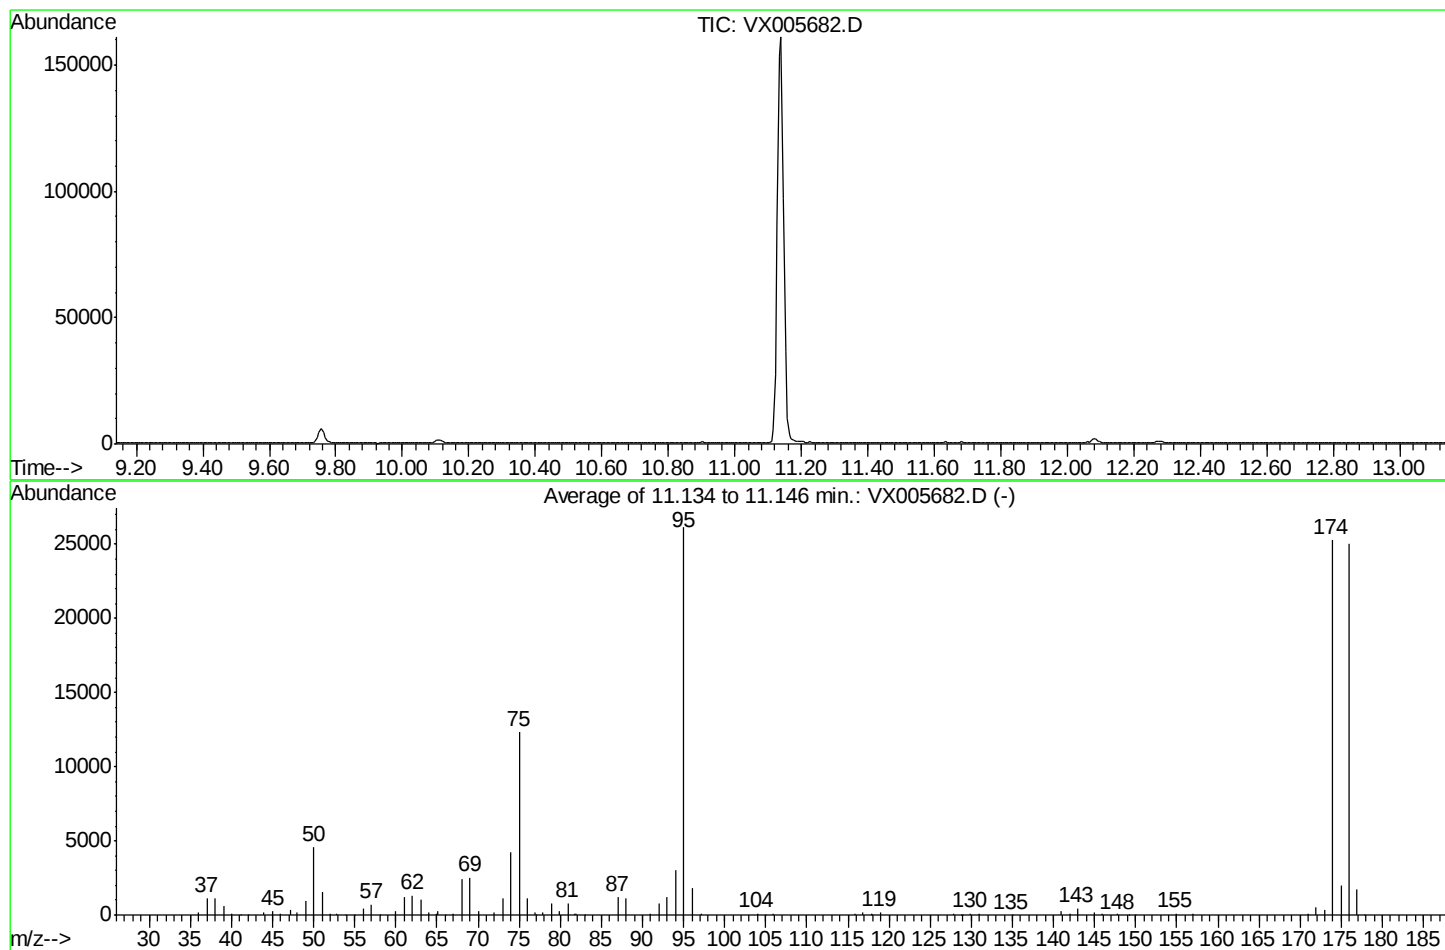

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	4612	PASS
75	95	30	60	47.3	12352	PASS
95	95	100	100	100.0	26141	PASS
96	95	5	9	7.1	1843	PASS
173	174	0.00	2	1.5	380	PASS
174	95	50	100	96.9	25328	PASS
175	174	5	9	7.8	1965	PASS
176	174	95	101	98.7	24997	PASS
177	176	5	9	6.8	1700	PASS