

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX103020\
 Data File : VX019182.D
 Acq On : 29 Oct 2020 10:38
 Operator : JC/MD
 Sample : VX1030WBL04
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK304

Quant Time: Oct 30 07:59:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 30 08:55:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.82	114	214180	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.09	117	188177	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.06	152	88966	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	53759	3.88	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.60%
7) Chloroethane-d5	1.70	69	45620	3.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.00%
11) 1,1-Dichloroethene-d2	2.34	63	80656	2.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.60%#
20) 2-Butanone-d5	4.56	46	126003	41.61	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.22%
24) Chloroform-d	5.14	84	102277	3.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.40%
26) 1,2-Dichloroethane-d4	6.03	65	55601	3.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.60%
32) Benzene-d6	6.04	84	211455	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.40%
36) 1,2-Dichloropropane-d6	7.37	67	61090	4.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.20%
41) Toluene-d8	8.70	98	192140	3.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.20%
43) trans-1,3-Dichloropropene-	8.99	79	25489	4.07	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.40%
46) 2-Hexanone-d5	9.43	63	118596	43.30	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.60%
56) 1,1,2,2-Tetrachloroethane-	11.23	84	45618	4.09	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.80%
66) 1,2-Dichlorobenzene-d4	12.36	152	67644	4.10	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	82.00%


Target Compounds					Ovalue
16) Methylene chloride	2.84	84	1929	0.118 ug/L	88




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX103020\
Data File : VX019182.D
Acq On : 29 Oct 2020 10:38
Operator : JC/MD
Sample : VX1030WBL04
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK304

Quant Time: Oct 30 07:59:44 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 30 08:55:33 2020
Response via : Initial Calibration

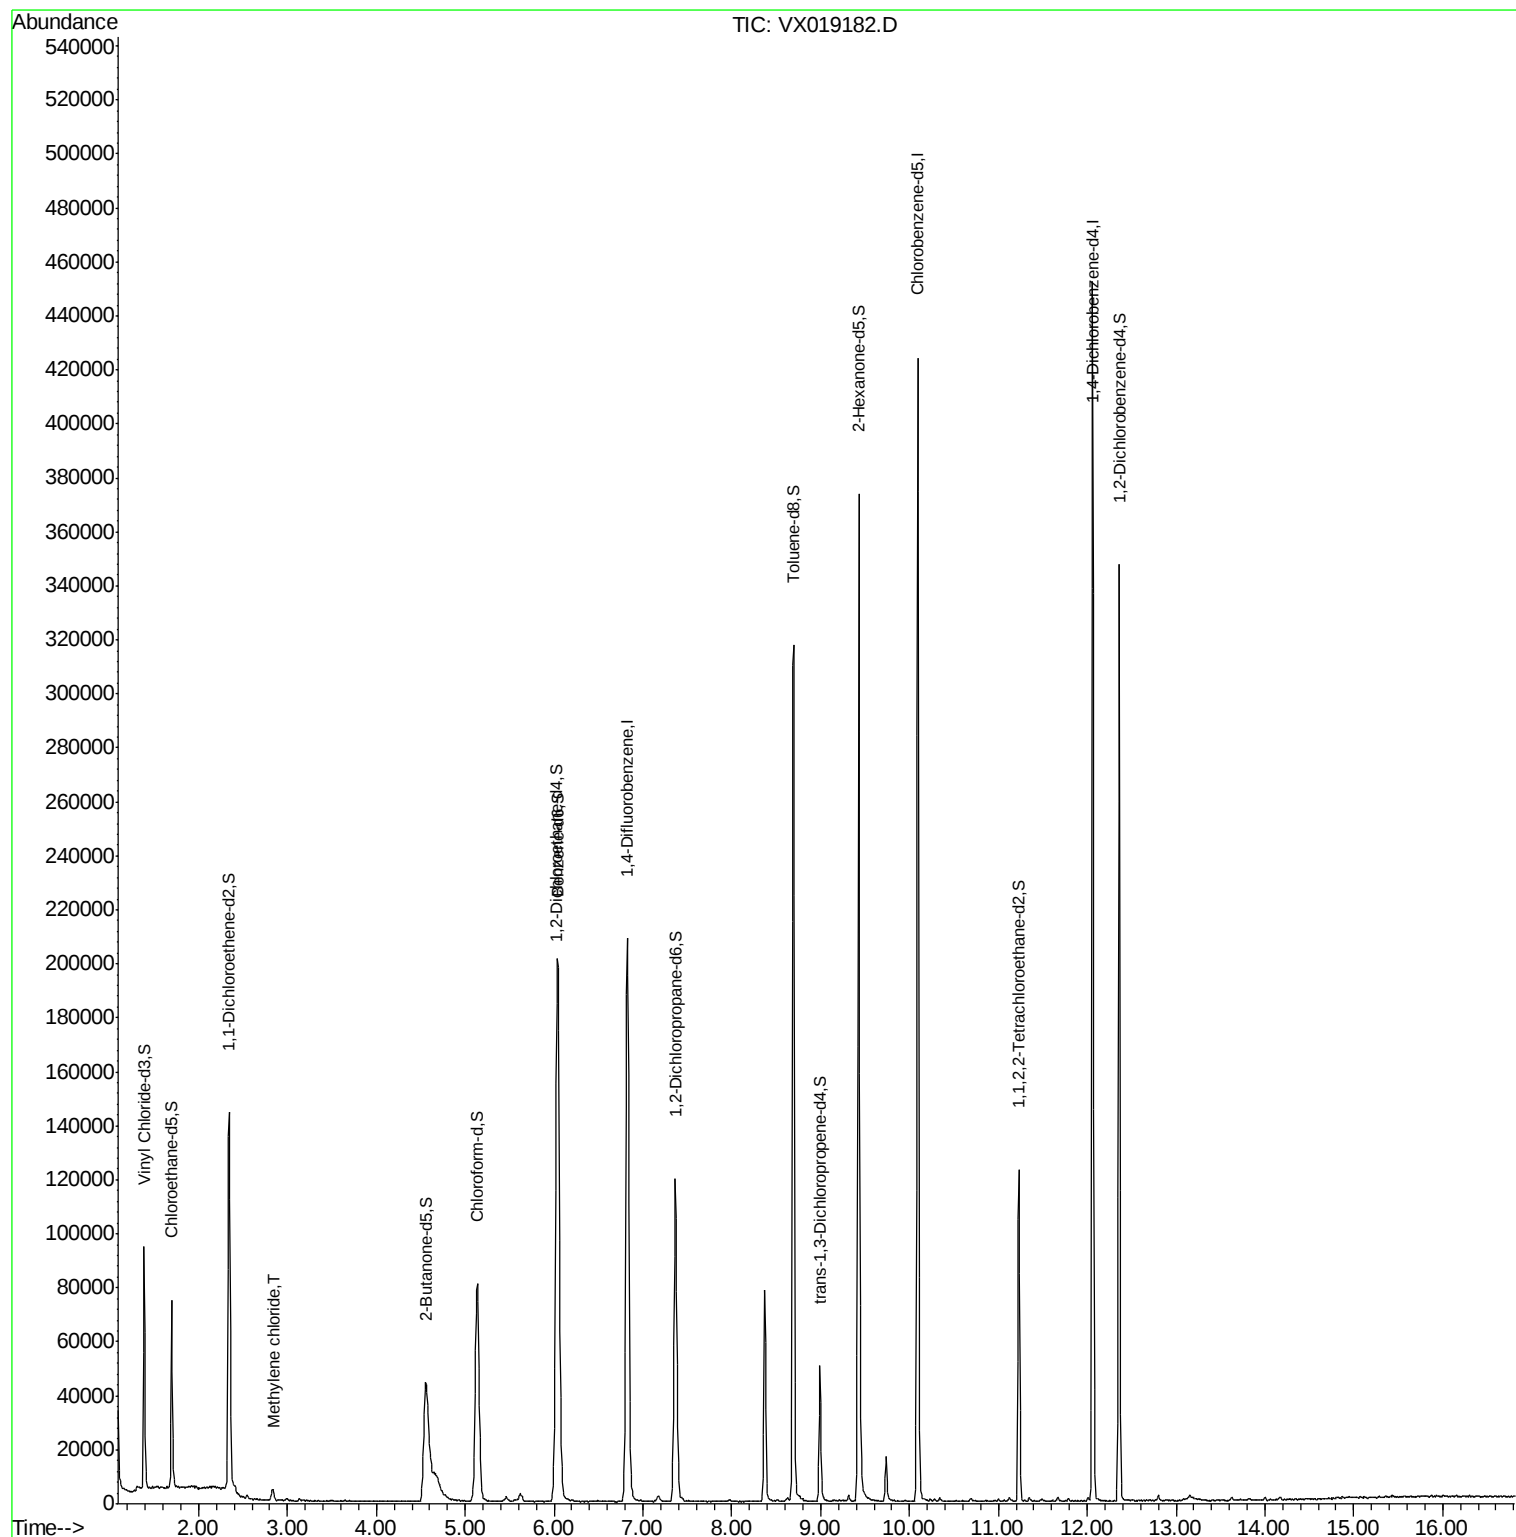

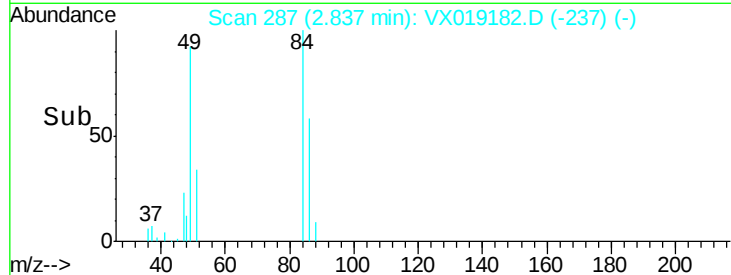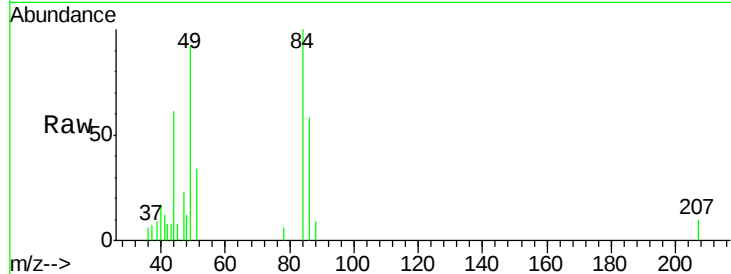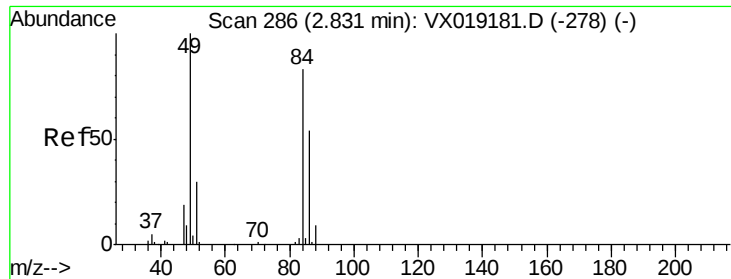

#16
Methvlene chloride
Concen: 0.118 ug/L
RT: 2.84 min Scan# 287
Delta R.T. 0.01 min
Lab File: VX019182.D
Acq: 29 Oct 2020 10:38

Instrument :
MSVOA_X
ClientSampleId :
VBLK304

Tot Ion: 84 Resp: 1929
Ion Ratio Lower Upper
84 100
86 58.0 42.2 78.4
49 92.1 77.5 143.9

