

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX103020\
 Data File : VX019183.D
 Acq On : 29 Oct 2020 11:03
 Operator : JC/MD
 Sample : VX1030WBL05
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK305

Quant Time: Oct 30 08:03:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 30 08:55:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	190073	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	167201	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.06	152	77922	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	61393	4.99	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.80%
7) Chloroethane-d5	1.70	69	51380	5.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.20%
11) 1,1-Dichloroethene-d2	2.34	63	92058	3.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.60%
20) 2-Butanone-d5	4.56	46	143880	53.54	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.08%
24) Chloroform-d	5.14	84	114089	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
26) 1,2-Dichloroethane-d4	6.03	65	64466	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
32) Benzene-d6	6.04	84	239744	5.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.20%
36) 1,2-Dichloropropane-d6	7.37	67	69047	5.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.00%
41) Toluene-d8	8.70	98	221629	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
43) trans-1,3-Dichloropropene-	8.99	79	28594	5.14	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.80%
46) 2-Hexanone-d5	9.43	63	135868	55.83	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.66%
56) 1,1,2,2-Tetrachloroethane-	11.23	84	51444	5.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.80%
66) 1,2-Dichlorobenzene-d4	12.36	152	76980	5.32	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.40%


Target Compounds					Ovalue
16) Methylene chloride	2.83	84	1688	0.116 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX103020\
Data File : VX019183.D
Acq On : 29 Oct 2020 11:03
Operator : JC/MD
Sample : VX1030WBL05
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK305

Quant Time: Oct 30 08:03:48 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 30 08:55:33 2020
Response via : Initial Calibration

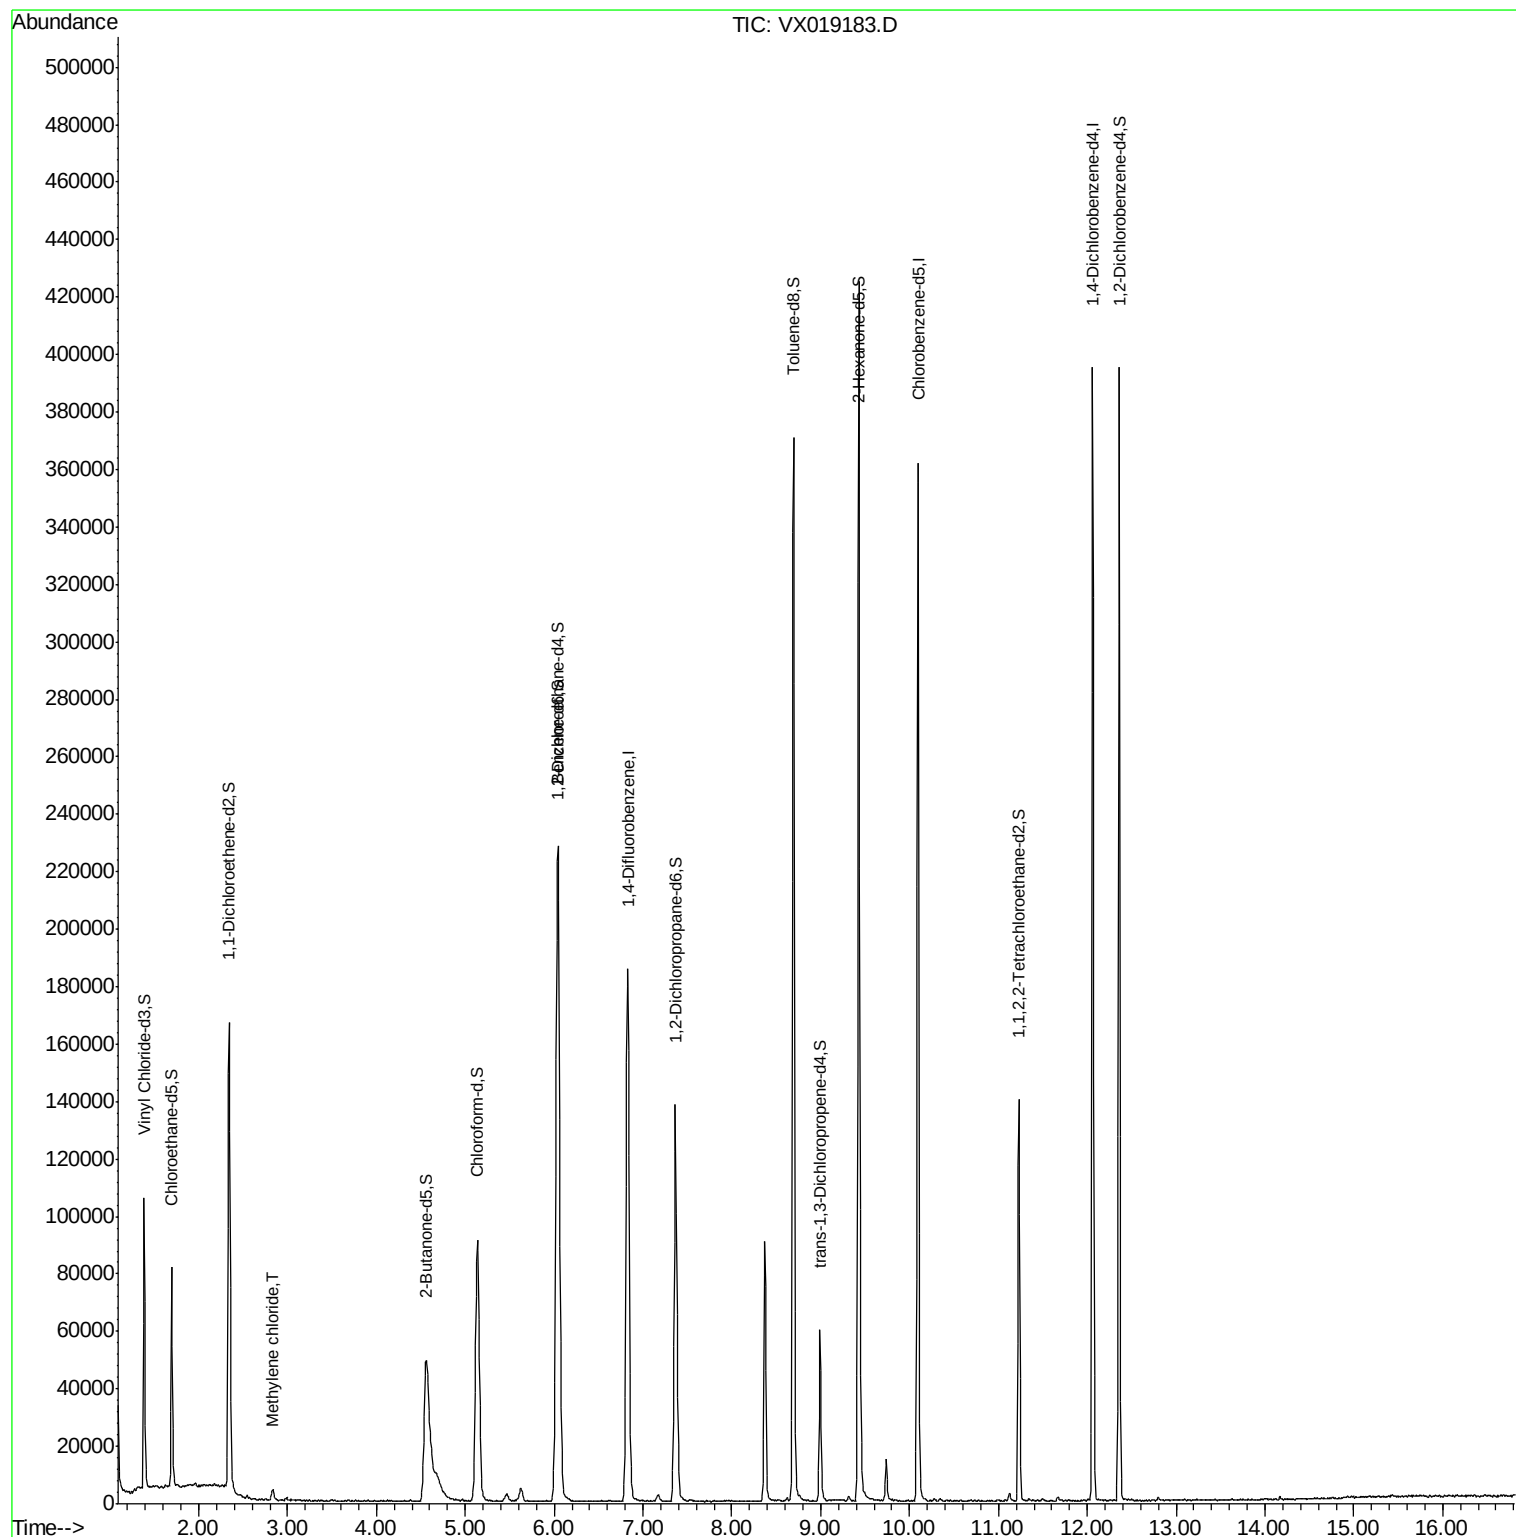

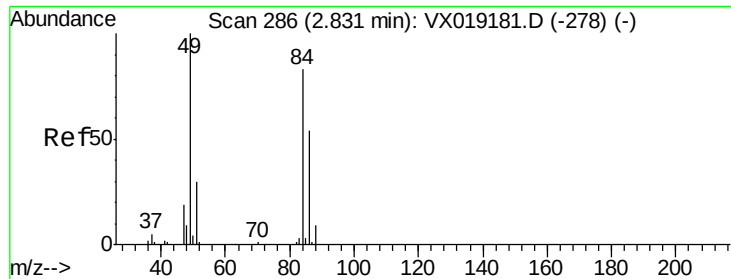

#16
Methylene chloride
Concen: 0.116 ug/L
RT: 2.83 min Scan# 286
Delta R.T. -0.00 min
Lab File: VX019183.D
Acq: 29 Oct 2020 11:03

Instrument :
MSVOA_X
ClientSampleId :
VBLK305

Tot Ion: 84 Resp: 1688

Ion	Ratio	Lower	Upper
84	100		
86	68.6	42.2	78.4
49	110.6	77.5	143.9

