

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX103020\
 Data File : VX019184.D
 Acq On : 29 Oct 2020 11:41
 Operator : JC/MD
 Sample : VX1030WBL04
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK306

Quant Time: Oct 30 08:06:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 30 08:55:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.82	114	195508	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.09	117	177675	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.06	152	81738	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	62452	4.94	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.80%
7) Chloroethane-d5	1.70	69	52777	5.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.20%
11) 1,1-Dichloroethene-d2	2.34	63	92704	3.75	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.00%
20) 2-Butanone-d5	4.56	46	145313	52.57	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.14%
24) Chloroform-d	5.14	84	117397	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
26) 1,2-Dichloroethane-d4	6.03	65	65013	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	6.04	84	241440	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
36) 1,2-Dichloropropane-d6	7.37	67	70761	5.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.20%
41) Toluene-d8	8.70	98	225426	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
43) trans-1,3-Dichloropropene-	8.99	79	29182	4.94	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.80%
46) 2-Hexanone-d5	9.43	63	134882	52.16	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.32%
56) 1,1,2,2-Tetrachloroethane-	11.23	84	51304	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.40%
66) 1,2-Dichlorobenzene-d4	12.36	152	77866	5.13	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.60%


Target Compounds					Ovalue
16) Methylene chloride	2.83	84	3834	0.256 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX103020\
Data File : VX019184.D
Acq On : 29 Oct 2020 11:41
Operator : JC/MD
Sample : VX1030WBL04
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK306

Quant Time: Oct 30 08:06:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 30 08:55:33 2020
Response via : Initial Calibration

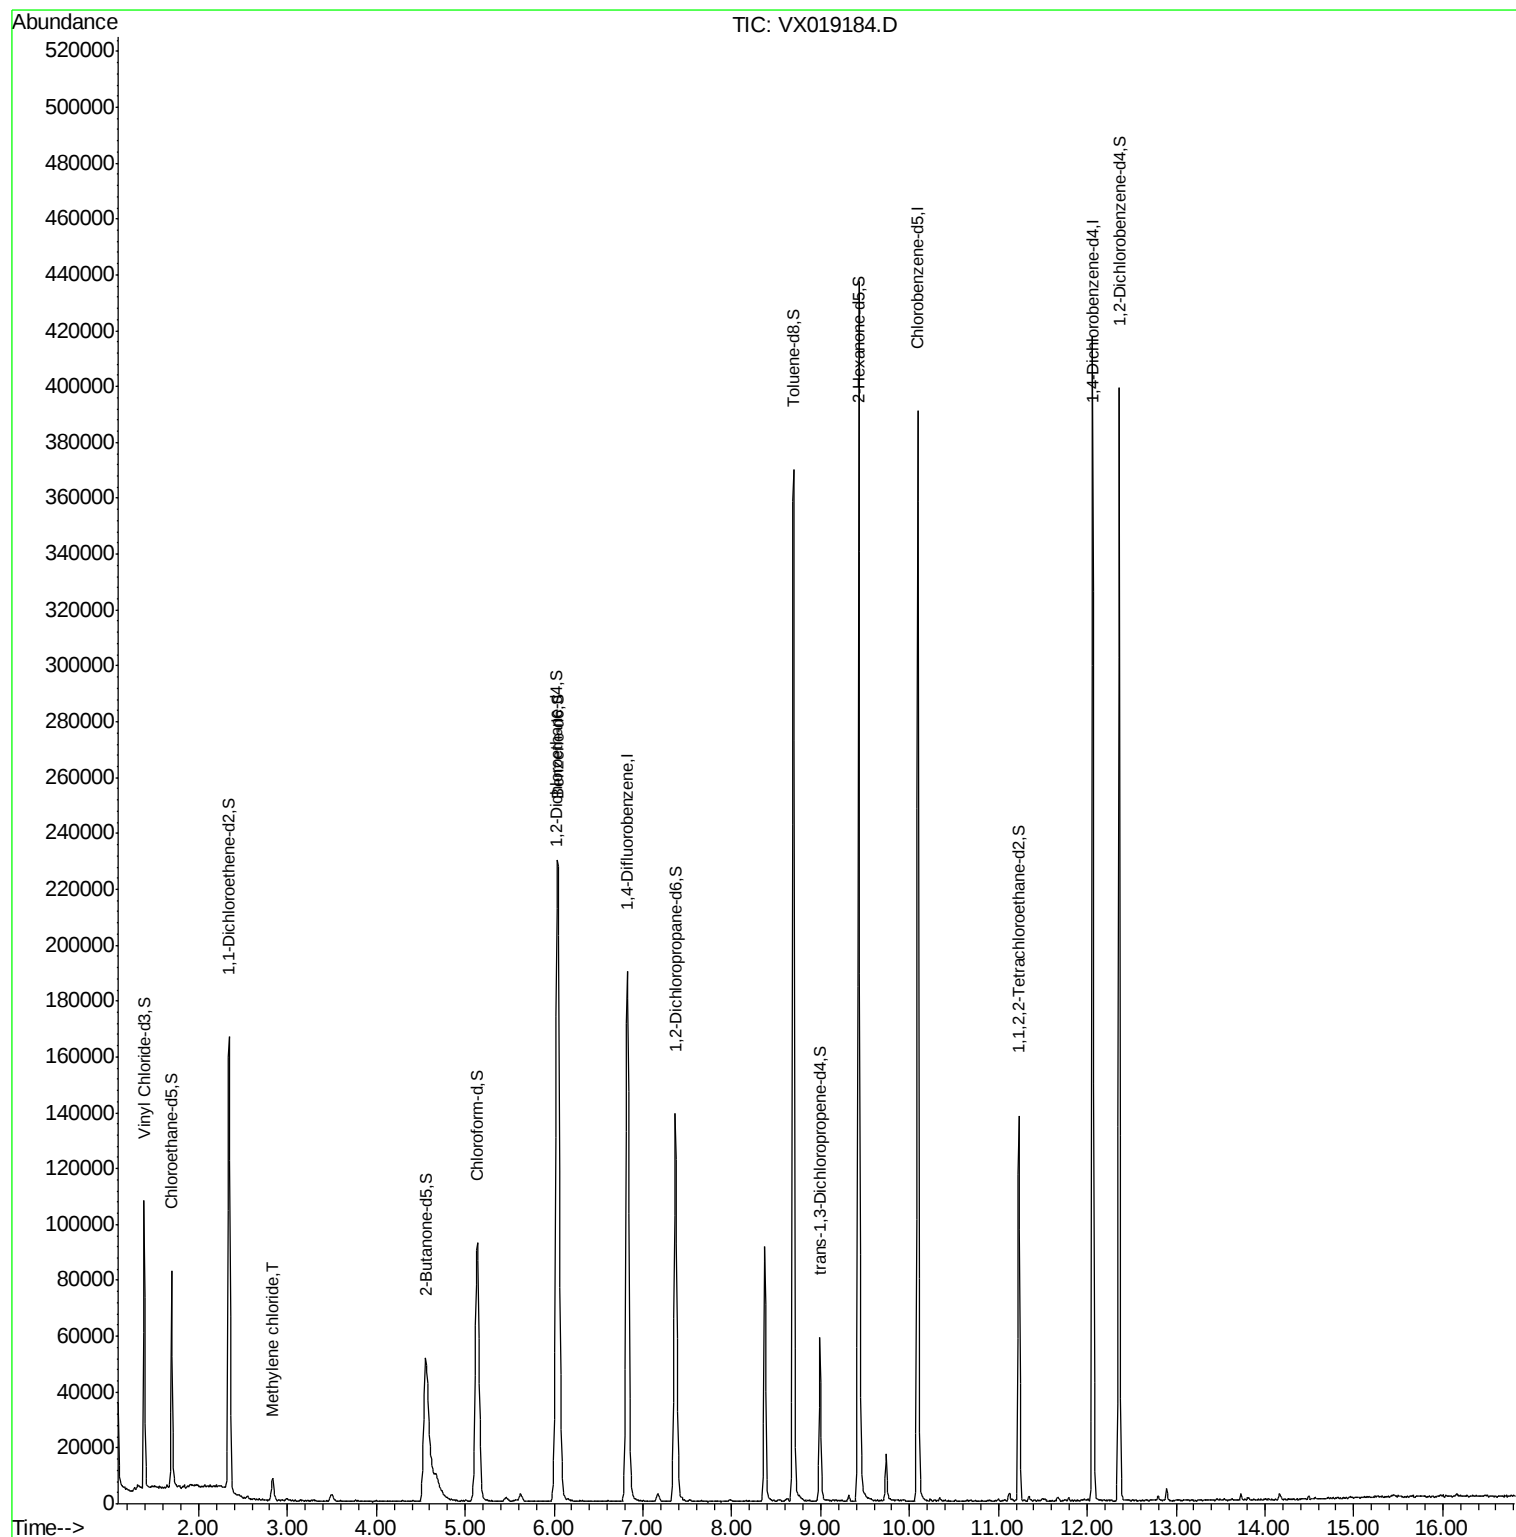

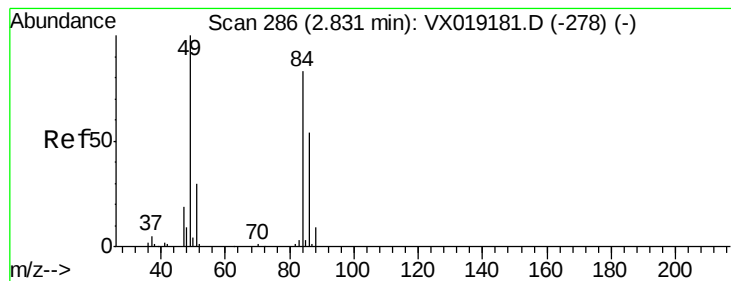

#16
 Methvlene chloride
 Concen: 0.256 ug/L
 RT: 2.83 min Scan# 286
 Delta R.T. 0.00 min
 Lab File: VX019184.D
 Acq: 29 Oct 2020 11:41

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK306

Tot Ion: 84 Resp: 3834
 Ion Ratio Lower Upper
 84 100
 86 62.0 42.2 78.4
 49 108.1 77.5 143.9

