


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX103020\
Data File : VX019180.D
Acq On : 29 Oct 2020 09:23
Operator : JC/MD
Sample : BFB62
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB62

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Oct 30 08:55:33 2020

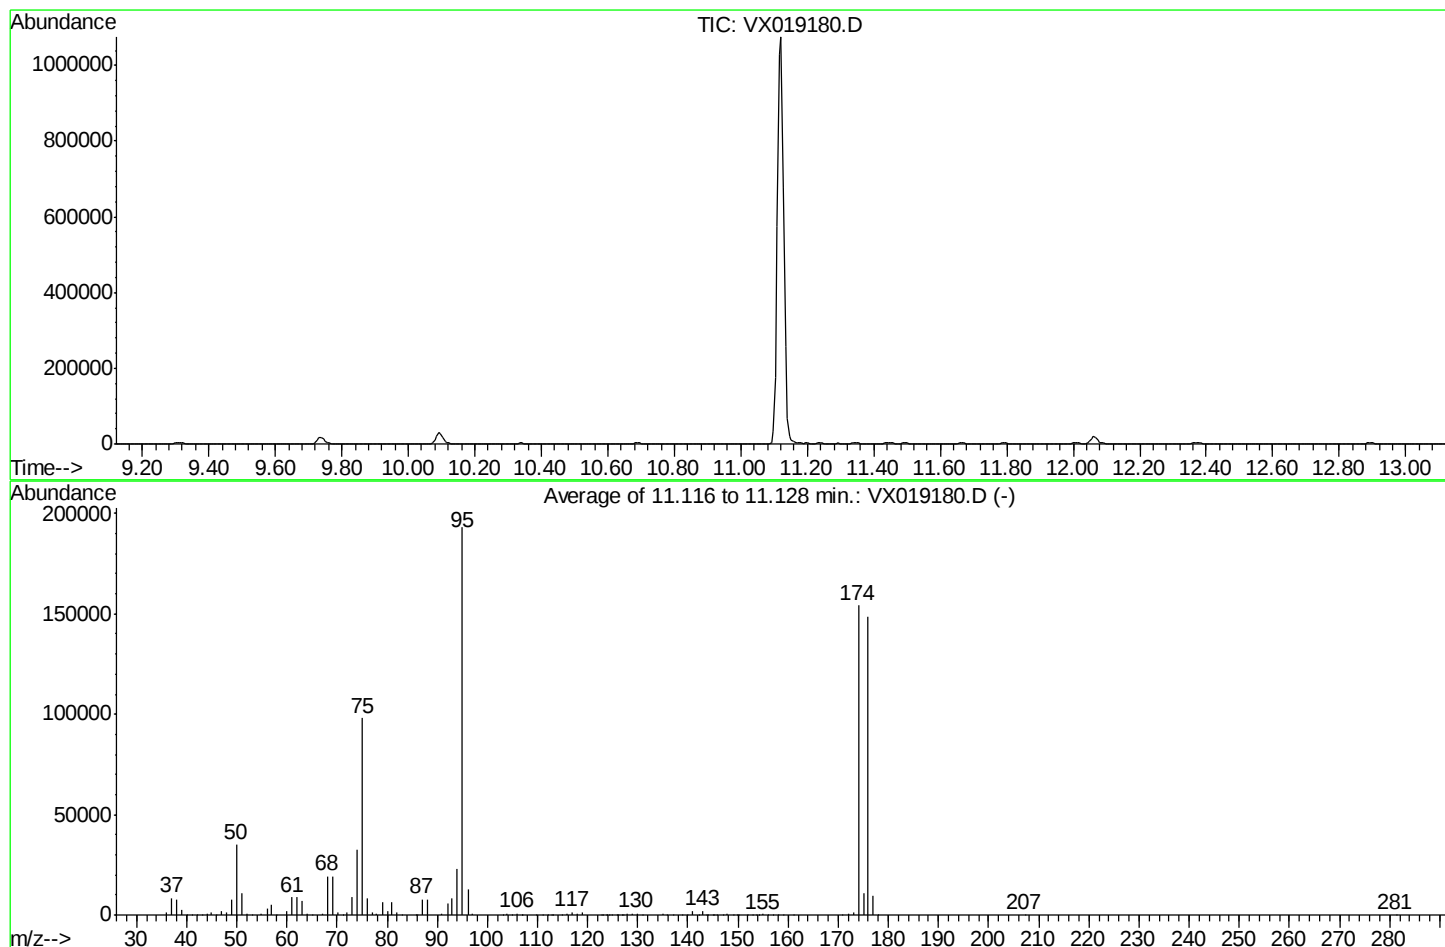

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	34789	PASS
75	95	30	80	50.8	98106	PASS
95	95	100	100	100.0	193109	PASS
96	95	5	9	6.7	12887	PASS
173	174	0.00	2	0.8	1247	PASS
174	95	50	120	79.9	154248	PASS
175	174	5	9	6.9	10615	PASS
176	174	95	105	96.2	148320	PASS
177	176	5	10	6.3	9319	PASS

m/z	Abundance
36.00	1690.0
37.00	10208.0
38.00	9043.0
39.00	3313.0
39.90	367.0
41.10	84.0
42.10	64.0
43.10	130.0
44.10	1657.0
45.00	1754.0
45.90	221.0
47.00	2378.0
48.00	1296.0
49.10	8845.0
50.00	42664.0
51.00	13030.0
52.00	581.0
53.00	55.0
55.00	687.0
56.10	3510.0
57.00	6069.0
58.00	258.0
60.00	2069.0
61.00	10934.0
62.00	11321.0
63.00	8366.0
64.00	934.0
65.10	226.0
67.00	563.0
68.00	22752.0
69.00	23328.0
70.10	1917.0
72.00	1264.0
73.00	10625.0
74.10	39144.0
75.00	115464.0
76.10	10021.0
77.00	1304.0
77.90	872.0
79.00	7343.0
80.00	2022.0
80.90	7621.0
81.90	1577.0
83.10	198.0
86.00	301.0
87.00	9311.0
88.00	8716.0
91.00	854.0
92.10	6298.0
93.00	9545.0
94.00	26184.0
95.10	218496.0
96.10	15365.0
97.10	532.0
103.00	70.0
103.90	978.0
104.90	316.0
105.90	1082.0
106.90	236.0
109.90	139.0
110.90	220.0
111.90	213.0
112.90	178.0
114.90	261.0
115.90	765.0
116.90	1523.0
117.90	876.0
119.00	1172.0
122.80	117.0
123.70	127.0
124.20	59.0
124.90	146.0
125.80	64.0
126.80	58.0
127.90	839.0
128.90	334.0
129.90	880.0
130.90	331.0
135.00	411.0
135.90	60.0
137.00	327.0
138.90	64.0
139.90	145.0
140.90	2185.0
142.00	291.0
142.90	2279.0
144.00	156.0
145.30	145.0
145.80	315.0
147.00	121.0
147.90	465.0
149.00	179.0

Instrument :
MSVOA_X
ClientSampleId :
BFB62

149.90	227.0
152.00	64.0
152.90	290.0
154.00	91.0
154.90	442.0
155.90	96.0
156.90	363.0
159.00	274.0
161.00	190.0
170.70	51.0
172.00	427.0
173.10	1354.0
174.00	153536.0
175.00	11250.0
176.00	147776.0
177.00	9713.0
178.00	319.0
207.10	150.0

Instrument :
MSVOA_X
ClientSampleId :
BFB62

m/z	Abundance
36.00	1697.0
37.00	9541.0
38.00	8644.0
39.00	3223.0
40.00	325.0
41.10	57.0
42.00	65.0
42.90	198.0
44.00	1592.0
45.00	1903.0
46.00	208.0
47.00	2193.0
47.90	1226.0
49.00	8935.0
50.00	39360.0
51.10	12033.0
52.00	477.0
54.90	511.0
56.00	3462.0
57.00	5976.0
58.00	212.0
60.00	2097.0
61.00	10120.0
62.00	10182.0
63.00	7617.0
64.10	759.0
65.10	242.0
67.00	734.0
68.00	22432.0
69.10	21688.0
70.00	1861.0
71.20	77.0
72.10	1129.0
73.00	10236.0
74.10	37048.0
75.10	110888.0
76.10	10016.0
77.00	1173.0
78.00	951.0
79.00	7287.0
80.00	1861.0
81.00	7468.0
81.90	1751.0
83.00	216.0
86.10	253.0
87.00	8916.0
88.00	8655.0
90.90	1073.0
92.00	6412.0
93.00	9580.0
94.00	26872.0
95.00	225472.0
96.10	15188.0
97.10	353.0
103.00	85.0
103.90	1161.0
104.90	341.0
106.00	1184.0
106.80	158.0
107.10	147.0
109.80	131.0
110.90	276.0
112.00	220.0
113.10	207.0
114.90	252.0
116.00	756.0
117.00	1574.0
117.90	822.0
118.90	1276.0
123.00	89.0
123.90	133.0
124.80	55.0
126.00	66.0
127.00	64.0
128.00	714.0
128.90	466.0
129.90	840.0
130.90	388.0
135.00	393.0
135.80	88.0
137.00	412.0
138.90	61.0
140.00	169.0
141.00	2447.0
142.10	256.0
143.00	2554.0
144.10	169.0
144.90	223.0
145.90	314.0
146.90	101.0
147.90	481.0
148.80	127.0

Instrument :
MSVOA_X
ClientSampleId :
BFB62

149.90	309.0
151.80	89.0
152.80	209.0
154.10	135.0
155.00	526.0
157.00	379.0
157.90	64.0
159.00	210.0
160.90	268.0
171.90	482.0
173.00	1212.0
174.00	184128.0
175.00	12373.0
176.00	172224.0
177.00	10710.0
178.00	228.0
207.20	119.0
281.30	62.0

Instrument :
MSVOA_X
ClientSampleId :
BFB62

m/z	Abundance
36.10	816.0
37.00	5229.0
38.00	4720.0
39.00	1857.0
40.00	255.0
41.00	122.0
43.00	139.0
44.00	1245.0
45.00	956.0
46.10	98.0
47.10	1006.0
48.00	728.0
49.00	4898.0
50.00	22344.0
51.00	6894.0
52.00	324.0
55.00	373.0
56.00	1742.0
57.10	3357.0
58.10	147.0
60.00	1025.0
61.00	5652.0
62.00	5849.0
63.00	4366.0
64.00	413.0
65.00	205.0
67.00	323.0
68.00	13117.0
69.00	13170.0
70.10	848.0
71.10	54.0
72.10	675.0
73.00	5746.0
74.00	21888.0
75.00	67968.0
76.10	5230.0
77.00	720.0
78.00	524.0
78.90	4016.0
80.00	1285.0
81.00	4505.0
81.90	953.0
83.10	86.0
85.70	108.0
87.00	5041.0
88.00	5096.0
90.90	555.0
92.00	3882.0
93.10	5389.0
94.00	16151.0
95.10	135360.0
96.10	8110.0
97.00	279.0
103.90	636.0
104.80	234.0
105.90	658.0
107.00	139.0
109.70	110.0
111.00	218.0
111.90	122.0
112.90	137.0
114.90	166.0
116.00	546.0
116.90	971.0
117.80	538.0
119.00	879.0
123.90	105.0
126.00	84.0
128.00	493.0
128.90	263.0
130.00	466.0
131.00	211.0
134.90	331.0
135.70	73.0
136.90	282.0
138.80	67.0
140.00	98.0
140.90	1533.0
142.00	163.0
143.00	1731.0
143.80	100.0
144.90	215.0
145.80	273.0
147.00	100.0
147.90	323.0
149.00	159.0
150.10	109.0
151.90	127.0
152.90	94.0
153.70	62.0
155.00	465.0
157.00	202.0

Instrument :
MSVOA_X
ClientSampleId :
BFB62

158.90	146.0
161.00	209.0
171.90	323.0
173.10	1177.0
174.00	125080.0
175.00	8224.0
176.00	124960.0
177.00	7534.0
178.00	250.0
207.30	69.0
281.30	68.0

Instrument :
MSVOA_X
ClientSampleId :
BFB62

Scan 1637 (11.067 min): VX019180.D
BFB62

m/z	Abundance
40.00	190.0
44.00	769.0
55.20	56.0
72.90	68.0
207.30	95.0

Instrument :
MSVOA_X
ClientSampleId :
BFB62