


Chloroethane

Response Ratio

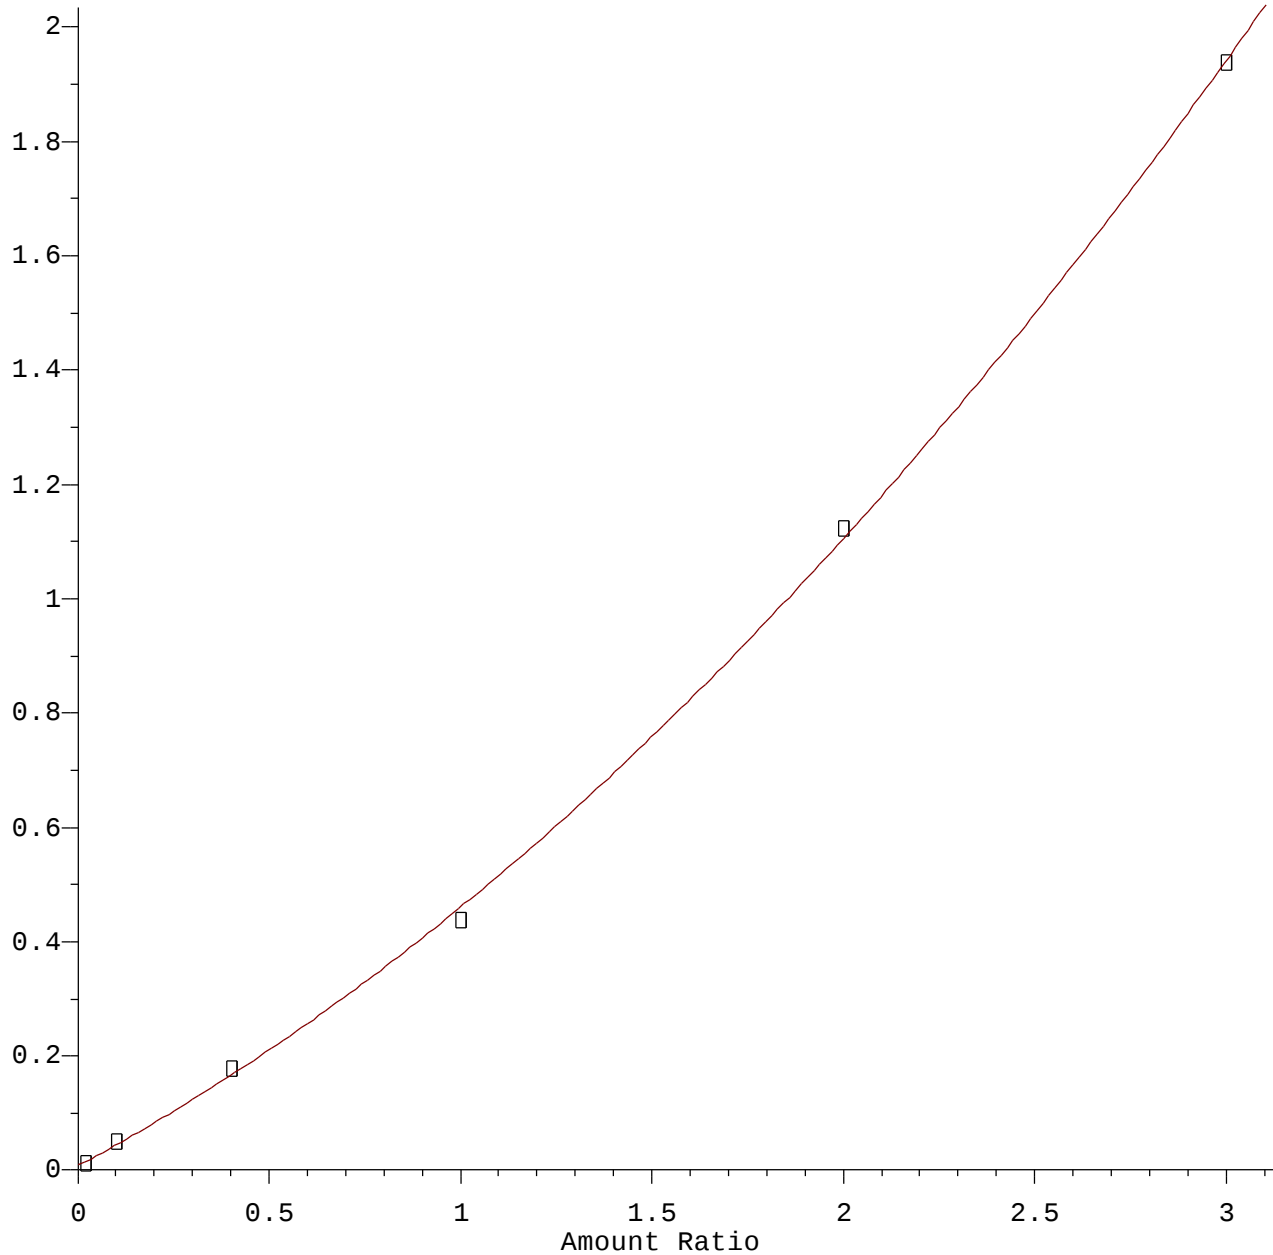


$R = 9.59e-002 A^2 + 3.57e-001 A + 7.52e-003$
Coef of Det (r^2) = 1.000 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103118W.M
Calibration Table Last Updated: Thu Nov 01 11:24:18 2018


2-Chloroethyl Vinyl ether

Response Ratio

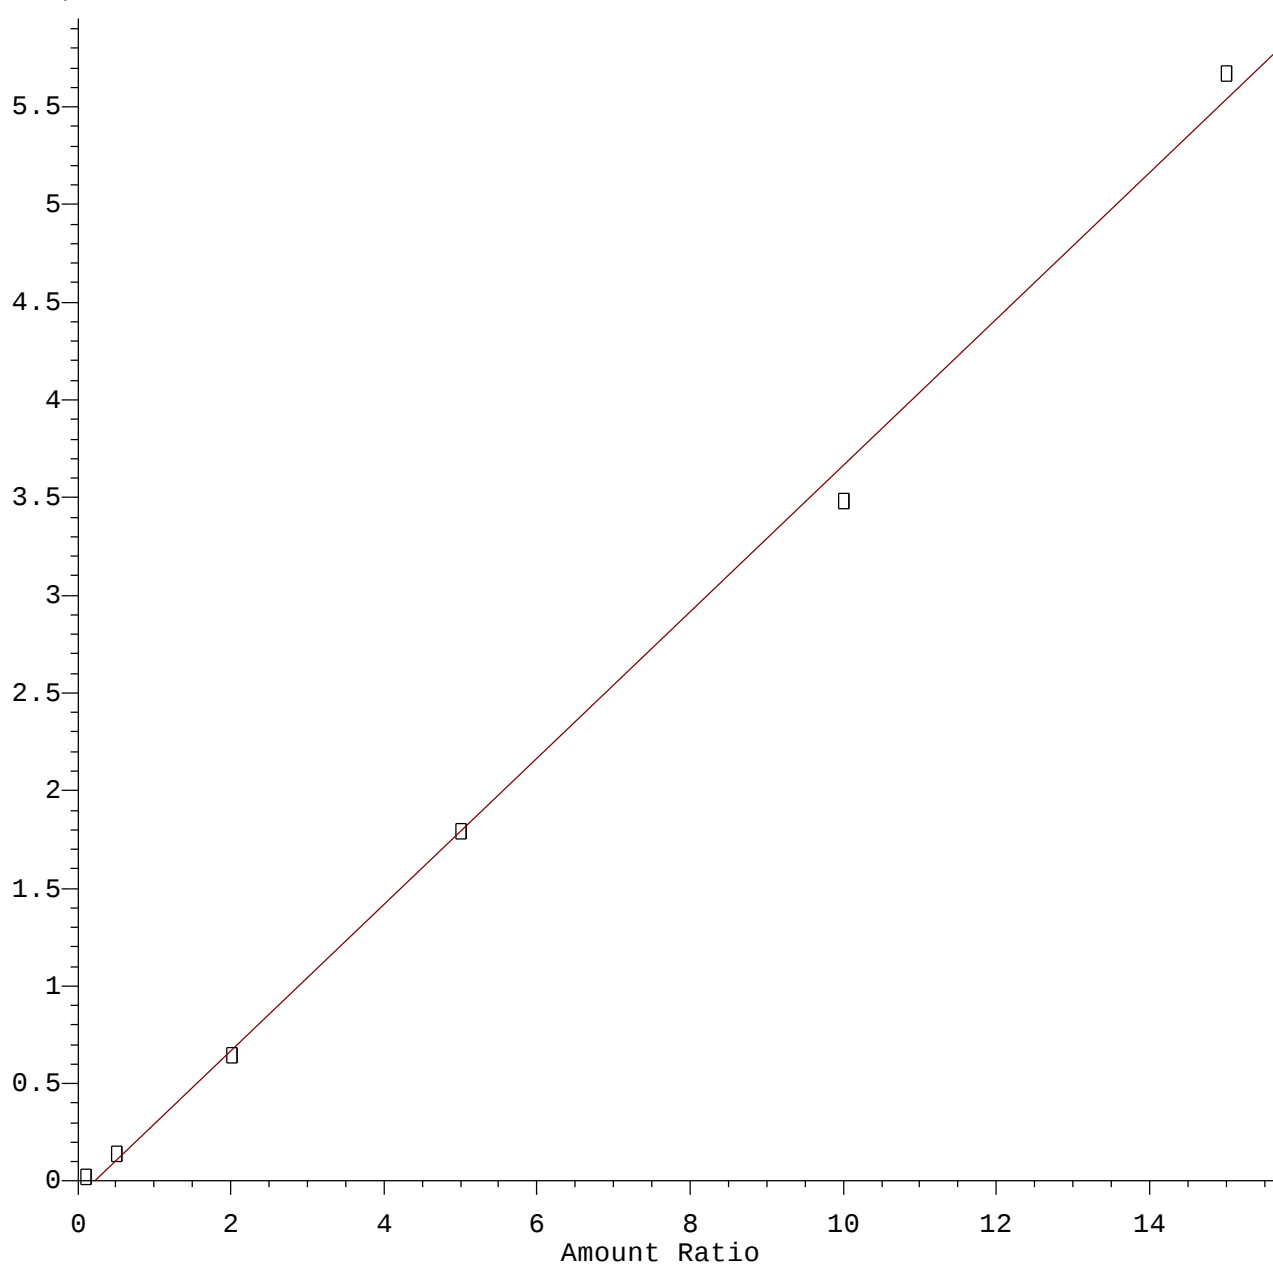


Resp Ratio = $3.74 \times 10^{-1} \times \text{Amt} - 7.74 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103118W.M
Calibration Table Last Updated: Thu Nov 01 11:24:18 2018

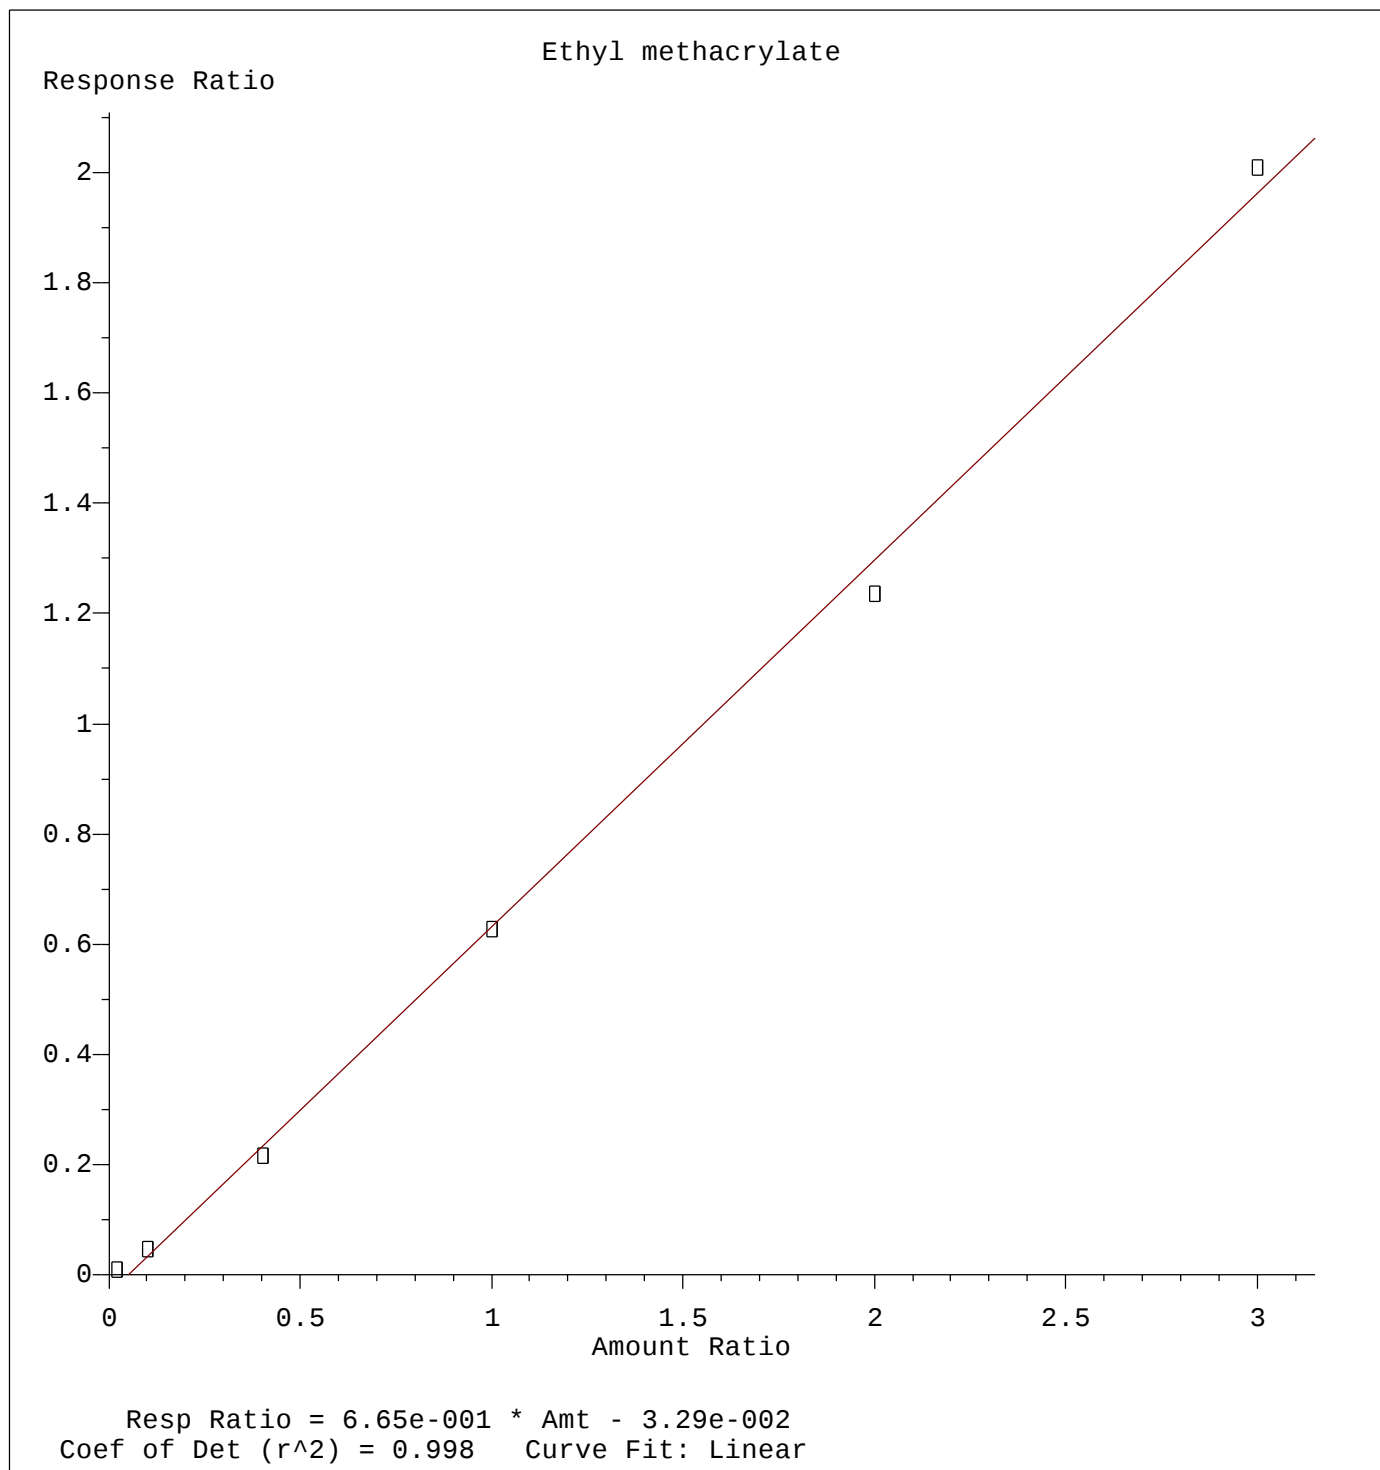


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103118W.M
Calibration Table Last Updated: Thu Nov 01 11:24:18 2018

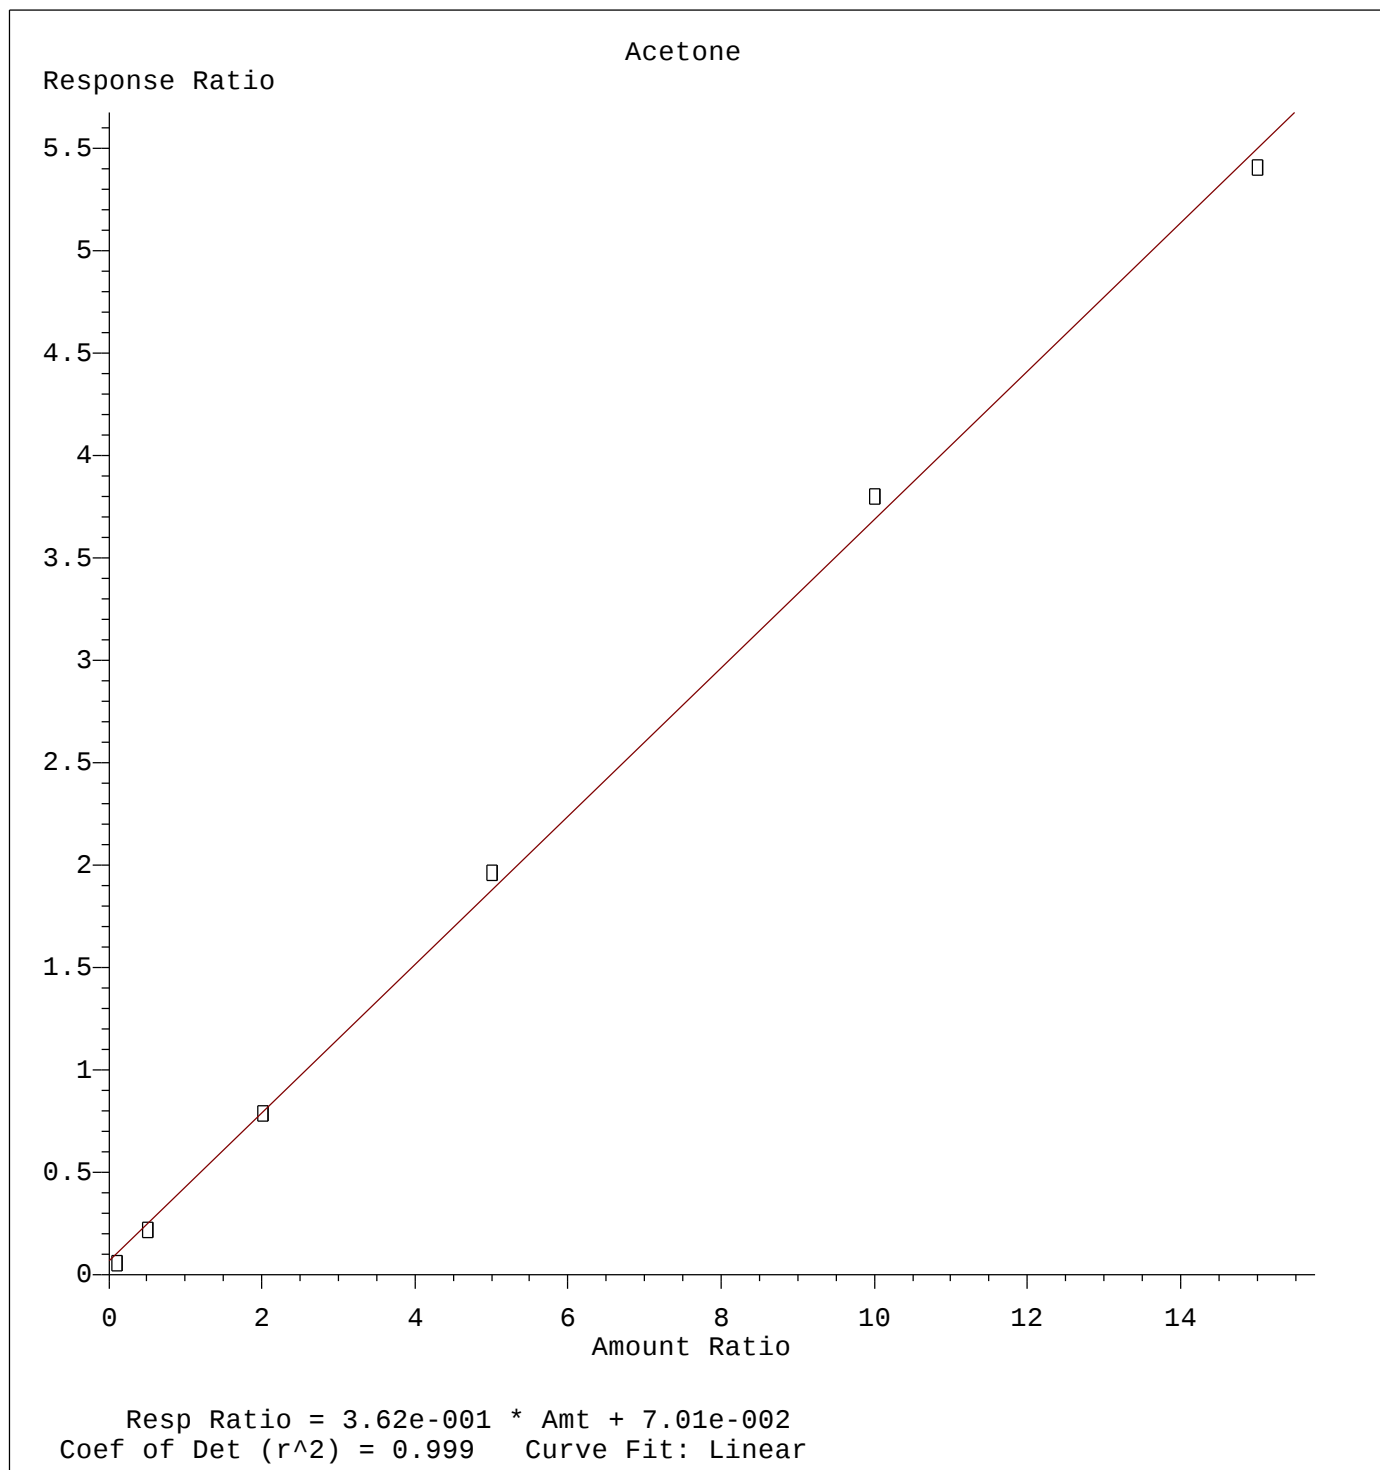

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103118W.M
Calibration Table Last Updated: Thu Nov 01 11:24:18 2018


Acrolein

Response Ratio

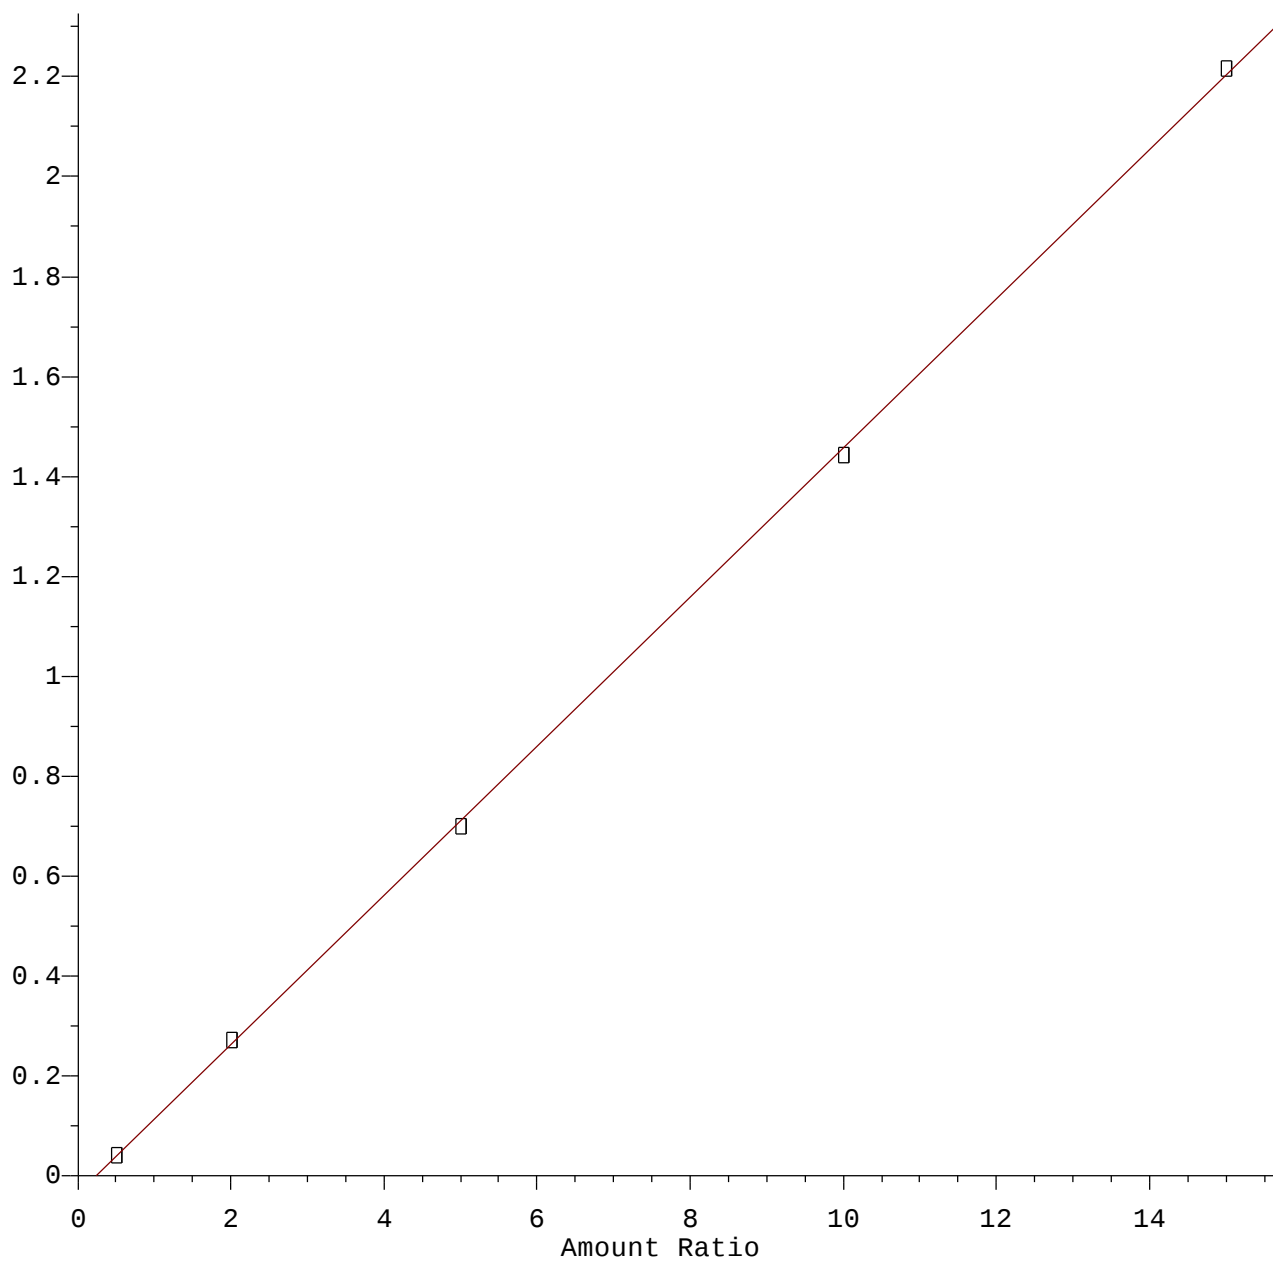

Resp Ratio = $1.49 \times 10^{-1} \times \text{Amt} - 3.64 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103118W.M
Calibration Table Last Updated: Thu Nov 01 11:24:18 2018

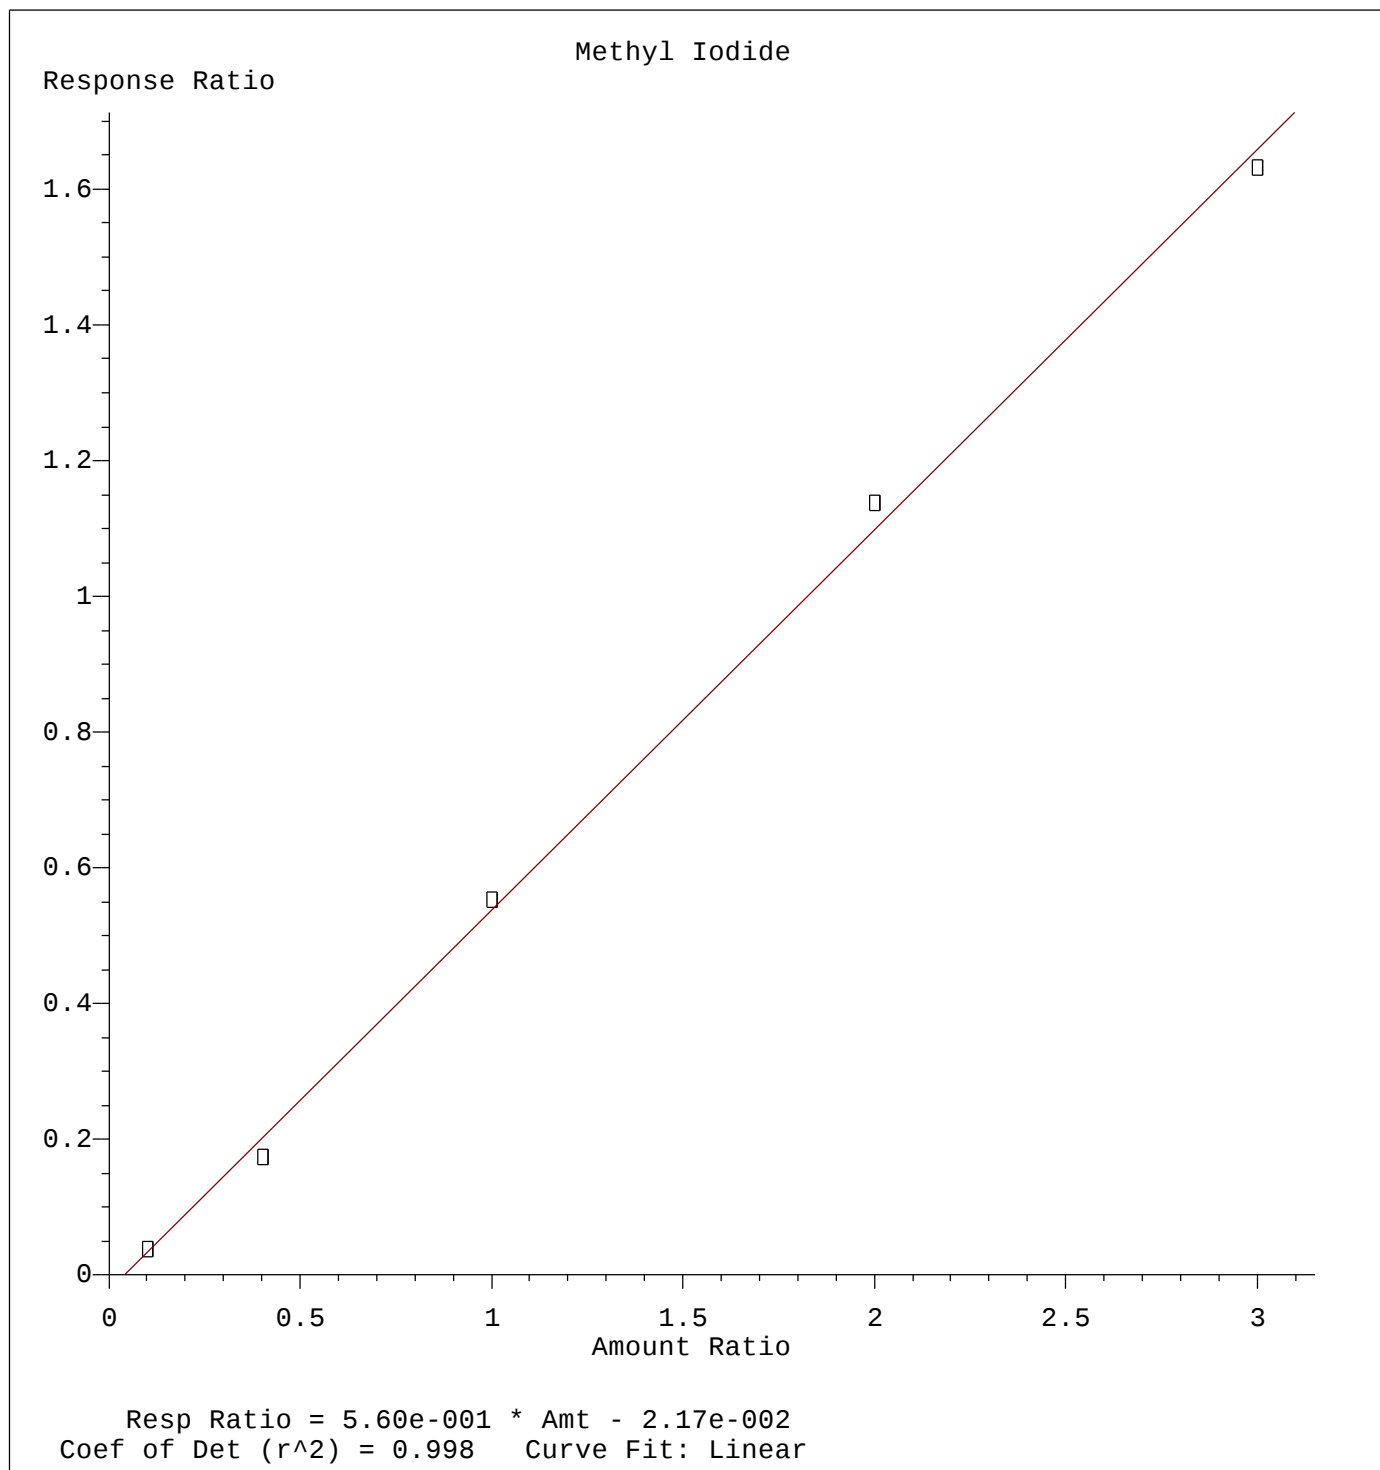

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103118W.M
Calibration Table Last Updated: Thu Nov 01 11:24:18 2018