

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103122\
 Data File : VX032491.D
 Acq On : 31 Oct 2022 16:30
 Operator : JC/MD
 Sample : N5340-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-4R-102722

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	36	rBV	58012	56760	9.15%	1.657%
2	2.562	231	242	254	rBV	4150	14708	2.37%	0.429%
3	2.946	297	305	317	rBV	6585	14888	2.40%	0.435%
4	4.568	560	571	585	rBV	2964	10918	1.76%	0.319%
5	5.385	694	705	721	rBV2	76165	222026	35.80%	6.483%
6	5.550	721	732	746	rVV	127680	366975	59.17%	10.715%
7	5.958	788	799	813	rBV2	81069	218867	35.29%	6.391%
8	6.763	921	931	948	rBV	199476	466915	75.28%	13.634%
9	8.647	1234	1240	1249	rBV	389624	620204	100.00%	18.110%
10	10.055	1465	1471	1487	rVB	388253	524819	84.62%	15.324%
11	11.079	1634	1639	1652	rBV	338582	443691	71.54%	12.955%
12	12.024	1789	1794	1807	rBV	383033	463961	74.81%	13.547%




Sum of corrected areas: 3424732

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103122\
Data File : VX032491.D
Acq On : 31 Oct 2022 16:30
Operator : JC/MD
Sample : N5340-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-4R-102722

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

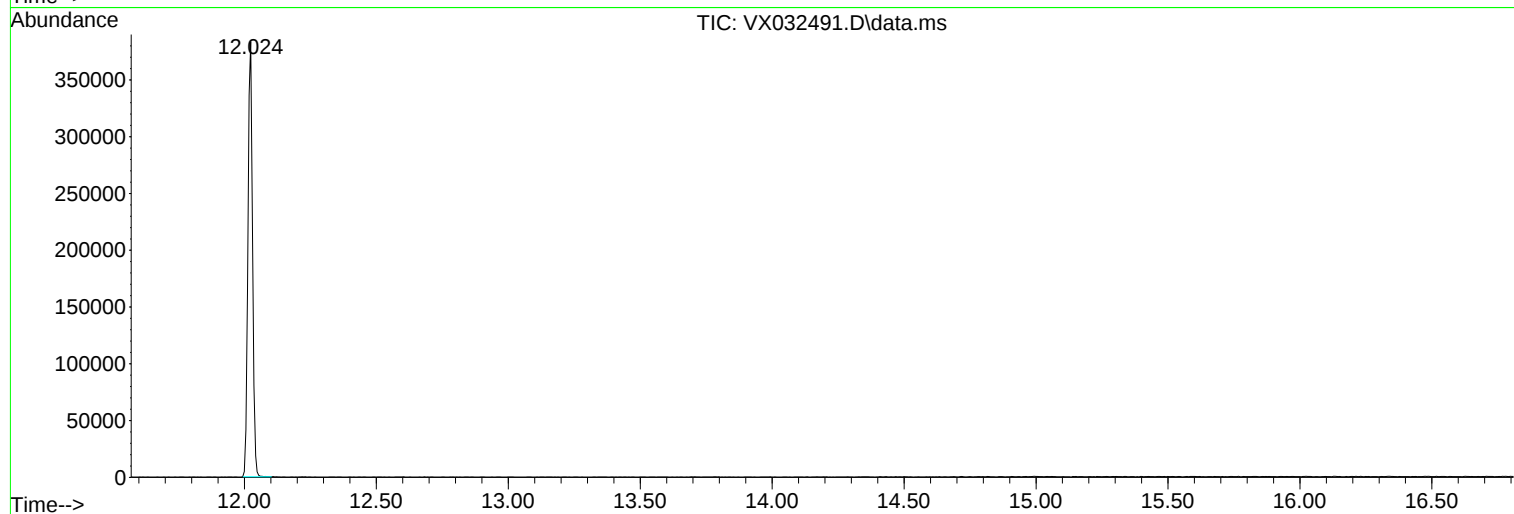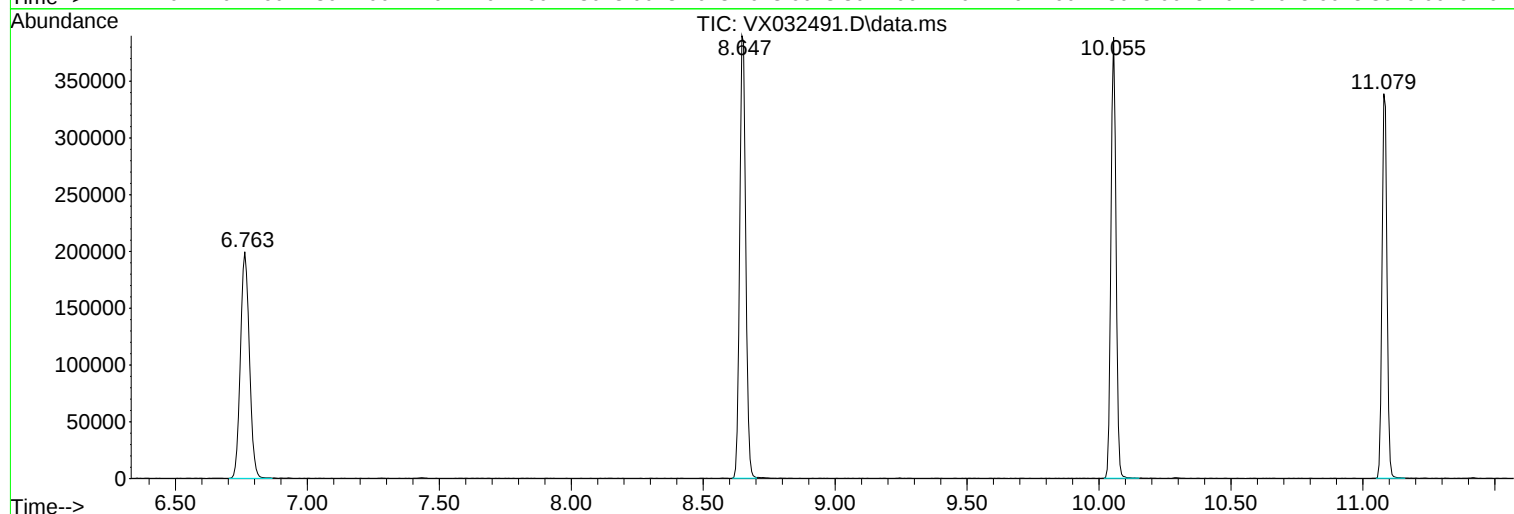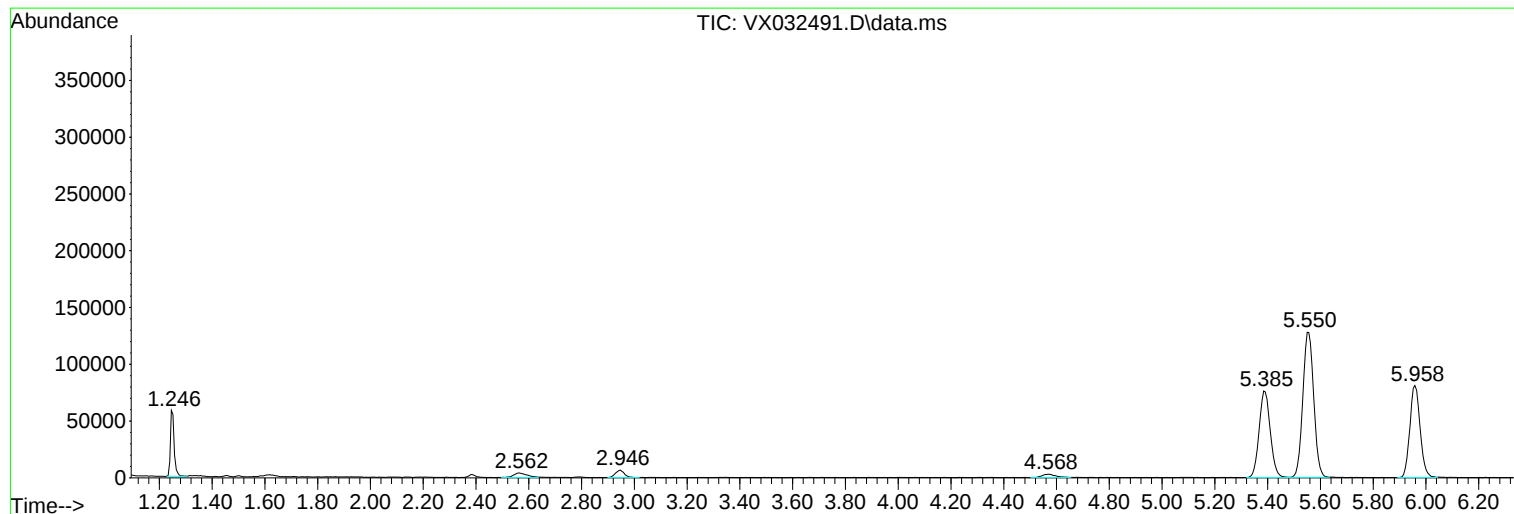

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103122\
Data File : VX032491.D
Acq On : 31 Oct 2022 16:30
Operator : JC/MD
Sample : N5340-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-4R-102722

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103122\
Data File : VX032491.D
Acq On : 31 Oct 2022 16:30
Operator : JC/MD
Sample : N5340-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-4R-102722

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------