

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103122\
Data File : VX032492.D
Acq On : 31 Oct 2022 16:53
Operator : JC/MD
Sample : N5340-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6-102722

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	33	rBV	47586	45961	7.03%	1.266%
2	2.550	231	240	254	rVB	3764	10269	1.57%	0.283%
3	2.940	296	304	315	rBV	5856	13437	2.05%	0.370%
4	4.562	561	570	581	rBV2	3305	10420	1.59%	0.287%
5	5.385	693	705	720	rBV	78273	228385	34.91%	6.291%
6	5.550	722	732	747	rVB2	131908	375924	57.46%	10.355%
7	5.958	788	799	813	rBV	84117	223574	34.18%	6.158%
8	6.763	921	931	952	rBV	204975	486698	74.40%	13.406%
9	8.653	1234	1241	1251	rBV	411936	654201	100.00%	18.020%
10	10.055	1465	1471	1481	rBV	421636	562146	85.93%	15.484%
11	11.079	1634	1639	1654	rBV	371311	482509	73.76%	13.291%
12	12.024	1788	1794	1803	rBV	435803	536864	82.06%	14.788%




Sum of corrected areas: 3630388

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103122\
Data File : VX032492.D
Acq On : 31 Oct 2022 16:53
Operator : JC/MD
Sample : N5340-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6-102722

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

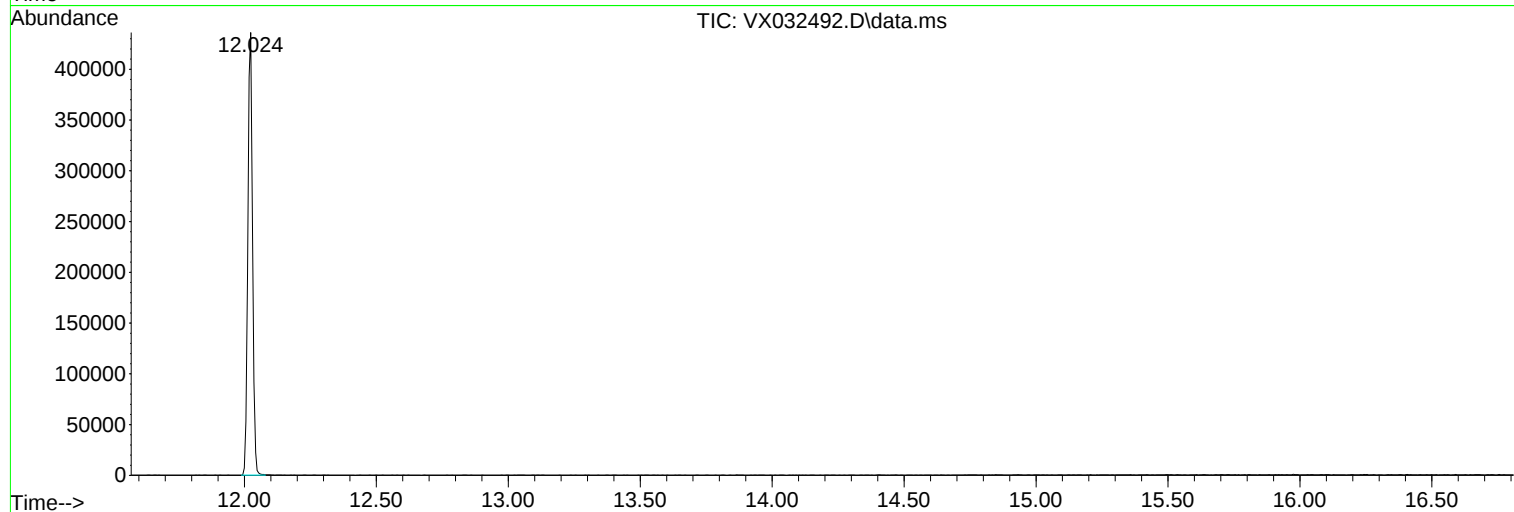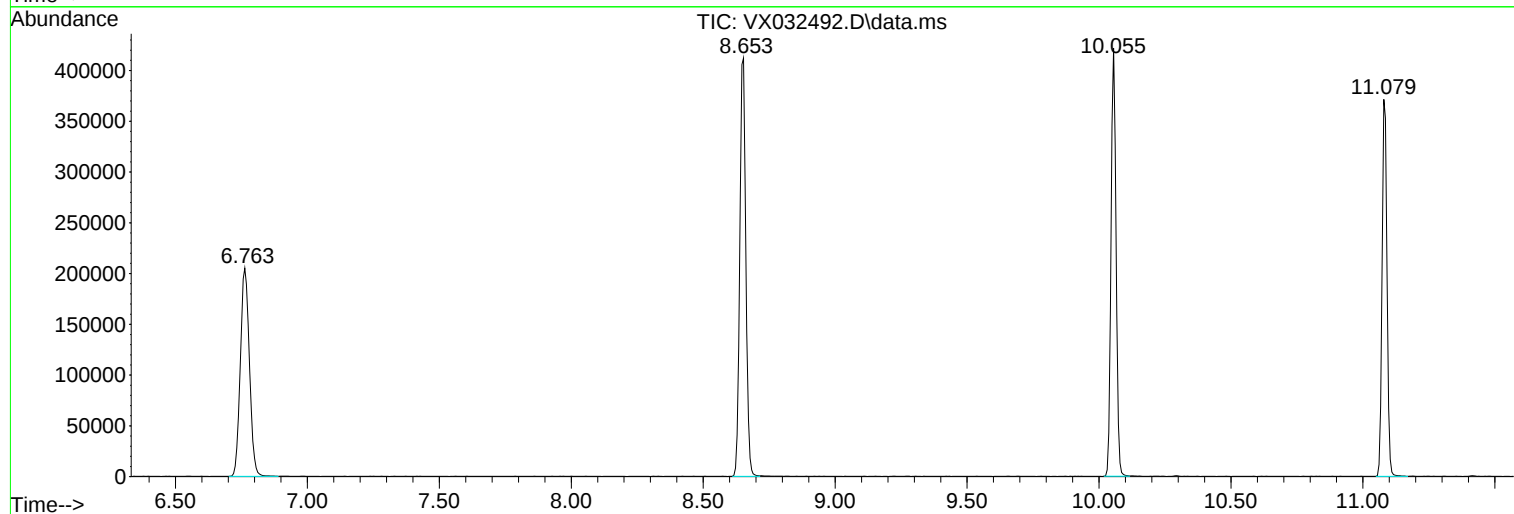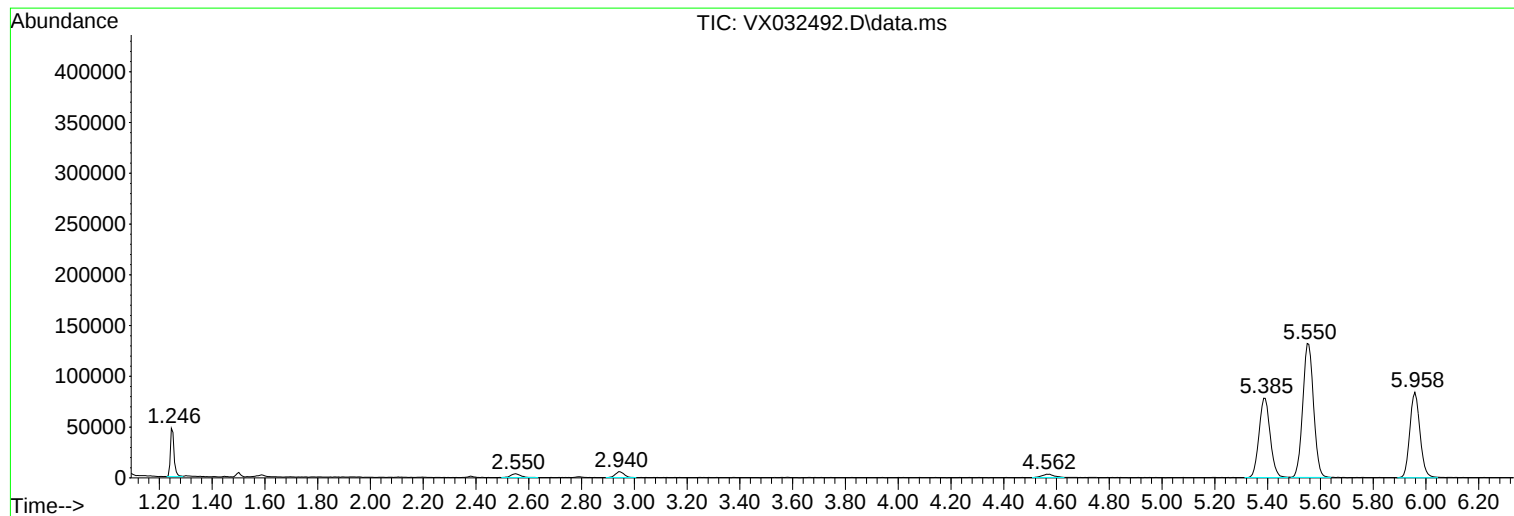

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103122\
Data File : VX032492.D
Acq On : 31 Oct 2022 16:53
Operator : JC/MD
Sample : N5340-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6-102722

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103122\
Data File : VX032492.D
Acq On : 31 Oct 2022 16:53
Operator : JC/MD
Sample : N5340-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6-102722

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------