

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103125\
 Data File : VX048434.D
 Acq On : 31 Oct 2025 15:50
 Operator : JC/MD
 Sample : Q3506-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Quant Time: Oct 31 23:07:22 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102925W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 30 02:37:17 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	102796	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	201134	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	248761	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	129205	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	79283	53.629	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 107.260%	
35) Dibromofluoromethane	5.379	113	58250	50.796	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 101.600%	
50) Toluene-d8	8.635	98	290942	57.476	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 114.960%#	
62) 4-Bromofluorobenzene	11.061	95	128044	67.620	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 135.240%#	
Target Compounds						Qvalue
10) Methyl Iodide	2.459	142	1075	0.227	ug/l #	87
16) Acetone	2.392	43	1457	4.348	ug/l #	77
18) Methyl Acetate	2.703	43	480	0.428	ug/l #	66
31) Cyclohexane	5.538	56	1849	0.905	ug/l #	1
36) 1,1-Dichloropropene	5.538	75	7346	3.815	ug/l #	49
38) Carbon Tetrachloride	5.544	117	9991	4.493	ug/l #	15
76) 1,2,3-Trichloropropane	11.061	75	67286	36.212	ug/l #	33
81) trans-1,4-Dichloro-2-b...	11.061	75	67286	125.314	ug/l #	10


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX103125\
Data File : VX048434.D
Acq On : 31 Oct 2025 15:50
Operator : JC/MD
Sample : Q3506-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Time: Oct 31 23:07:22 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102925W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 30 02:37:17 2025
Response via : Initial Calibration




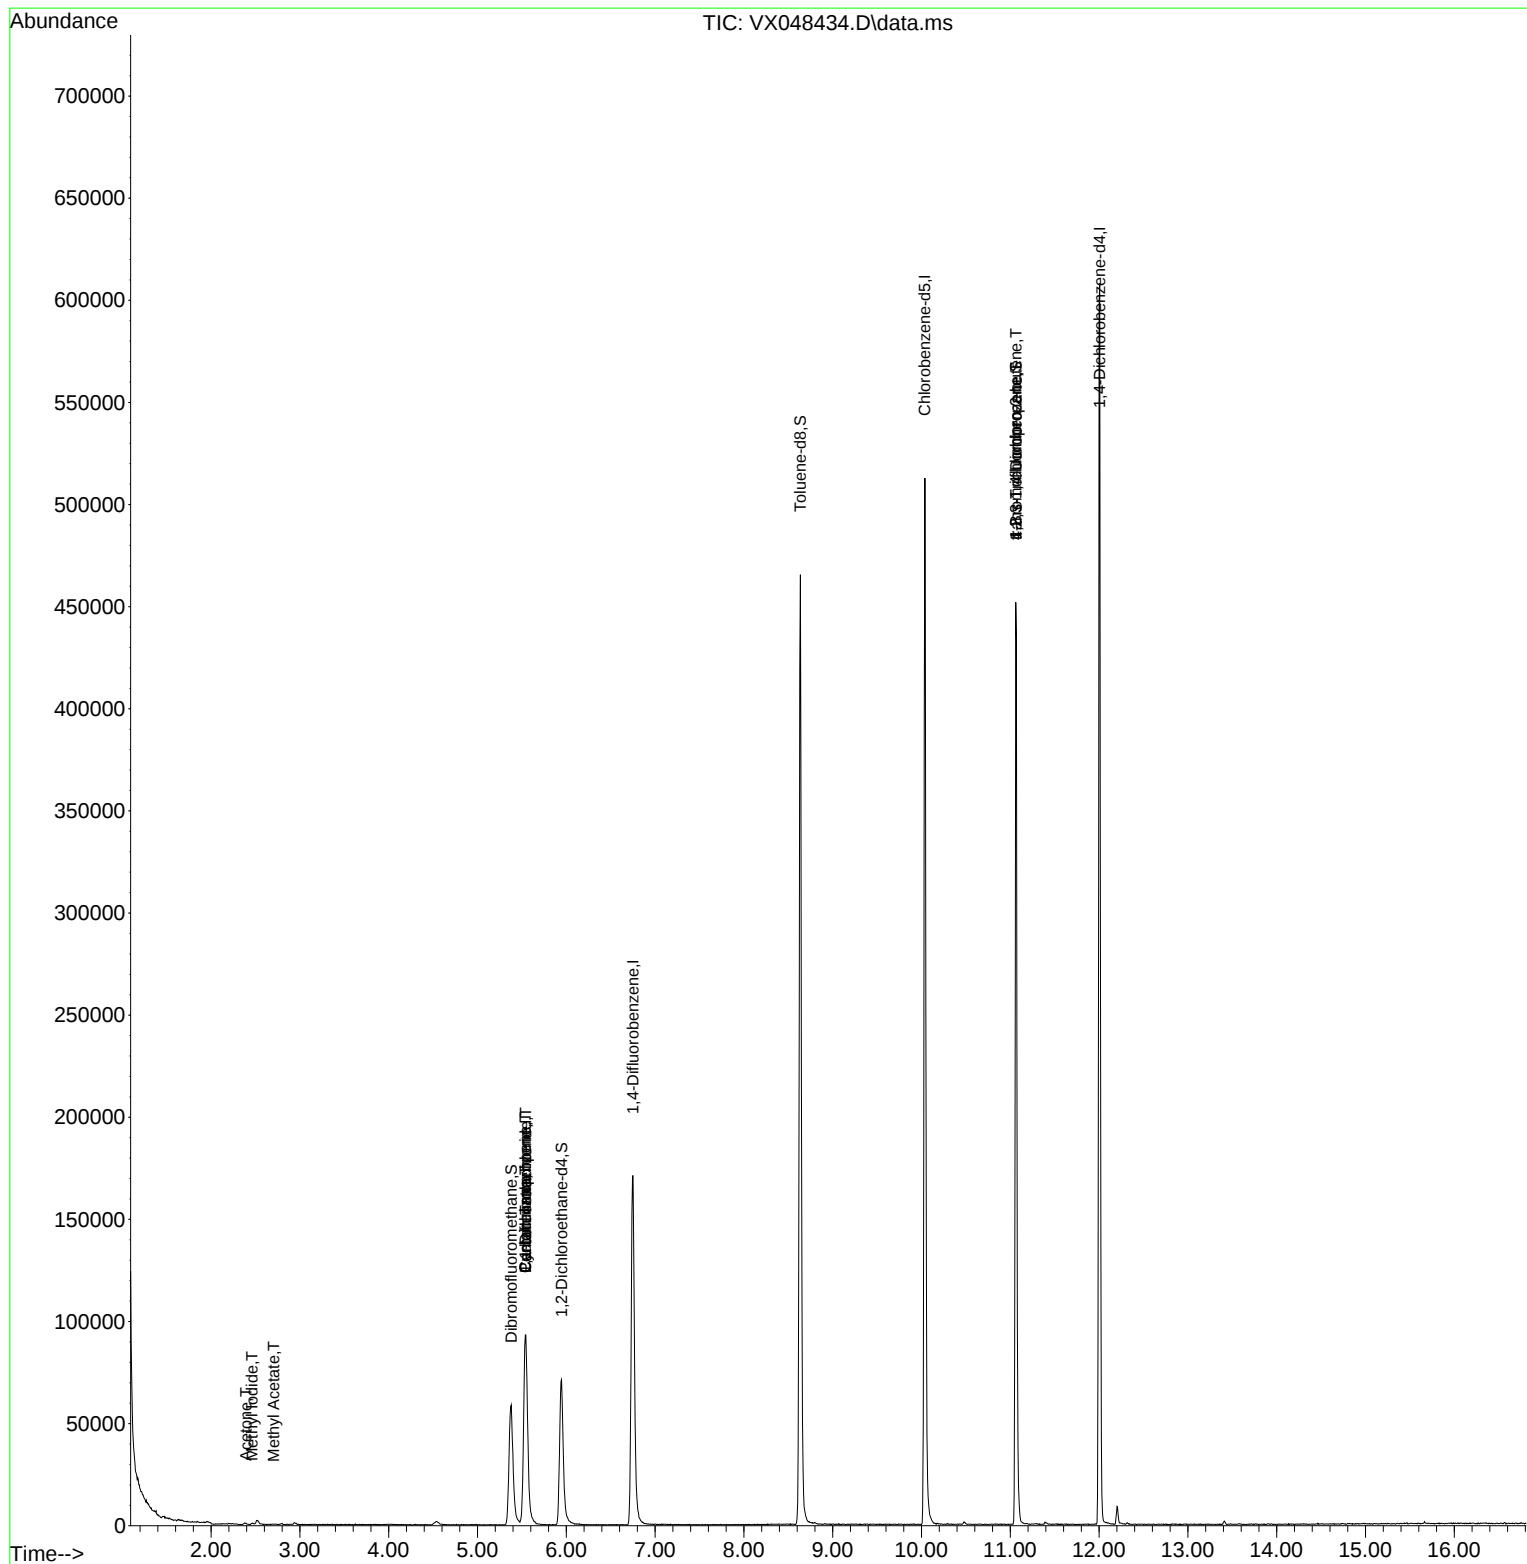




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. 0.007 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:168 Resp: 102796
Ion Ratio Lower Upper
168 100
99 56.6 46.4 69.6

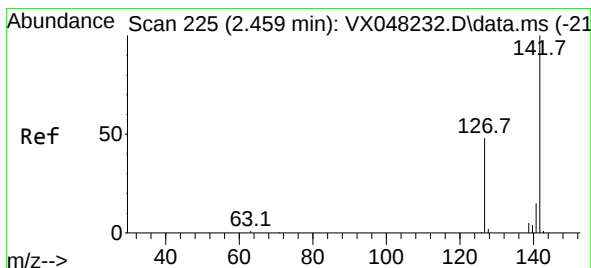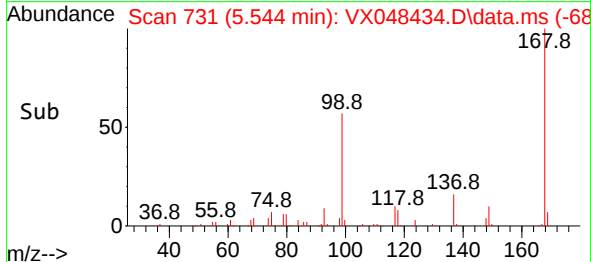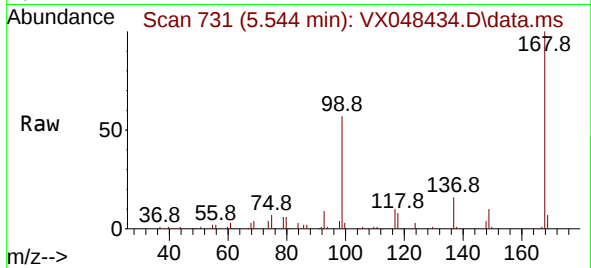

#10
Methyl Iodide
Concen: 0.227 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.000 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50

Tgt Ion:142 Resp: 1075
Ion Ratio Lower Upper
142 100
127 52.0 38.5 57.7
141 0.0 11.6 17.4#


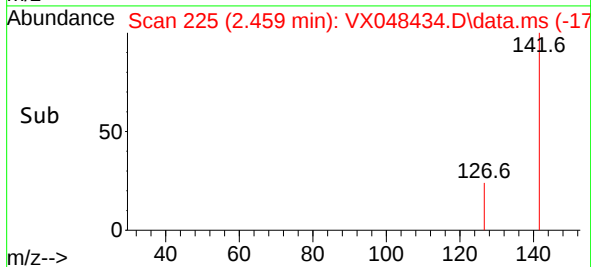

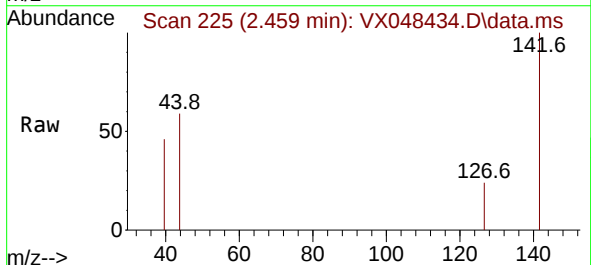




#16
Acetone
Concen: 4.348 ug/l
RT: 2.392 min Scan# 211
Delta R.T. 0.018 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion: 43 Resp: 1457
Ion Ratio Lower Upper
43 100
58 16.8 23.4 35.2#

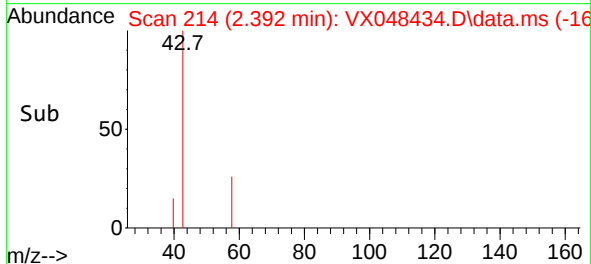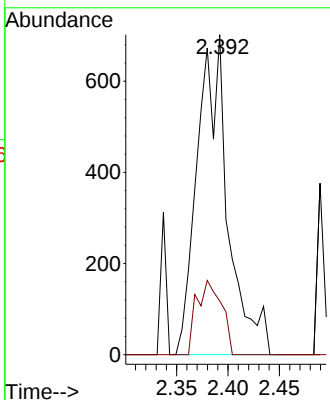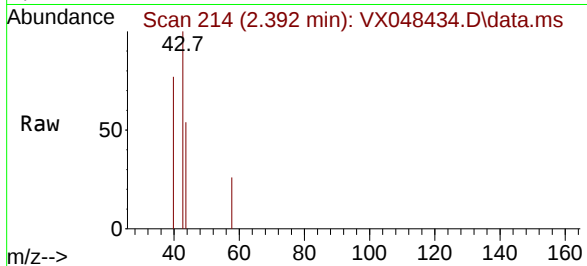

#18
Methyl Acetate
Concen: 0.428 ug/l
RT: 2.703 min Scan# 265
Delta R.T. 0.006 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50

Tgt Ion: 43 Resp: 480
Ion Ratio Lower Upper
43 100
74 5.6 17.5 26.3#


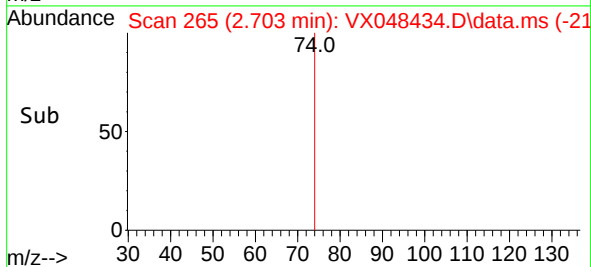
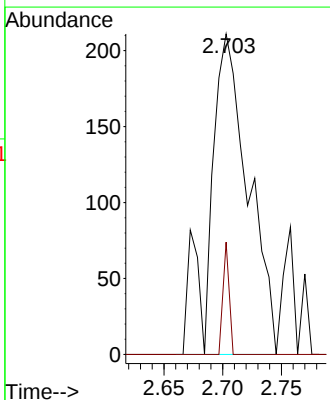
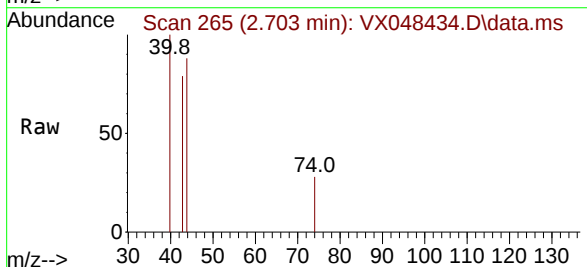


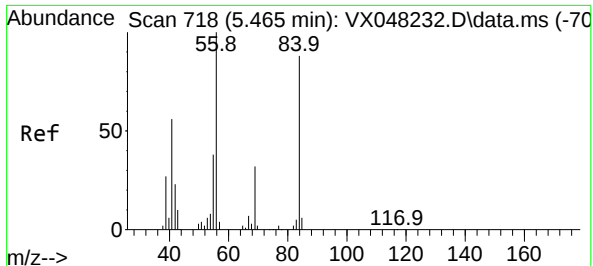

#31
Cyclohexane
Concen: 0.905 ug/l
RT: 5.538 min Scan# 718
Delta R.T. 0.073 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion: 56 Resp: 1849
Ion Ratio Lower Upper
56 100
69 166.0 23.0 34.6#
84 173.0 64.6 97.0#

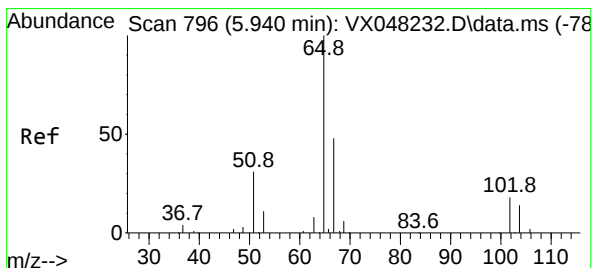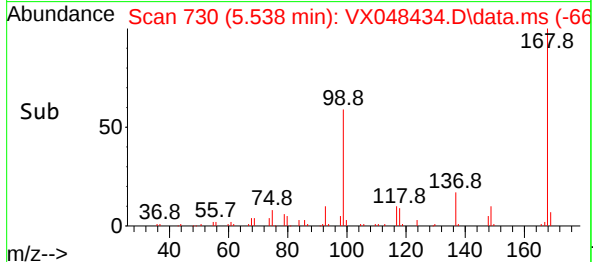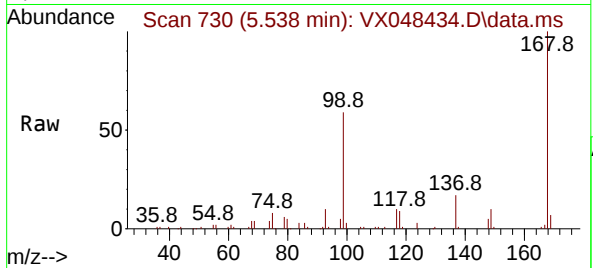

#33
1,2-Dichloroethane-d4
Concen: 53.629 ug/l
RT: 5.946 min Scan# 797
Delta R.T. 0.006 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50

Tgt Ion: 65 Resp: 79283
Ion Ratio Lower Upper
65 100
67 52.4 0.0 105.0


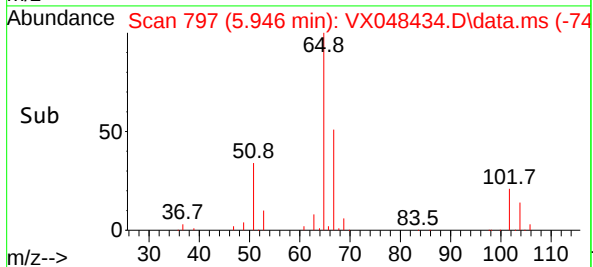

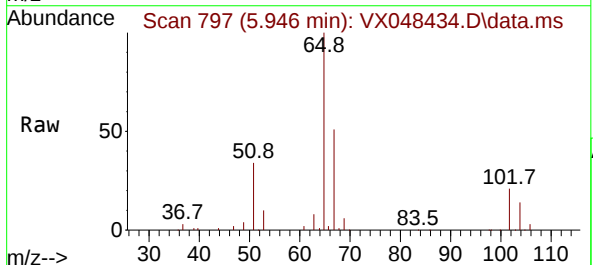




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.751 min Scan# 911
Delta R.T. 0.006 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:114 Resp: 201134
Ion Ratio Lower Upper
114 100
63 19.2 0.0 43.2
88 16.0 0.0 33.6

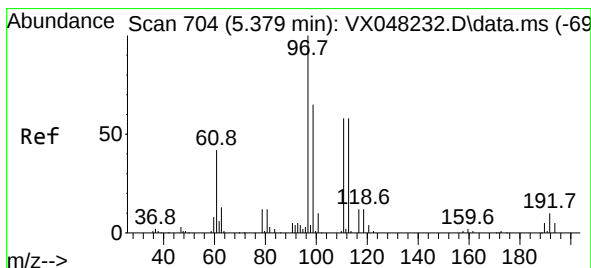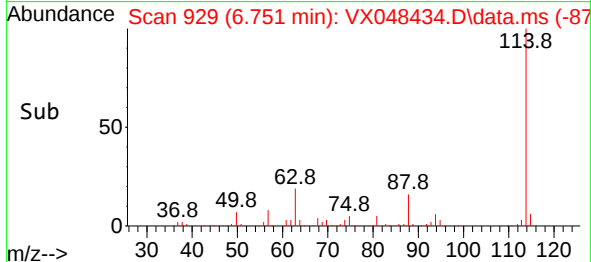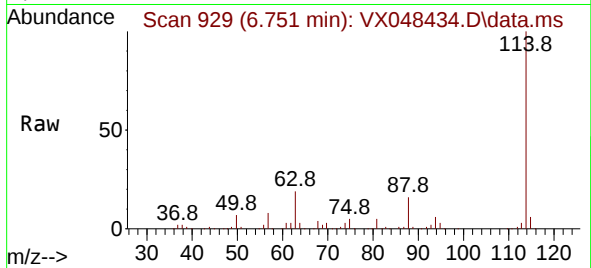

#35
Dibromofluoromethane
Concen: 50.796 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50

Tgt Ion:113 Resp: 58250
Ion Ratio Lower Upper
113 100
111 104.5 82.2 123.4
192 19.6 15.1 22.7

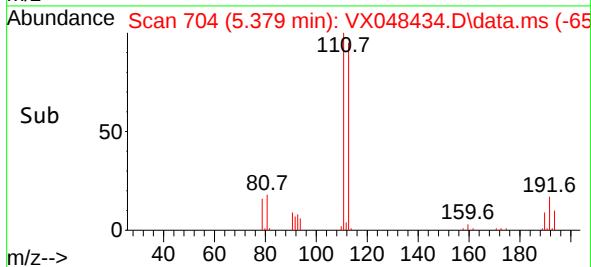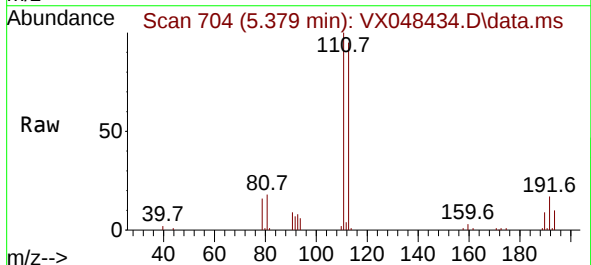



#36

1,1-Dichloropropene

Concen: 3.815 ug/l

RT: 5.538 min Scan# 71

Delta R.T. -0.146 min

Lab File: VX048434.D

Acq: 31 Oct 2025 15:50

Instrument :

MSVOA_X

ClientSampleId :

STORAGE-BLANK-WATER-REF-5





Tgt Ion: 75 Resp: 7346

Ion Ratio Lower Upper

75 100

110 8.4 17.7 53.1#

77 0.0 24.3 36.5#

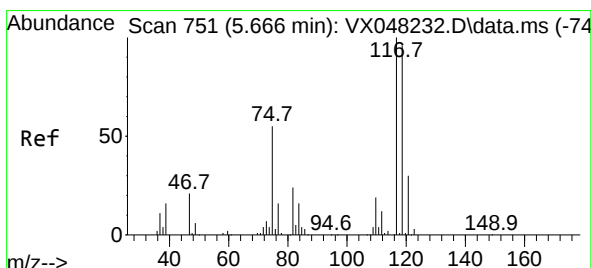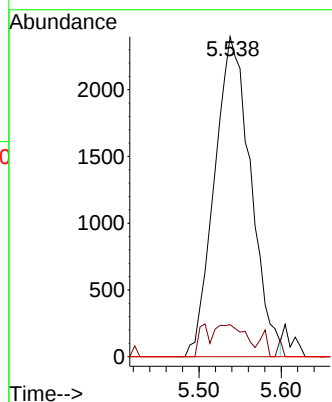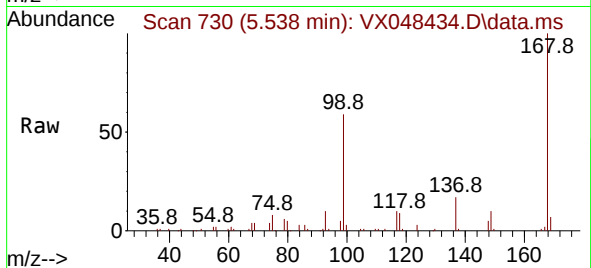

#38

Carbon Tetrachloride

Concen: 4.493 ug/l

RT: 5.544 min Scan# 731

Delta R.T. -0.122 min

Lab File: VX048434.D

Acq: 31 Oct 2025 15:50




Tgt Ion: 117 Resp: 9991


Ion Ratio Lower Upper

117 100

119 4.6 77.2 115.8#

121 0.0 24.8 37.2#


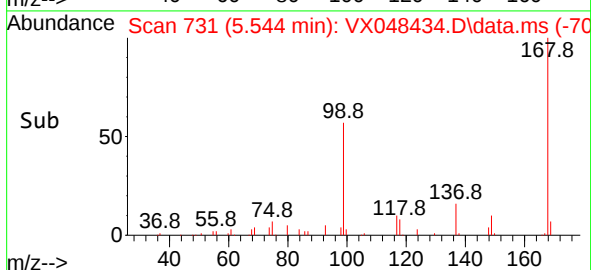






#50
Toluene-d8
Concen: 57.476 ug/l
RT: 8.635 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion: 98 Resp: 290942
Ion Ratio Lower Upper
98 100
100 66.5 53.0 79.4

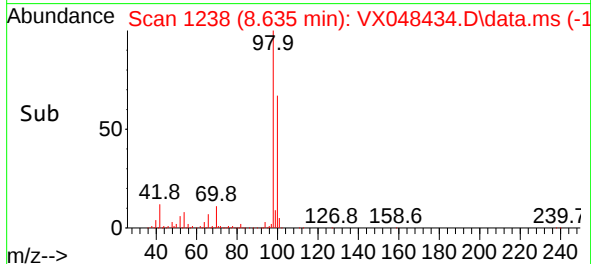

#62
4-Bromofluorobenzene
Concen: 67.620 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. 0.000 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50

Tgt Ion: 95 Resp: 128044
Ion Ratio Lower Upper
95 100
174 76.0 0.0 147.8
176 72.6 0.0 142.8


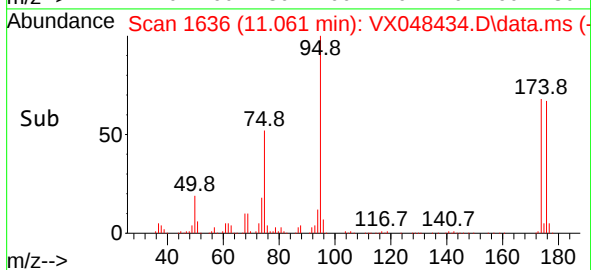

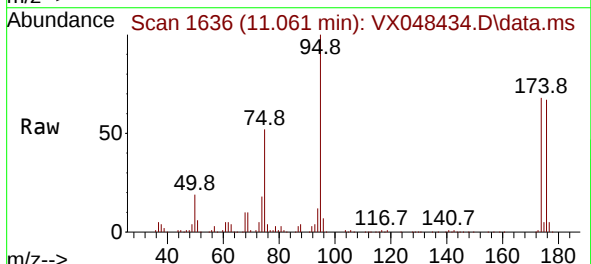


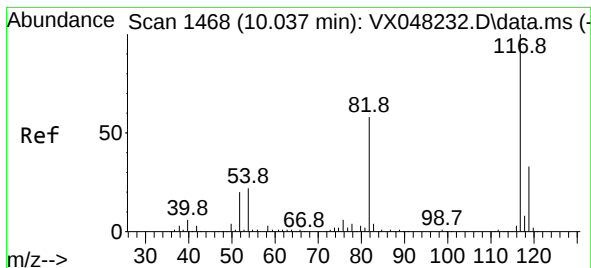

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. 0.000 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:117 Resp: 248761
Ion Ratio Lower Upper
117 100
82 55.4 46.5 69.7
119 31.2 25.9 38.9

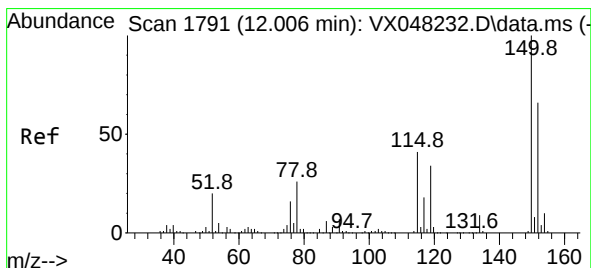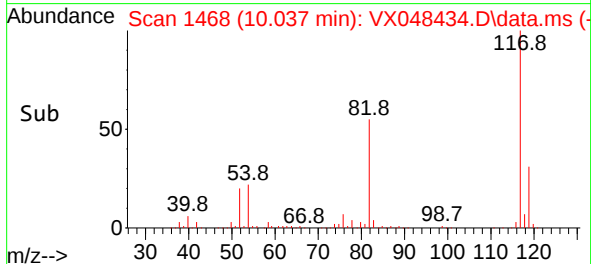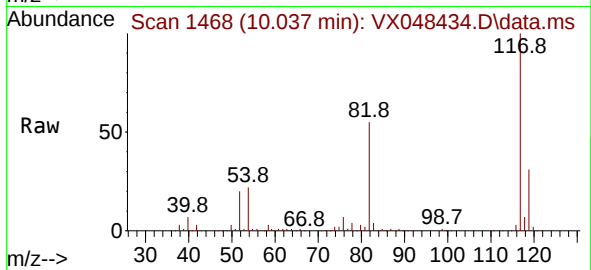

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. 0.000 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50

Tgt Ion:152 Resp: 129205
Ion Ratio Lower Upper
152 100
115 61.7 43.1 129.4
150 157.6 0.0 353.0


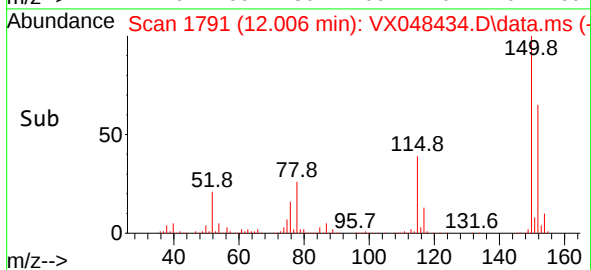

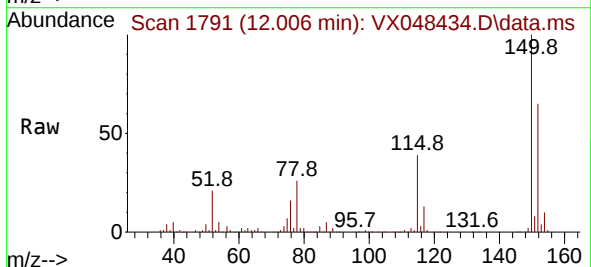




#76
1,2,3-Trichloropropane
Concen: 36.212 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.158 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion: 75 Resp: 67286
Ion Ratio Lower Upper
75 100
77 1.2 22.4 67.2#

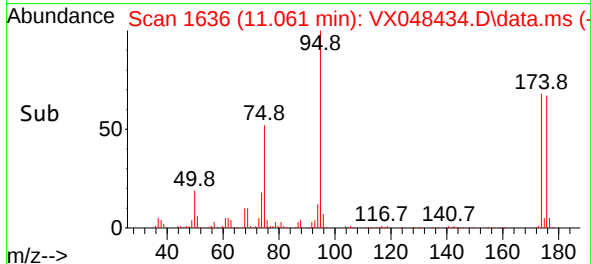

#81
trans-1,4-Dichloro-2-butene
Concen: 125.314 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. 0.061 min
Lab File: VX048434.D
Acq: 31 Oct 2025 15:50

Tgt Ion: 75 Resp: 67286
Ion Ratio Lower Upper
75 100
53 0.0 79.5 119.3#
89 0.0 36.8 55.2#

