


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX110118\
Data File : VX005719.D
Acq On : 01 Nov 2018 09:29
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103118W.M
Title : SW846 8260
Last Update : Wed Oct 31 18:23:06 2018

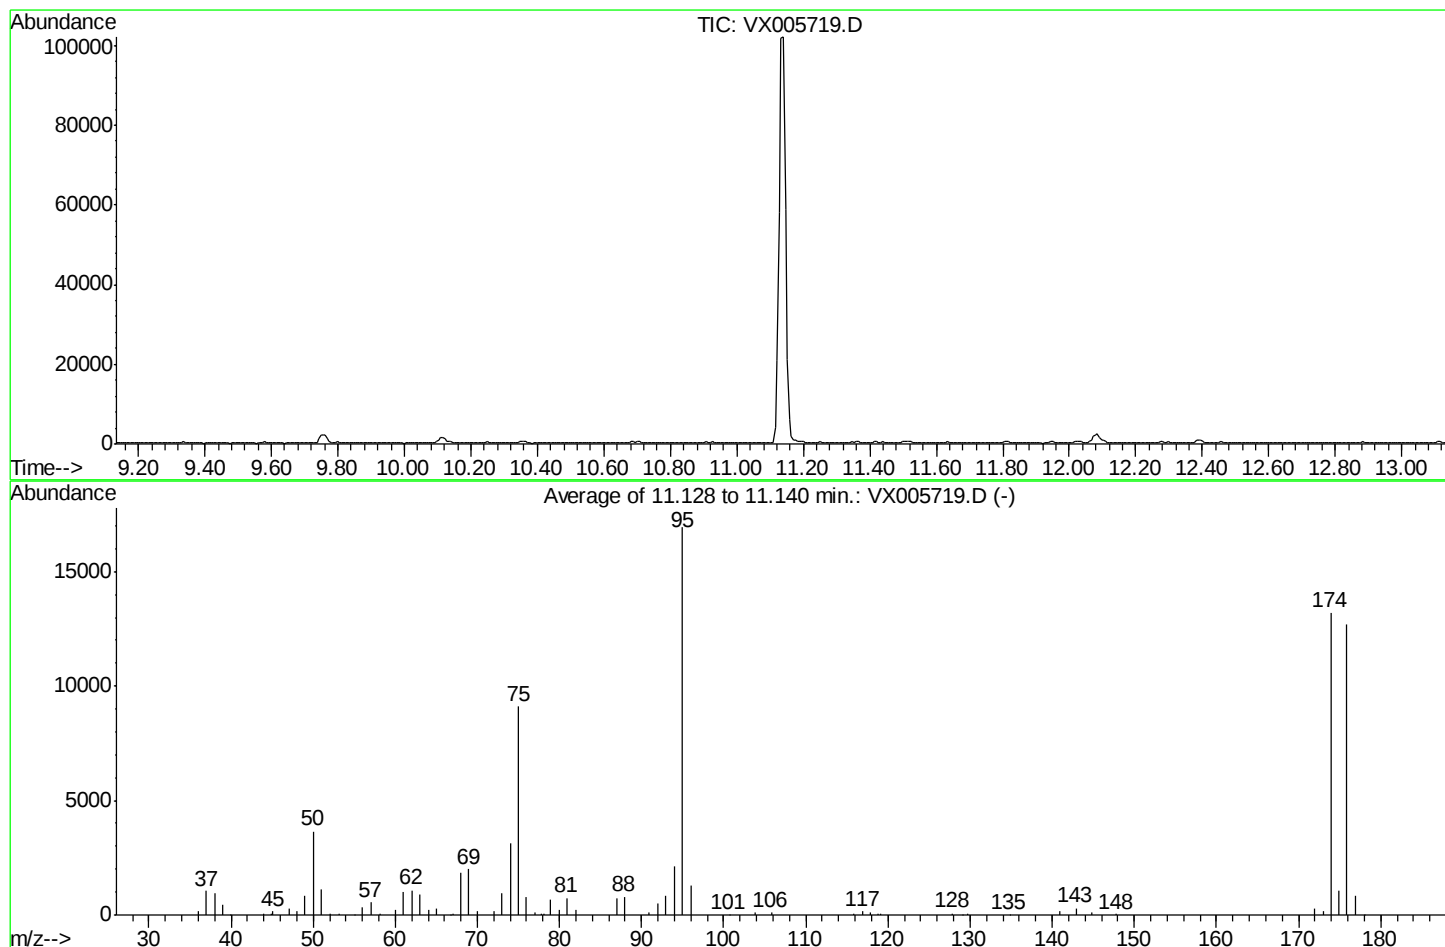

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	3656	PASS
75	95	30	60	53.8	9108	PASS
95	95	100	100	100.0	16932	PASS
96	95	5	9	7.6	1293	PASS
173	174	0.00	2	1.3	177	PASS
174	95	50	100	78.1	13216	PASS
175	174	5	9	8.0	1062	PASS
176	174	95	101	96.1	12694	PASS
177	176	5	9	6.5	823	PASS