

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX110119\
 Data File : VX013303.D
 Acq On : 01 Nov 2019 12:00
 Operator : JC/SP
 Sample : K5626-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S1TB2-191030

Quant Time: Nov 04 00:51:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 02 07:06:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	741626	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	1118941	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	982479	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	450661	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	425064	48.38	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.76%	
35) Dibromofluoromethane	5.49	113	331339	47.21	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.42%	
50) Toluene-d8	8.71	98	1311804	49.58	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.16%	
62) 4-Bromofluorobenzene	11.13	95	429343	44.96	ug/l	0.00
Spiked Amount	50.000		Recovery	=	89.92%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX110119\
Data File : VX013303.D
Acq On : 01 Nov 2019 12:00
Operator : JC/SP
Sample : K5626-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S1TB2-191030

Quant Time: Nov 04 00:51:08 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 02 07:06:38 2019
Response via : Initial Calibration

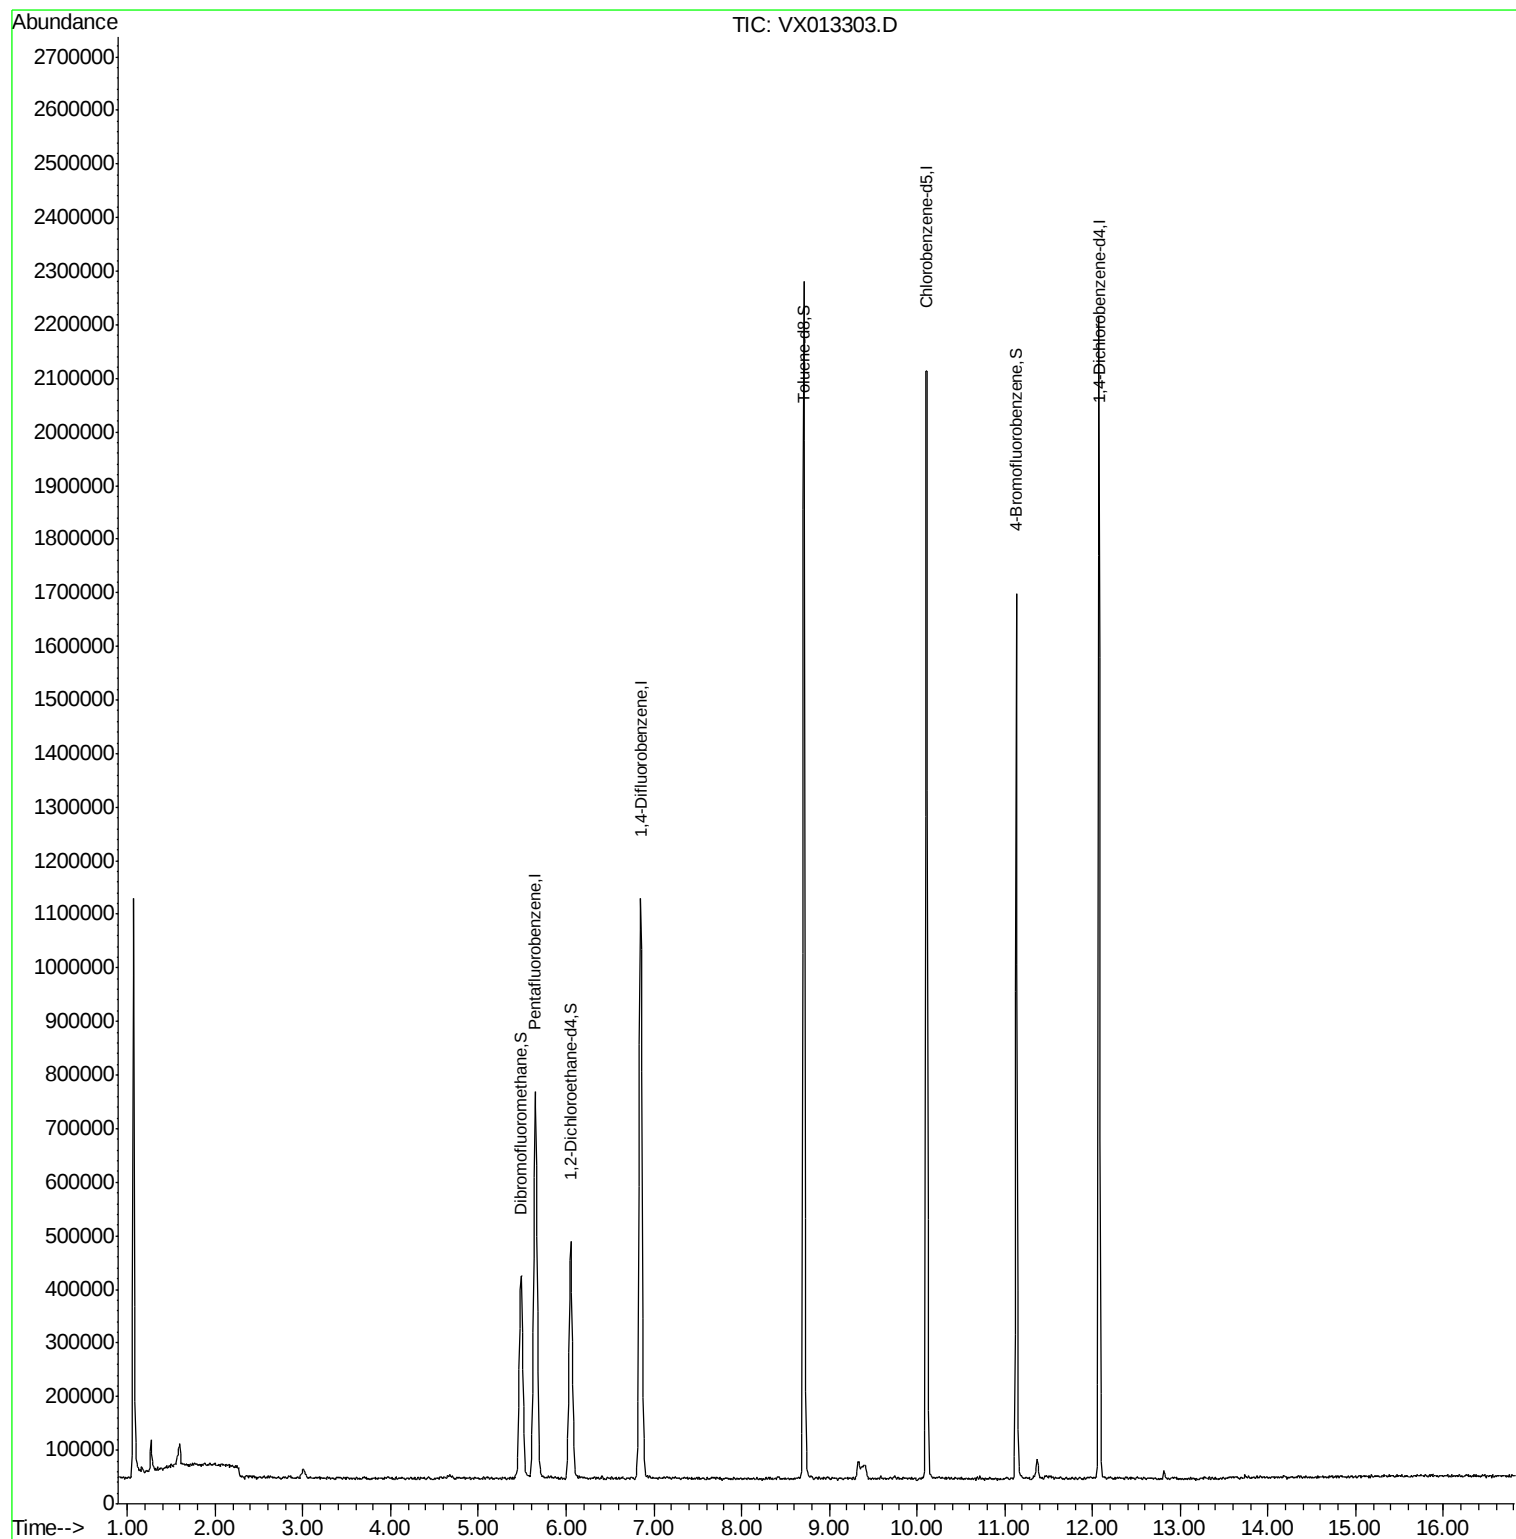

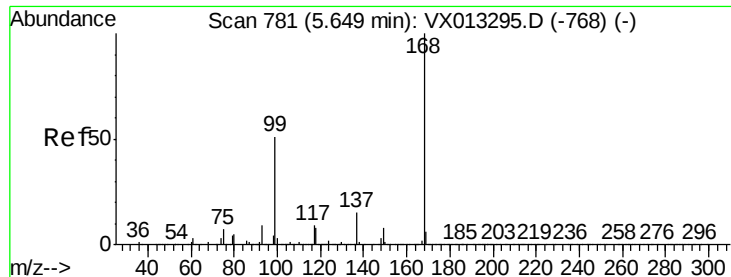

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 781

Delta R.T. -0.00 min

Lab File: VX013303.D

Acq: 01 Nov 2019 12:00

Instrument :

MSVOA_X

ClientSampleId :


S1TB2-191030

Tgt Ion:168 Resp: 741626

Ion Ratio Lower Upper

168 100

99 49.5 40.8 61.2

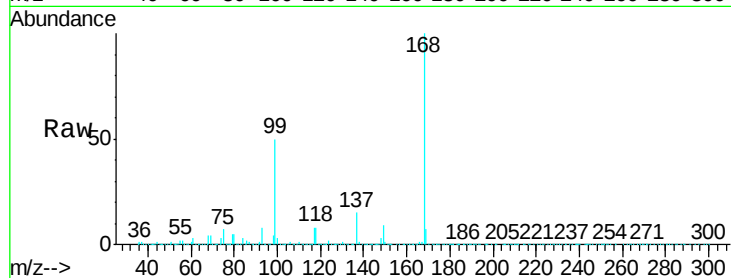

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

250000

200000



150000

100000

50000

0

Time-->

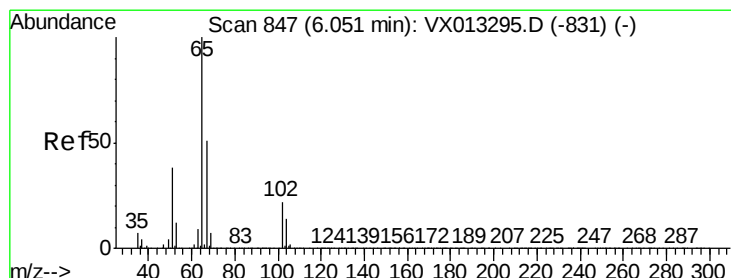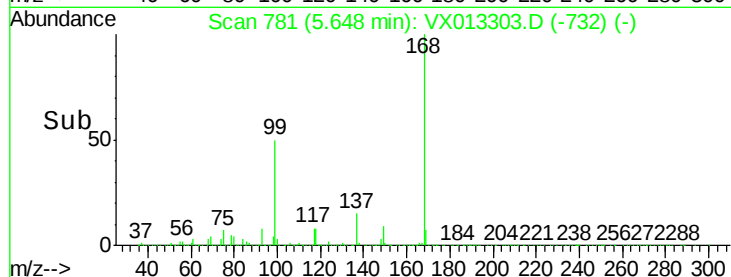

#33

1,2-Dichloroethane-d4

Concen: 48.379 ug/l

RT: 6.05 min Scan# 847

Delta R.T. -0.00 min

Lab File: VX013303.D


Acq: 01 Nov 2019 12:00

Tgt Ion: 65 Resp: 425064

Ion Ratio Lower Upper

65 100

67 51.1 0.0 104.2

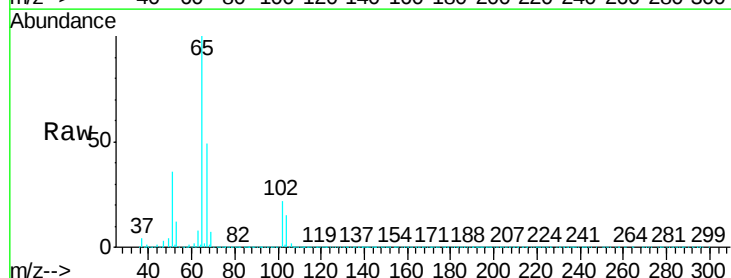

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.05


150000


100000

50000

0

Time-->

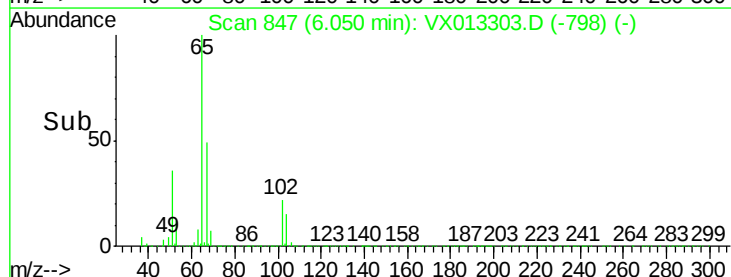

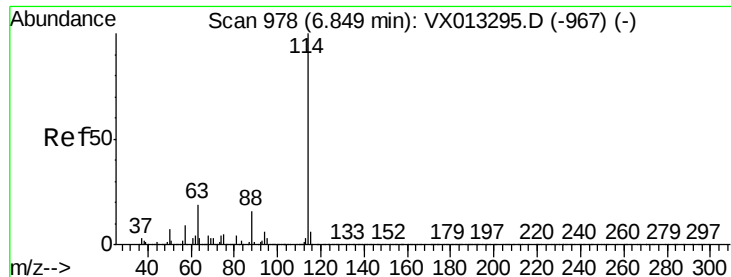

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. -0.00 min

Lab File: VX013303.D

Acq: 01 Nov 2019 12:00

Instrument :

MSVOA_X

ClientSampleId :

S1TB2-191030


Tgt Ion:114 Resp: 1118941

Ion Ratio Lower Upper

114 100

63 19.8 0.0 38.4

88 15.4 0.0 32.2

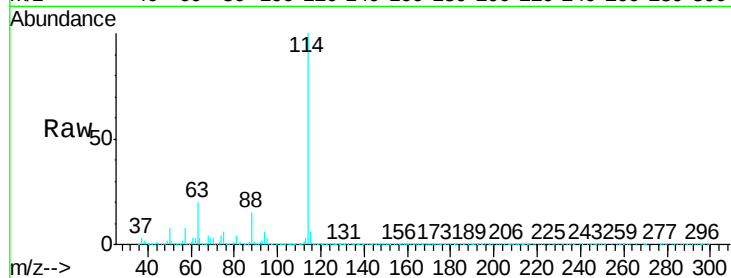

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

6.85

600000

500000

400000



300000

200000

100000

0

Time-->

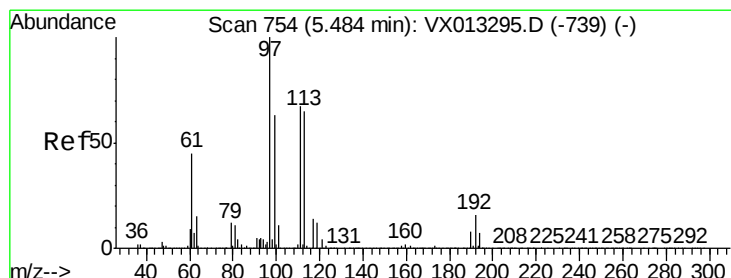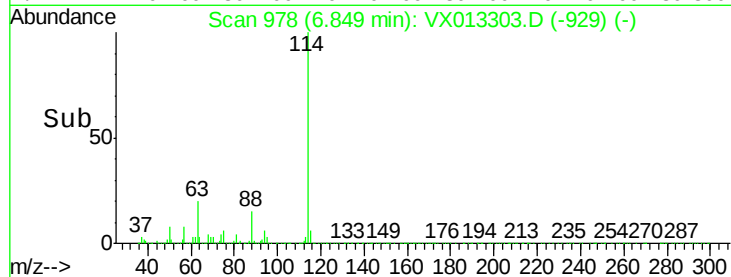

#35

Dibromofluoromethane

Concen: 47.212 ug/l

RT: 5.49 min Scan# 755

Delta R.T. 0.01 min

Lab File: VX013303.D

Acq: 01 Nov 2019 12:00


Tgt Ion:113 Resp: 331339

Ion Ratio Lower Upper

113 100

111 103.1 81.9 122.9

192 23.2 19.1 28.7

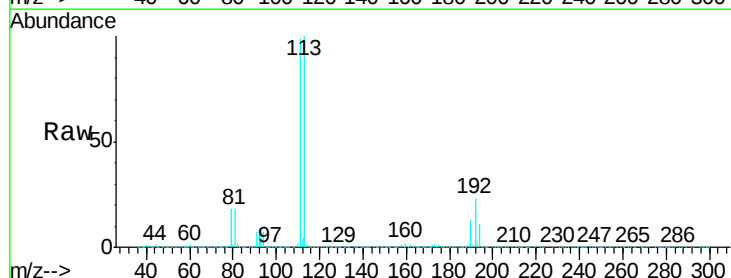

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

5.49


150000


100000

50000

0

Time-->

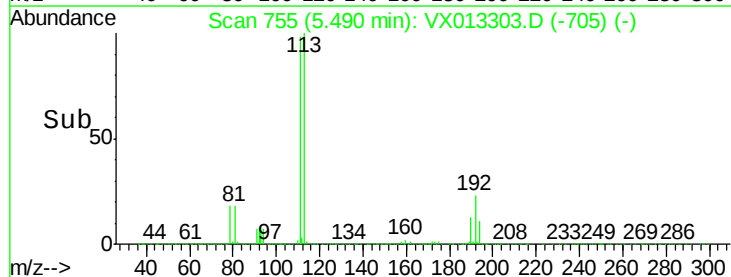

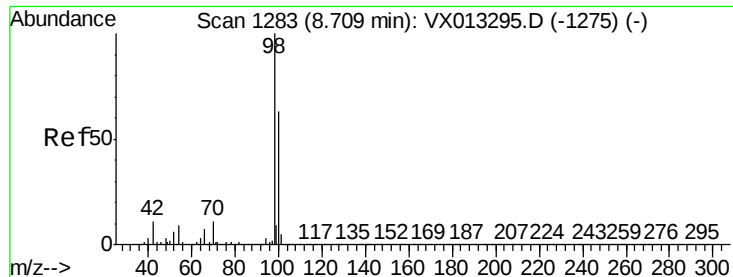

#50

Toluene-d8

Concen: 49.581 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. -0.00 min

Lab File: VX013303.D

Acq: 01 Nov 2019 12:00

Instrument :

MSVOA_X

ClientSampleId :





S1TB2-191030

Tgt Ion: 98 Resp: 1311804

Ion Ratio Lower Upper

98 100

100 65.1 52.2 78.2

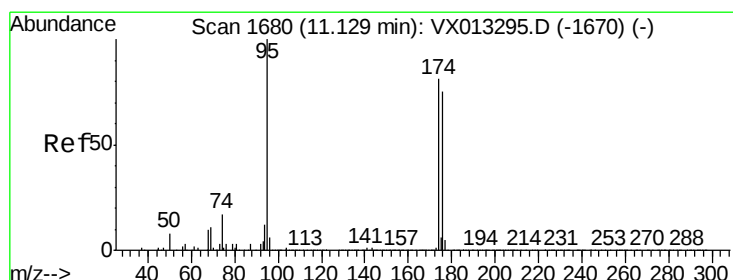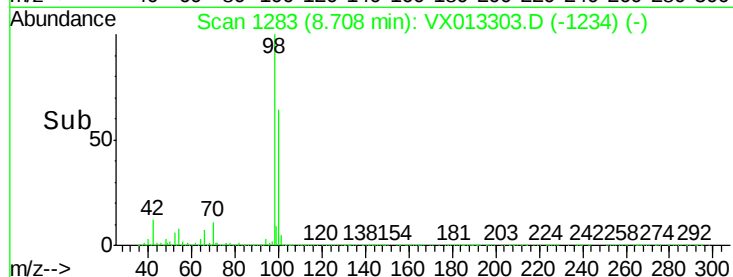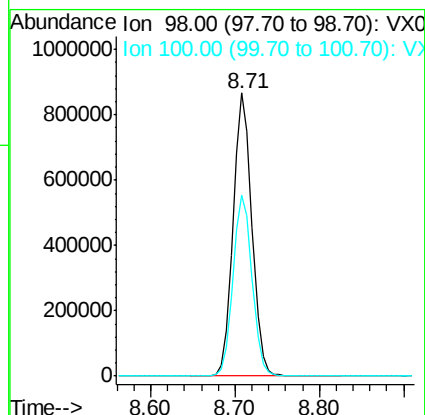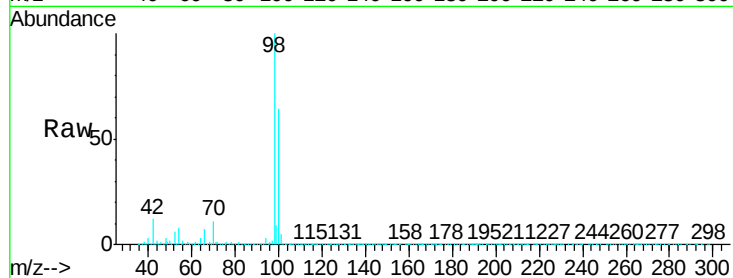

#62

4-Bromofluorobenzene

Concen: 44.963 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.00 min

Lab File: VX013303.D

Acq: 01 Nov 2019 12:00




Tgt Ion: 95 Resp: 429343


Ion Ratio Lower Upper

95 100

174 91.9 0.0 179.8

176 88.0 0.0 173.0


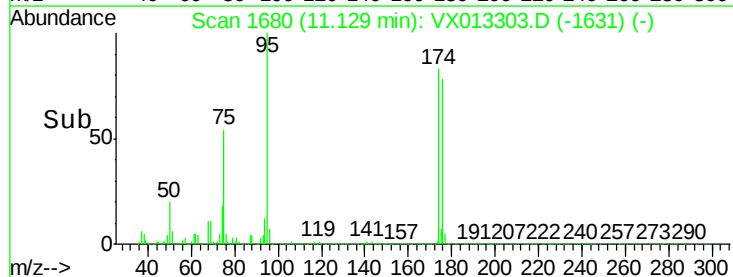
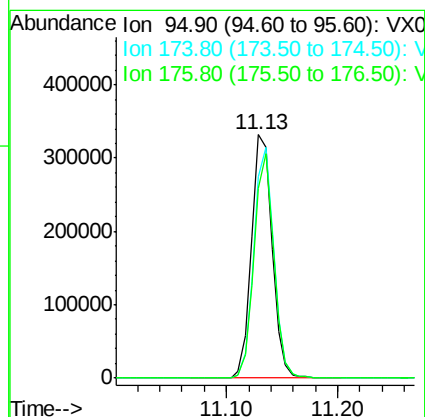
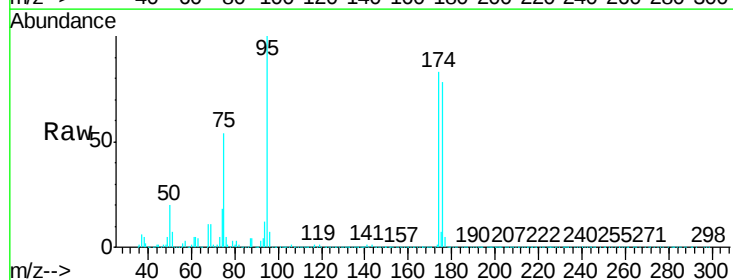


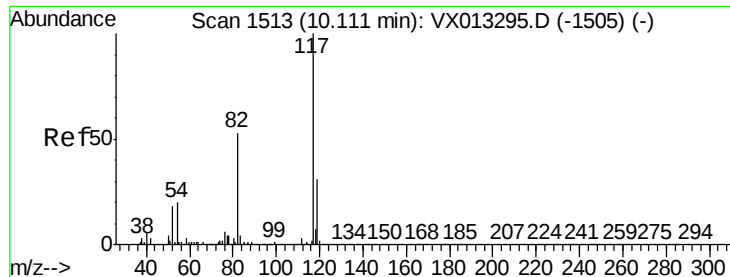

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1513
Delta R.T. -0.00 min
Lab File: VX013303.D
Acq: 01 Nov 2019 12:00

Instrument :
MSVOA_X
ClientSampleId :
S1TB2-191030

Tgt Ion	Ratio	Lower	Upper
117	100		
82	52.3	42.6	64.0
119	32.0	24.8	37.2

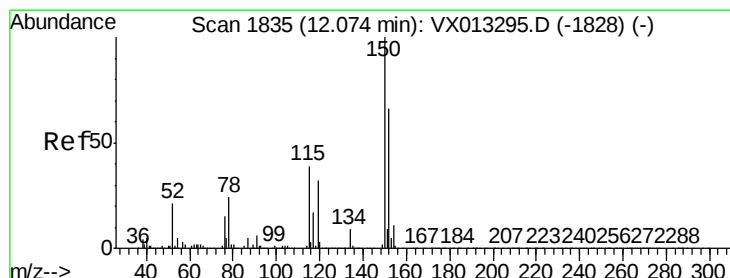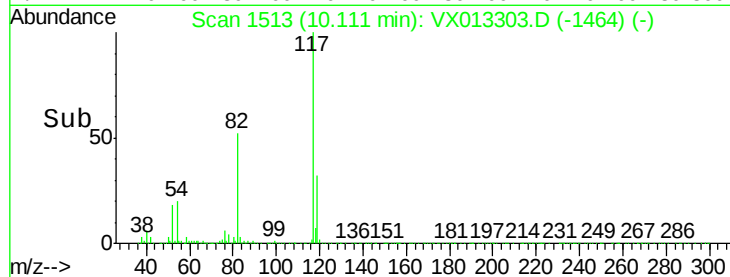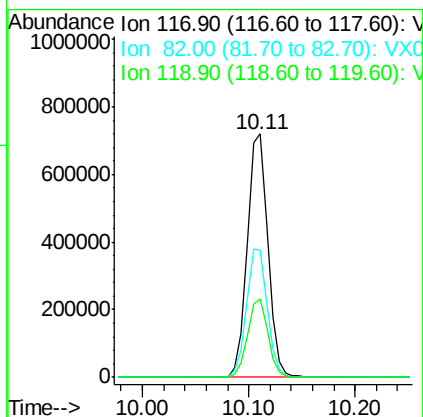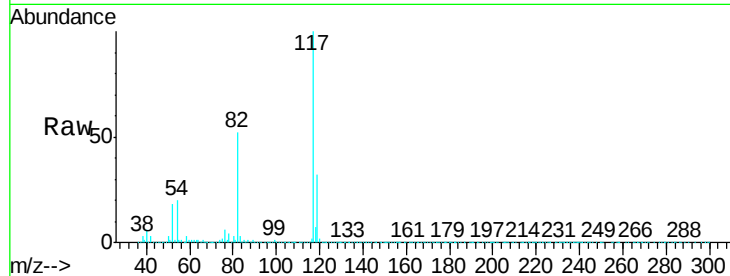

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. -0.00 min
Lab File: VX013303.D
Acq: 01 Nov 2019 12:00

Tgt Ion	Ratio	Lower	Upper
152	100		
115	54.8	39.5	118.3
150	155.9	0.0	344.4

