


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110119\
 Data File : VX013299.D
 Acq On : 01 Nov 2019 09:17
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
 Title : SW846 8260
 Last Update : Sat Nov 02 07:06:38 2019

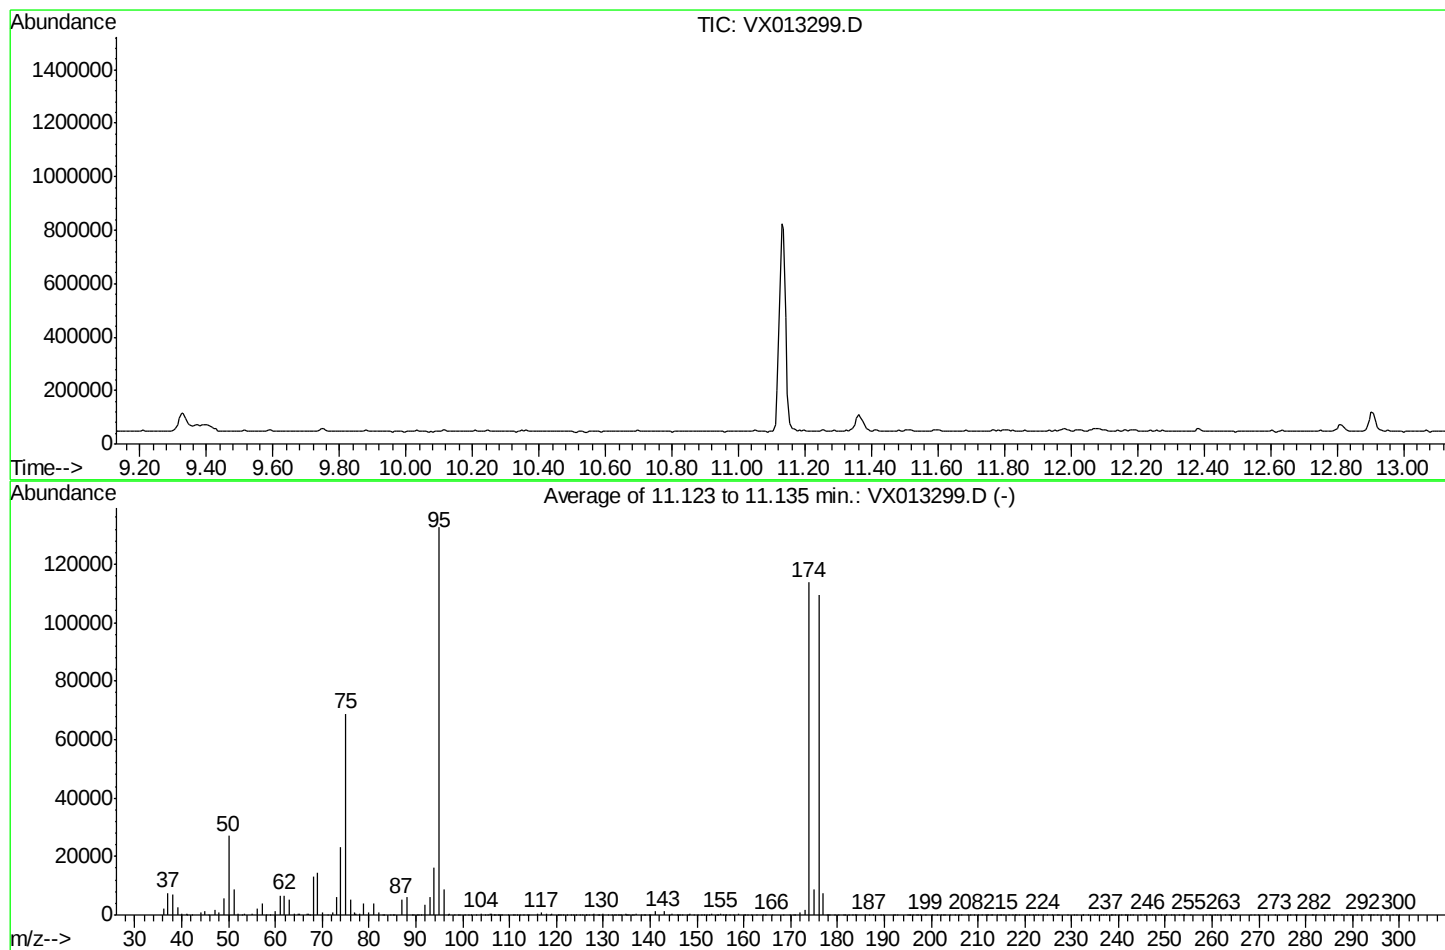

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	26982	PASS
75	95	30	60	51.9	68829	PASS
95	95	100	100	100.0	132609	PASS
96	95	5	9	6.7	8899	PASS
173	174	0.00	2	1.5	1697	PASS
174	95	50	100	85.8	113728	PASS
175	174	5	9	7.9	8931	PASS
176	174	95	101	96.1	109302	PASS
177	176	5	9	6.8	7463	PASS