

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX110120\
 Data File : VX019198.D
 Acq On : 30 Oct 2020 10:33
 Operator : JC/MD
 Sample : VX1101WBL06
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK307

Quant Time: Oct 30 14:10:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 30 08:55:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.82	114	207473	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.09	117	186243	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.06	152	86823	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	62668	4.67	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.40%
7) Chloroethane-d5	1.70	69	54022	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.60%
11) 1,1-Dichloroethene-d2	2.34	63	94690	3.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.20%
20) 2-Butanone-d5	4.56	46	155517	53.02	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.04%
24) Chloroform-d	5.14	84	119844	4.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.80%
26) 1,2-Dichloroethane-d4	6.03	65	67344	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
32) Benzene-d6	6.04	84	248205	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
36) 1,2-Dichloropropane-d6	7.37	67	72134	5.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.40%
41) Toluene-d8	8.70	98	229949	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.00%
43) trans-1,3-Dichloropropene-	8.99	79	29436	4.75	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.00%
46) 2-Hexanone-d5	9.43	63	143099	52.79	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.58%
56) 1,1,2,2-Tetrachloroethane-	11.23	84	55028	4.99	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.80%
66) 1,2-Dichlorobenzene-d4	12.36	152	79156	4.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.20%


Target Compounds					Ovalue
16) Methylene chloride	2.83	84	4632	0.292 ug/L	94




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX110120\
Data File : VX019198.D
Acq On : 30 Oct 2020 10:33
Operator : JC/MD
Sample : VX1101WBL06
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK307

Quant Time: Oct 30 14:10:51 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 30 08:55:33 2020
Response via : Initial Calibration

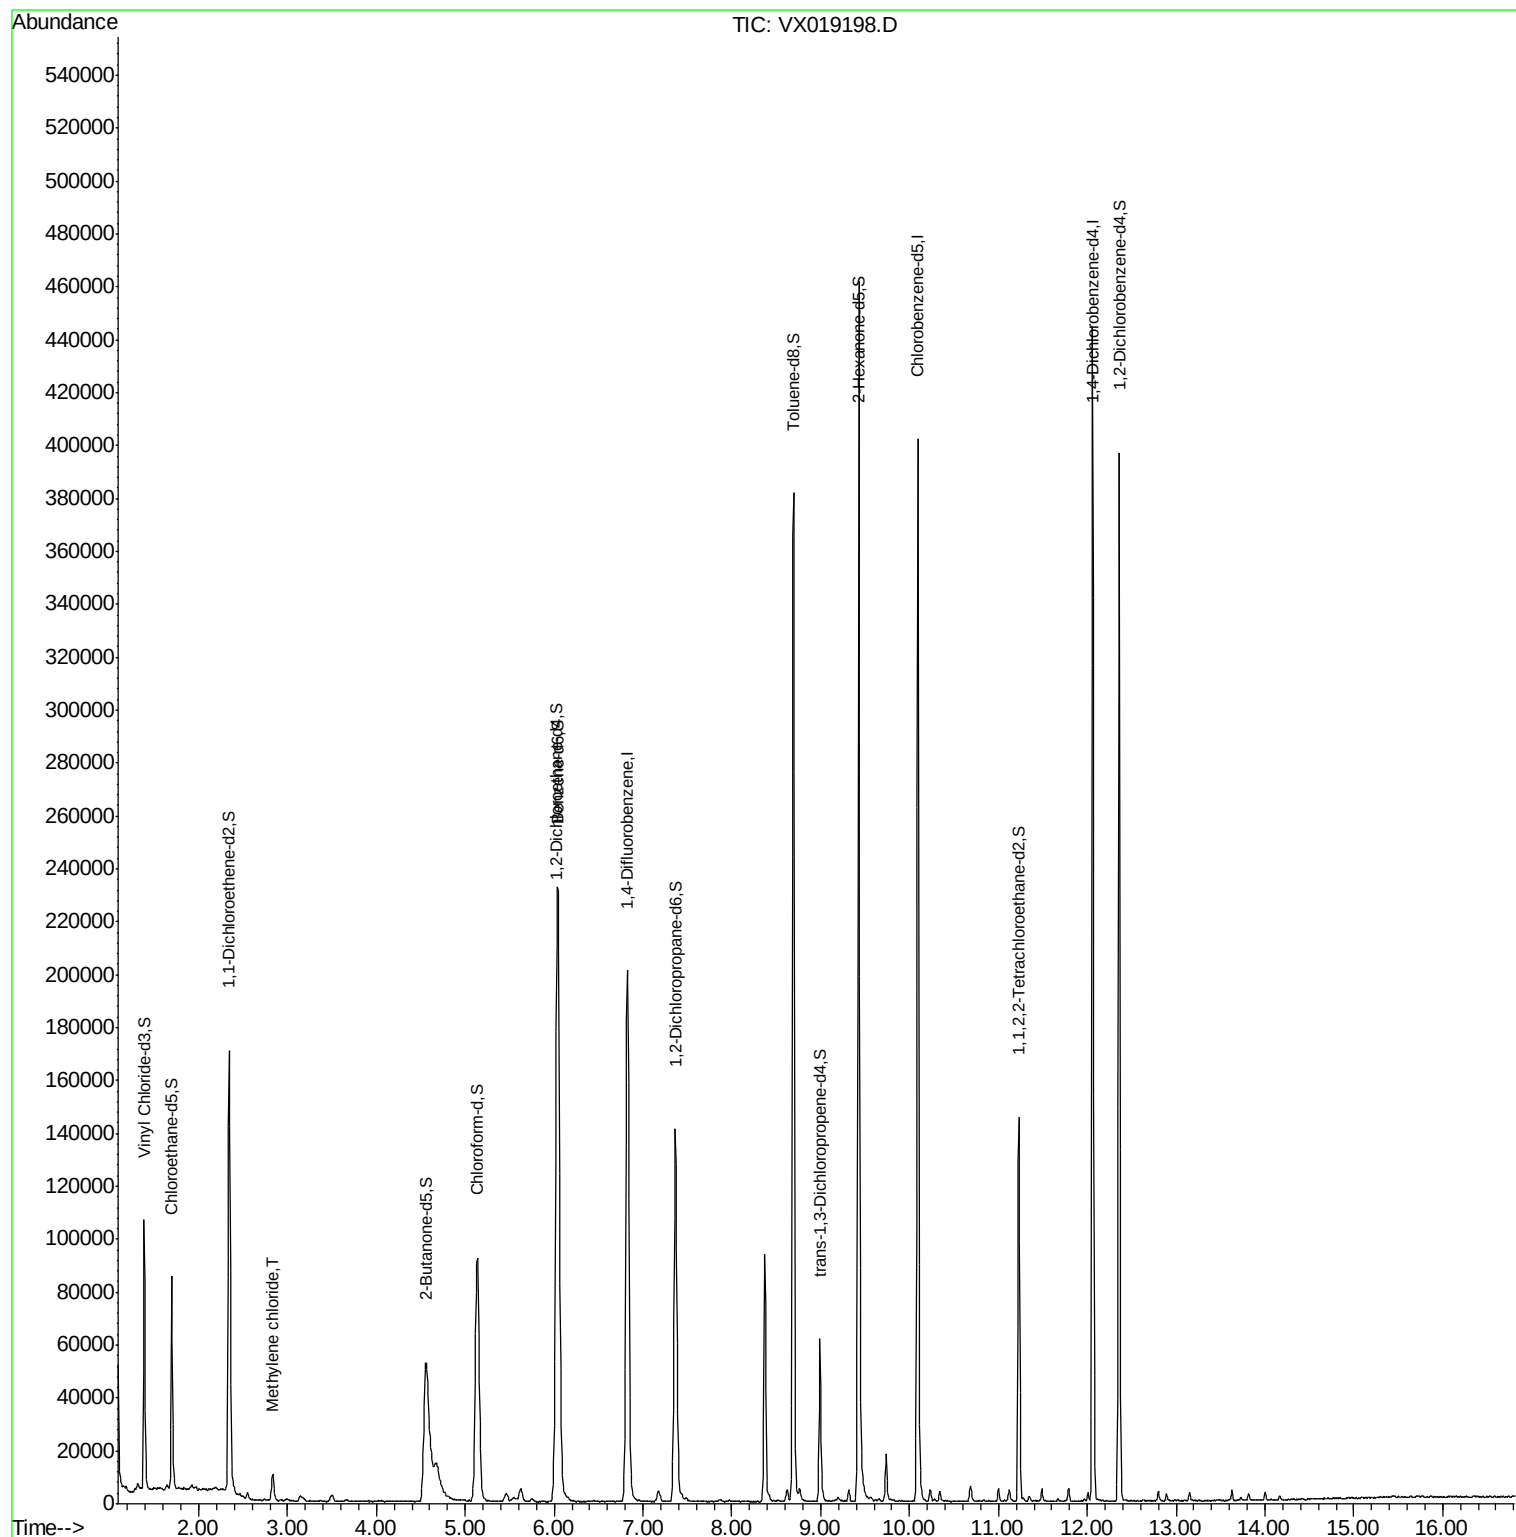

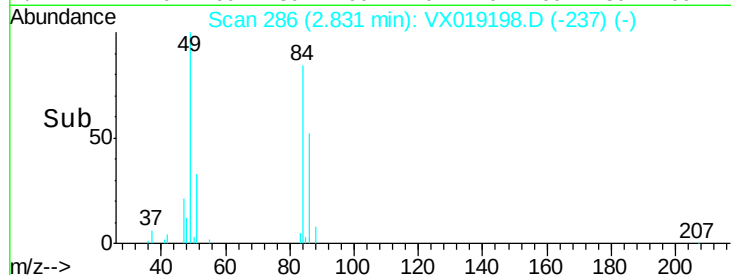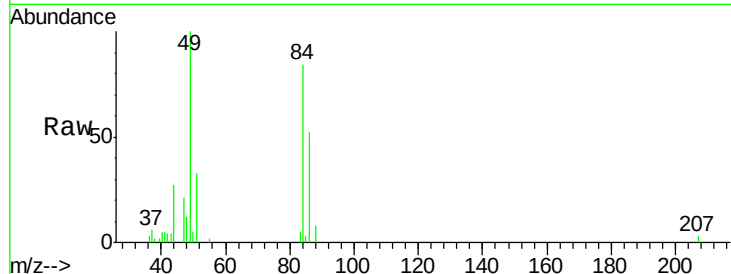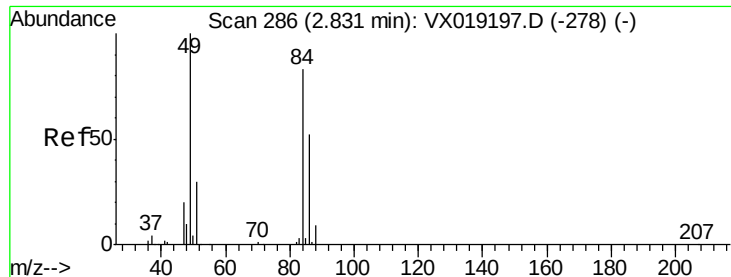

#16
Methylene chloride
Concen: 0.292 ug/L
RT: 2.83 min Scan# 286
Delta R.T. -0.00 min
Lab File: VX019198.D
Acq: 30 Oct 2020 10:33

Instrument :
MSVOA_X
ClientSampleId :
VBLK307

Tot Ion: 84 Resp: 4632
Ion Ratio Lower Upper
84 100
86 62.4 42.2 78.4
49 119.1 77.5 143.9

