

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX110120\
 Data File : VX019199.D
 Acq On : 30 Oct 2020 10:58
 Operator : JC/MD
 Sample : VX1101WBL07
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK308

Quant Time: Oct 30 14:07:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 30 08:55:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	196249	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	172410	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.06	152	79680	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	60548	4.77	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.40%
7) Chloroethane-d5	1.70	69	51617	4.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.60%
11) 1,1-Dichloroethene-d2	2.34	63	90936	3.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.40%
20) 2-Butanone-d5	4.56	46	147809	53.27	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.54%
24) Chloroform-d	5.14	84	116785	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
26) 1,2-Dichloroethane-d4	6.03	65	64774	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.20%
32) Benzene-d6	6.04	84	240209	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.20%
36) 1,2-Dichloropropane-d6	7.37	67	69887	5.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.00%
41) Toluene-d8	8.70	98	221279	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.60%
43) trans-1,3-Dichloropropene-	8.99	79	29008	5.06	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	101.20%
46) 2-Hexanone-d5	9.43	63	137580	54.83	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.66%
56) 1,1,2,2-Tetrachloroethane-	11.23	84	52064	5.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.00%
66) 1,2-Dichlorobenzene-d4	12.36	152	75901	5.13	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.60%


Target Compounds					Ovalue
16) Methylene chloride	2.83	84	2252	0.150 ug/L	92




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX110120\
Data File : VX019199.D
Acq On : 30 Oct 2020 10:58
Operator : JC/MD
Sample : VX1101WBL07
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK308

Quant Time: Oct 30 14:07:54 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 30 08:55:33 2020
Response via : Initial Calibration

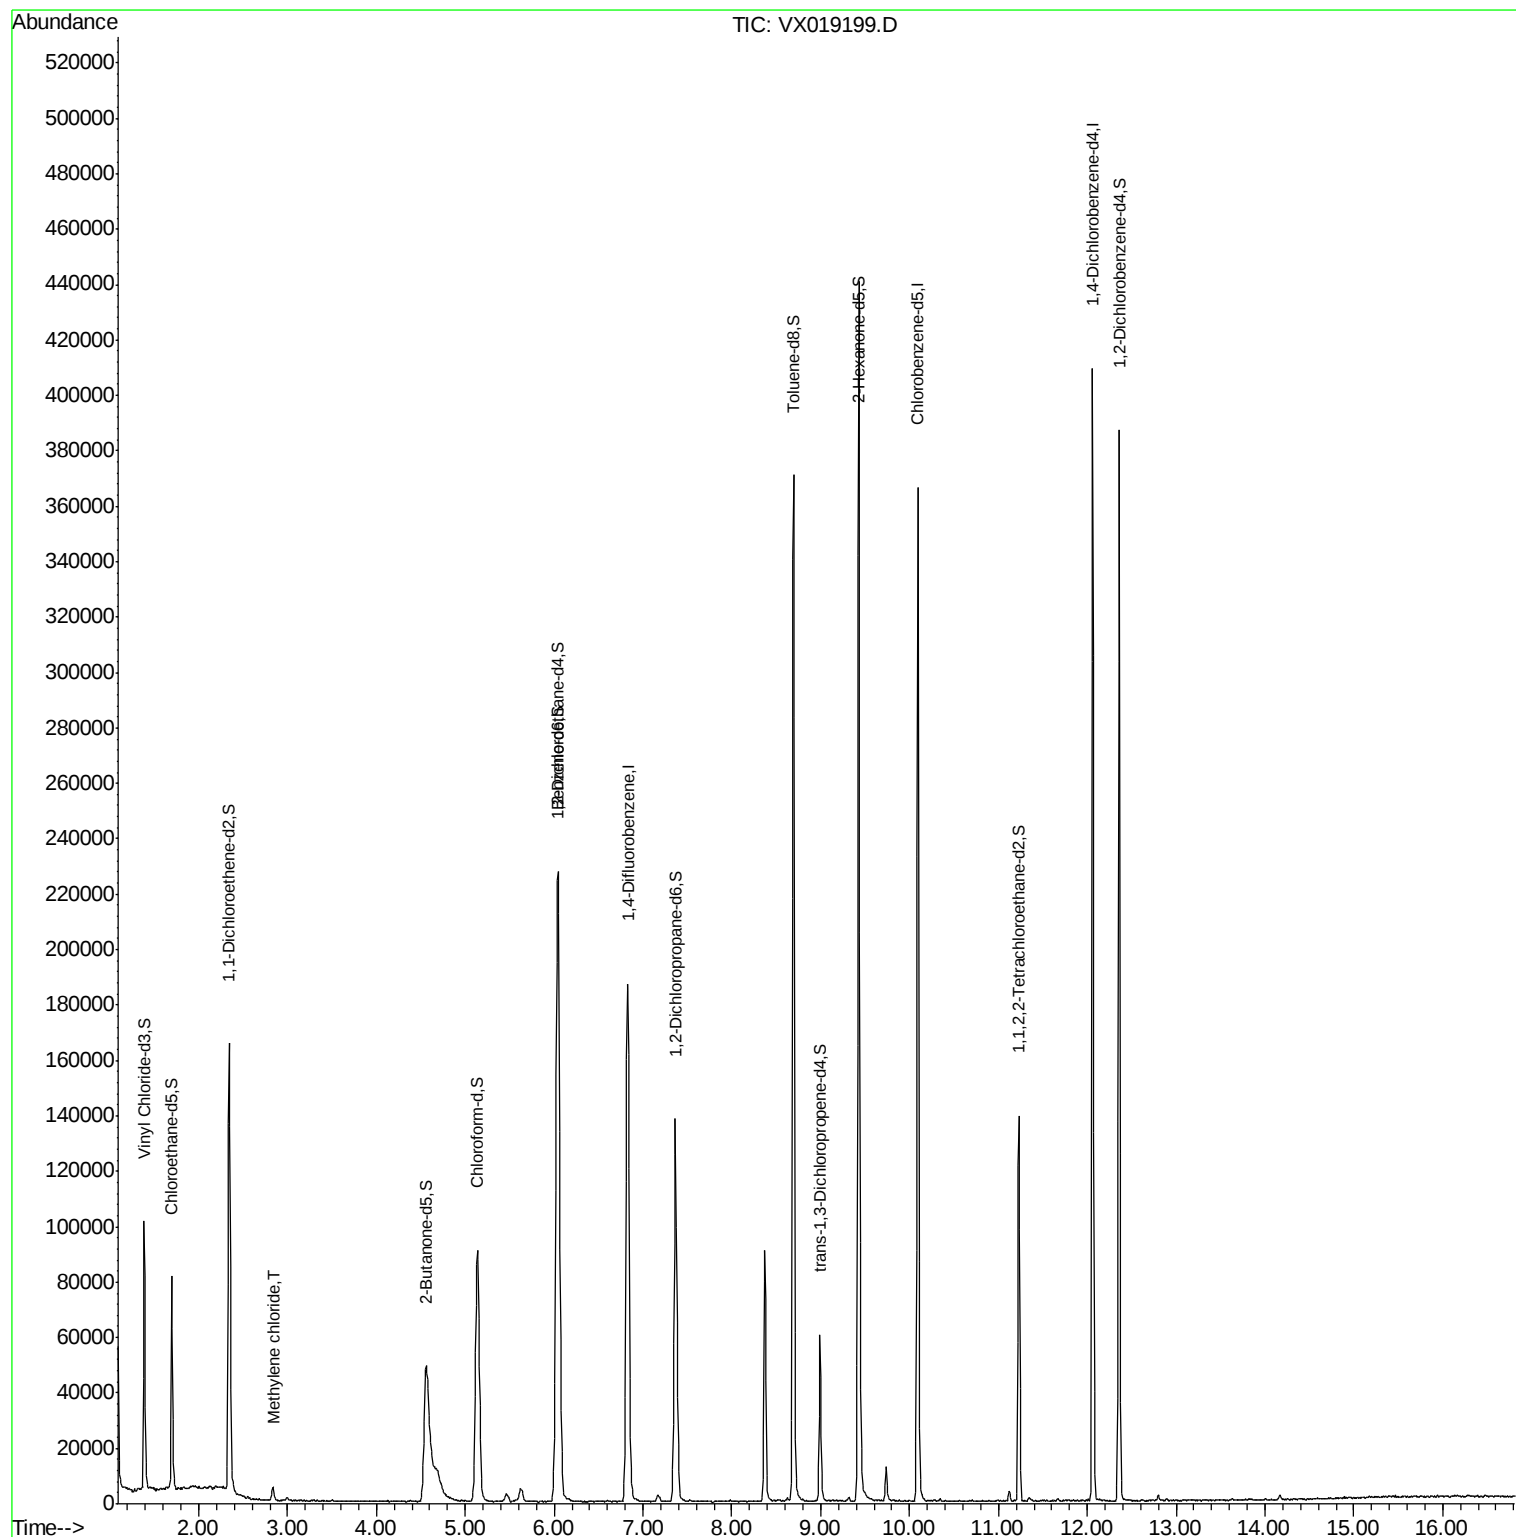

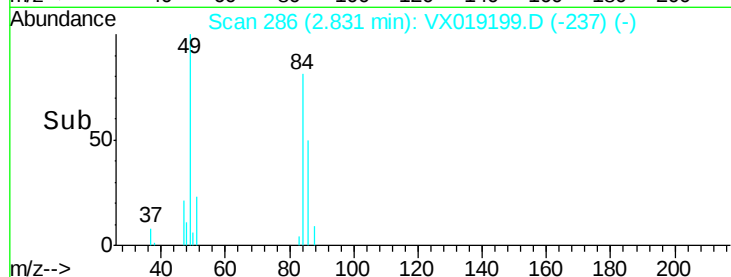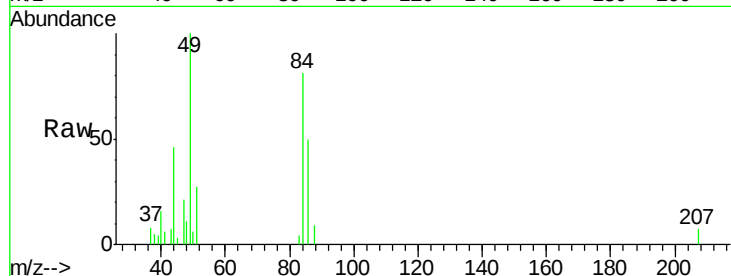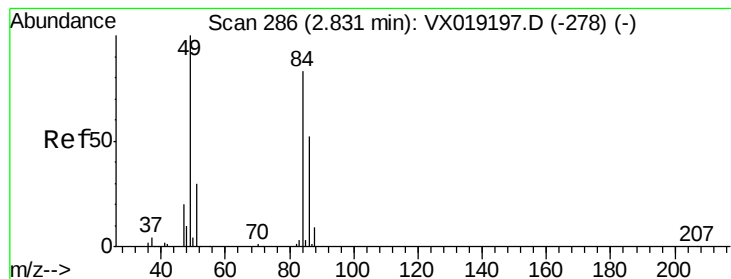

#16

Methylene chloride

Concen: 0.150 ug/L

RT: 2.83 min Scan# 286

Delta R.T. -0.00 min

Lab File: VX019199.D

Acq: 30 Oct 2020 10:58

Instrument :

MSVOA_X

ClientSampleId :

VBLK308

Tot Ion: 84 Resp: 2252

Ion Ratio Lower Upper

84 100

86 61.9 42.2 78.4

49 123.1 77.5 143.9

