


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX110120\
 Data File : VX019196.D
 Acq On : 30 Oct 2020 09:28
 Operator : JC/MD
 Sample : BFB63
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB63

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR102920WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Oct 30 08:55:33 2020

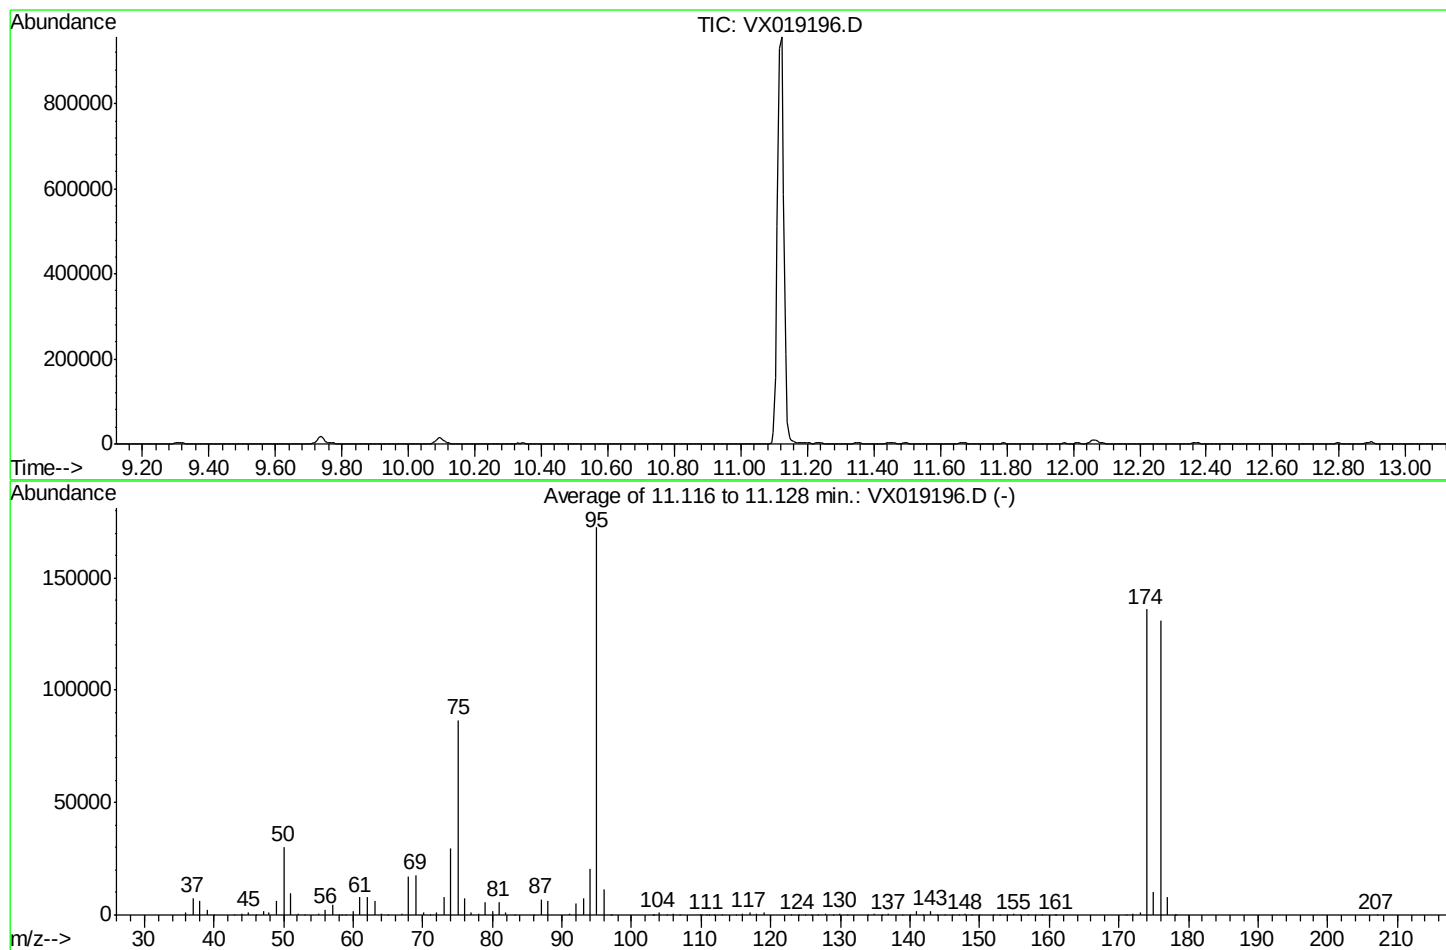

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	30362	PASS
75	95	30	80	50.2	86666	PASS
95	95	100	100	100.0	172528	PASS
96	95	5	9	6.6	11399	PASS
173	174	0.00	2	0.8	1151	PASS
174	95	50	120	78.8	135922	PASS
175	174	5	9	7.4	10069	PASS
176	174	95	105	96.5	131229	PASS
177	176	5	10	6.3	8273	PASS

m/z	Abundance
36.00	1656.0
37.00	9090.0
38.00	8023.0
39.10	3350.0
40.00	260.0
40.90	55.0
43.00	168.0
44.00	1807.0
45.00	1733.0
47.10	2254.0
48.00	1282.0
49.00	7943.0
50.00	38008.0
51.10	11926.0
52.10	464.0
55.00	632.0
56.00	3307.0
57.00	5645.0
58.10	196.0
59.00	54.0
60.00	1926.0
61.00	9342.0
62.00	9529.0
63.10	7516.0
64.00	782.0
65.00	316.0
67.10	491.0
68.00	20672.0
69.00	21616.0
70.10	1727.0
71.10	110.0
71.90	1073.0
73.00	9460.0
74.10	35440.0
75.10	103832.0
76.10	9388.0
77.00	1195.0
78.00	933.0
79.00	6654.0
80.00	1937.0
80.90	6929.0
81.90	1475.0
83.10	210.0
86.10	321.0
87.00	8009.0
88.00	7459.0
91.00	814.0
92.10	5672.0
93.10	8821.0
94.10	24336.0
95.00	198016.0
96.10	13793.0
97.00	492.0
103.10	81.0
103.90	1135.0
105.00	267.0
105.90	958.0
107.00	162.0
109.80	149.0
110.80	159.0
111.90	104.0
112.90	244.0
115.00	281.0
115.90	833.0
117.00	1266.0
118.00	733.0
118.90	1087.0
124.00	113.0
124.90	96.0
125.70	56.0
126.80	68.0
127.90	741.0
128.90	285.0
130.00	664.0
130.90	298.0
133.90	63.0
134.80	381.0
135.90	72.0
137.00	389.0
140.90	1991.0
141.90	281.0
142.90	1900.0
143.90	101.0
145.00	170.0
146.00	195.0
147.00	153.0
147.90	389.0
148.90	133.0
149.90	184.0
151.90	115.0
153.00	167.0
154.10	99.0

Instrument :
MSVOA_X
ClientSampleId :
BFB63

155.00	419.0
157.00	346.0
159.00	273.0
160.80	273.0
171.20	86.0
171.90	388.0
173.00	1200.0
174.00	139712.0
175.00	10924.0
176.00	132928.0
177.00	8670.0
178.00	248.0
207.20	95.0

Instrument :
MSVOA_X
ClientSampleId :
BFB63

m/z	Abundance
36.00	1538.0
37.00	8421.0
38.00	7110.0
39.00	2582.0
40.00	288.0
42.90	92.0
44.00	1602.0
45.00	1433.0
46.00	132.0
47.00	1922.0
47.90	1179.0
49.00	7544.0
50.00	34136.0
51.00	10841.0
52.00	465.0
53.00	59.0
55.00	549.0
56.00	2820.0
57.00	5457.0
58.00	252.0
58.90	54.0
60.00	1741.0
61.00	9094.0
62.00	9111.0
63.00	7219.0
64.10	614.0
64.90	184.0
67.00	516.0
68.00	20712.0
69.00	20224.0
70.00	1578.0
71.10	89.0
72.00	1152.0
73.00	8749.0
74.00	34752.0
75.10	99224.0
76.10	8368.0
77.00	1211.0
78.00	732.0
79.00	6428.0
80.00	1875.0
80.90	6638.0
82.00	1380.0
83.10	189.0
86.00	212.0
87.00	7899.0
88.00	7943.0
91.00	718.0
92.00	5652.0
93.00	8330.0
94.00	23616.0
95.00	200768.0
96.00	12877.0
97.20	250.0
102.90	91.0
103.90	912.0
105.00	259.0
105.90	924.0
106.90	282.0
109.90	151.0
110.90	191.0
112.00	186.0
113.00	249.0
115.00	203.0
116.00	787.0
116.90	1157.0
118.00	753.0
119.00	1068.0
124.10	84.0
124.90	106.0
125.80	79.0
126.90	81.0
127.90	768.0
129.00	374.0
129.90	798.0
131.00	275.0
133.90	62.0
134.90	317.0
136.90	363.0
138.90	98.0
140.10	174.0
141.00	1974.0
141.80	228.0
143.00	2253.0
144.00	162.0
145.00	218.0
146.00	368.0
146.90	146.0
148.00	487.0
148.90	198.0
150.00	220.0
151.90	112.0

Instrument :
MSVOA_X
ClientSampleId :
BFB63

152.90	179.0
154.10	118.0
155.00	557.0
155.80	98.0
156.90	329.0
158.90	253.0
161.00	324.0
172.00	455.0
173.00	1332.0
174.00	158528.0
175.00	11811.0
176.00	157248.0
177.00	9981.0
178.20	228.0
207.00	101.0

Instrument :
MSVOA_X
ClientSampleId :
BFB63

m/z	Abundance
36.00	801.0
37.00	4763.0
38.00	3924.0
39.00	1618.0
39.90	207.0
41.00	102.0
43.00	153.0
44.10	1340.0
45.00	808.0
46.10	113.0
47.00	885.0
47.90	590.0
49.00	4148.0
50.00	18944.0
51.00	6169.0
52.00	283.0
55.00	337.0
56.10	1620.0
57.00	2982.0
58.30	102.0
60.00	939.0
61.00	5360.0
62.00	4850.0
63.10	4019.0
64.10	411.0
65.00	171.0
67.10	284.0
68.00	10508.0
69.00	11736.0
70.00	757.0
71.20	55.0
72.00	509.0
73.00	5247.0
74.00	19424.0
75.10	56944.0
76.00	4750.0
77.00	684.0
77.90	490.0
79.00	3775.0
80.00	1120.0
80.90	3998.0
82.00	744.0
83.00	112.0
85.90	130.0
87.00	5074.0
88.00	4089.0
90.90	422.0
92.10	3387.0
93.00	5157.0
94.00	13664.0
95.10	118800.0
96.00	7527.0
97.10	200.0
103.20	73.0
103.90	599.0
105.00	243.0
106.00	618.0
106.90	201.0
110.10	68.0
110.70	64.0
111.20	84.0
111.80	107.0
113.00	138.0
115.00	145.0
115.90	542.0
116.90	717.0
117.90	466.0
119.00	843.0
122.90	51.0
123.90	78.0
127.90	371.0
128.90	192.0
129.80	462.0
131.00	173.0
133.90	58.0
135.00	264.0
137.00	284.0
138.90	63.0
139.90	88.0
141.00	1436.0
142.00	126.0
143.00	1430.0
143.90	116.0
144.80	184.0
146.00	184.0
146.80	131.0
147.90	322.0
148.90	128.0
149.80	159.0
151.90	111.0
153.00	79.0
153.90	119.0

Instrument :
MSVOA_X
ClientSampleId :
BFB63

154.80	334.0
155.90	61.0
156.90	215.0
158.00	61.0
158.90	152.0
161.00	159.0
171.10	54.0
172.00	291.0
173.10	921.0
174.00	109528.0
175.00	7472.0
176.00	103512.0
177.00	6170.0
178.00	201.0
207.00	97.0

Instrument :
MSVOA_X
ClientSampleId :
BFB63

Scan 1638 (11.073 min): VX019196.D
BFB63

m/z	Abundance
40.00	160.0
41.10	73.0
43.00	71.0
44.00	704.0
207.30	65.0

Instrument :
MSVOA_X
ClientSampleId :
BFB63