

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110121\
 Data File : VX025030.D
 Acq On : 01 Nov 2021 11:27
 Operator : JC/MD
 Sample : VX1101MBL06
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK627

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
 Title : VOC Analysis

Signal : TIC: VX025030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	56540	58212	9.37%	1.152%
2	1.672	91	96	107	rVB	41630	52444	8.44%	1.038%
3	2.306	194	200	210	rBV	118156	192173	30.93%	3.803%
4	2.514	228	234	242	rBV3	1322	3016	0.49%	0.060%
5	2.782	274	278	285	rBV2	1452	3044	0.49%	0.060%
6	2.879	292	294	295	rBV	476	226	0.04%	0.004%
7	3.087	326	328	330	rBV	746	802	0.13%	0.016%
8	3.142	335	337	339	rBV	497	490	0.08%	0.010%
9	3.203	345	347	350	rBV	338	286	0.05%	0.006%
10	3.227	350	351	356	rVB2	471	577	0.09%	0.011%
11	3.587	407	410	414	rBV	454	739	0.12%	0.015%
12	3.623	414	416	417	rBV	570	425	0.07%	0.008%
13	3.666	421	423	424	rBV	327	181	0.03%	0.004%
14	3.934	465	467	471	rVV	410	363	0.06%	0.007%
15	3.965	471	472	474	rVB	666	315	0.05%	0.006%
16	4.062	486	488	491	rBV	378	305	0.05%	0.006%
17	4.093	491	493	494	rBV	324	146	0.02%	0.003%
18	4.458	545	553	565	rBV2	53798	156733	25.23%	3.102%
19	4.727	595	597	601	rBV2	666	744	0.12%	0.015%
20	4.916	626	628	630	rBV	420	434	0.07%	0.009%
21	4.952	632	634	635	rBV	457	280	0.05%	0.006%
22	5.062	639	652	668	rBV	93048	289281	46.56%	5.725%
23	5.342	696	698	699	rBV	338	196	0.03%	0.004%
24	5.605	739	741	744	rBV	577	729	0.12%	0.014%
25	5.678	749	753	754	rBV2	608	542	0.09%	0.011%
26	5.970	788	801	816	rBV2	202600	621331	100.00%	12.296%
27	6.348	861	863	866	rBV2	585	410	0.07%	0.008%
28	6.373	866	867	869	rBV	349	304	0.05%	0.006%
29	6.592	902	903	905	rBV	381	313	0.05%	0.006%
30	6.659	912	914	915	rBV	482	392	0.06%	0.008%
31	6.763	922	931	943	rBV	191610	457270	73.60%	9.050%
32	6.964	963	964	967	rVB	343	268	0.04%	0.005%
33	7.104	980	987	996	rBV4	3343	8506	1.37%	0.168%
34	7.312	1012	1021	1032	rBV	131572	287284	46.24%	5.685%
35	7.464	1044	1046	1048	rBV	745	562	0.09%	0.011%
36	7.482	1048	1049	1052	rVV	905	859	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110121\
 Data File : VX025030.D
 Acq On : 01 Nov 2021 11:27
 Operator : JC/MD
 Sample : VX1101MBL06
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK627

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

37	7.537	1056	1058	1061	rVB	602	517	0.08%	0.010%
38	7.574	1062	1064	1065	rVB	414	210	0.03%	0.004%
39	7.598	1065	1068	1069	rBV	129	142	0.02%	0.003%
40	7.793	1098	1100	1104	rBV	518	669	0.11%	0.013%
41	8.049	1140	1142	1144	rBV2	533	424	0.07%	0.008%
42	8.324	1181	1187	1196	rBV	97033	157671	25.38%	3.120%
43	8.519	1217	1219	1222	rBV	552	581	0.09%	0.011%
44	8.543	1222	1223	1225	rBV	353	263	0.04%	0.005%
45	8.653	1234	1241	1249	rBV	293266	468646	75.43%	9.275%
46	8.952	1284	1290	1300	rBV	76744	110574	17.80%	2.188%
47	9.153	1321	1323	1325	rVB	825	628	0.10%	0.012%
48	9.183	1325	1328	1329	rBV	355	363	0.06%	0.007%
49	9.238	1335	1337	1338	rBV	277	125	0.02%	0.002%
50	9.317	1348	1350	1353	rVB	534	481	0.08%	0.010%
51	9.384	1353	1361	1375	rBV	249213	355550	57.22%	7.036%
52	9.519	1381	1383	1385	rBV2	864	593	0.10%	0.012%
53	9.598	1394	1396	1397	rBV2	523	543	0.09%	0.011%
54	9.640	1401	1403	1404	rBV2	319	262	0.04%	0.005%
55	9.768	1422	1424	1425	rBV2	663	360	0.06%	0.007%
56	10.055	1465	1471	1480	rBV	404300	527203	84.85%	10.434%
57	10.244	1498	1502	1503	rBV	466	553	0.09%	0.011%
58	10.268	1505	1506	1508	rVV	619	570	0.09%	0.011%
59	10.299	1508	1511	1518	rVB	1333	2202	0.35%	0.044%
60	10.421	1530	1531	1532	rBV	461	280	0.05%	0.006%
61	10.732	1581	1582	1583	rBV	272	179	0.03%	0.004%
62	10.835	1598	1599	1602	rBV	690	610	0.10%	0.012%
63	10.939	1615	1616	1617	rBV	335	195	0.03%	0.004%
64	11.006	1625	1627	1629	rBV	503	465	0.07%	0.009%
65	11.091	1637	1641	1642	rBV	521	688	0.11%	0.014%
66	11.195	1652	1658	1665	rBV	262379	333606	53.69%	6.602%
67	11.427	1695	1696	1698	rBV	652	559	0.09%	0.011%
68	11.604	1723	1725	1728	rBV	445	414	0.07%	0.008%
69	11.640	1728	1731	1734	rVB2	877	988	0.16%	0.020%
70	11.756	1746	1750	1752	rBV3	1902	2390	0.38%	0.047%
71	11.921	1774	1777	1778	rBV3	711	615	0.10%	0.012%
72	11.975	1784	1786	1788	rVB3	1595	947	0.15%	0.019%
73	12.024	1788	1794	1802	rBV	401047	490561	78.95%	9.708%
74	12.323	1837	1843	1850	rBV	349587	443378	71.36%	8.775%
75	12.518	1873	1875	1876	rBV	386	197	0.03%	0.004%
76	12.707	1905	1906	1908	rBV	338	212	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110121\
 Data File : VX025030.D
 Acq On : 01 Nov 2021 11:27
 Operator : JC/MD
 Sample : VX1101MBL06
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK627

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

77	12.762	1913	1915	1919	rBV	660	947	0.15%	0.019%
78	13.158	1978	1980	1981	rVB	522	291	0.05%	0.006%
79	13.243	1992	1994	1995	rVB	455	195	0.03%	0.004%
80	13.365	2012	2014	2017	rVB	620	605	0.10%	0.012%
81	13.658	2059	2062	2063	rBV	550	414	0.07%	0.008%
82	13.719	2071	2072	2075	rBV	558	354	0.06%	0.007%
83	13.835	2090	2091	2092	rBV	269	175	0.03%	0.003%
84	13.969	2110	2113	2115	rBV2	1174	1187	0.19%	0.023%
85	14.158	2143	2144	2146	rBV	526	310	0.05%	0.006%
86	14.335	2171	2173	2174	rBV	484	227	0.04%	0.004%
87	14.402	2182	2184	2187	rBV	585	604	0.10%	0.012%
88	14.463	2193	2194	2195	rBV	229	111	0.02%	0.002%
89	14.481	2195	2197	2199	rBV	486	438	0.07%	0.009%
90	14.780	2243	2246	2248	rBV2	657	1080	0.17%	0.021%
91	15.335	2335	2337	2339	rBV2	655	435	0.07%	0.009%


Sum of corrected areas: 5052969

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110121\
Data File : VX025030.D
Acq On : 01 Nov 2021 11:27
Operator : JC/MD
Sample : VX1101MBL06
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK627

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

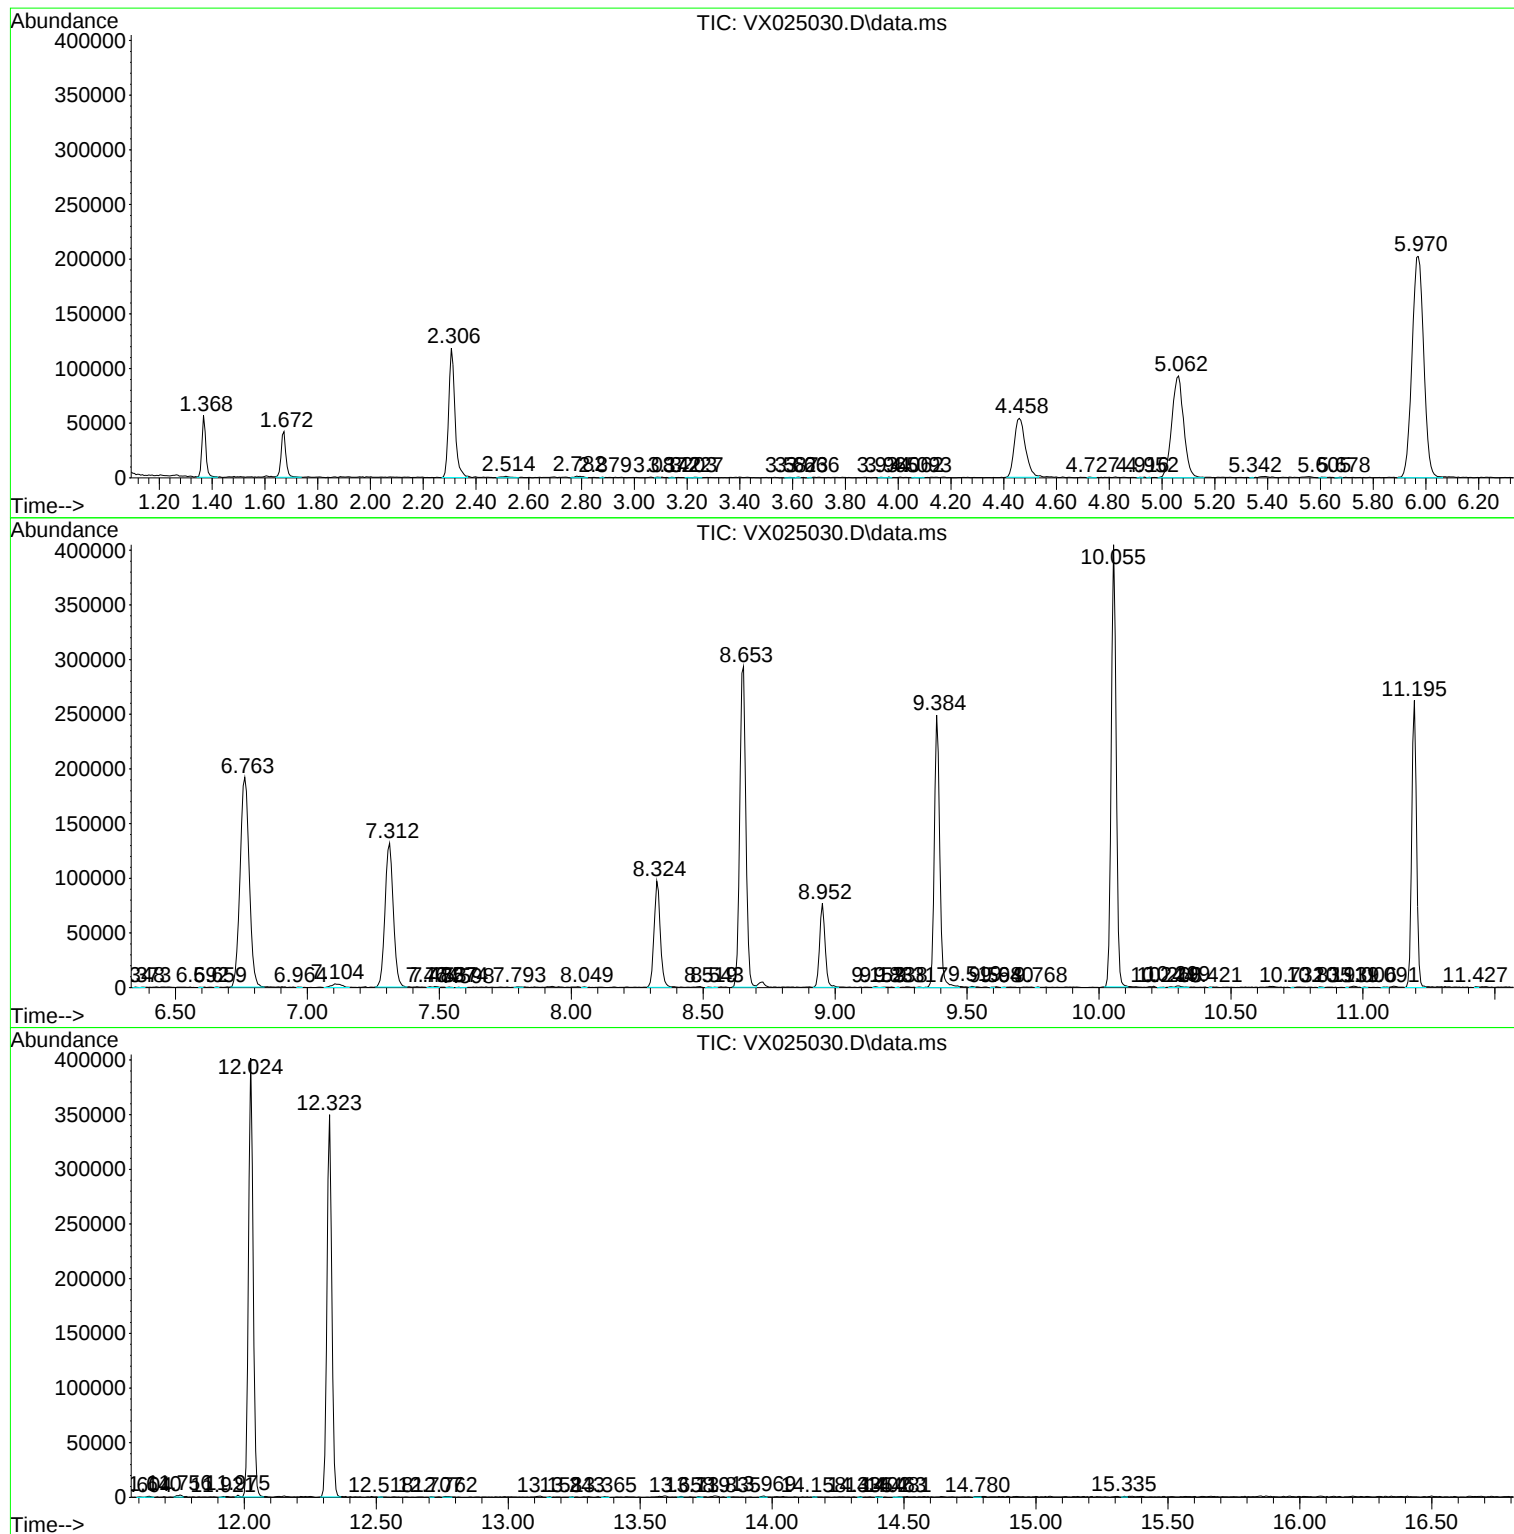

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110121\
Data File : VX025030.D
Acq On : 01 Nov 2021 11:27
Operator : JC/MD
Sample : VX1101MBL06
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK627

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110121\
Data File : VX025030.D
Acq On : 01 Nov 2021 11:27
Operator : JC/MD
Sample : VX1101MBL06
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK627

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc