

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110121\
 Data File : VX025032.D
 Acq On : 01 Nov 2021 14:13
 Operator : JC/MD
 Sample : VX1101WBL06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK629

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
 Title : VOC Analysis

Signal : TIC: VX025032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rBV	67470	69408	10.14%	1.327%
2	1.666	91	95	107	rVB	45864	57729	8.44%	1.104%
3	2.246	188	190	191	rBV	577	333	0.05%	0.006%
4	2.307	194	200	213	rVB	144698	232797	34.02%	4.452%
5	2.575	243	244	245	rBV	439	243	0.04%	0.005%
6	2.611	248	250	252	rVB	358	297	0.04%	0.006%
7	2.770	272	276	277	rBV	451	574	0.08%	0.011%
8	2.886	294	295	298	rBV	358	388	0.06%	0.007%
9	2.983	307	311	312	rBV	604	716	0.10%	0.014%
10	3.008	312	315	316	rBV	272	252	0.04%	0.005%
11	3.160	337	340	342	rVB	514	335	0.05%	0.006%
12	3.197	342	346	347	rBB	398	356	0.05%	0.007%
13	3.434	384	385	387	rBV	639	405	0.06%	0.008%
14	3.483	391	393	395	rVB	440	272	0.04%	0.005%
15	3.501	395	396	397	rBV	302	213	0.03%	0.004%
16	3.538	401	402	404	rVB	445	279	0.04%	0.005%
17	3.660	421	422	424	rBV	368	257	0.04%	0.005%
18	3.697	426	428	430	rVB	294	230	0.03%	0.004%
19	3.745	434	436	438	rBV2	429	299	0.04%	0.006%
20	3.849	449	453	455	rBV	647	620	0.09%	0.012%
21	3.873	455	457	459	rVB	721	545	0.08%	0.010%
22	3.904	459	462	465	rBV	326	372	0.05%	0.007%
23	4.007	477	479	481	rBV	202	251	0.04%	0.005%
24	4.044	484	485	487	rVV	414	346	0.05%	0.007%
25	4.068	487	489	490	rVB	542	284	0.04%	0.005%
26	4.300	525	527	528	rBV	252	150	0.02%	0.003%
27	4.459	545	553	566	rBV2	53173	152282	22.25%	2.912%
28	4.648	582	584	587	rVB	525	472	0.07%	0.009%
29	4.757	600	602	604	rBV	432	263	0.04%	0.005%
30	4.776	604	605	606	rBV	520	230	0.03%	0.004%
31	4.849	614	617	618	rBV	212	222	0.03%	0.004%
32	4.946	631	633	634	rBV	440	363	0.05%	0.007%
33	5.056	642	651	666	rVB2	99178	301325	44.03%	5.763%
34	5.263	684	685	686	rBV	302	119	0.02%	0.002%
35	5.330	692	696	697	rBV2	529	543	0.08%	0.010%
36	5.367	700	702	703	rVV2	519	262	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110121\
 Data File : VX025032.D
 Acq On : 01 Nov 2021 14:13
 Operator : JC/MD
 Sample : VX1101WBL06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK629

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

37	5.446	713	715	716	rBV2	621	449	0.07%	0.009%
38	5.513	724	726	727	rBV	341	131	0.02%	0.003%
39	5.544	727	731	734	rBV	814	1103	0.16%	0.021%
40	5.678	752	753	754	rBV	367	162	0.02%	0.003%
41	5.836	777	779	780	rVB	321	193	0.03%	0.004%
42	5.867	780	784	786	rBV2	750	782	0.11%	0.015%
43	5.971	789	801	813	rBV2	232869	684303	100.00%	13.087%
44	6.385	868	869	871	rVB	478	308	0.05%	0.006%
45	6.684	917	918	919	rBV	251	128	0.02%	0.002%
46	6.763	921	931	944	rVV	178790	425971	62.25%	8.147%
47	7.190	999	1001	1003	rBV	698	530	0.08%	0.010%
48	7.208	1003	1004	1005	rVV	247	105	0.02%	0.002%
49	7.312	1012	1021	1033	rBV	139593	314073	45.90%	6.007%
50	7.464	1043	1046	1047	rBV	502	487	0.07%	0.009%
51	7.574	1063	1064	1066	rBV	409	310	0.05%	0.006%
52	7.690	1081	1083	1086	rBV	425	502	0.07%	0.010%
53	7.879	1113	1114	1115	rBV	398	218	0.03%	0.004%
54	8.074	1143	1146	1149	rBV	599	630	0.09%	0.012%
55	8.123	1152	1154	1155	rBV	294	305	0.04%	0.006%
56	8.171	1158	1162	1164	rBV	394	586	0.09%	0.011%
57	8.202	1166	1167	1168	rBV	438	230	0.03%	0.004%
58	8.324	1181	1187	1197	rBV	101571	169397	24.75%	3.240%
59	8.653	1234	1241	1248	rBV	343136	550645	80.47%	10.531%
60	8.952	1284	1290	1300	rBV	84210	121100	17.70%	2.316%
61	9.171	1323	1326	1328	rBV	492	536	0.08%	0.010%
62	9.385	1353	1361	1372	rBV	244203	348678	50.95%	6.669%
63	9.641	1402	1403	1406	rBV	327	345	0.05%	0.007%
64	9.665	1406	1407	1408	rVB	557	208	0.03%	0.004%
65	9.848	1434	1437	1438	rBB	407	396	0.06%	0.008%
66	9.866	1438	1440	1443	rBV	262	299	0.04%	0.006%
67	9.903	1443	1446	1450	rVV2	508	702	0.10%	0.013%
68	10.055	1465	1471	1480	rBV	364935	489995	71.60%	9.371%
69	10.275	1506	1507	1508	rBV	331	139	0.02%	0.003%
70	10.397	1525	1527	1529	rBV2	437	317	0.05%	0.006%
71	10.573	1554	1556	1557	rBV2	314	224	0.03%	0.004%
72	10.653	1568	1569	1571	rBV2	497	271	0.04%	0.005%
73	10.707	1575	1578	1580	rBV2	417	543	0.08%	0.010%
74	10.939	1614	1616	1617	rBV	446	240	0.04%	0.005%
75	11.073	1636	1638	1640	rBV	457	462	0.07%	0.009%
76	11.122	1642	1646	1650	rBV2	3103	4208	0.61%	0.080%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110121\
 Data File : VX025032.D
 Acq On : 01 Nov 2021 14:13
 Operator : JC/MD
 Sample : VX1101WBL06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK629

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
 Title : VOC Analysis

77	11.195	1653	1658	1666	rVB	263037	336655	49.20%	6.439%
78	11.756	1746	1750	1754	rVB4	2861	3378	0.49%	0.065%
79	11.933	1776	1779	1782	rBV3	1156	1427	0.21%	0.027%
80	12.024	1789	1794	1800	rBV	359858	452115	66.07%	8.647%
81	12.256	1830	1832	1833	rVB	670	271	0.04%	0.005%
82	12.274	1833	1835	1836	rBV	681	414	0.06%	0.008%
83	12.323	1837	1843	1850	rVV	382445	481543	70.37%	9.210%
84	12.482	1867	1869	1874	rBV	932	942	0.14%	0.018%
85	12.603	1887	1889	1891	rBV	413	353	0.05%	0.007%
86	13.000	1952	1954	1957	rBV	672	426	0.06%	0.008%
87	13.250	1992	1995	1996	rBV	378	404	0.06%	0.008%
88	13.286	2000	2001	2002	rVV	550	307	0.04%	0.006%
89	13.305	2002	2004	2006	rVV	1005	627	0.09%	0.012%
90	13.341	2008	2010	2012	rVV	428	381	0.06%	0.007%
91	13.359	2012	2013	2015	rVB2	552	335	0.05%	0.006%
92	14.201	2150	2151	2155	rVB2	997	718	0.10%	0.014%
93	14.243	2155	2158	2160	rBV2	426	498	0.07%	0.010%
94	14.475	2194	2196	2197	rBV2	659	389	0.06%	0.007%
95	14.597	2214	2216	2220	rBV2	401	429	0.06%	0.008%
96	14.816	2248	2252	2257	rBV3	500	732	0.11%	0.014%
97	14.853	2257	2258	2261	rBV2	531	464	0.07%	0.009%
98	15.024	2285	2286	2289	rBV	444	421	0.06%	0.008%
99	16.243	2485	2486	2489	rBV2	592	520	0.08%	0.010%
100	16.700	2559	2561	2567	rBV3	546	719	0.11%	0.014%




Sum of corrected areas: 5228711

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110121\
Data File : VX025032.D
Acq On : 01 Nov 2021 14:13
Operator : JC/MD
Sample : VX1101WBL06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK629

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

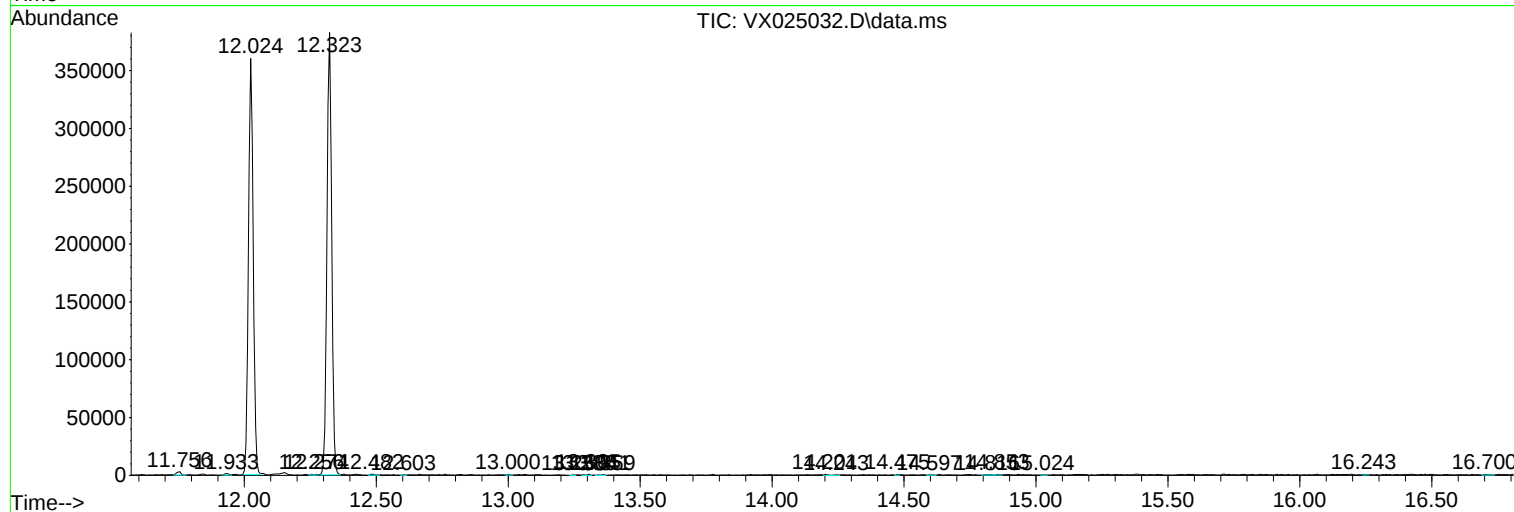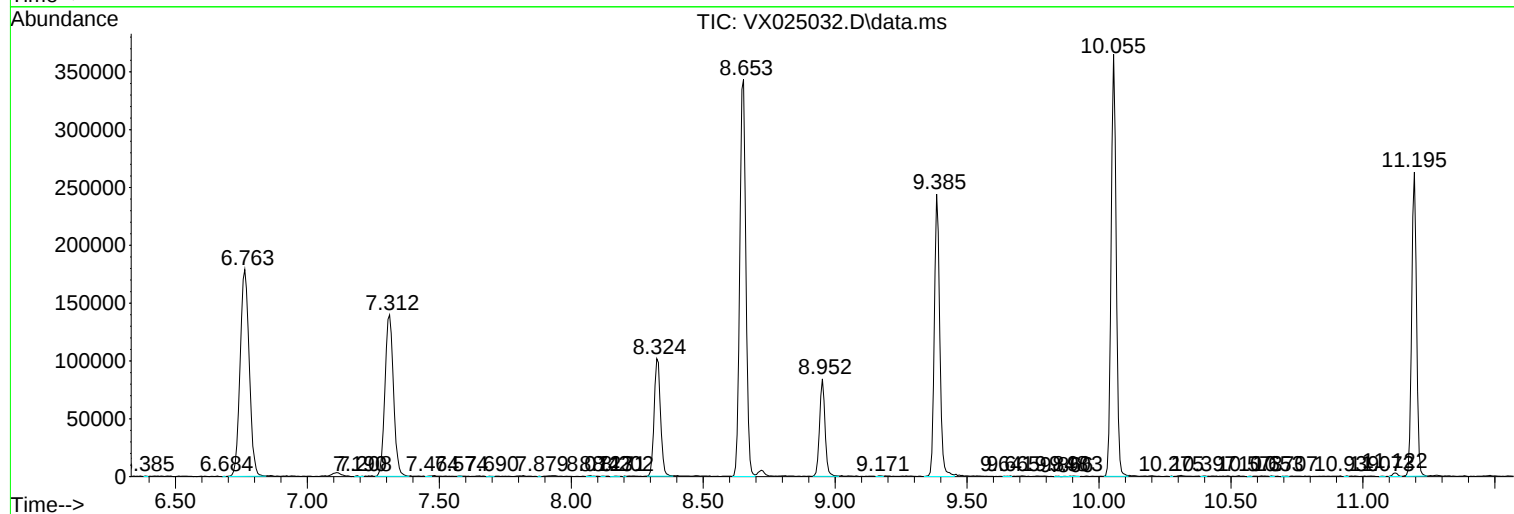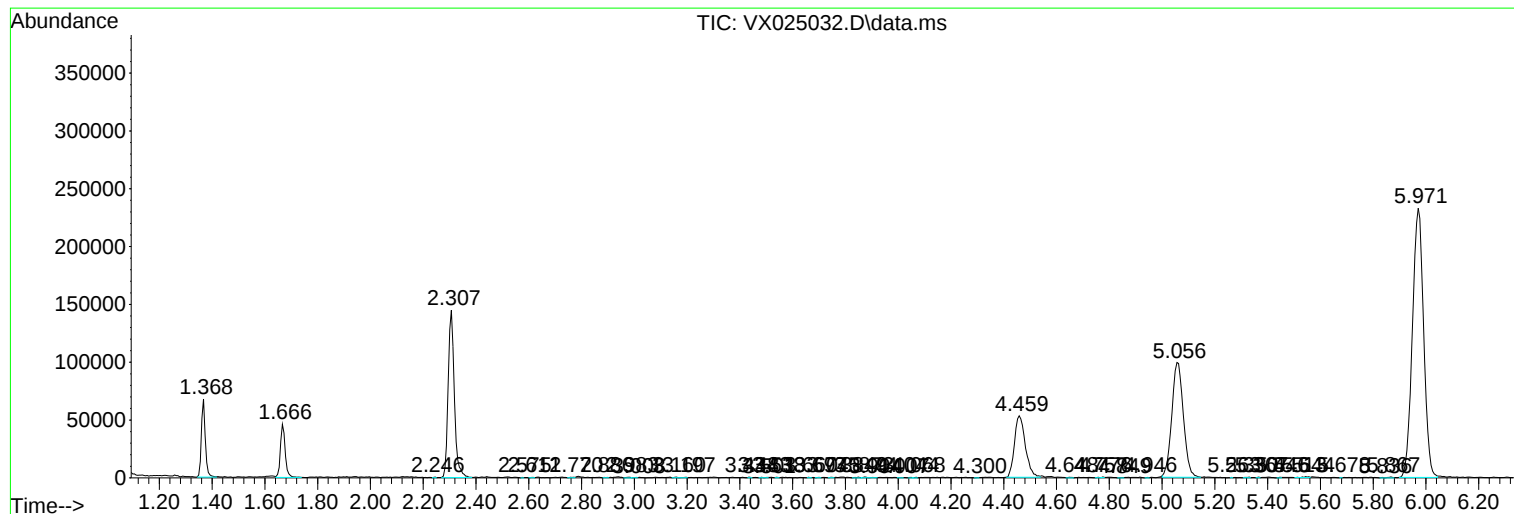

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110121\
Data File : VX025032.D
Acq On : 01 Nov 2021 14:13
Operator : JC/MD
Sample : VX1101WBL06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK629

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110121\
Data File : VX025032.D
Acq On : 01 Nov 2021 14:13
Operator : JC/MD
Sample : VX1101WBL06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK629

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc