
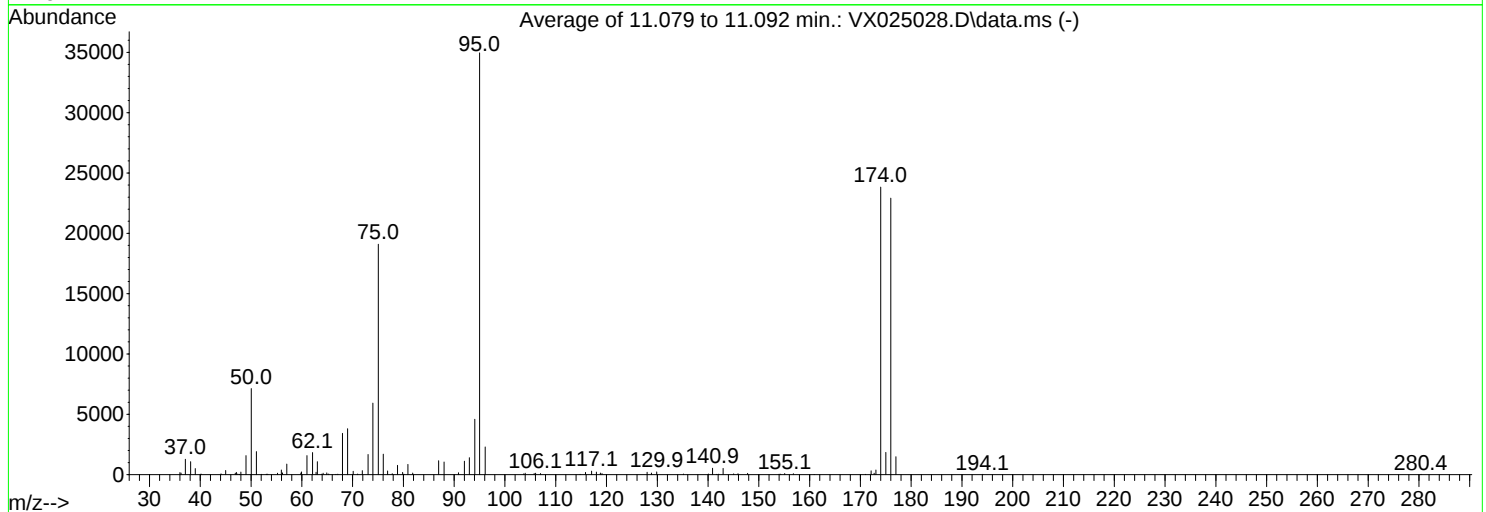


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110121\
Data File : VX025028.D
Acq On : 01 Nov 2021 09:52
Operator : JC/MD
Sample : BFB609
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB609

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM102821WMA.M
Title : VOC Analysis
Last Update : Tue Nov 02 03:29:47 2021

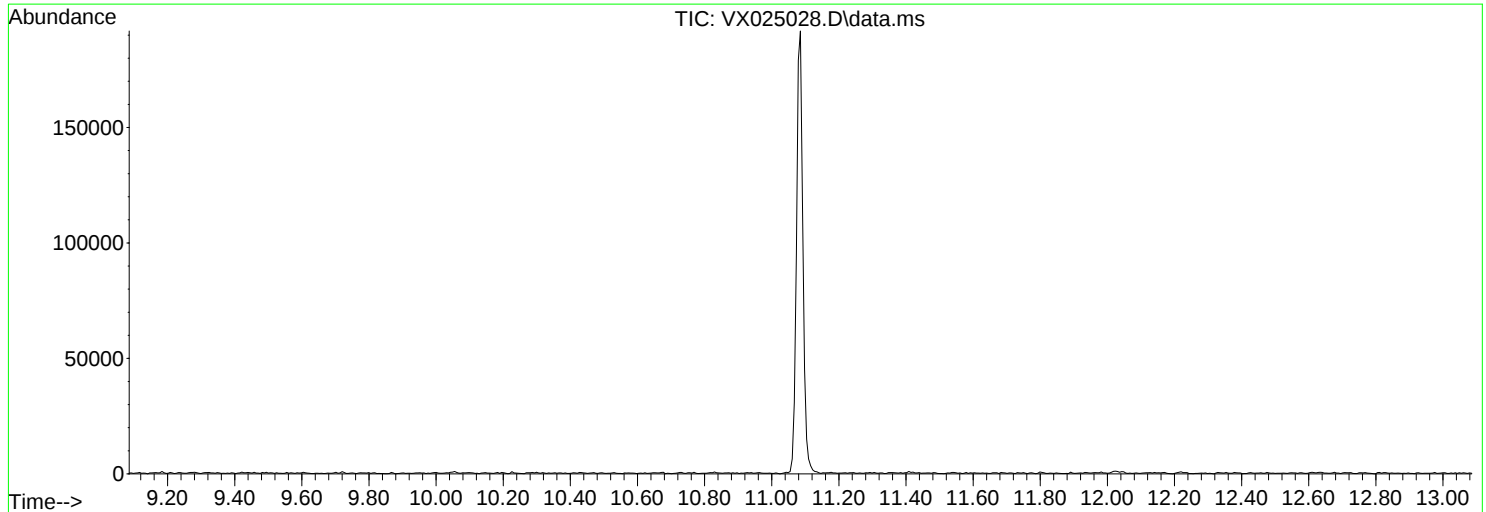

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1634

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	7138	PASS
75	95	30	80	54.6	19101	PASS
95	95	100	100	100.0	34957	PASS
96	95	5	9	6.6	2298	PASS
173	174	0.00	2	1.6	381	PASS
174	95	50	120	68.2	23835	PASS
175	174	5	9	7.7	1840	PASS
176	174	95	101	96.1	22909	PASS
177	176	5	9	6.5	1491	PASS

m/z	Abundance
39.90	203.0
44.20	128.0
52.00	96.0
57.20	112.0

Instrument :
MSVOA_X
ClientSampleId :
BFB609

m/z	Abundance
36.00	319.0
37.10	1681.0
38.10	1299.0
39.00	720.0
44.20	274.0
45.00	446.0
46.90	366.0
47.40	152.0
48.00	376.0
49.00	2079.0
50.10	8557.0
51.00	1960.0
52.10	140.0
53.30	110.0
55.30	174.0
56.00	531.0
57.00	1221.0
59.80	400.0
61.00	2083.0
62.10	2078.0
63.00	1838.0
64.20	190.0
64.90	204.0
66.70	70.0
68.00	4199.0
69.00	4325.0
70.20	372.0
71.00	77.0
71.90	445.0
73.00	1745.0
74.00	7060.0
75.00	23096.0
76.10	1695.0
76.90	406.0
77.80	72.0
78.80	814.0
79.90	211.0
81.00	918.0
81.90	124.0
86.90	1310.0
88.10	1161.0
90.90	182.0
92.00	1120.0
93.00	1681.0
94.10	5136.0
95.00	38968.0
96.10	2652.0
103.70	205.0
105.70	108.0
106.10	162.0
107.00	129.0
115.80	236.0
117.00	337.0
118.00	244.0
118.80	290.0
128.10	196.0
128.80	89.0
129.80	218.0
140.90	582.0
141.70	84.0
143.00	530.0
145.00	77.0
145.90	73.0
147.80	97.0
150.00	61.0
154.30	103.0
155.10	75.0
156.80	91.0
160.90	60.0
171.00	79.0
172.10	337.0
172.70	359.0
173.10	271.0
174.00	23008.0
175.00	1631.0
176.00	22648.0
177.00	1561.0

Instrument :
MSVOA_X
ClientSampleId :
BFB609

m/z	Abundance
36.00	207.0
37.00	1112.0
38.10	1291.0
39.00	457.0
40.10	65.0
44.00	178.0
45.00	390.0
47.10	358.0
48.00	249.0
49.00	1550.0
50.00	8507.0
51.10	2405.0
52.10	221.0
55.10	176.0
55.90	611.0
57.10	1074.0
60.00	461.0
61.00	1678.0
62.10	2287.0
63.10	1371.0
64.20	183.0
64.90	246.0
67.10	138.0
68.00	3912.0
69.00	4467.0
70.00	306.0
71.00	83.0
71.90	385.0
73.00	1936.0
74.00	6856.0
75.10	21696.0
76.00	1959.0
76.90	328.0
77.80	89.0
78.90	951.0
79.80	214.0
80.90	1024.0
81.90	151.0
87.00	1386.0
87.90	1345.0
90.80	143.0
92.10	1344.0
93.00	1758.0
94.00	5198.0
95.00	41824.0
96.10	2649.0
104.00	220.0
105.80	190.0
107.00	153.0
114.80	79.0
115.90	237.0
117.10	341.0
118.00	221.0
119.10	280.0
128.00	176.0
128.90	160.0
129.90	181.0
135.10	70.0
140.10	76.0
140.90	663.0
142.10	69.0
143.00	644.0
145.10	139.0
145.90	74.0
147.80	204.0
154.00	57.0
155.10	193.0
156.80	85.0
172.00	389.0
173.00	460.0
174.00	29200.0
175.00	2666.0
176.00	27464.0
177.00	1843.0

Instrument :
MSVOA_X
ClientSampleId :
BFB609

m/z	Abundance
36.20	394.0
37.00	1024.0
38.00	618.0
39.10	354.0
40.20	111.0
44.00	120.0
45.00	216.0
47.10	204.0
47.70	91.0
49.00	1104.0
50.00	4349.0
51.00	1383.0
53.00	120.0
56.20	425.0
57.00	681.0
59.90	236.0
61.10	966.0
62.00	1109.0
62.80	616.0
63.90	121.0
65.30	182.0
68.00	2153.0
69.00	2626.0
70.20	176.0
72.00	167.0
73.10	1349.0
73.90	3865.0
75.10	12510.0
76.10	1448.0
76.90	186.0
77.80	91.0
78.90	532.0
79.80	131.0
80.10	135.0
80.80	601.0
81.70	131.0
86.90	761.0
88.00	622.0
90.80	162.0
91.90	870.0
93.10	799.0
94.00	3430.0
95.10	24080.0
96.00	1593.0
104.00	132.0
106.00	186.0
115.80	106.0
117.00	213.0
117.90	153.0
118.80	124.0
127.90	225.0
128.90	134.0
130.00	281.0
135.20	107.0
140.00	89.0
141.00	352.0
142.10	60.0
142.90	401.0
145.90	97.0
154.00	63.0
156.80	55.0
172.20	224.0
173.00	411.0
174.00	19296.0
175.00	1222.0
176.00	18616.0
177.10	1070.0
194.10	76.0
280.40	81.0

Instrument :
MSVOA_X
ClientSampleId :
BFB609