

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110122\
Data File : VX032515.D
Acq On : 01 Nov 2022 15:58
Operator : JC/MD
Sample : N5390-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	694	705	722	rBV	76598	223319	35.10%	6.502%
2	5.556	722	733	746	rVV	128230	366239	57.56%	10.662%
3	5.958	788	799	815	rBV	82825	221827	34.87%	6.458%
4	6.763	921	931	945	rBV	197430	474163	74.53%	13.804%
5	8.647	1234	1240	1255	rBV	401161	636219	100.00%	18.522%
6	10.055	1465	1471	1481	rBV	408010	545135	85.68%	15.871%
7	11.079	1634	1639	1650	rBV	365689	465513	73.17%	13.553%
8	12.024	1788	1794	1803	rBV	395415	502443	78.97%	14.628%




Sum of corrected areas: 3434858

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110122\
Data File : VX032515.D
Acq On : 01 Nov 2022 15:58
Operator : JC/MD
Sample : N5390-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

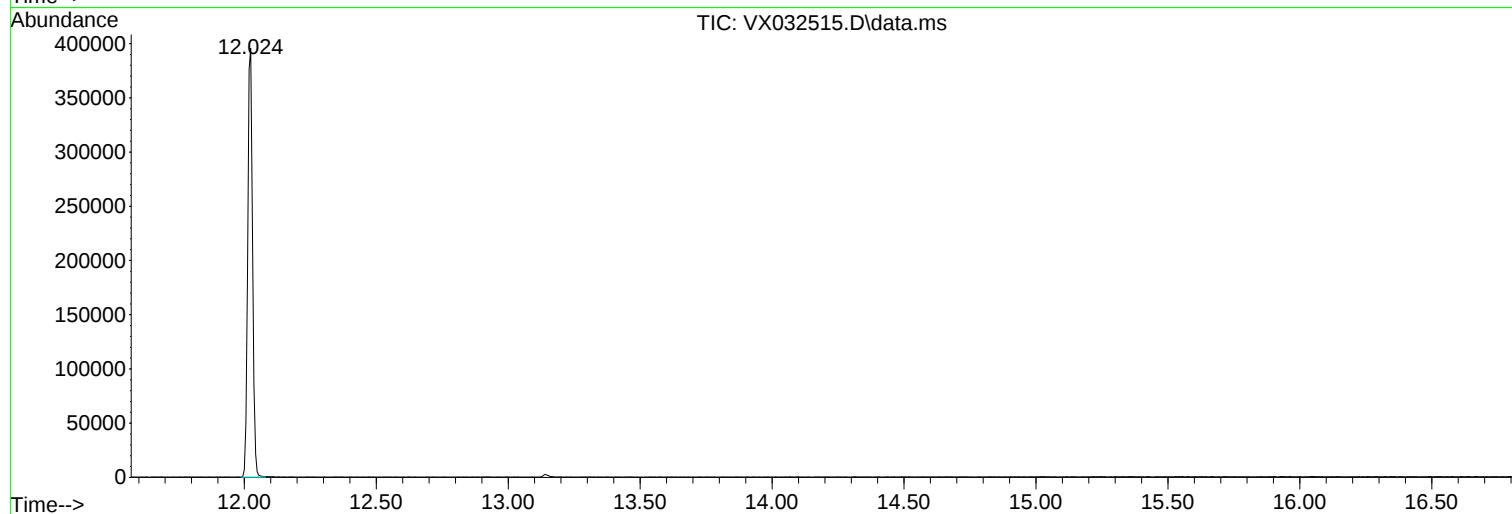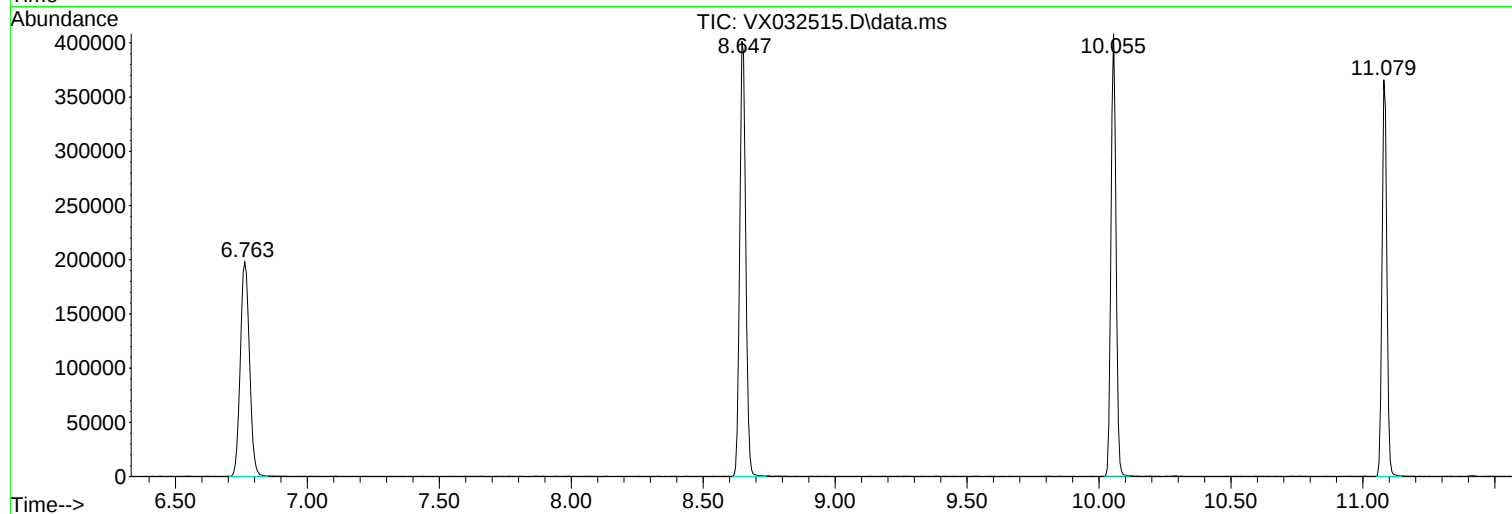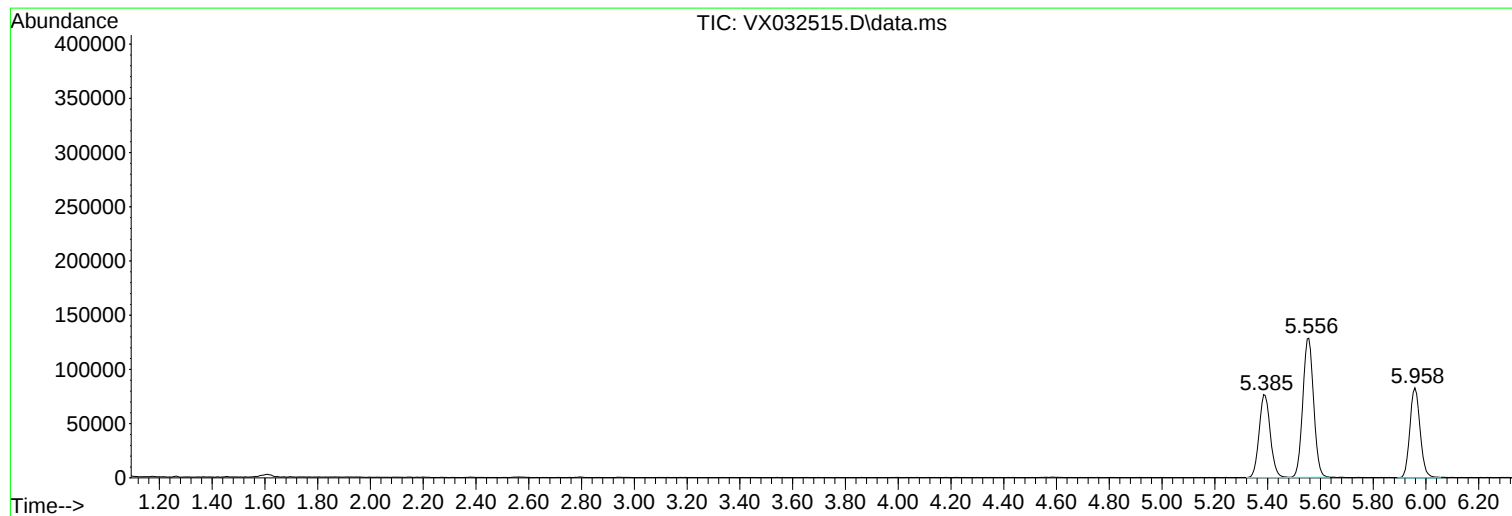

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110122\
Data File : VX032515.D
Acq On : 01 Nov 2022 15:58
Operator : JC/MD
Sample : N5390-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110122\
Data File : VX032515.D
Acq On : 01 Nov 2022 15:58
Operator : JC/MD
Sample : N5390-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc