

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110122\
Data File : VX032517.D
Acq On : 01 Nov 2022 16:45
Operator : JC/MD
Sample : N4955-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032517.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.391	693	706	721	rBV	69084	204137	38.50%	6.846%
2	5.556	721	733	747	rVB	115689	325371	61.36%	10.912%
3	5.958	789	799	813	rBV2	72741	195747	36.91%	6.565%
4	6.763	921	931	947	rBV	170243	408790	77.09%	13.709%
5	8.653	1234	1241	1249	rBV	333075	530275	100.00%	17.784%
6	10.055	1465	1471	1482	rBV	361520	474326	89.45%	15.907%
7	11.079	1634	1639	1651	rBV	291562	384237	72.46%	12.886%
8	12.024	1789	1794	1804	rBV	369506	458922	86.54%	15.391%




Sum of corrected areas: 2981805

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110122\
Data File : VX032517.D
Acq On : 01 Nov 2022 16:45
Operator : JC/MD
Sample : N4955-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

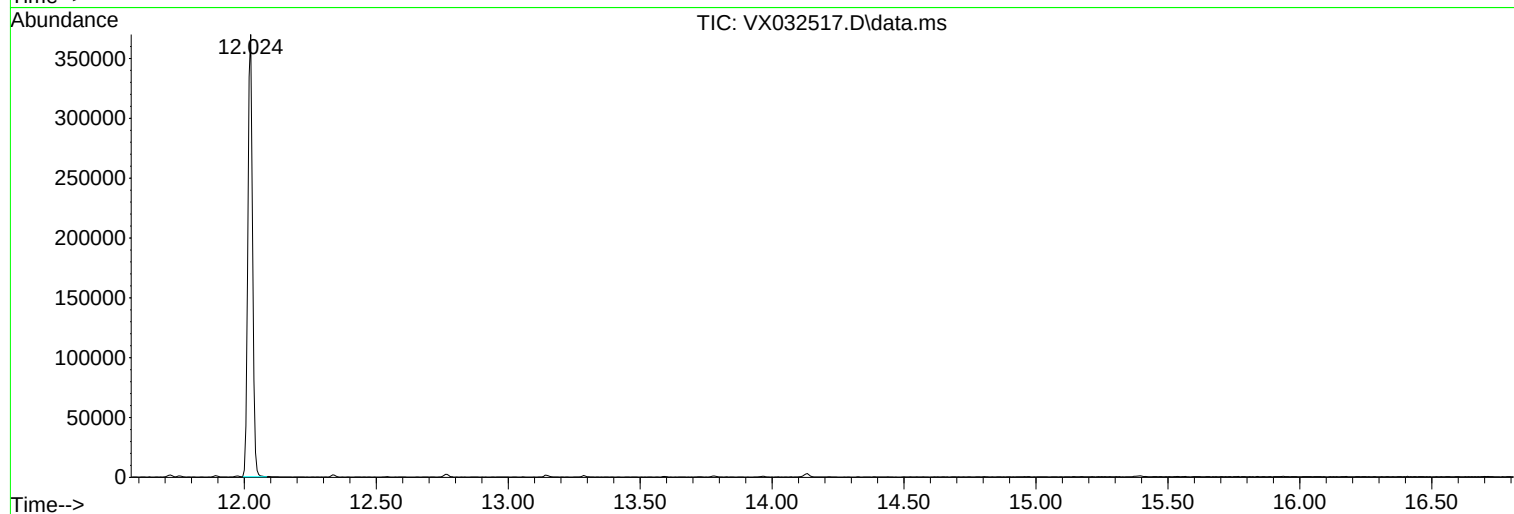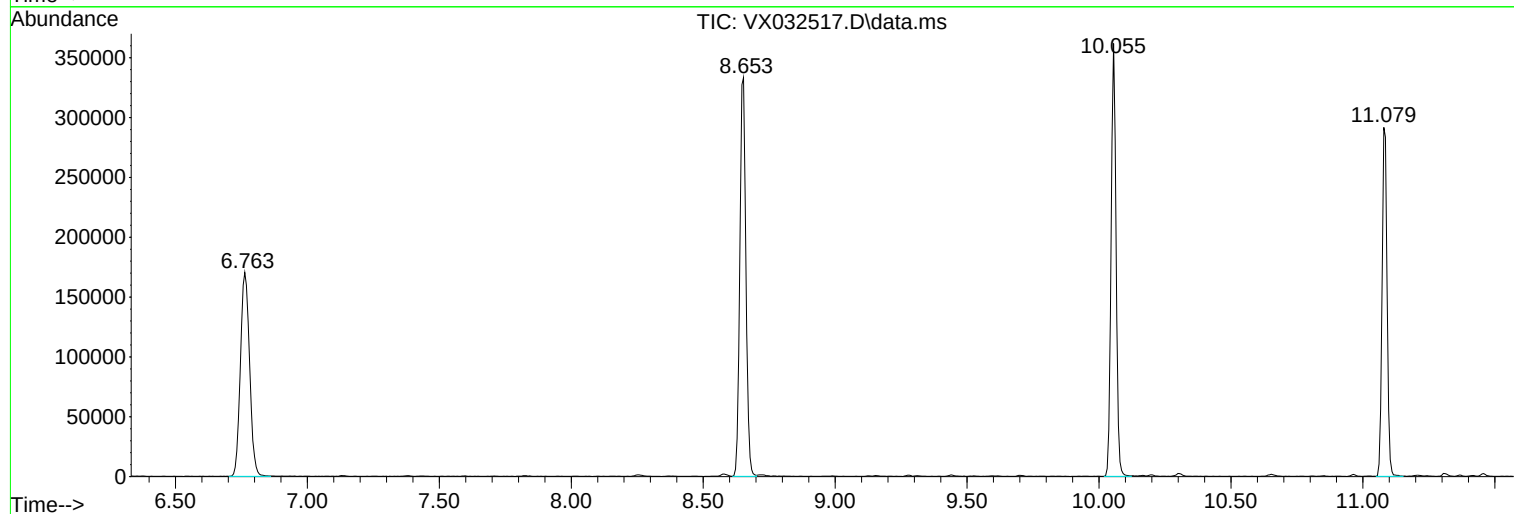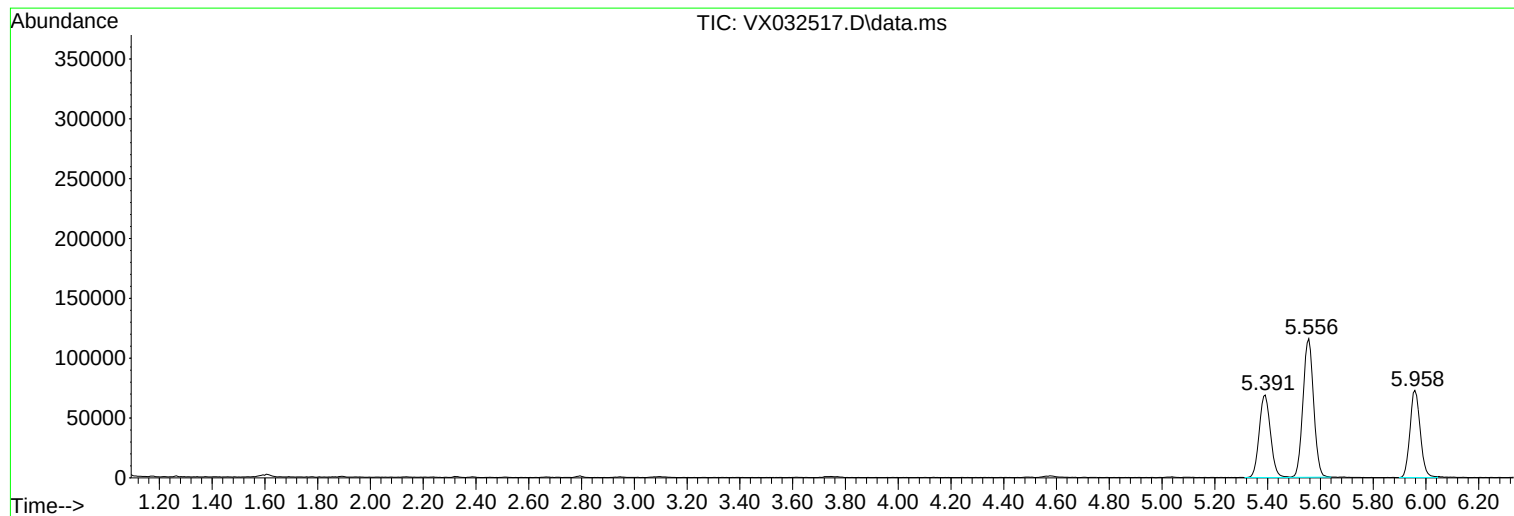

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110122\
Data File : VX032517.D
Acq On : 01 Nov 2022 16:45
Operator : JC/MD
Sample : N4955-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110122\
Data File : VX032517.D
Acq On : 01 Nov 2022 16:45
Operator : JC/MD
Sample : N4955-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------