


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX110220\
 Data File : VX019203.D
 Acq On : 02 Nov 2020 09:16
 Operator : JC/MD
 Sample : BFB64
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB64

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM110220WMA.M
 Title : VOC Analysis
 Last Update : Wed Nov 04 01:20:42 2020

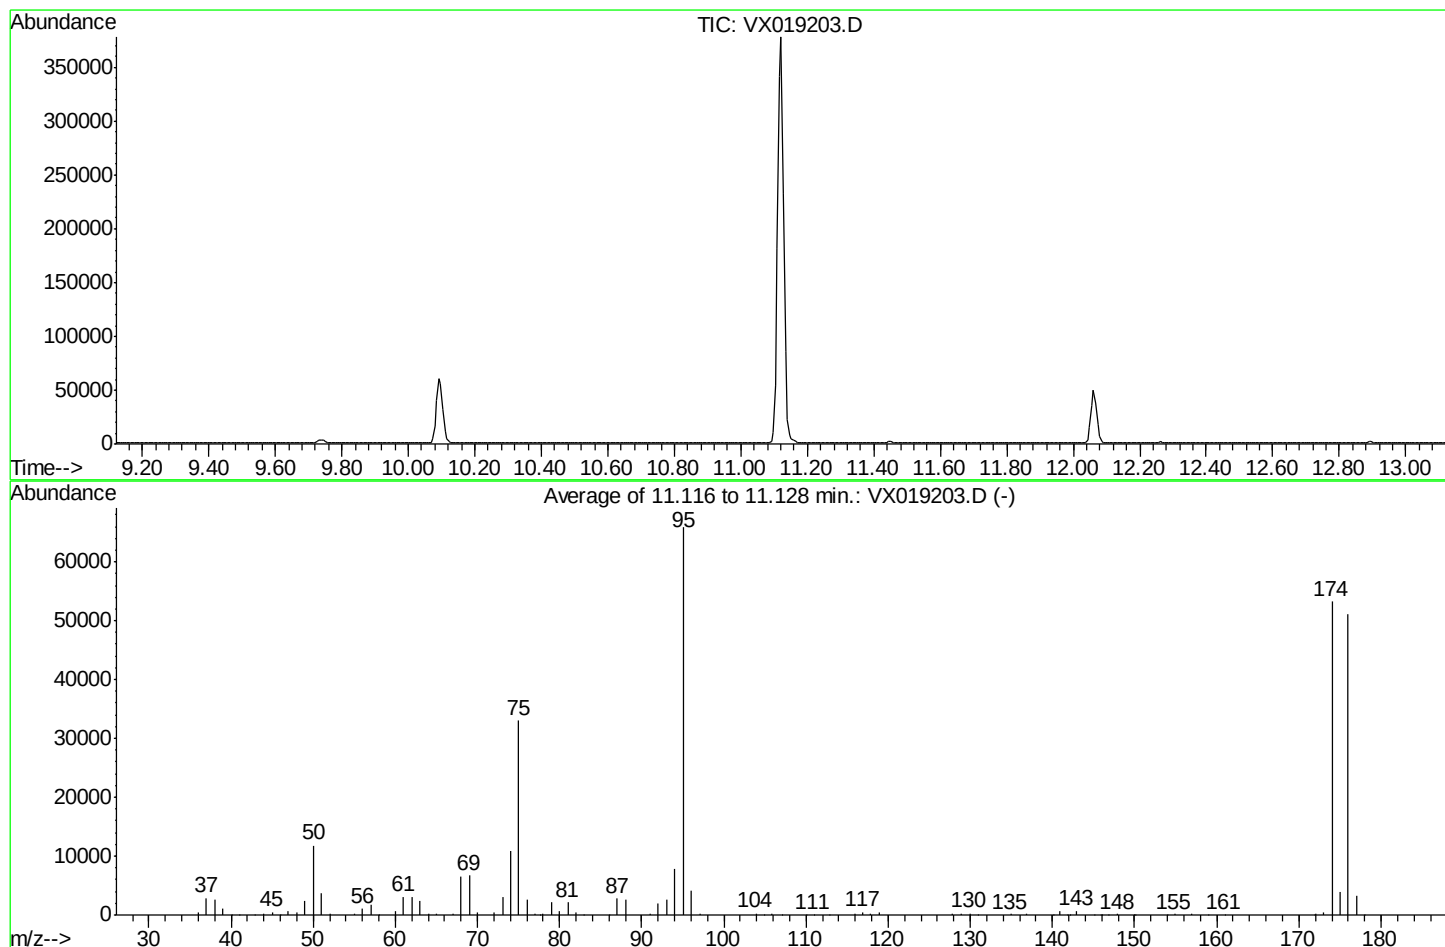

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	11829	PASS
75	95	30	80	50.0	32952	PASS
95	95	100	100	100.0	65861	PASS
96	95	5	9	6.3	4153	PASS
173	174	0.00	2	0.9	465	PASS
174	95	50	120	80.8	53218	PASS
175	174	5	9	7.2	3845	PASS
176	174	95	101	96.2	51189	PASS
177	176	5	9	6.4	3278	PASS

m/z	Abundance
36.10	586.0
37.00	3631.0
38.00	3164.0
39.00	1362.0
40.00	217.0
41.00	86.0
43.00	106.0
44.00	1023.0
45.00	572.0
45.90	82.0
46.90	793.0
47.90	367.0
49.00	3054.0
50.00	14392.0
51.00	4478.0
52.10	164.0
55.00	256.0
56.00	1286.0
57.00	2021.0
58.10	114.0
60.00	698.0
61.00	3494.0
62.10	3491.0
63.10	2658.0
64.00	223.0
65.10	231.0
67.10	219.0
68.00	7664.0
69.00	7794.0
70.00	553.0
72.00	453.0
73.00	3541.0
74.00	12666.0
75.00	38152.0
76.10	3260.0
77.10	390.0
77.90	384.0
79.00	2330.0
79.90	788.0
81.00	2358.0
82.00	585.0
82.90	80.0
86.10	99.0
87.00	3277.0
88.10	2817.0
90.90	277.0
92.00	2181.0
93.00	3118.0
94.00	8619.0
95.10	72208.0
96.00	4673.0
97.10	190.0
104.00	357.0
105.00	112.0
105.80	322.0
107.00	74.0
110.90	74.0
112.90	71.0
116.00	314.0
117.00	499.0
117.90	294.0
118.90	491.0
127.80	256.0
129.00	119.0
130.00	229.0
131.00	124.0
134.90	189.0
136.90	146.0
140.10	107.0
141.00	761.0
141.80	63.0
142.90	728.0
145.10	78.0
145.90	108.0
146.80	52.0
148.00	121.0
154.90	164.0
157.00	171.0
158.90	68.0
160.90	95.0
171.90	258.0
172.10	254.0
173.00	435.0
174.00	51776.0
175.00	3943.0
176.00	47368.0
177.00	3351.0
177.90	93.0
207.10	116.0

Instrument :
MSVOA_X
ClientSampleId :
BFB64

Scan 1639 (11.079 min): VX019203.D
BFB64

m/z	Abundance
40.00	170.0
41.00	72.0
41.20	72.0
44.00	590.0
207.20	119.0
281.20	87.0

Instrument :
MSVOA_X
ClientSampleId :
BFB64

m/z	Abundance
36.10	272.0
37.00	1643.0
38.00	1739.0
39.00	666.0
40.00	256.0
40.90	54.0
42.80	107.0
44.00	611.0
45.00	375.0
46.10	56.0
47.00	429.0
47.90	185.0
49.00	1552.0
50.00	7295.0
51.00	2344.0
52.00	75.0
55.20	100.0
56.10	609.0
57.00	1142.0
60.00	429.0
61.00	2050.0
62.00	2011.0
63.00	1586.0
63.90	137.0
64.90	121.0
67.00	158.0
68.00	4656.0
69.10	4618.0
70.10	327.0
72.00	228.0
73.00	2010.0
74.00	7273.0
75.10	22160.0
76.00	1844.0
77.00	279.0
77.80	147.0
79.00	1552.0
79.90	444.0
80.90	1434.0
81.90	411.0
82.80	57.0
86.00	76.0
87.00	1775.0
87.90	1737.0
91.00	195.0
92.10	1398.0
93.10	1896.0
94.10	5678.0
95.10	46888.0
96.00	3007.0
97.00	115.0
103.90	263.0
104.80	92.0
105.90	196.0
115.80	178.0
117.00	385.0
117.90	219.0
118.90	332.0
127.90	166.0
129.00	76.0
129.80	221.0
130.90	103.0
134.90	106.0
136.90	74.0
140.90	561.0
142.10	56.0
143.00	594.0
146.10	72.0
146.80	51.0
147.90	131.0
150.10	68.0
154.80	120.0
157.10	82.0
161.00	60.0
172.00	245.0
173.10	406.0
174.00	43592.0
175.00	3110.0
176.00	43344.0
177.00	2406.0
178.00	86.0
207.10	91.0
281.10	52.0

Instrument :
MSVOA_X
ClientSampleId :
BFB64

m/z	Abundance
36.00	635.0
37.00	3258.0
38.00	3141.0
39.00	1251.0
40.00	288.0
40.90	85.0
42.90	59.0
44.00	1085.0
45.00	643.0
46.00	75.0
47.00	870.0
48.00	483.0
49.00	2859.0
50.10	13802.0
51.00	4352.0
52.10	218.0
55.10	216.0
56.00	1154.0
57.00	2036.0
58.00	124.0
60.00	819.0
61.00	3922.0
62.10	3614.0
63.00	2662.0
64.10	340.0
65.10	176.0
67.00	220.0
68.00	7351.0
69.00	7619.0
70.10	737.0
72.00	459.0
73.10	3411.0
74.00	12854.0
75.10	38544.0
76.10	3004.0
77.00	335.0
77.60	244.0
78.00	252.0
79.00	2611.0
79.90	810.0
81.00	2470.0
82.00	606.0
83.00	64.0
86.00	82.0
87.00	3289.0
88.00	3191.0
90.90	280.0
92.00	2254.0
93.10	3078.0
94.00	9102.0
95.10	78488.0
96.10	4781.0
97.00	214.0
103.80	369.0
104.90	117.0
105.80	346.0
107.00	73.0
110.00	53.0
110.90	68.0
112.90	64.0
116.00	282.0
116.90	513.0
117.90	343.0
119.00	476.0
127.90	283.0
128.90	242.0
130.00	316.0
131.00	54.0
134.90	169.0
136.90	151.0
140.00	62.0
141.00	787.0
141.90	127.0
143.00	844.0
145.00	87.0
145.90	126.0
148.00	226.0
149.90	100.0
154.00	61.0
154.90	150.0
157.00	155.0
158.90	83.0
161.00	131.0
172.10	297.0
173.10	556.0
174.00	64288.0
175.00	4484.0
176.00	62856.0
177.00	4079.0
178.00	135.0
207.00	113.0
281.20	55.0

Instrument :
MSVOA_X
ClientSampleId :
BFB64