

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110221\
 Data File : VX025041.D
 Acq On : 02 Nov 2021 10:40
 Operator : JC/MD
 Sample : VX1102WBL01
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK610

Quant Time: Nov 03 00:54:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 03 00:53:58 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	82883	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	76592	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	34991	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	14759	6.065	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 121.400%		
7) Chloroethane-d5	1.672	69	11815	5.389	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 107.800%		
11) 1,1-Dichloroethene-d2	2.313	63	30358	3.347	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 67.000%		
20) 2-Butanone-d5	4.477	46	52218	58.696	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 117.400%		
24) Chloroform-d	5.056	84	50118	4.278	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 85.600%		
26) 1,2-Dichloroethane-d4	5.958	65	27466	4.290	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 85.800%		
32) Benzene-d6	5.977	84	81619	4.573	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 91.400%		
36) 1,2-Dichloropropane-d6	7.312	67	27126	4.764	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 95.200%		
41) Toluene-d8	8.647	98	79536	4.445	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 89.000%		
43) trans-1,3-Dichloroprop...	8.952	79	12957	4.958	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 99.200%		
46) 2-Hexanone-d5	9.384	63	43752	46.519	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 93.040%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	19097	4.388	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 87.800%		
66) 1,2-Dichlorobenzene-d4	12.323	152	26954	4.571	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 91.400%		
Target Compounds						
16) Methylene chloride	2.788	84	2472	0.418	ug/L	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110221\
Data File : VX025041.D
Acq On : 02 Nov 2021 10:40
Operator : JC/MD
Sample : VX1102WBL01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK610


Quant Time: Nov 03 00:54:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 03 00:53:58 2021
Response via : Initial Calibration

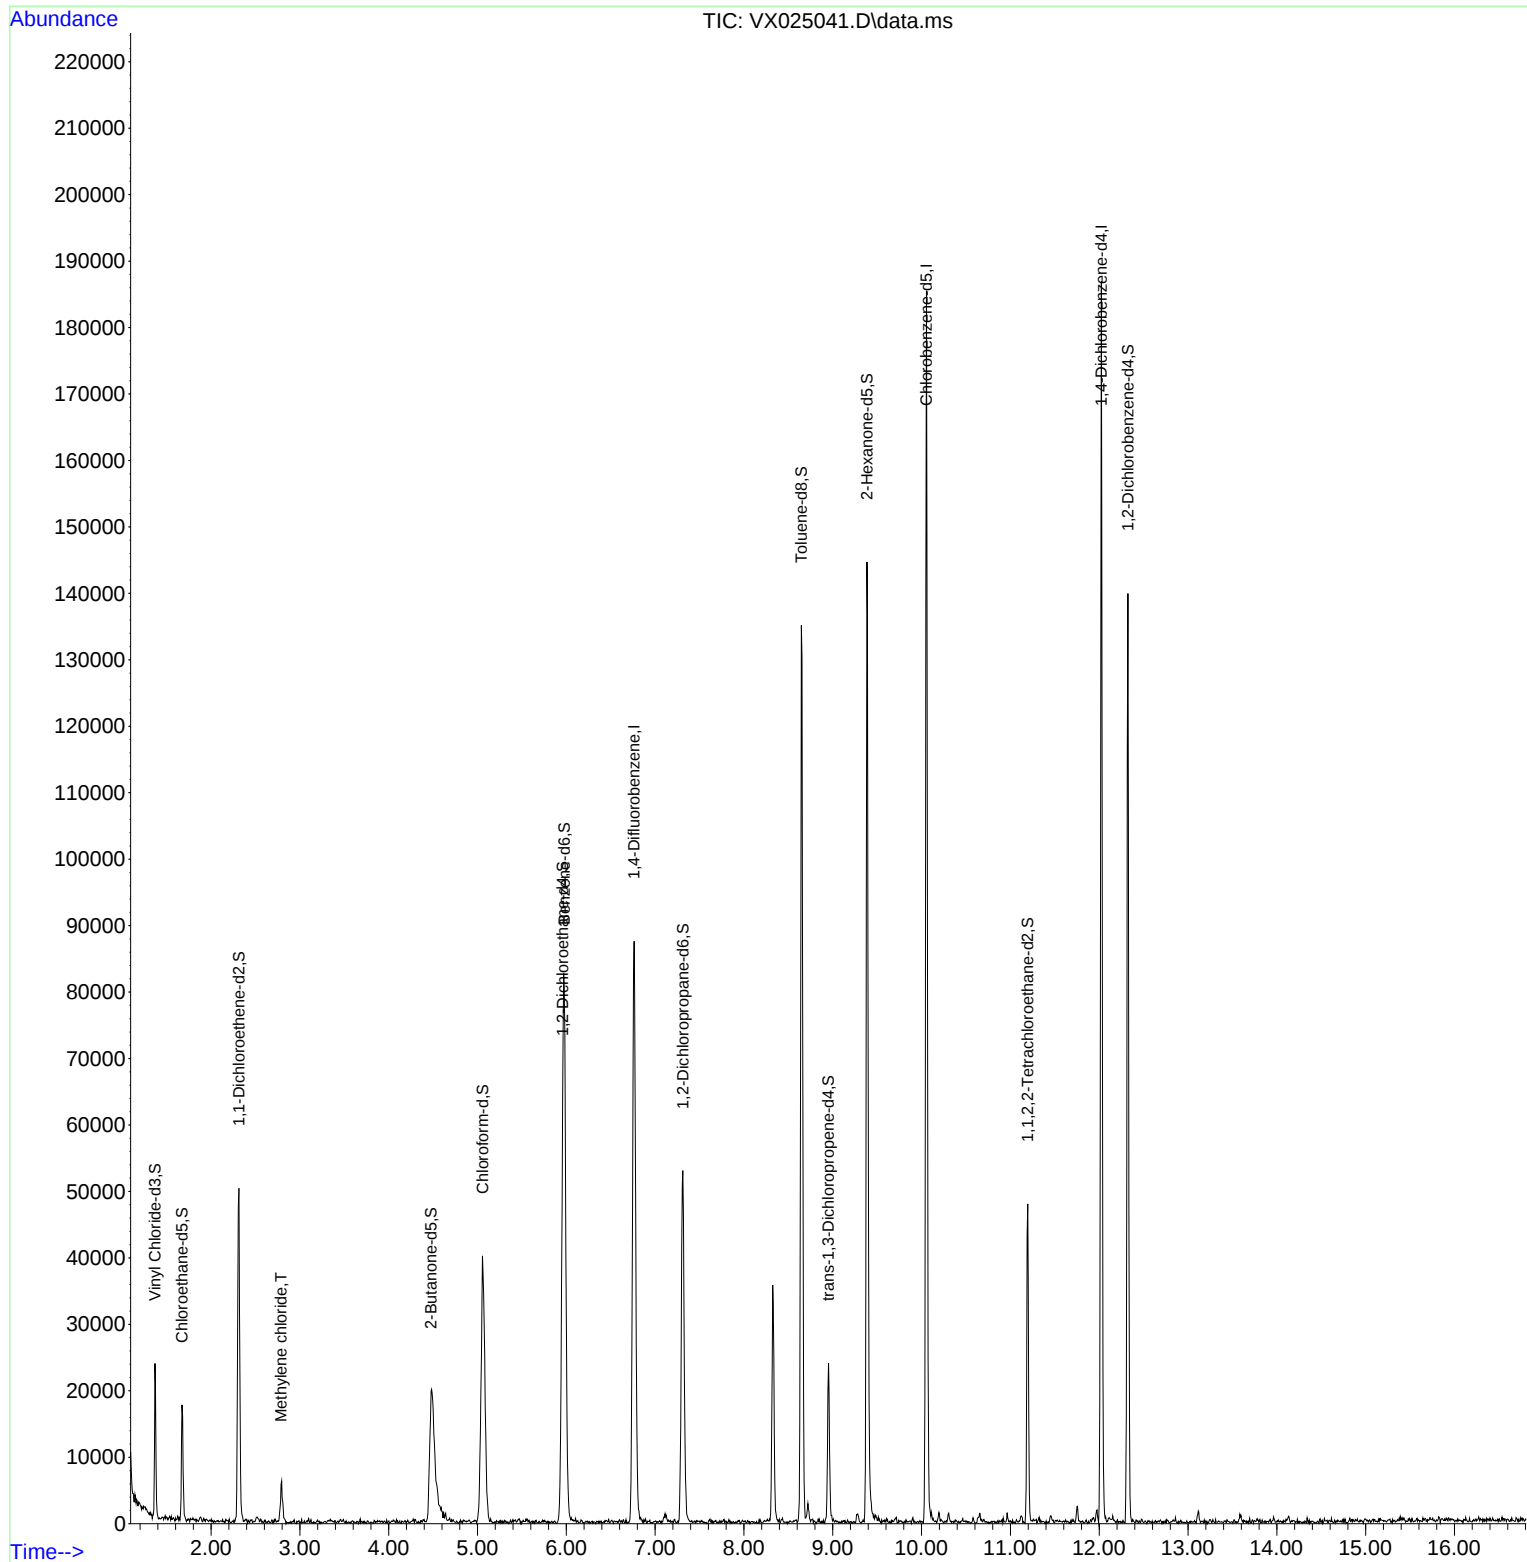

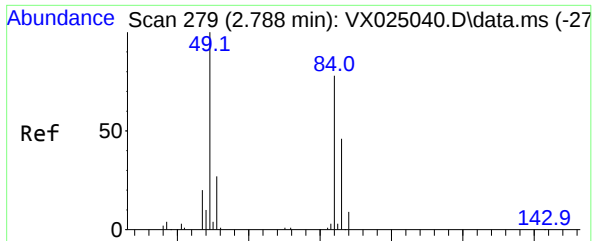

#16
Methylene chloride
Concen: 0.418 ug/L
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX025041.D
Acq: 02 Nov 2021 10:40

Instrument :
MSVOA_X
ClientSampleId :
VBLK610

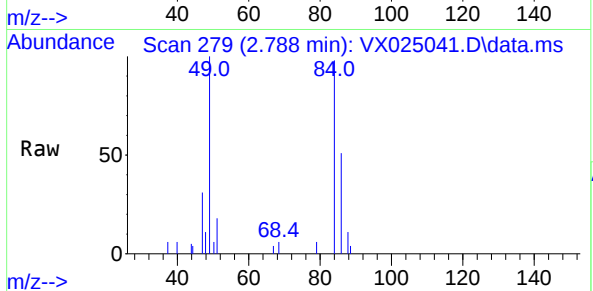

Tgt Ion: 84 Resp: 2472

Ion	Ratio	Lower	Upper
84	100		
86	51.5	49.5	91.9
49	101.8	62.7	116.5

