

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110221\
 Data File : VX025042.D
 Acq On : 02 Nov 2021 11:13
 Operator : JC/MD
 Sample : VX1102WBL02
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK611

Quant Time: Nov 03 00:54:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 03 00:53:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	77997	5.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	69901	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	31963	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	14723	6.430	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	128.600%
7) Chloroethane-d5	1.672	69	12393	6.007	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	120.200%
11) 1,1-Dichloroethene-d2	2.307	63	31869	3.734	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.600%
20) 2-Butanone-d5	4.489	46	50507	60.330	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.660%
24) Chloroform-d	5.062	84	51659	4.686	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.800%
26) 1,2-Dichloroethane-d4	5.964	65	28088	4.662	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%
32) Benzene-d6	5.977	84	82178	5.046	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.000%
36) 1,2-Dichloropropane-d6	7.312	67	26092	5.021	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.400%
41) Toluene-d8	8.647	98	80415	4.924	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%
43) trans-1,3-Dichloroprop...	8.952	79	11332	4.751	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.000%
46) 2-Hexanone-d5	9.391	63	43146	50.265	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.540%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	18915	4.763	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.200%
66) 1,2-Dichlorobenzene-d4	12.323	152	26850	4.985	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.600%
Target Compounds						Qvalue
16) Methylene chloride	2.794	84	1469	0.264	ug/L	# 75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110221\
Data File : VX025042.D
Acq On : 02 Nov 2021 11:13
Operator : JC/MD
Sample : VX1102WBL02
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK611


Quant Time: Nov 03 00:54:48 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 03 00:53:58 2021
Response via : Initial Calibration

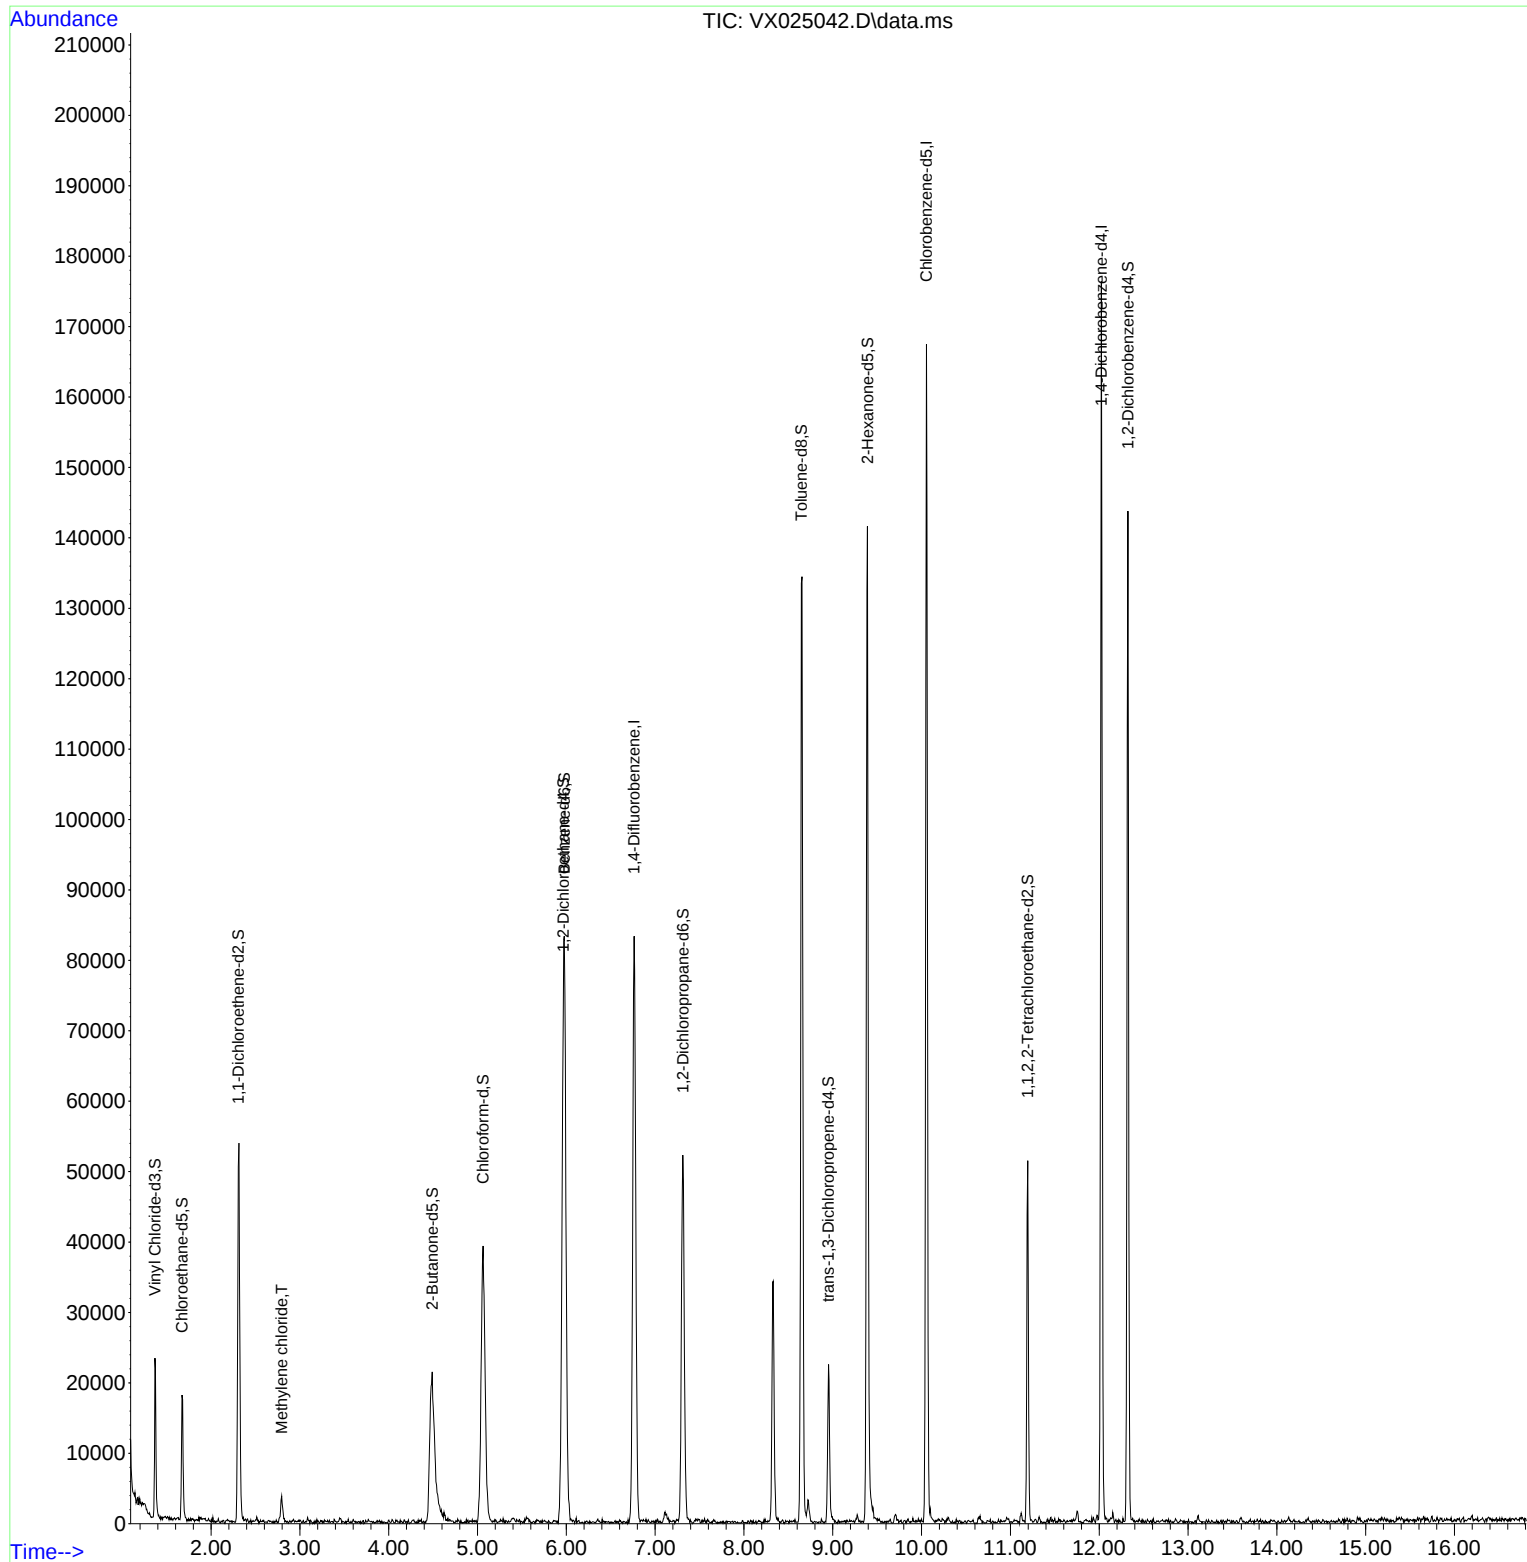

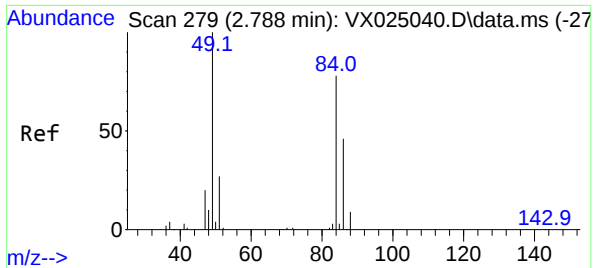

#16
Methylene chloride
Concen: 0.264 ug/L
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX025042.D
Acq: 02 Nov 2021 11:13

Instrument :
MSVOA_X
ClientSampleId :
VBLK611

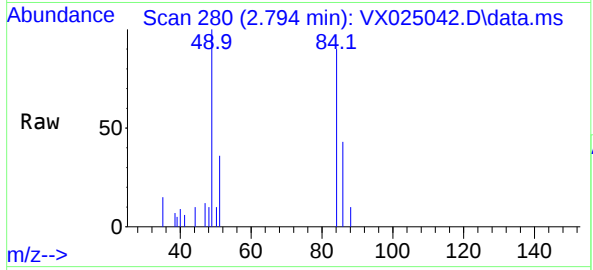

Tgt Ion: 84 Resp: 1469
Ion Ratio Lower Upper
84 100
86 47.7 49.5 91.9#
49 111.1 62.7 116.5

