

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110221\
 Data File : VX025043.D
 Acq On : 02 Nov 2021 12:01
 Operator : JC/MD
 Sample : VX1102WBL03
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK612

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VX0250MB.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	53	rVB	23169	23513	9.84%	1.123%
2	1.673	93	96	102	rVB	17923	21788	9.12%	1.041%
3	2.313	193	201	212	rBV	46841	76482	32.01%	3.653%
4	2.794	272	280	285	rBV4	2617	5596	2.34%	0.267%
5	4.489	547	558	570	rBV2	19637	74891	31.35%	3.577%
6	4.568	570	571	576	rVV4	2408	3418	1.43%	0.163%
7	5.068	642	653	667	rBV2	37013	112615	47.14%	5.379%
8	5.977	792	802	813	rBV2	79151	233762	97.85%	11.166%
9	6.763	923	931	943	rVB	83004	202597	84.80%	9.678%
10	7.117	983	989	994	rBV3	1589	3180	1.33%	0.152%
11	7.312	1011	1021	1032	rBV	50531	110601	46.30%	5.283%
12	8.330	1180	1188	1199	rBV	33566	56474	23.64%	2.698%
13	8.653	1232	1241	1248	rBV	138056	206884	86.60%	9.882%
14	8.726	1248	1253	1256	rVB3	1932	3434	1.44%	0.164%
15	8.952	1284	1290	1297	rBV2	22655	32792	13.73%	1.566%
16	9.391	1356	1362	1375	rBV	140449	211444	88.51%	10.100%
17	10.055	1465	1471	1483	rBV	170271	238900	100.00%	11.412%
18	11.195	1652	1658	1664	rBV	48128	64620	27.05%	3.087%
19	12.024	1789	1794	1803	rVB	182505	232970	97.52%	11.128%
20	12.323	1836	1843	1850	rBV	142342	177504	74.30%	8.479%




Sum of corrected areas: 2093465

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110221\
Data File : VX025043.D
Acq On : 02 Nov 2021 12:01
Operator : JC/MD
Sample : VX1102WBL03
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

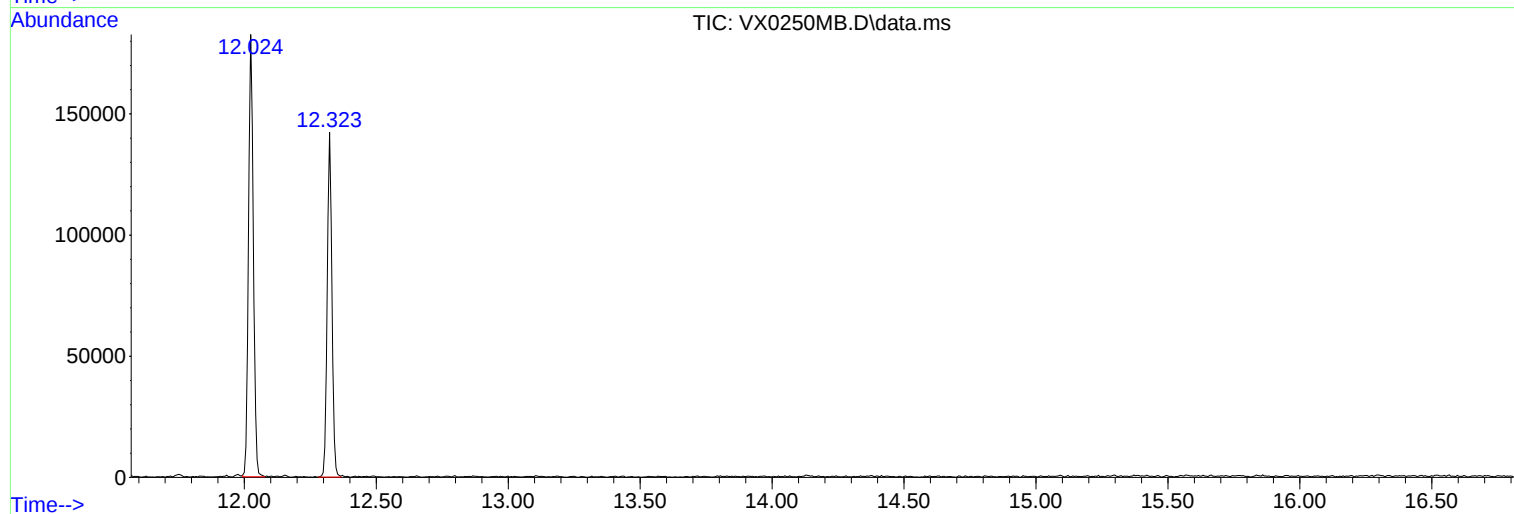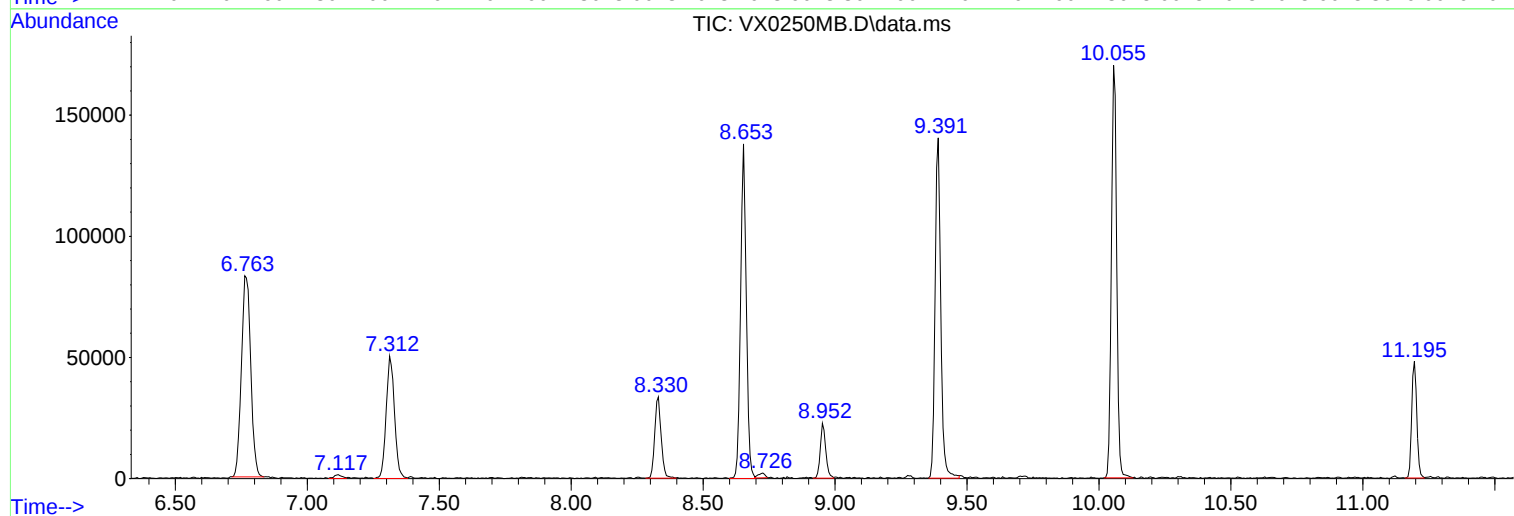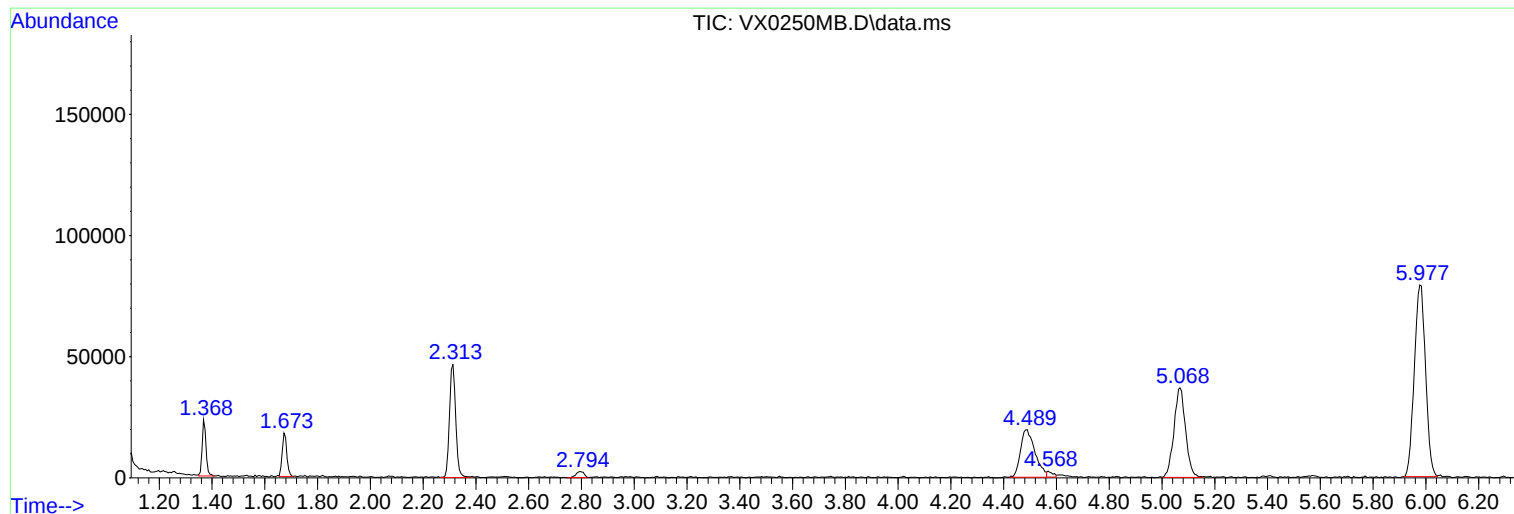

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110221\
Data File : VX025043.D
Acq On : 02 Nov 2021 12:01
Operator : JC/MD
Sample : VX1102WBL03
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110221\
Data File : VX025043.D
Acq On : 02 Nov 2021 12:01
Operator : JC/MD
Sample : VX1102WBL03
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK612

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc