
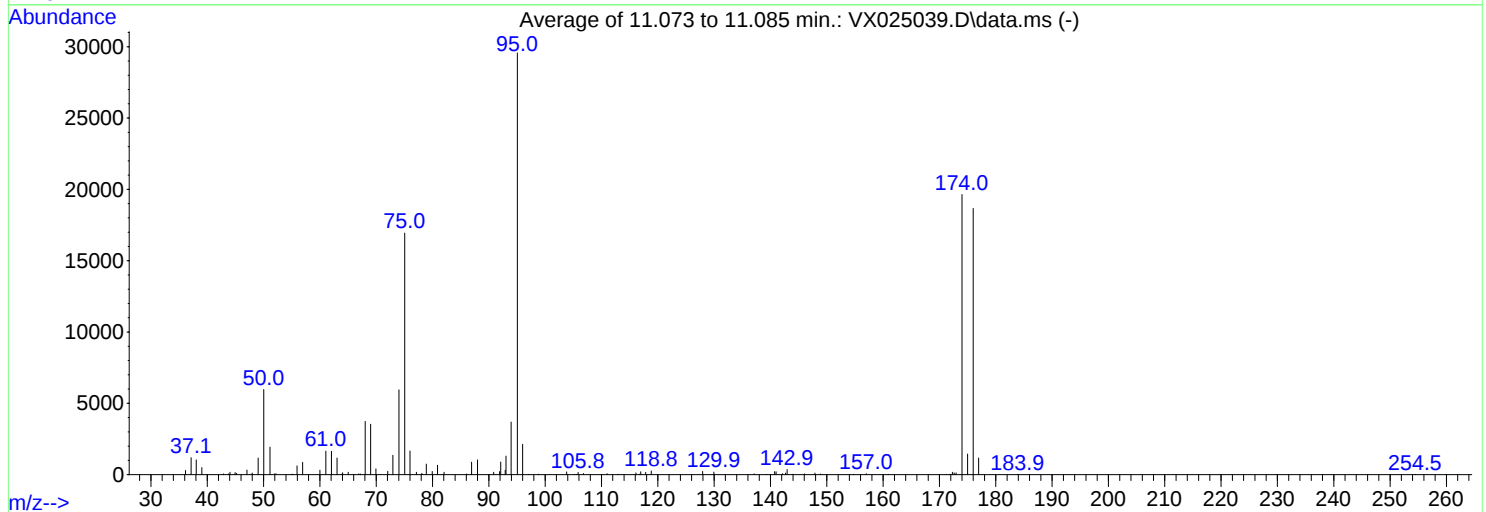


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110221\
 Data File : VX025039.D
 Acq On : 02 Nov 2021 08:27
 Operator : JC/MD
 Sample : BFB612
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB612

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR102221WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Nov 09 06:29:58 2021

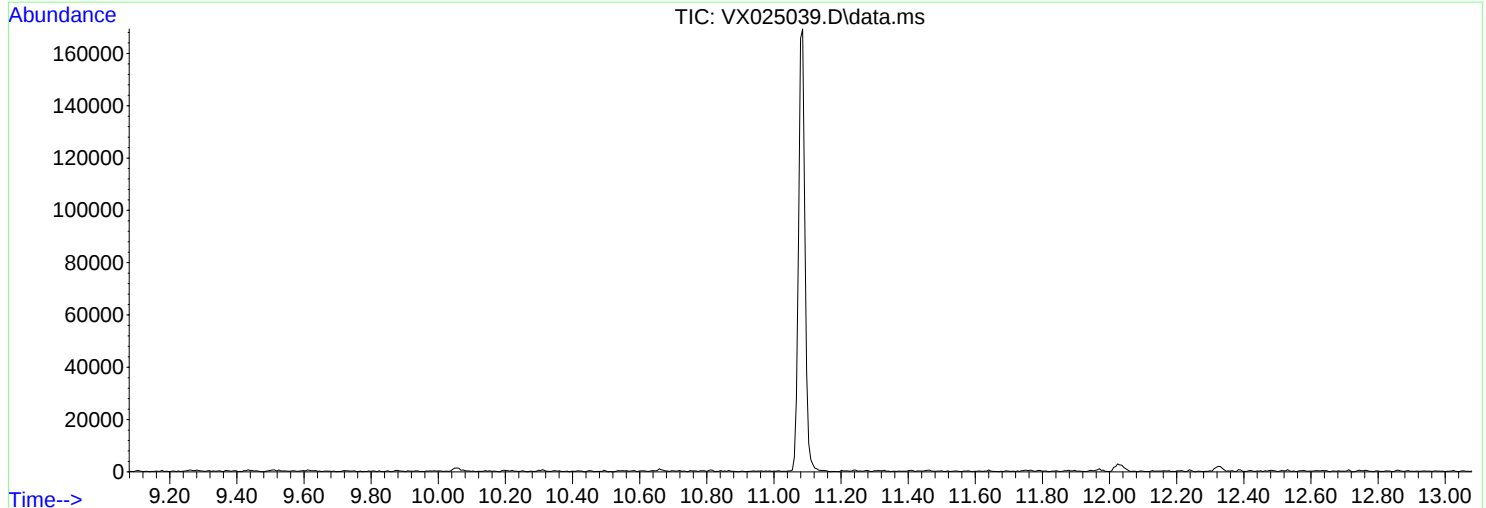

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	5966	PASS
75	95	30	80	57.3	16943	PASS
95	95	100	100	100.0	29571	PASS
96	95	5	9	7.2	2129	PASS
173	174	0.00	2	0.6	122	PASS
174	95	50	120	66.4	19643	PASS
175	174	5	9	7.3	1442	PASS
176	174	95	105	95.0	18665	PASS
177	176	5	10	6.2	1163	PASS