

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110222\
 Data File : VX032540.D
 Acq On : 02 Nov 2022 16:03
 Operator : JC/MD
 Sample : N5424-03DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 INF1122DL

Quant Time: Nov 03 03:13:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 08:28:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	121423	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	200266	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	178351	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	88572	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	82977	49.182	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	98.360%		
35) Dibromofluoromethane	5.385	113	64826	45.380	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	90.760%		
50) Toluene-d8	8.647	98	239688	48.253	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	96.500%		
62) 4-Bromofluorobenzene	11.079	95	93897	48.392	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	96.780%		
Target Compounds						Qvalue
11) Tert butyl alcohol	2.940	59	2172	8.845	ug/l #	72
13) Acrolein	2.215	56	429	1.750	ug/l #	1
15) Acrylonitrile	3.099	53	308	0.462	ug/l #	30
16) Acetone	2.380	43	445	0.726	ug/l #	45
18) Methyl Acetate	2.782	43	7864	3.944	ug/l #	51
20) Methylene Chloride	2.788	84	820	0.583	ug/l #	79
29) Tetrahydrofuran	5.190	42	387	0.639	ug/l #	31
30) Chloroform	5.172	83	571	0.215	ug/l #	18
31) Cyclohexane	5.477	56	7845	3.835	ug/l #	95
36) 1,1-Dichloropropene	5.556	75	9645	4.848	ug/l #	49
38) Carbon Tetrachloride	5.550	117	13015	5.899	ug/l #	16
39) Methylcyclohexane	7.379	83	3646	1.549	ug/l	93
40) Benzene	6.037	78	178596	31.726	ug/l	100
42) 1,2-Dichloroethane	6.025	62	2052	0.892	ug/l #	77
48) Methyl methacrylate	7.665	41	443	0.270	ug/l #	66
52) Toluene	8.720	92	17906	4.875	ug/l	99
58) 2-Chloroethyl Vinyl ether	8.147	63	231	0.216	ug/l #	46
67) Ethyl Benzene	10.195	91	116818	16.351	ug/l	99
68) m/p-Xylenes	10.305	106	144614	52.129	ug/l	99
69) o-Xylene	10.640	106	17957	6.658	ug/l	99
70) Styrene	10.640	104	994	0.222	ug/l #	1
73) Isopropylbenzene	10.963	105	16734	2.384	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	51911	26.344	ug/l #	37
78) n-propylbenzene	11.305	91	32398	4.006	ug/l	99
79) 2-Chlorotoluene	11.402	91	6936	1.432	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.451	105	30012	5.003	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	51911	83.827	ug/l #	6
82) 4-Chlorotoluene	11.451	91	3355	0.592	ug/l #	45
83) tert-Butylbenzene	11.756	119	12411	2.072	ug/l #	56
84) 1,2,4-Trimethylbenzene	11.750	105	104349	17.490	ug/l	98
85) sec-Butylbenzene	11.750	105	104349	14.481	ug/l #	57
89) n-Butylbenzene	12.317	91	2737	0.515	ug/l #	36
90) Hexachloroethane	12.646	117	3363	3.367	ug/l #	12
95) Naphthalene	13.774	128	49219	7.078	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110222\
Data File : VX032540.D
Acq On : 02 Nov 2022 16:03
Operator : JC/MD
Sample : N5424-03DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
INF1122DL

Quant Time: Nov 03 03:13:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 08:28:06 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110222\
 Data File : VX032540.D
 Acq On : 02 Nov 2022 16:03
 Operator : JC/MD
 Sample : N5424-03DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 INF1122DL

Quant Time: Nov 03 03:13:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 08:28:06 2022
 Response via : Initial Calibration




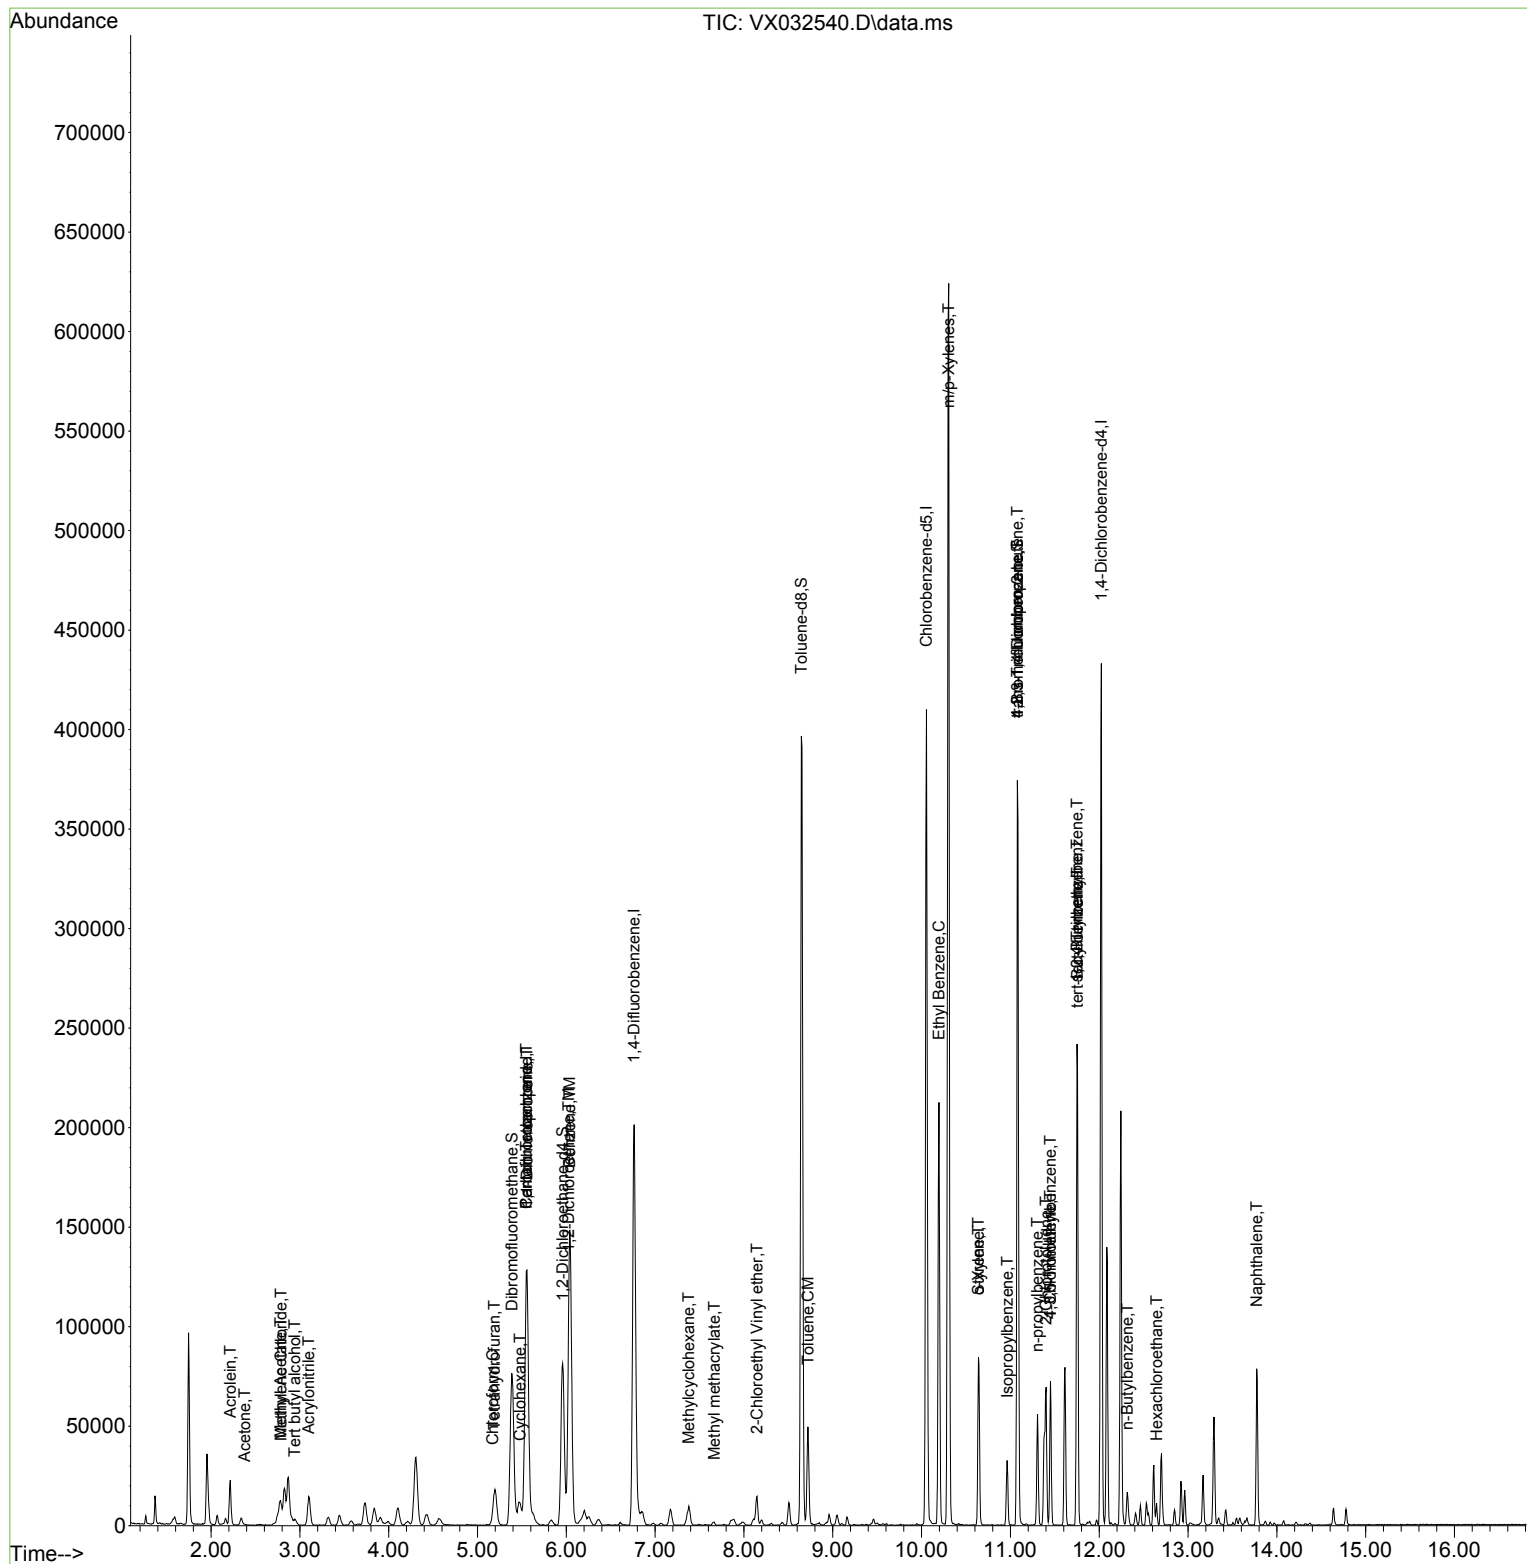


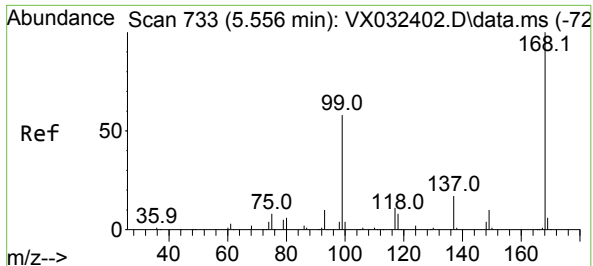

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03




Instrument :
MSVOA_X
ClientSampleId :
INF1122DL


Tgt Ion:168 Resp: 121423
Ion Ratio Lower Upper
168 100
99 57.3 46.1 69.1

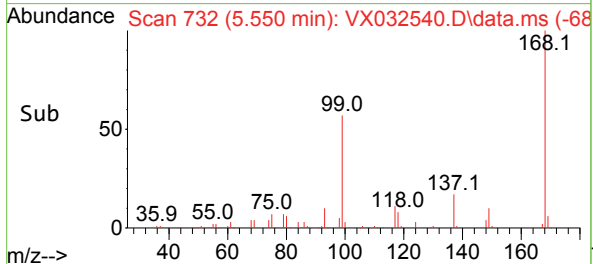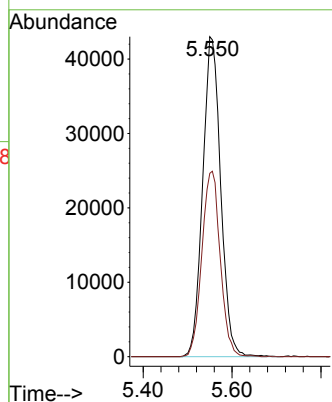

#11
Tert butyl alcohol
Concen: 8.845 ug/l
RT: 2.940 min Scan# 304
Delta R.T. -0.024 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Tgt Ion: 59 Resp: 2172
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#


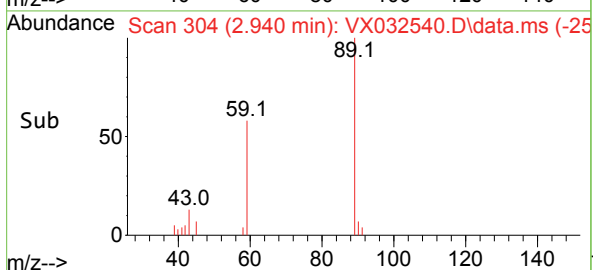

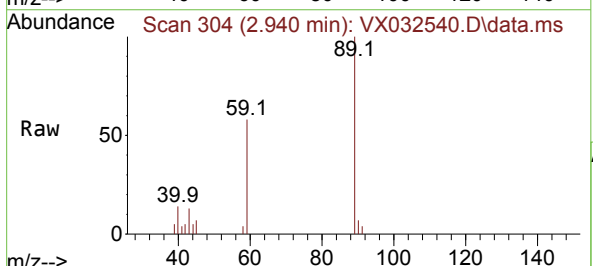


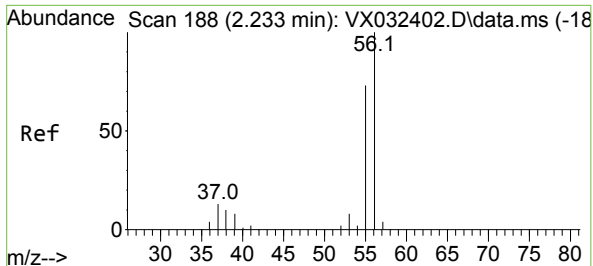

#13
Acrolein
Concen: 1.750 ug/l
RT: 2.215 min Scan# 11
Delta R.T. -0.018 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03




Instrument :
MSVOA_X
ClientSampleId :
INF1122DL


Tgt Ion: 56 Resp: 429
Ion Ratio Lower Upper
56 100
55 2516.8 56.9 85.3#

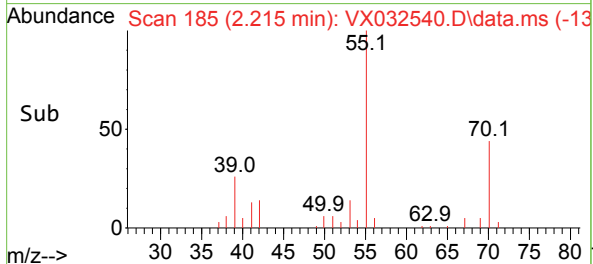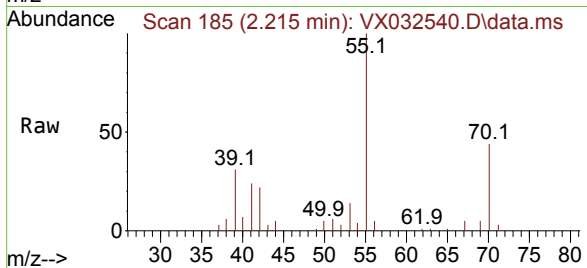

#15
Acrylonitrile
Concen: 0.462 ug/l
RT: 3.099 min Scan# 330
Delta R.T. 0.037 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Tgt Ion: 53 Resp: 308
Ion Ratio Lower Upper
53 100
52 0.0 67.4 101.0#
51 50.3 30.3 45.5#


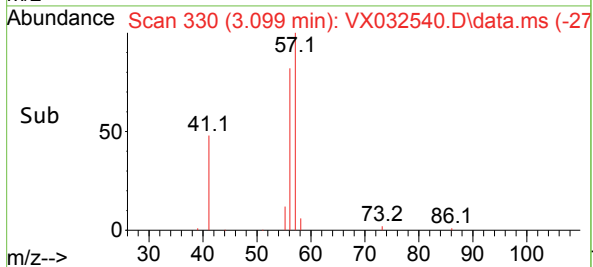

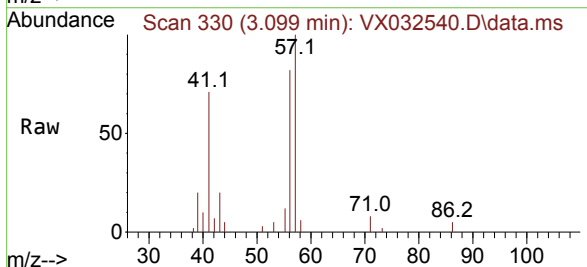




#16
Acetone
Concen: 0.726 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03




Instrument :
MSVOA_X
ClientSampleId :
INF1122DL


Tgt Ion: 43 Resp: 445
Ion Ratio Lower Upper
43 100
58 0.0 23.8 35.8#



#18
Methyl Acetate
Concen: 3.944 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.079 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Tgt Ion: 43 Resp: 7864
Ion Ratio Lower Upper
43 100
74 0.0 19.4 29.0#


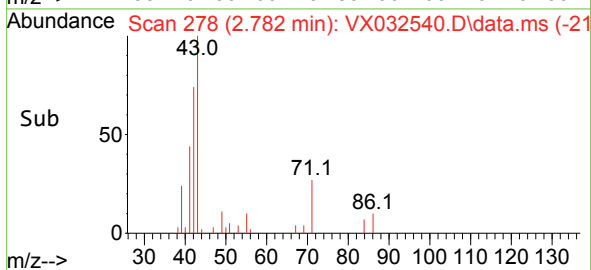






#20
Methylene Chloride
Concen: 0.583 ug/l
RT: 2.788 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03




Instrument :
MSVOA_X
ClientSampleId :
INF1122DL


Tgt Ion:	84	Resp:	820
Ion	Ratio	Lower	Upper
84	100		
49	105.6	101.0	151.6
51	15.7	31.1	46.7#
86	52.7	52.3	78.5



#29
Tetrahydrofuran
Concen: 0.639 ug/l
RT: 5.190 min Scan# 673
Delta R.T. 0.189 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Tgt Ion:	42	Resp:	387
Ion	Ratio	Lower	Upper
42	100		
72	0.0	37.6	56.4#
71	0.0	34.7	52.1#


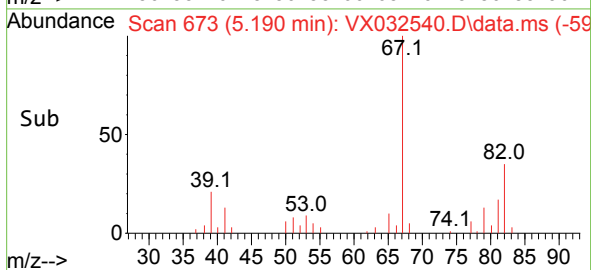




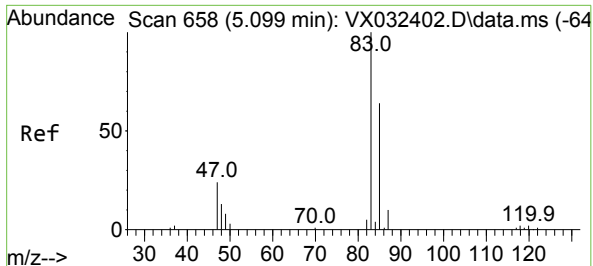

#30
Chloroform
Concen: 0.215 ug/l
RT: 5.172 min Scan# 61
Delta R.T. 0.073 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03




Instrument :
MSVOA_X
ClientSampleId :
INF1122DL


Tgt Ion: 83 Resp: 571
Ion Ratio Lower Upper
83 100
85 0.0 51.1 76.7#

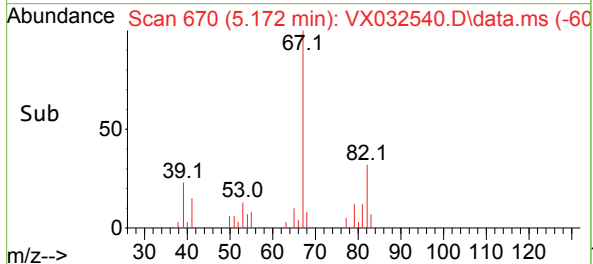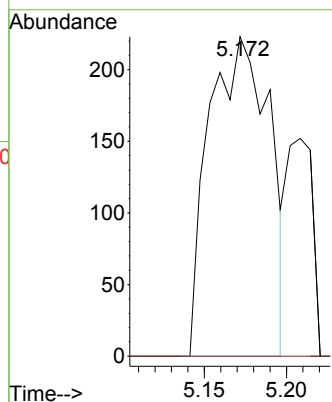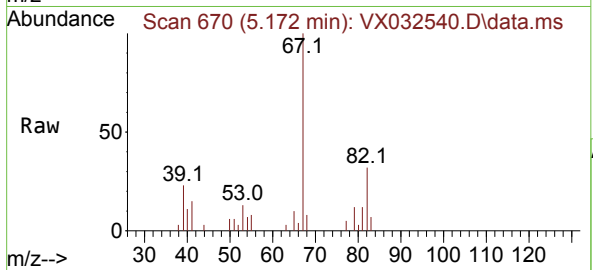

#31
Cyclohexane
Concen: 3.835 ug/l
RT: 5.477 min Scan# 720
Delta R.T. 0.006 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Tgt Ion: 56 Resp: 7845
Ion Ratio Lower Upper
56 100
69 23.4 24.1 36.1#
84 81.3 66.9 100.3

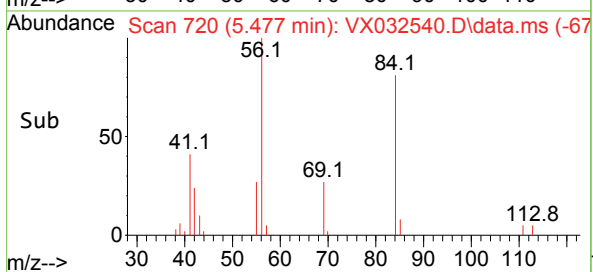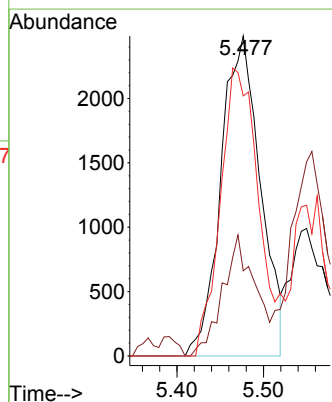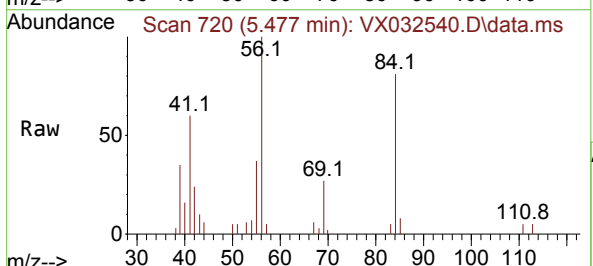



#33

1,2-Dichloroethane-d4

Concen: 49.182 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.000 min

Lab File: VX032540.D

Acq: 02 Nov 2022 16:03

Instrument :

MSVOA_X

ClientSampleId :





INF1122DL

Tgt Ion: 65 Resp: 82977

Ion Ratio Lower Upper

65 100

67 49.9 0.0 101.8

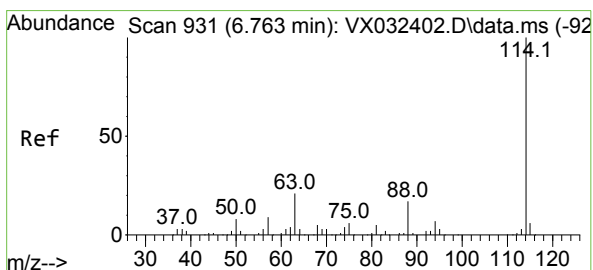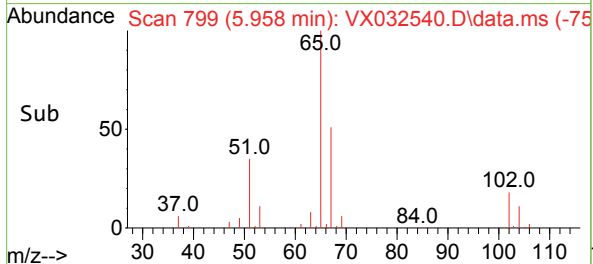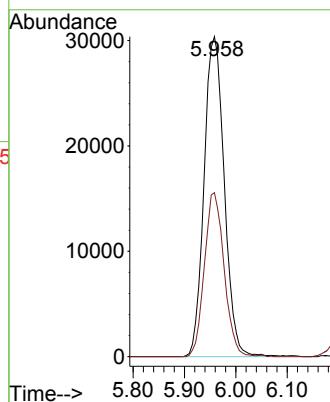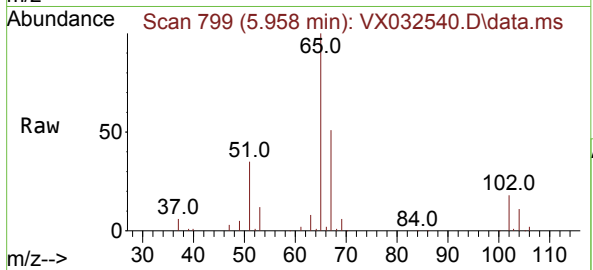

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX032540.D

Acq: 02 Nov 2022 16:03




Tgt Ion: 114 Resp: 200266


Ion Ratio Lower Upper

114 100

63 19.9 0.0 41.6

88 16.1 0.0 33.4


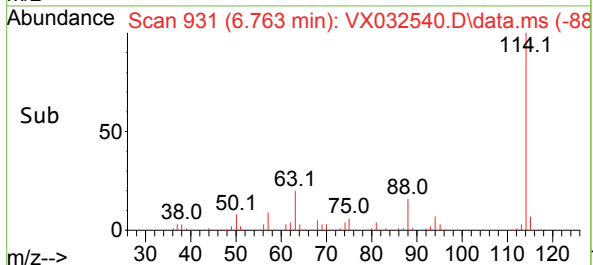

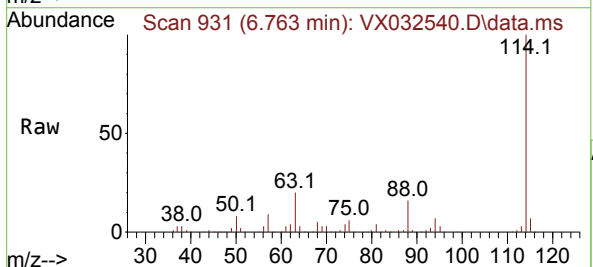


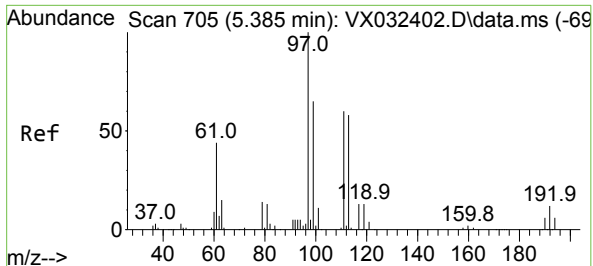

#35
Dibromofluoromethane
Concen: 45.380 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03




Instrument :
MSVOA_X
ClientSampleId :
INF1122DL


Tgt Ion:113 Resp: 64826
Ion Ratio Lower Upper
113 100
111 103.6 82.4 123.6
192 19.4 15.4 23.2

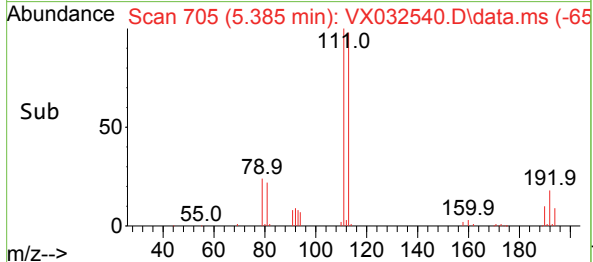

#36
1,1-Dichloropropene
Concen: 4.848 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.140 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03


Tgt Ion: 75 Resp: 9645
Ion Ratio Lower Upper
75 100
110 9.1 18.4 55.2#
77 0.0 24.5 36.7#

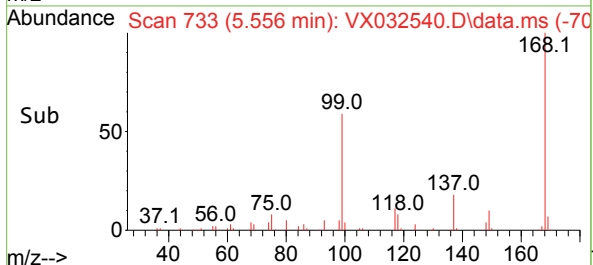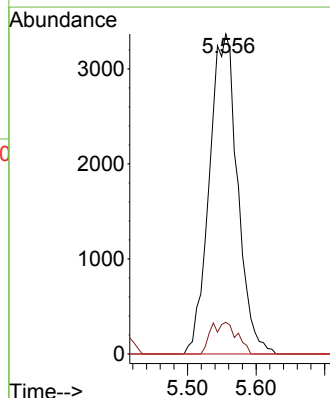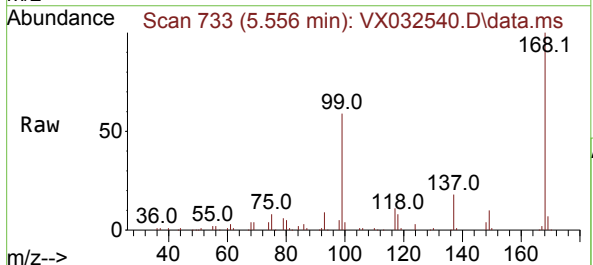






#38
Carbon Tetrachloride
Concen: 5.899 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03


Instrument :
MSVOA_X
ClientSampleId :
INF1122DL





Tgt Ion:117 Resp: 13015
Ion Ratio Lower Upper
117 100
119 4.9 77.2 115.8#
121 0.0 25.8 38.6#




#39
Methylcyclohexane
Concen: 1.549 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03



Tgt Ion: 83 Resp: 3646
Ion Ratio Lower Upper
83 100
55 78.7 58.4 87.6
98 51.5 37.2 55.8



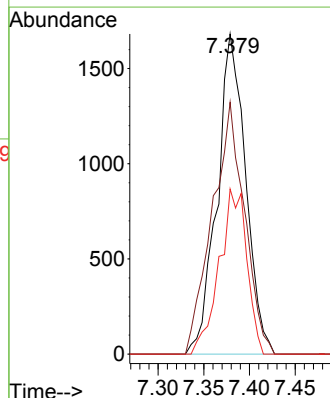



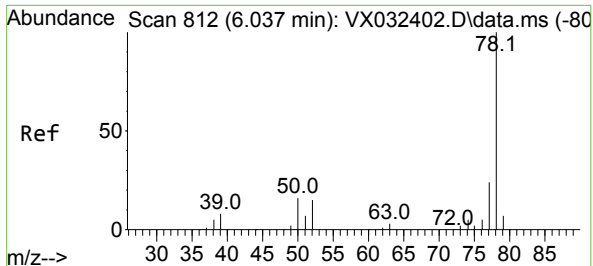

#40
Benzene
Concen: 31.726 ug/l
RT: 6.037 min Scan# 812
Delta R.T. -0.000 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03




Instrument :
MSVOA_X
ClientSampleId :
INF1122DL


Tgt Ion: 78 Resp: 178596
Ion Ratio Lower Upper
78 100
77 23.5 19.0 28.4

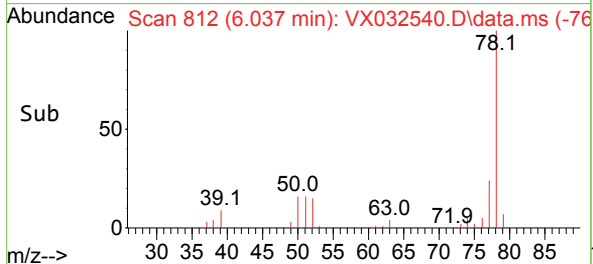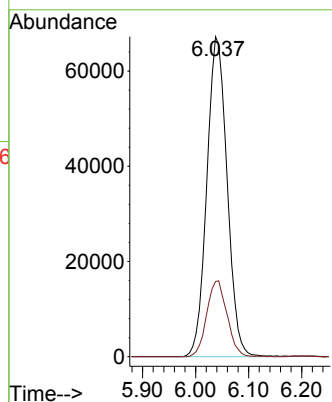

#42
1,2-Dichloroethane
Concen: 0.892 ug/l
RT: 6.025 min Scan# 810
Delta R.T. -0.061 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Tgt Ion: 62 Resp: 2052
Ion Ratio Lower Upper
62 100
98 0.0 0.0 16.0

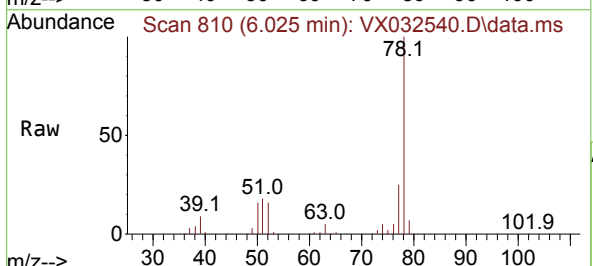



#48

Methyl methacrylate

Concen: 0.270 ug/l

RT: 7.665 min Scan# 1

Delta R.T. -0.030 min

Lab File: VX032540.D

Acq: 02 Nov 2022 16:03

Instrument :

MSVOA_X

ClientSampleId :

INF1122DL





Tgt Ion: 41 Resp: 443

Ion Ratio Lower Upper

41 100

69 128.4 65.1 97.7#

39 56.0 51.9 77.9



#50

Toluene-d8

Concen: 48.253 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.006 min

Lab File: VX032540.D




Acq: 02 Nov 2022 16:03


Tgt Ion: 98 Resp: 239688

Ion Ratio Lower Upper

98 100

100 63.6 50.9 76.3


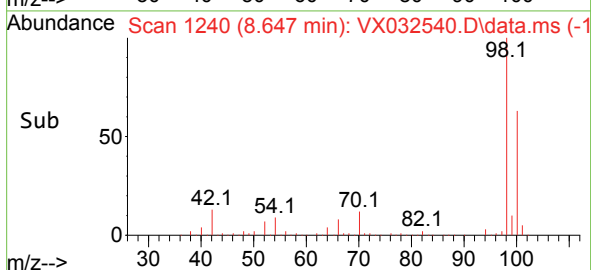






#52
Toluene
Concen: 4.875 ug/l
RT: 8.720 min Scan# 1158
Delta R.T. -0.000 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03




Instrument :
MSVOA_X
ClientSampleId :
INF1122DL


Tgt Ion: 92 Resp: 17906
Ion Ratio Lower Upper
92 100
91 173.7 138.3 207.5

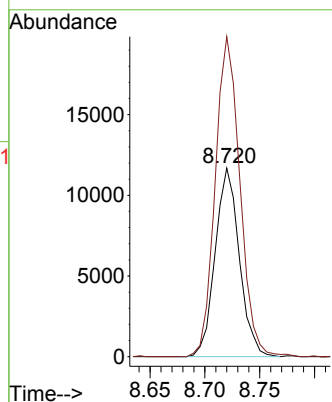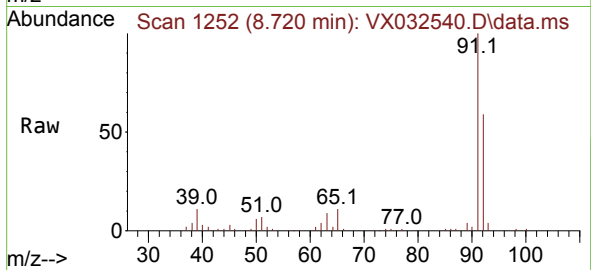

#58
2-Chloroethyl Vinyl ether
Concen: 0.216 ug/l
RT: 8.147 min Scan# 1158
Delta R.T. -0.098 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Tgt Ion: 63 Resp: 231
Ion Ratio Lower Upper
63 100
106 0.0 23.3 34.9#


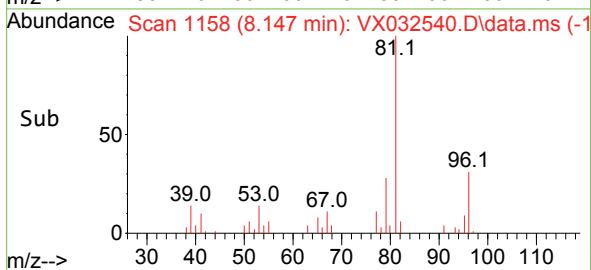
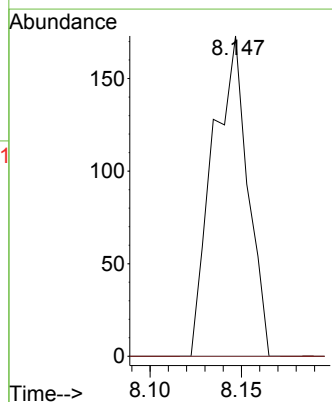
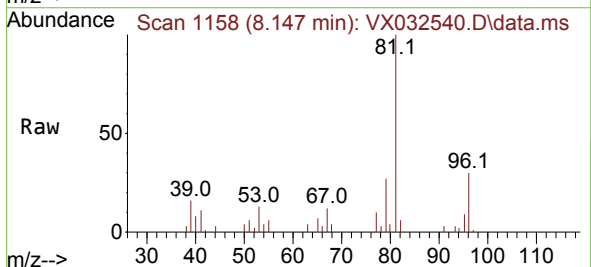




#62
4-Bromofluorobenzene
Concen: 48.392 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03




Instrument :
MSVOA_X
ClientSampleId :
INF1122DL


Tgt Ion: 95 Resp: 93897
Ion Ratio Lower Upper
95 100
174 83.1 0.0 164.0
176 79.6 0.0 154.4

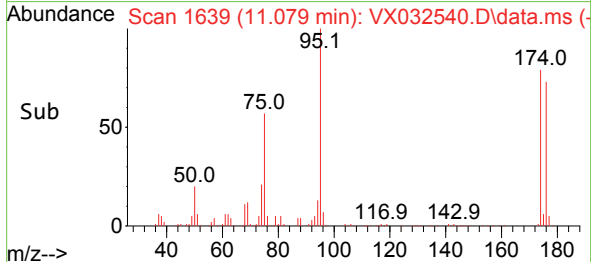

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Tgt Ion: 117 Resp: 178351
Ion Ratio Lower Upper
117 100
82 55.0 44.3 66.5
119 31.4 25.7 38.5

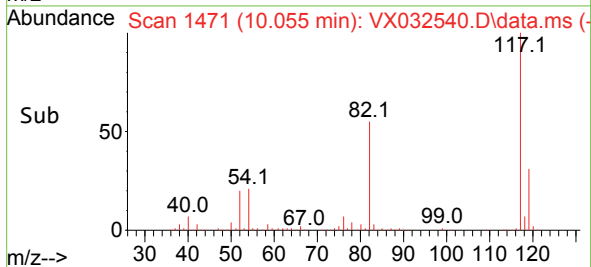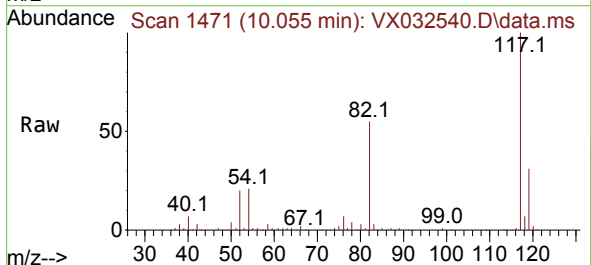



#67

Ethyl Benzene

Concen: 16.351 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. -0.000 min

Lab File: VX032540.D

Acq: 02 Nov 2022 16:03

Instrument :

MSVOA_X

ClientSampleId :





INF1122DL

Tgt Ion: 91 Resp: 116818

Ion Ratio Lower Upper

91 100

106 31.0 25.0 37.6



#68

m/p-Xylenes

Concen: 52.129 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. -0.000 min

Lab File: VX032540.D




Acq: 02 Nov 2022 16:03


Tgt Ion: 106 Resp: 144614

Ion Ratio Lower Upper

106 100

91 207.2 164.5 246.7


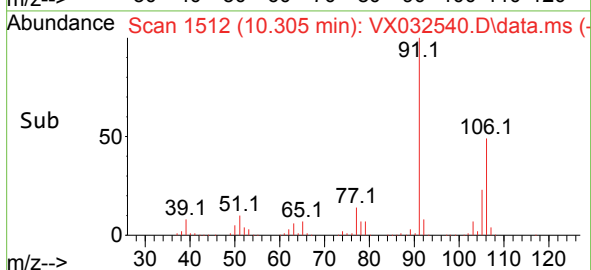






#69
o-Xylene
Concen: 6.658 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03




Instrument :
MSVOA_X
ClientSampleId :
INF1122DL


Tgt Ion:106 Resp: 17957
Ion Ratio Lower Upper
106 100
91 220.6 109.2 327.6

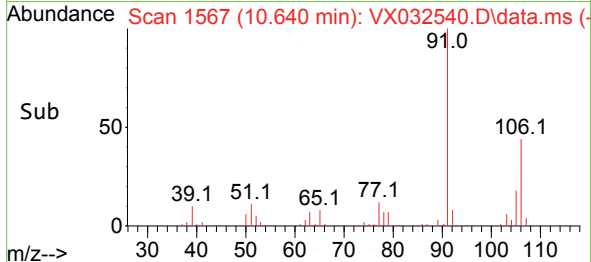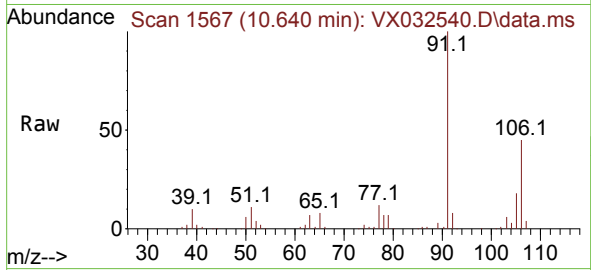

#70
Styrene
Concen: 0.222 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.018 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Tgt Ion:104 Resp: 994
Ion Ratio Lower Upper
104 100
78 310.1 41.8 62.8#
103 264.8 44.5 66.7#

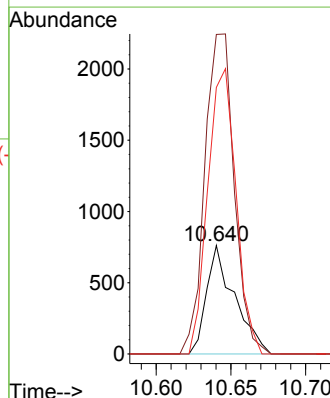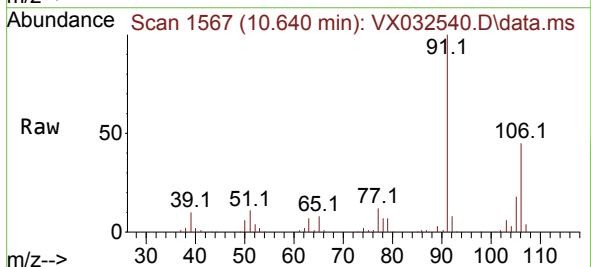



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX032540.D

Acq: 02 Nov 2022 16:03

Instrument :

MSVOA_X

ClientSampleId :

INF1122DL





Tgt Ion:152 Resp: 88572

Ion Ratio Lower Upper

152 100

115 59.5 44.0 132.0

150 155.6 0.0 351.8

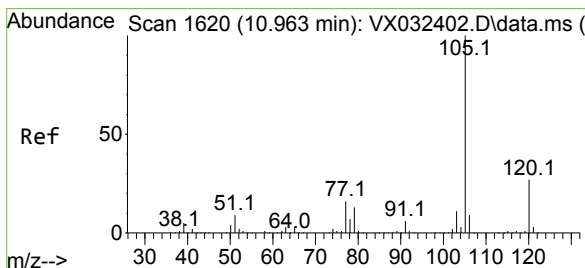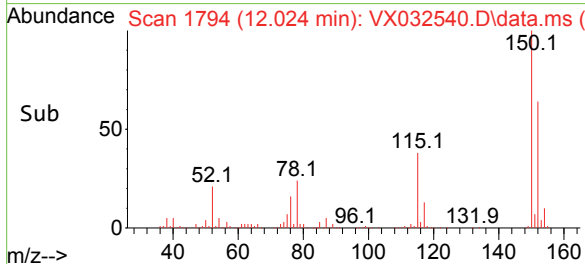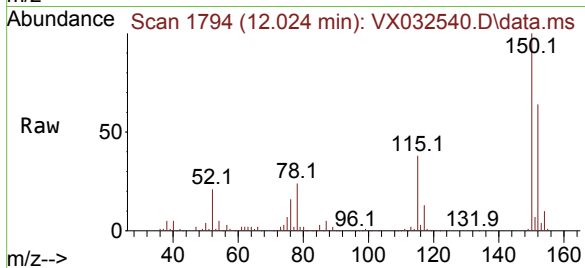

#73

Isopropylbenzene

Concen: 2.384 ug/l

RT: 10.963 min Scan# 1620

Delta R.T. -0.000 min

Lab File: VX032540.D




Acq: 02 Nov 2022 16:03


Tgt Ion:105 Resp: 16734

Ion Ratio Lower Upper

105 100

120 25.8 13.1 39.3


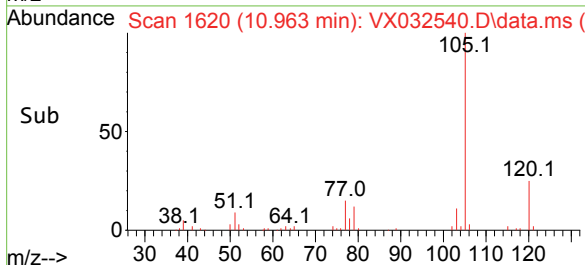
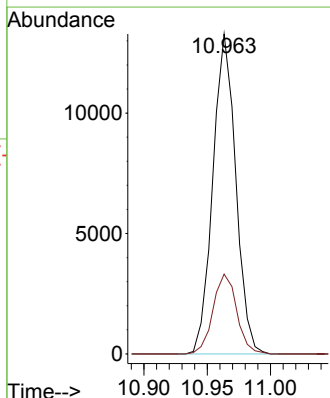
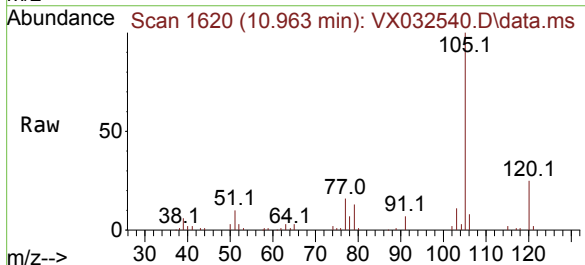




#76
1,2,3-Trichloropropane
Concen: 26.344 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03




Instrument :
MSVOA_X
ClientSampleId :
INF1122DL


Tgt Ion: 75 Resp: 51911
Ion Ratio Lower Upper
75 100
77 1.0 20.0 60.0#

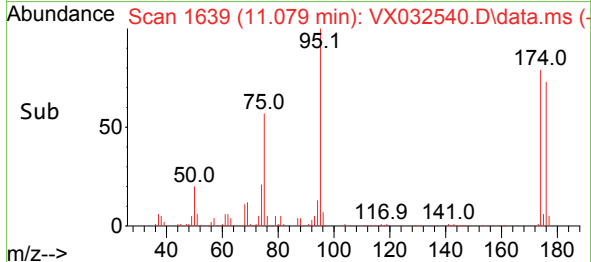

#78
n-propylbenzene
Concen: 4.006 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Tgt Ion: 91 Resp: 32398
Ion Ratio Lower Upper
91 100
120 22.5 11.6 34.8


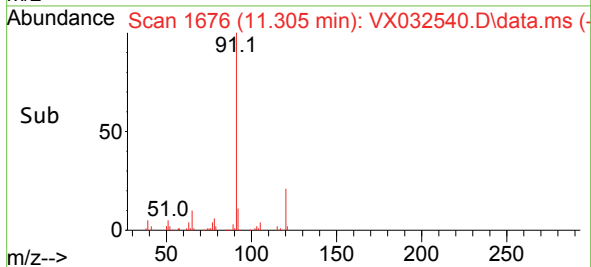

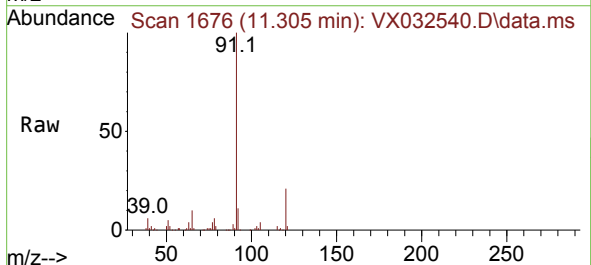


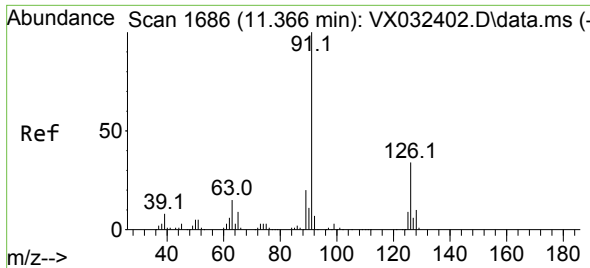

#79
2-Chlorotoluene
Concen: 1.432 ug/l
RT: 11.402 min Scan# 11
Delta R.T. 0.037 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03




Instrument :
MSVOA_X
ClientSampleId :
INF1122DL


Tgt Ion: 91 Resp: 6936
Ion Ratio Lower Upper
91 100
126 0.0 17.1 51.2#

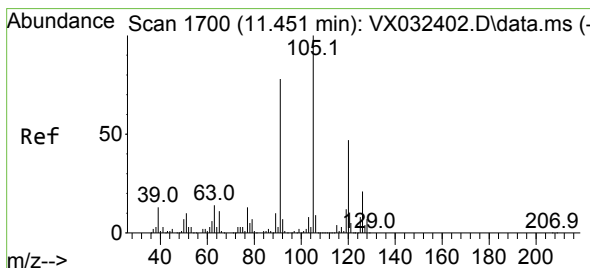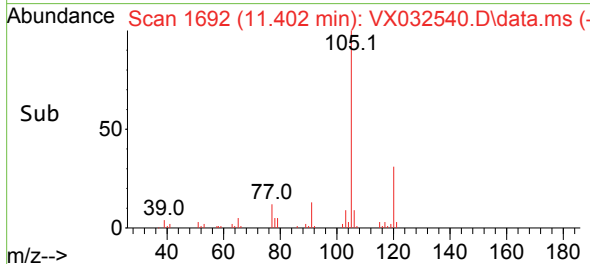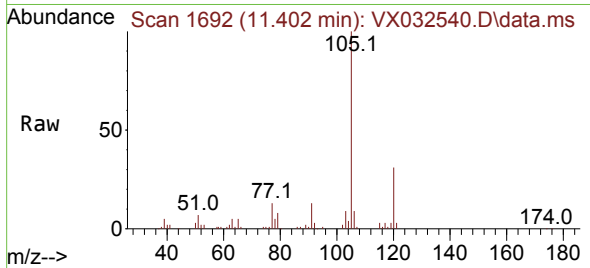

#80
1,3,5-Trimethylbenzene
Concen: 5.003 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Tgt Ion: 105 Resp: 30012
Ion Ratio Lower Upper
105 100
120 46.5 23.6 71.0


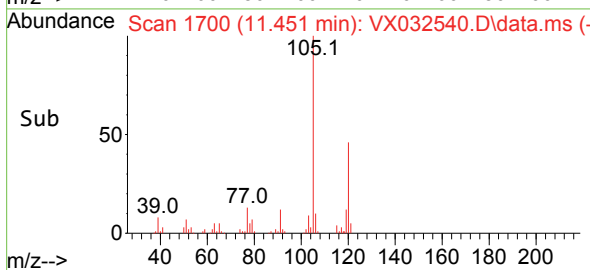

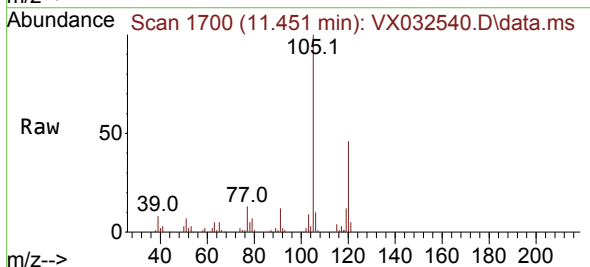




#81
trans-1,4-Dichloro-2-butene
Concen: 83.827 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03




Instrument :
MSVOA_X
ClientSampleId :
INF1122DL


Tgt Ion: 75 Resp: 51911
Ion Ratio Lower Upper
75 100
53 0.0 86.9 130.3#
89 0.0 38.3 57.5#

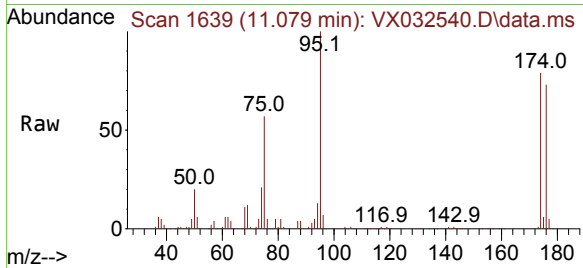

#82
4-Chlorotoluene
Concen: 0.592 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Tgt Ion: 91 Resp: 3355
Ion Ratio Lower Upper
91 100
126 0.0 14.8 44.4#

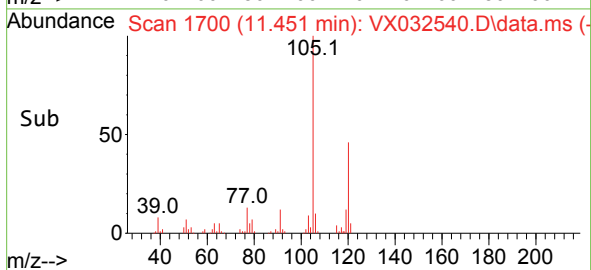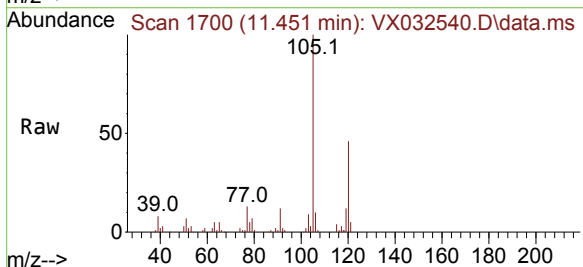



#83

tert-Butylbenzene

Concen: 2.072 ug/l

RT: 11.756 min Scan# 11

Delta R.T. 0.043 min

Lab File: VX032540.D

Acq: 02 Nov 2022 16:03

Instrument :

MSVOA_X

ClientSampleId :

INF1122DL





Tgt Ion:119 Resp: 12411

Ion Ratio Lower Upper

119 100

91 91.5 29.4 88.2#

134 0.0 11.0 33.0#

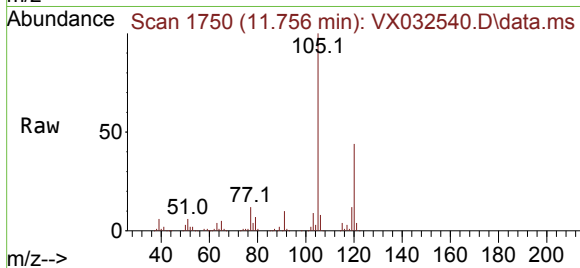

#84

1,2,4-Trimethylbenzene

Concen: 17.490 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX032540.D




Acq: 02 Nov 2022 16:03


Tgt Ion:105 Resp: 104349

Ion Ratio Lower Upper

105 100

120 44.8 21.9 65.5


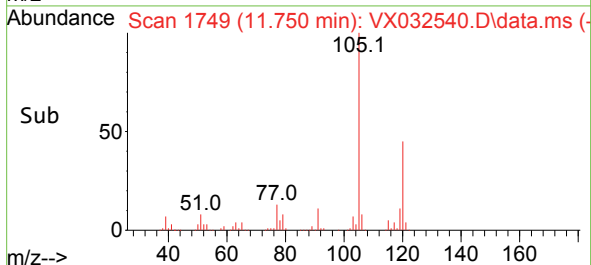
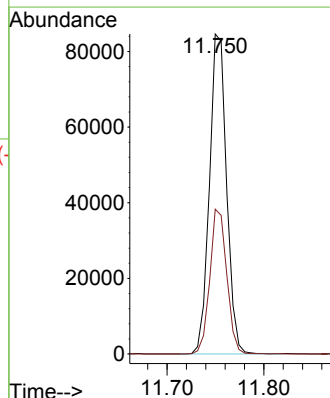
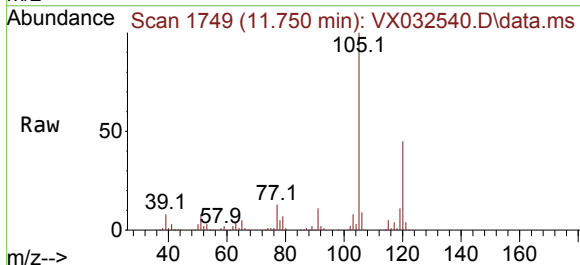




#85
 sec-Butylbenzene
 Concen: 14.481 ug/l
 RT: 11.750 min Scan# 11
 Delta R.T. -0.140 min
 Lab File: VX032540.D
 Acq: 02 Nov 2022 16:03




Instrument :
 MSVOA_X
 ClientSampleId :
 INF1122DL


Tgt Ion:105 Resp: 104349
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.9 29.7#

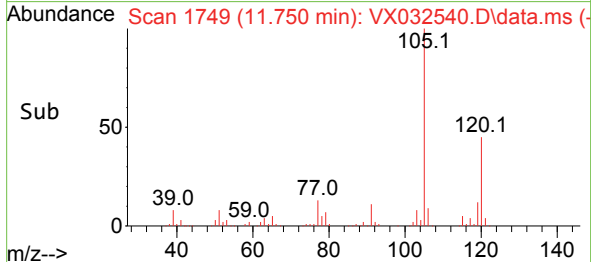

#89
 n-Butylbenzene
 Concen: 0.515 ug/l
 RT: 12.317 min Scan# 1842
 Delta R.T. -0.018 min
 Lab File: VX032540.D
 Acq: 02 Nov 2022 16:03

Tgt Ion: 91 Resp: 2737
 Ion Ratio Lower Upper
 91 100
 92 31.0 26.2 78.6
 134 92.7 12.9 38.6#


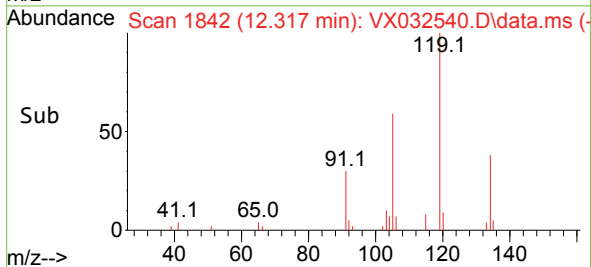

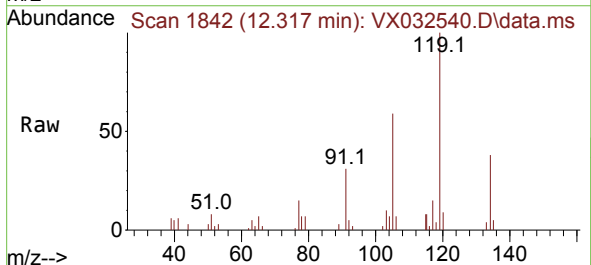




#90
Hexachloroethane
Concen: 3.367 ug/l
RT: 12.646 min Scan# 1879
Delta R.T. 0.104 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Instrument :
MSVOA_X
ClientSampleId :
INF1122DL

Tgt Ion:117 Resp: 3363
Ion Ratio Lower Upper
117 100
201 0.0 37.6 112.9#

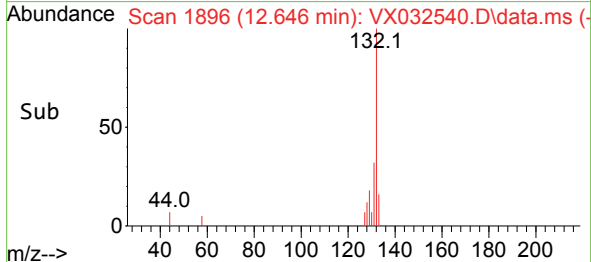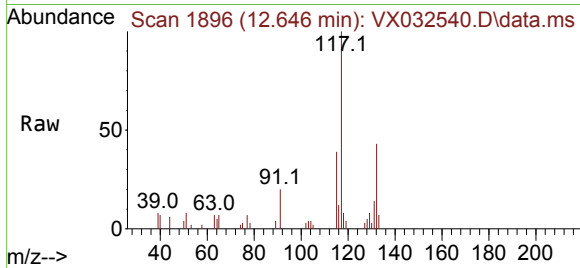

#95
Naphthalene
Concen: 7.078 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.006 min
Lab File: VX032540.D
Acq: 02 Nov 2022 16:03

Tgt Ion:128 Resp: 49219
Ion Ratio Lower Upper
128 100
127 13.0 10.2 15.4
129 10.5 8.9 13.3

