


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX110320\
 Data File : VX019219.D
 Acq On : 03 Nov 2020 08:46
 Operator : JC/MD
 Sample : BFB65
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB65

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM110220WMA.M
 Title : VOC Analysis
 Last Update : Wed Nov 04 01:20:42 2020

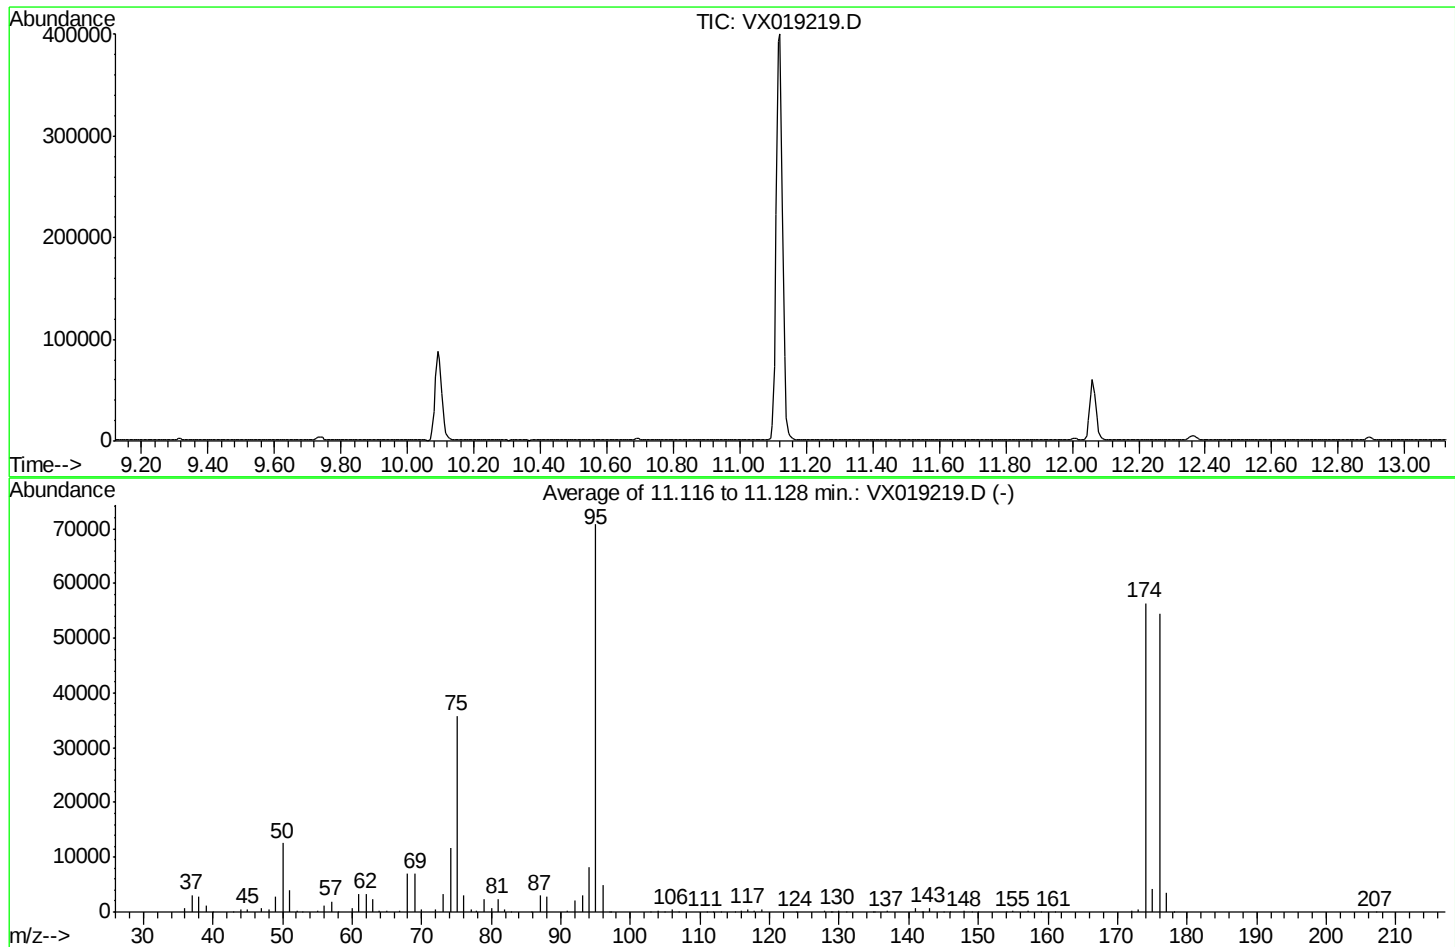

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	12533	PASS
75	95	30	80	50.6	35792	PASS
95	95	100	100	100.0	70800	PASS
96	95	5	9	6.8	4825	PASS
173	174	0.00	2	1.0	548	PASS
174	95	50	120	79.7	56448	PASS
175	174	5	9	7.3	4141	PASS
176	174	95	101	96.4	54394	PASS
177	176	5	9	6.5	3555	PASS

m/z	Abundance
36.00	715.0
37.00	3927.0
38.00	3808.0
39.10	1332.0
40.00	270.0
41.10	63.0
43.00	126.0
44.00	1149.0
45.00	637.0
47.10	970.0
48.10	463.0
49.00	3691.0
50.10	15699.0
51.10	4972.0
52.00	266.0
55.00	271.0
56.00	1340.0
57.00	2404.0
58.00	119.0
60.00	908.0
61.00	3928.0
62.00	4228.0
63.00	3199.0
64.00	250.0
65.00	188.0
66.90	281.0
68.00	8350.0
69.10	8679.0
70.00	749.0
72.00	413.0
73.00	3880.0
74.10	14201.0
75.10	43048.0
76.10	3655.0
77.00	670.0
78.10	396.0
78.90	2867.0
80.00	834.0
80.90	2822.0
81.90	614.0
85.80	149.0
87.00	3808.0
87.90	3084.0
91.00	302.0
92.00	2628.0
93.10	3588.0
94.10	9809.0
95.10	83048.0
96.10	5756.0
97.00	191.0
103.90	395.0
105.00	158.0
106.00	424.0
107.00	110.0
111.00	73.0
111.80	79.0
113.10	66.0
115.10	70.0
116.00	360.0
116.90	556.0
117.90	287.0
118.90	517.0
123.80	61.0
127.90	254.0
128.80	142.0
129.90	295.0
131.00	103.0
134.80	148.0
135.10	148.0
136.90	156.0
141.00	820.0
141.80	88.0
143.00	828.0
145.00	101.0
146.00	121.0
148.10	182.0
149.00	55.0
153.90	87.0
155.00	225.0
157.00	183.0
158.90	104.0
160.90	131.0
172.00	195.0
173.00	603.0
174.00	61144.0
175.00	4378.0
176.00	56168.0
177.00	4108.0
178.10	104.0
206.90	81.0
281.00	63.0

Instrument :
MSVOA_X
ClientSampleId :
BFB65

m/z	Abundance
36.00	766.0
37.00	3420.0
38.00	3398.0
39.00	1335.0
40.00	222.0
41.10	64.0
43.00	126.0
44.00	977.0
45.00	708.0
47.00	729.0
48.10	536.0
49.00	3263.0
50.00	14598.0
51.10	4653.0
52.10	149.0
55.00	269.0
56.00	1368.0
57.00	2455.0
58.10	119.0
60.00	708.0
61.00	3903.0
62.00	3794.0
63.00	2888.0
63.90	239.0
65.00	169.0
66.90	255.0
68.00	8171.0
69.10	8009.0
70.00	673.0
71.90	447.0
73.10	3767.0
74.10	13699.0
75.10	42376.0
76.00	3382.0
77.10	576.0
77.90	419.0
78.90	2668.0
80.00	770.0
81.00	2944.0
82.00	699.0
82.90	54.0
85.80	113.0
87.00	3258.0
88.00	3378.0
90.90	325.0
92.00	2251.0
93.00	3810.0
94.00	9391.0
95.00	83384.0
96.10	5769.0
97.00	109.0
97.20	111.0
102.80	65.0
103.90	419.0
104.90	117.0
105.90	428.0
106.90	89.0
110.90	107.0
111.80	55.0
113.00	112.0
115.10	100.0
115.90	290.0
116.90	592.0
117.90	257.0
119.00	534.0
123.80	57.0
128.00	337.0
129.00	181.0
129.90	391.0
130.90	164.0
134.90	132.0
136.90	232.0
140.90	881.0
142.00	102.0
143.00	927.0
144.90	123.0
145.90	158.0
147.90	147.0
149.00	67.0
149.90	85.0
154.00	52.0
155.00	199.0
157.10	164.0
159.00	101.0
160.90	133.0
172.00	342.0
173.00	558.0
174.00	66280.0
175.00	5017.0
176.00	64344.0
177.00	4211.0
178.00	173.0

Instrument :
MSVOA_X
ClientSampleId :
BFB65

207.1052.0

281.0057.0

Instrument :
MSVOA_X
ClientSampleId :
BFB65

m/z	Abundance
36.00	338.0
37.00	2016.0
38.00	1479.0
39.00	668.0
40.00	138.0
41.10	70.0
44.10	808.0
44.90	315.0
46.90	481.0
47.90	235.0
49.00	1683.0
50.10	7304.0
51.00	2511.0
52.10	83.0
52.90	51.0
55.00	124.0
56.00	713.0
57.10	1119.0
60.10	465.0
61.00	1996.0
62.00	2005.0
63.10	1281.0
64.00	151.0
65.00	70.0
66.90	128.0
68.00	4245.0
69.10	4304.0
70.00	217.0
72.10	295.0
73.00	1893.0
74.00	7337.0
75.10	21952.0
76.10	2042.0
77.00	326.0
77.80	173.0
79.00	1339.0
80.00	447.0
81.00	1553.0
81.90	343.0
87.00	1786.0
88.00	1934.0
90.90	232.0
92.00	1485.0
93.10	2092.0
94.00	5371.0
95.10	45968.0
96.10	2952.0
97.30	50.0
103.90	189.0
105.00	102.0
106.00	249.0
107.00	108.0
112.90	82.0
115.10	84.0
115.90	191.0
116.90	322.0
117.80	204.0
118.90	252.0
128.00	188.0
128.90	129.0
129.90	183.0
130.90	54.0
135.00	117.0
136.90	149.0
141.00	467.0
142.10	68.0
142.80	491.0
145.90	103.0
147.80	109.0
150.00	64.0
155.00	156.0
157.00	121.0
159.00	62.0
161.00	116.0
171.90	149.0
172.10	150.0
173.00	485.0
174.00	41920.0
175.00	3028.0
176.00	42672.0
177.10	2347.0
178.00	89.0
281.00	81.0

Instrument :
MSVOA_X
ClientSampleId :
BFB65

Scan 1639 (11.079 min): VX019219.D
BFB65

m/z	Abundance
40.10	186.0
40.90	81.0
42.10	51.0
44.00	499.0
206.90	77.0
280.90	73.0

Instrument :
MSVOA_X
ClientSampleId :
BFB65