

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110322\
 Data File : VX032561.D
 Acq On : 03 Nov 2022 17:24
 Operator : JC/MD
 Sample : N5454-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TRE-1674

Quant Time: Nov 04 06:19:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 08:28:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	139001	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	230765	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	208378	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	98388	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	97327	50.392	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 100.780%			
35) Dibromofluoromethane	5.385	113	75600	45.928	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 91.860%			
50) Toluene-d8	8.647	98	278220	48.608	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 97.220%			
62) 4-Bromofluorobenzene	11.079	95	103609	46.340	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 92.680%			
Target Compounds						Qvalue
6) Chloroethane	1.691	64	655	0.654	ug/l #	76
11) Tert butyl alcohol	2.940	59	1924	6.844	ug/l #	72
16) Acetone	2.398	43	10957	15.609	ug/l	93
18) Methyl Acetate	2.721	43	458	0.201	ug/l #	51
20) Methylene Chloride	2.788	84	327	0.203	ug/l	93
25) 2-Butanone	4.593	43	1612	1.482	ug/l	96
29) Tetrahydrofuran	5.044	42	643	0.927	ug/l #	51
31) Cyclohexane	5.544	56	3219	1.375	ug/l #	42
36) 1,1-Dichloropropene	5.550	75	10664	4.652	ug/l #	50
38) Carbon Tetrachloride	5.550	117	14521	5.712	ug/l #	15
41) Methacrylonitrile	5.044	41	295	0.243	ug/l #	44
51) 4-Methyl-2-Pentanone	8.580	43	583	0.253	ug/l	98
52) Toluene	8.726	92	1142	0.270	ug/l	99
59) 2-Hexanone	9.433	43	571	0.333	ug/l	69
67) Ethyl Benzene	10.195	91	10594	1.269	ug/l	95
68) m/p-Xylenes	10.305	106	14627	4.513	ug/l	97
69) o-Xylene	10.640	106	15431	4.897	ug/l	93
73) Isopropylbenzene	10.963	105	6447	0.827	ug/l	95
76) 1,2,3-Trichloropropane	11.079	75	56894	25.992	ug/l #	37
78) n-propylbenzene	11.305	91	16719	1.861	ug/l	99
79) 2-Chlorotoluene	11.378	91	9664	1.796	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.451	105	32186	4.830	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	56894	82.708	ug/l #	6
82) 4-Chlorotoluene	11.451	91	3747	0.595	ug/l #	45
83) tert-Butylbenzene	11.756	119	7495	1.127	ug/l #	53
84) 1,2,4-Trimethylbenzene	11.750	105	61745	9.317	ug/l	99
85) sec-Butylbenzene	11.890	105	9190	1.148	ug/l	89
86) p-Isopropyltoluene	12.012	119	7241	1.066	ug/l	94
89) n-Butylbenzene	12.329	91	25269	4.276	ug/l #	36
90) Hexachloroethane	12.555	117	2989	2.694	ug/l #	12
92) 1,2-Dibromo-3-Chloropr...	12.963	75	679	1.237	ug/l #	1
95) Naphthalene	13.774	128	17817	2.307	ug/l #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110322\
Data File : VX032561.D
Acq On : 03 Nov 2022 17:24
Operator : JC/MD
Sample : N5454-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRE-1674

Quant Time: Nov 04 06:19:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 08:28:06 2022
Response via : Initial Calibration




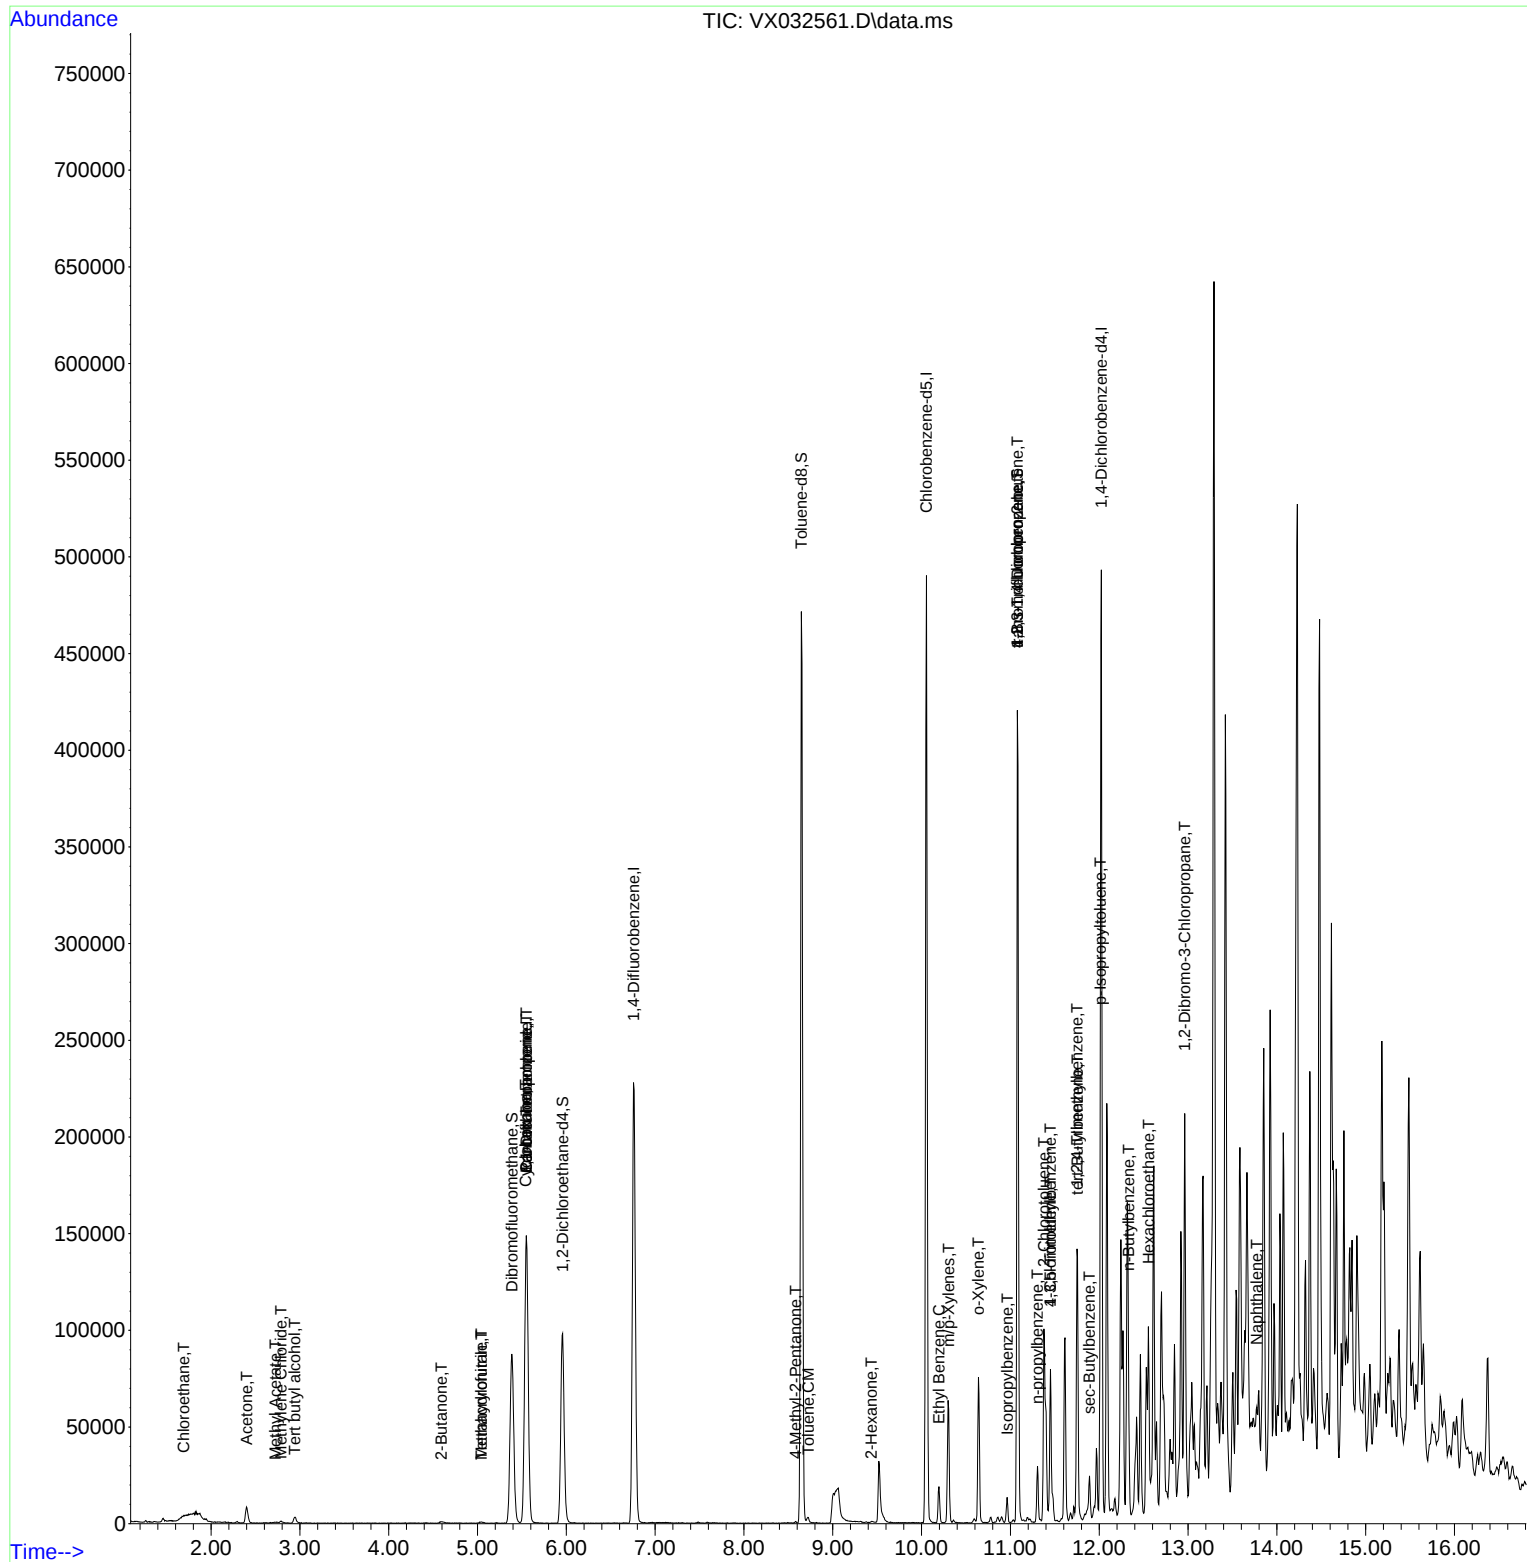




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24




Instrument :
MSVOA_X
ClientSampleId :
TRE-1674


Tgt Ion:168 Resp: 139001
Ion Ratio Lower Upper
168 100
99 58.1 46.1 69.1

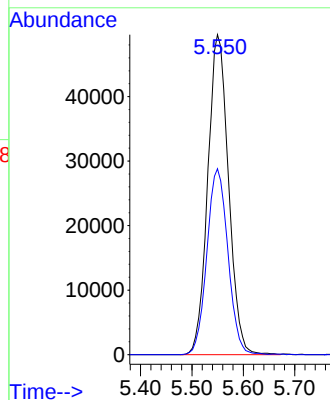

#6
Chloroethane
Concen: 0.654 ug/l
RT: 1.691 min Scan# 99
Delta R.T. 0.006 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion: 64 Resp: 655
Ion Ratio Lower Upper
64 100
66 19.0 26.0 39.0#



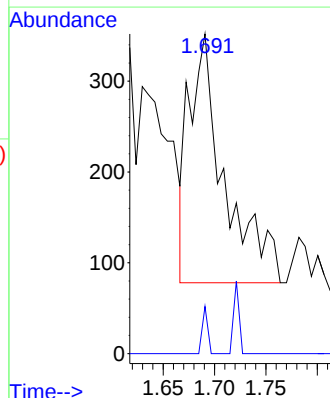





#11
Tert butyl alcohol
Concen: 6.844 ug/l
RT: 2.940 min Scan# 308
Delta R.T. -0.024 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24




Instrument :
MSVOA_X
ClientSampleId :
TRE-1674


Tgt Ion: 59 Resp: 1924
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

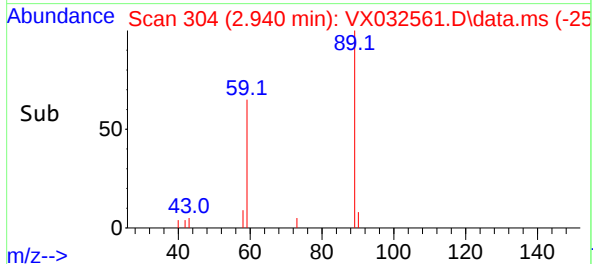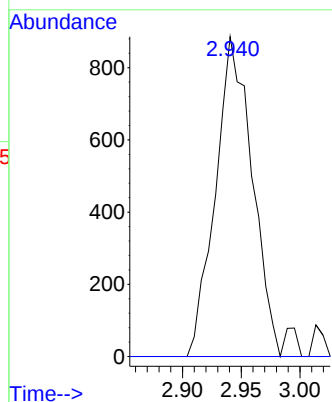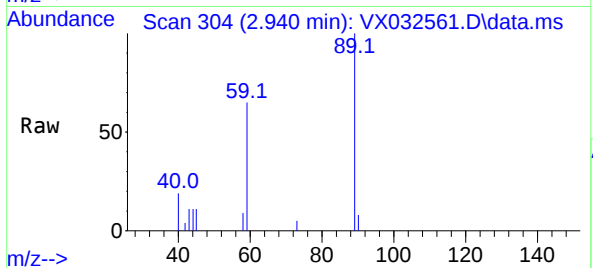

#16
Acetone
Concen: 15.609 ug/l
RT: 2.398 min Scan# 215
Delta R.T. 0.018 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion: 43 Resp: 10957
Ion Ratio Lower Upper
43 100
58 25.8 23.8 35.8


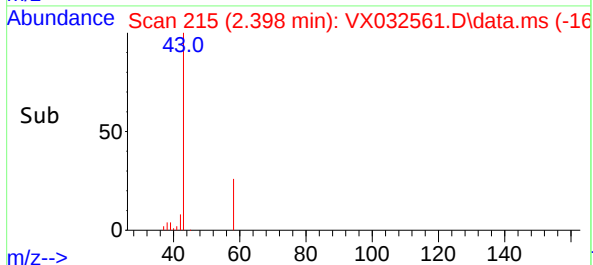

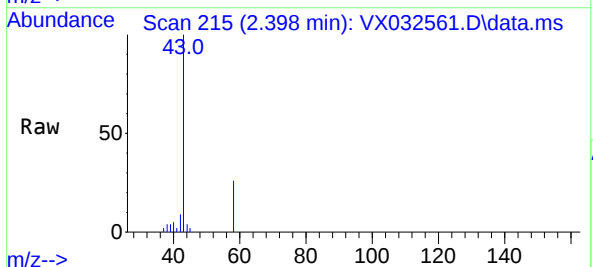




#18
Methyl Acetate
Concen: 0.201 ug/l
RT: 2.721 min Scan# 268
Delta R.T. 0.018 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24




Instrument :
MSVOA_X
ClientSampleId :
TRE-1674


Tgt Ion: 43 Resp: 458
Ion Ratio Lower Upper
43 100
74 0.0 19.4 29.0#



#20
Methylene Chloride
Concen: 0.203 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion: 84 Resp: 327
Ion Ratio Lower Upper
84 100
49 122.4 101.0 151.6
51 33.3 31.1 46.7
86 74.5 52.3 78.5



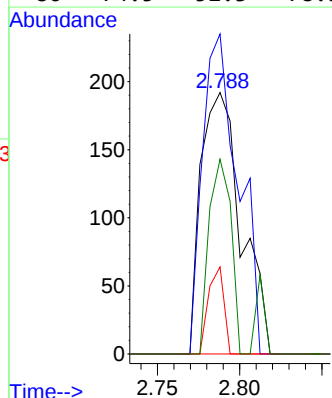





#25
2-Butanone
Concen: 1.482 ug/l
RT: 4.593 min Scan# 51
Delta R.T. 0.037 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24




Instrument :
MSVOA_X
ClientSampleId :
TRE-1674


Tgt Ion: 43 Resp: 1612
Ion Ratio Lower Upper
43 100
72 25.5 22.2 33.2

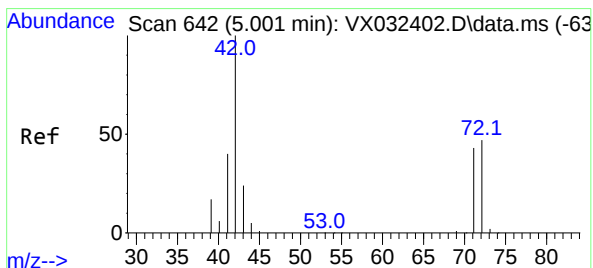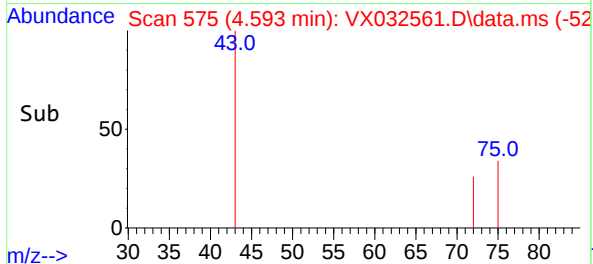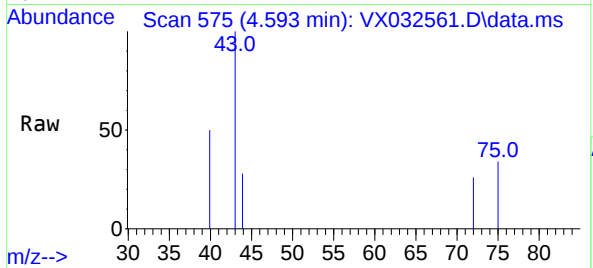

#29
Tetrahydrofuran
Concen: 0.927 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.043 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24


Tgt Ion: 42 Resp: 643
Ion Ratio Lower Upper
42 100
72 17.1 37.6 56.4#
71 9.5 34.7 52.1#

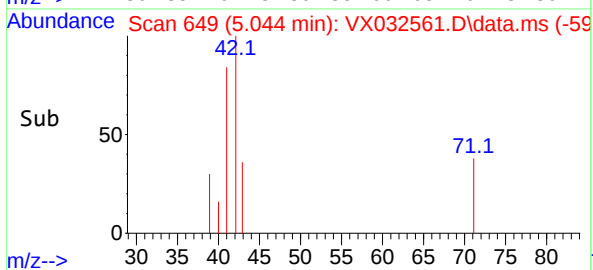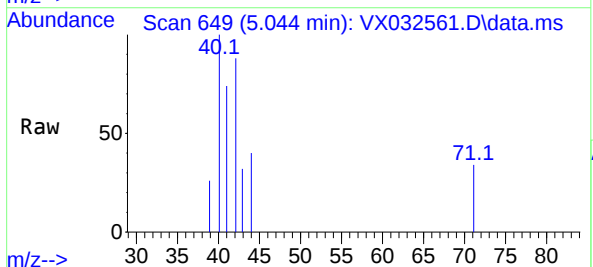



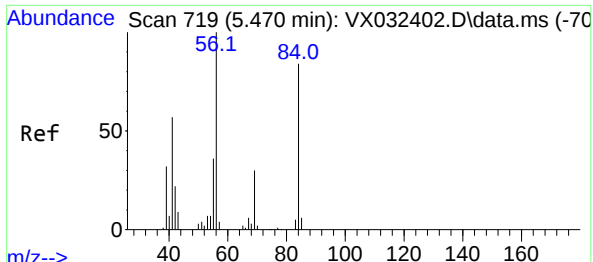


#31
Cyclohexane
Concen: 1.375 ug/l
RT: 5.544 min Scan# 719
Delta R.T. 0.073 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Instrument :
MSVOA_X
ClientSampleId :
TRE-1674



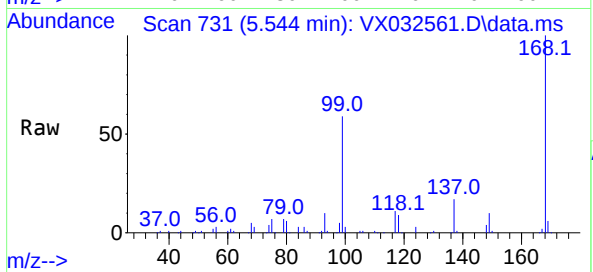



Tgt Ion: 56 Resp: 3219
Ion Ratio Lower Upper
56 100
69 127.0 24.1 36.1#
84 97.3 66.9 100.3

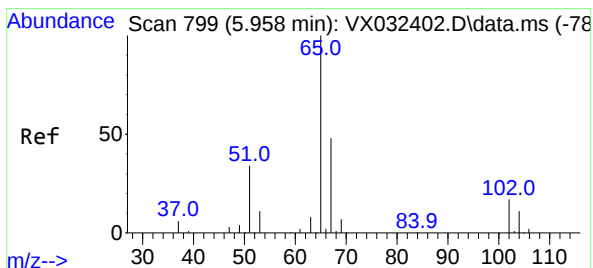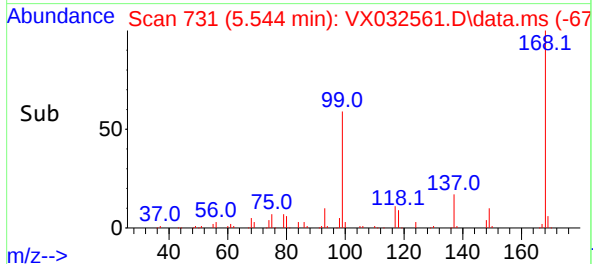

#33
1,2-Dichloroethane-d4
Concen: 50.392 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion: 65 Resp: 97327
Ion Ratio Lower Upper
65 100
67 51.1 0.0 101.8

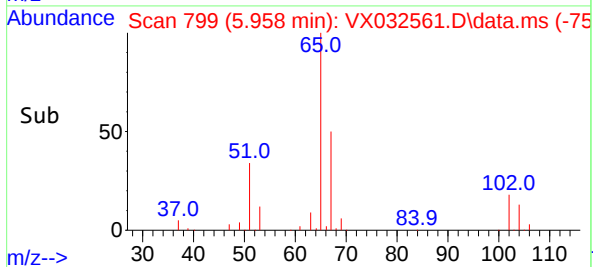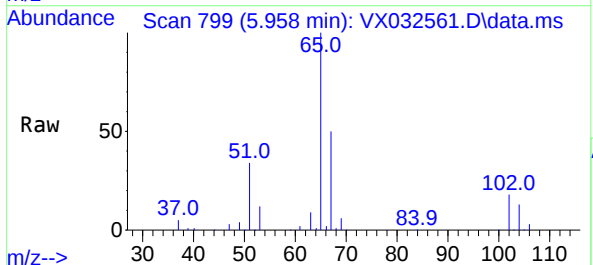



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 91

Delta R.T. -0.006 min

Lab File: VX032561.D

Acq: 03 Nov 2022 17:24

Instrument :

MSVOA_X

ClientSampleId :

TRE-1674





Tgt Ion:114 Resp: 230765

Ion Ratio Lower Upper

114 100

63 19.7 0.0 41.6

88 16.1 0.0 33.4

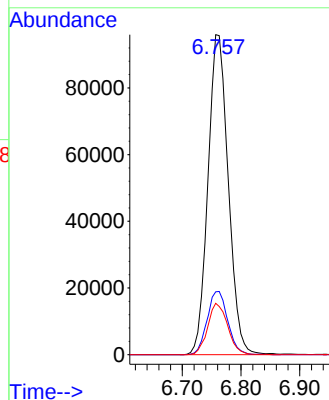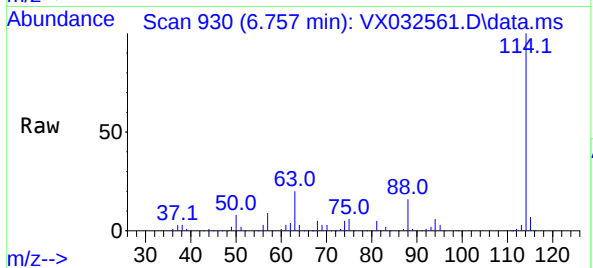

#35

Dibromofluoromethane

Concen: 45.928 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.000 min

Lab File: VX032561.D

Acq: 03 Nov 2022 17:24




Tgt Ion:113 Resp: 75600


Ion Ratio Lower Upper

113 100

111 101.9 82.4 123.6

192 19.3 15.4 23.2


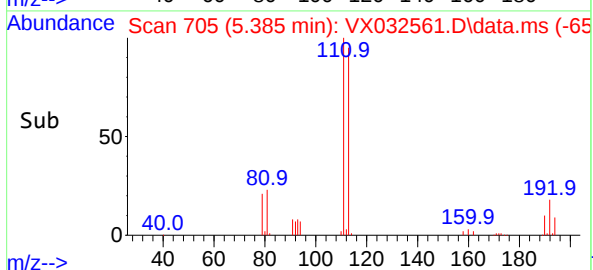
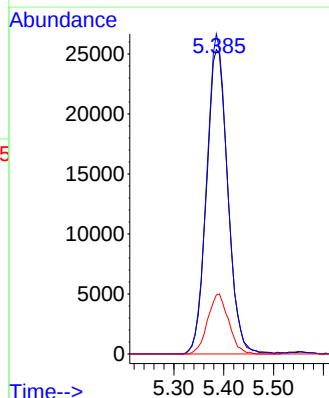





#36
1,1-Dichloropropene
Concen: 4.652 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.146 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24




Instrument :
MSVOA_X
ClientSampleId :
TRE-1674


Tgt Ion: 75 Resp: 10664
Ion Ratio Lower Upper
75 100
110 10.0 18.4 55.2#
77 0.0 24.5 36.7#

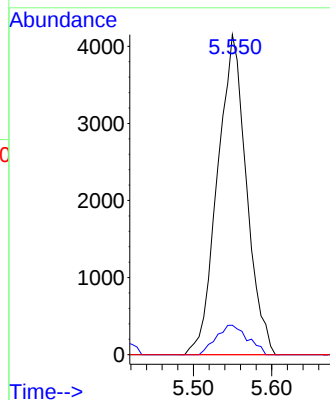

#38
Carbon Tetrachloride
Concen: 5.712 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.134 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion: 117 Resp: 14521
Ion Ratio Lower Upper
117 100
119 3.9 77.2 115.8#
121 0.0 25.8 38.6#

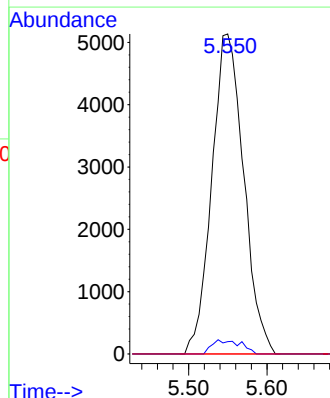




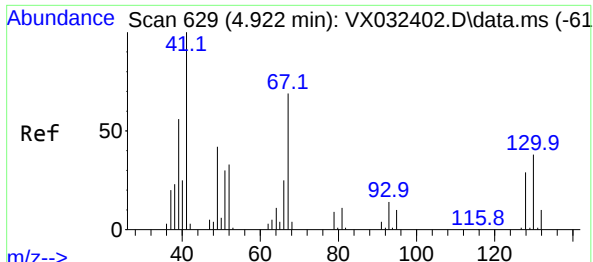


#41
Methacrylonitrile
Concen: 0.243 ug/l
RT: 5.044 min Scan# 64
Delta R.T. 0.122 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Instrument :
MSVOA_X
ClientSampleId :
TRE-1674

Tgt Ion: 41 Resp: 295




Ion	Ratio	Lower	Upper
41	100		
39	50.2	47.5	71.3
67	0.0	60.5	90.7#
52	0.0	27.0	40.6#

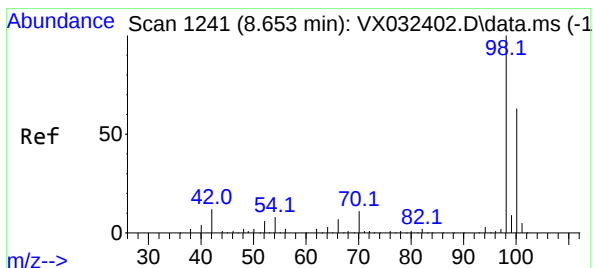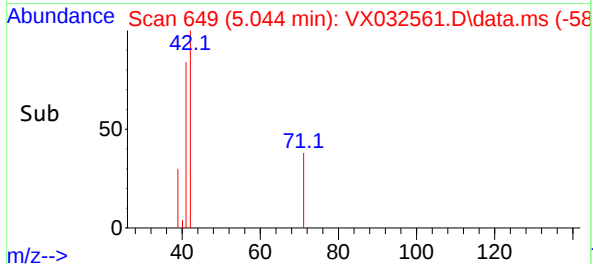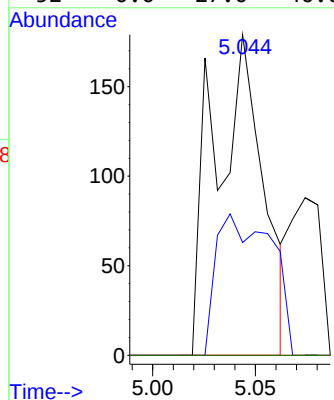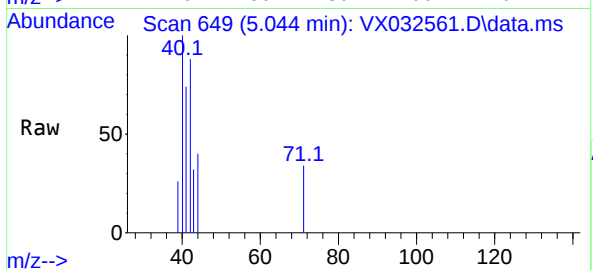


#50
Toluene-d8
Concen: 48.608 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.006 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion: 98 Resp: 278220

Ion	Ratio	Lower	Upper
98	100		
100	63.9	50.9	76.3

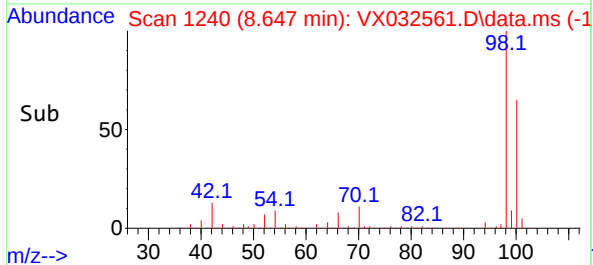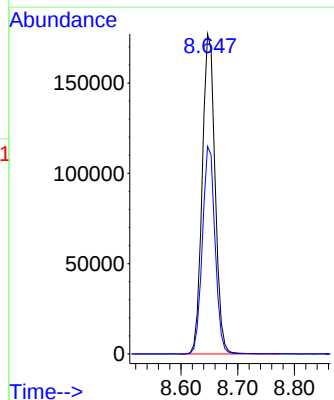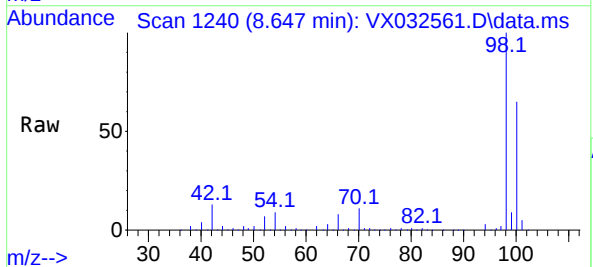



#51

4-Methyl-2-Pentanone

Concen: 0.253 ug/l

RT: 8.580 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX032561.D

Acq: 03 Nov 2022 17:24

Instrument :

MSVOA_X

ClientSampleId :





TRE-1674

Tgt Ion: 43 Resp: 583

Ion Ratio Lower Upper

43 100

58 37.6 30.9 46.3

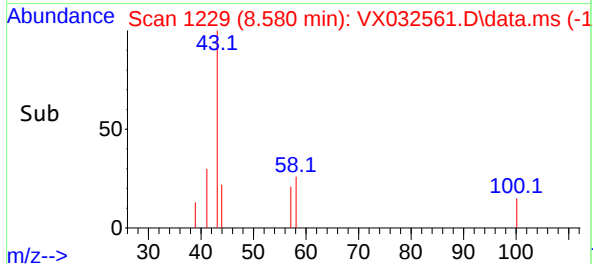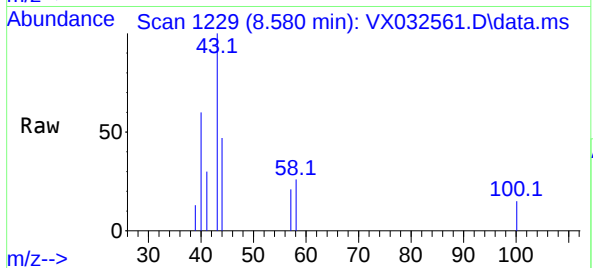

#52

Toluene

Concen: 0.270 ug/l

RT: 8.726 min Scan# 1253

Delta R.T. 0.006 min

Lab File: VX032561.D




Acq: 03 Nov 2022 17:24


Tgt Ion: 92 Resp: 1142

Ion Ratio Lower Upper

92 100

91 173.6 138.3 207.5

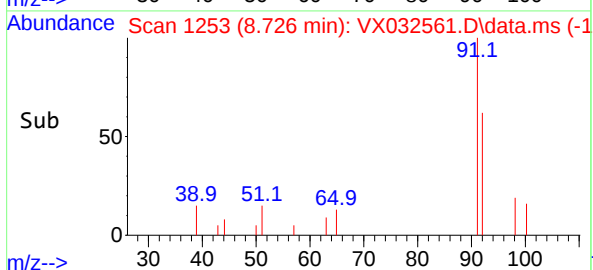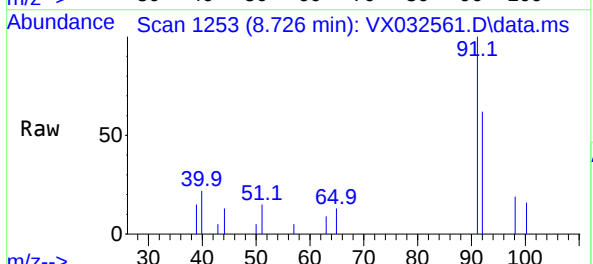



#59

2-Hexanone

Concen: 0.333 ug/l

RT: 9.433 min Scan# 1369

Delta R.T. 0.000 min

Lab File: VX032561.D

Acq: 03 Nov 2022 17:24

Instrument :

MSVOA_X

ClientSampleId :





TRE-1674

Tgt Ion: 43 Resp: 571

Ion Ratio Lower Upper

43 100

58 75.1 26.5 79.5

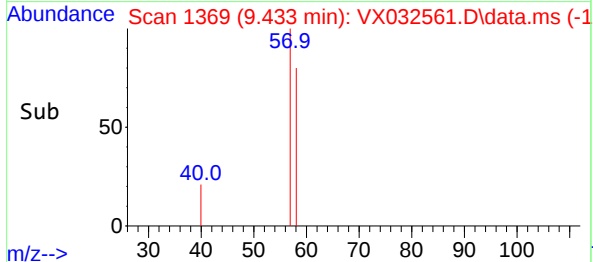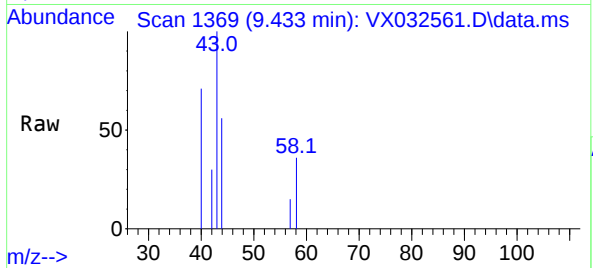

#62

4-Bromofluorobenzene

Concen: 46.340 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX032561.D

Acq: 03 Nov 2022 17:24




Tgt Ion: 95 Resp: 103609


Ion Ratio Lower Upper

95 100

174 81.7 0.0 164.0

176 79.6 0.0 154.4


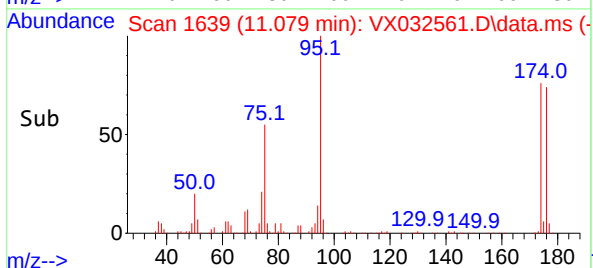
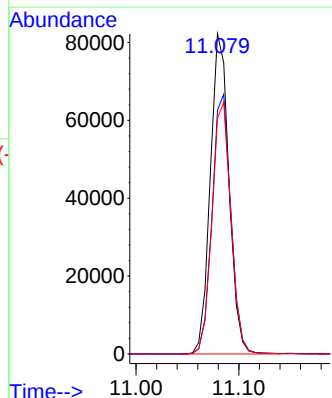
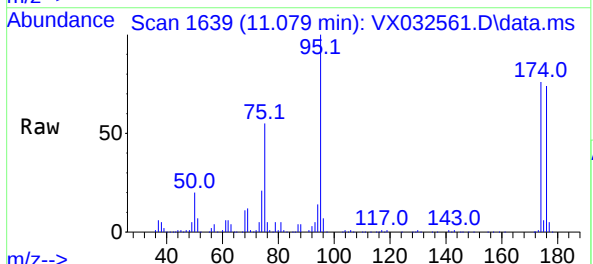




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24




Instrument :
MSVOA_X
ClientSampleId :
TRE-1674


Tgt Ion:117 Resp: 208378
Ion Ratio Lower Upper
117 100
82 55.0 44.3 66.5
119 32.5 25.7 38.5

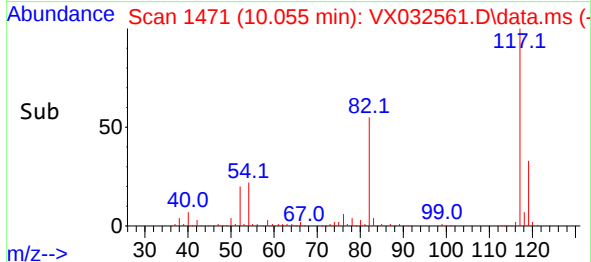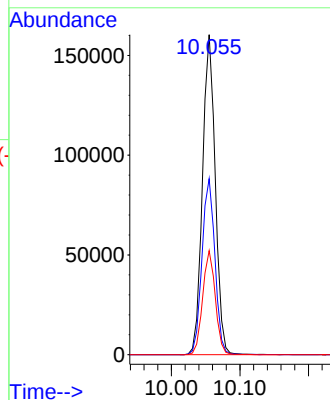

#67
Ethyl Benzene
Concen: 1.269 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion: 91 Resp: 10594
Ion Ratio Lower Upper
91 100
106 34.0 25.0 37.6


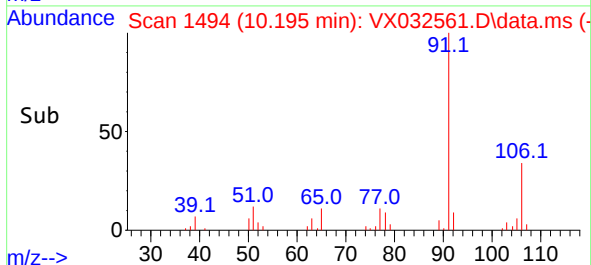
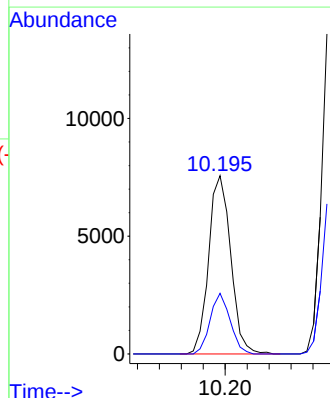
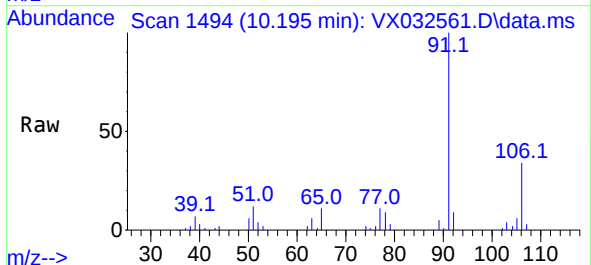




#68
m/p-Xylenes
Concen: 4.513 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24




Instrument :
MSVOA_X
ClientSampleId :
TRE-1674


Tgt Ion:106 Resp: 14627
Ion Ratio Lower Upper
106 100
91 209.7 164.5 246.7

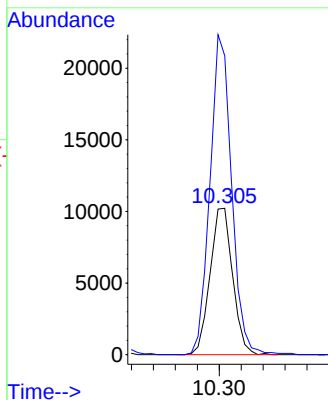

#69
o-Xylene
Concen: 4.897 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion:106 Resp: 15431
Ion Ratio Lower Upper
106 100
91 229.5 109.2 327.6


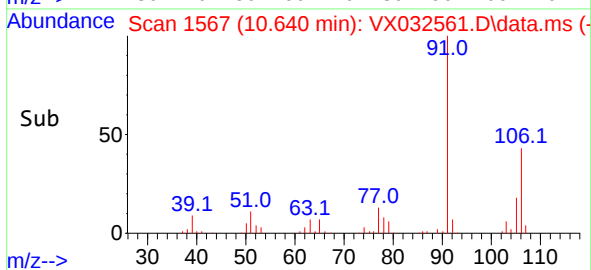
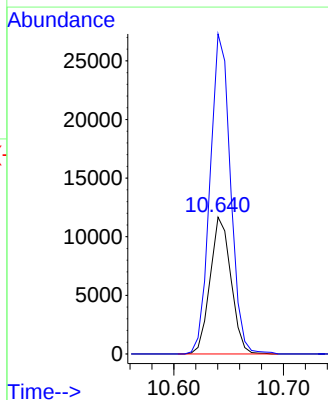





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24




Instrument :
MSVOA_X
ClientSampleId :
TRE-1674


Tgt Ion:152 Resp: 98388
Ion Ratio Lower Upper
152 100
115 60.9 44.0 132.0
150 156.3 0.0 351.8

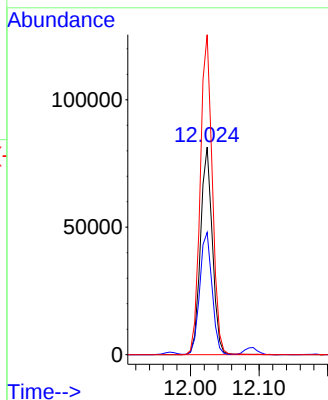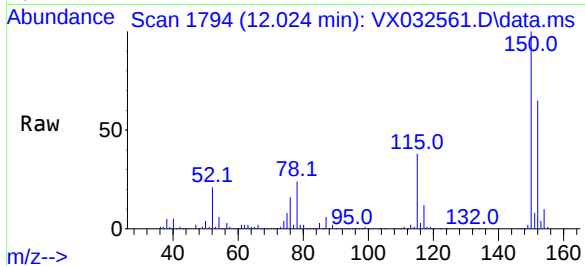

#73
Isopropylbenzene
Concen: 0.827 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion:105 Resp: 6447
Ion Ratio Lower Upper
105 100
120 23.8 13.1 39.3


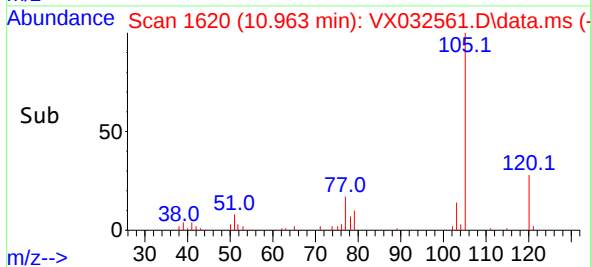
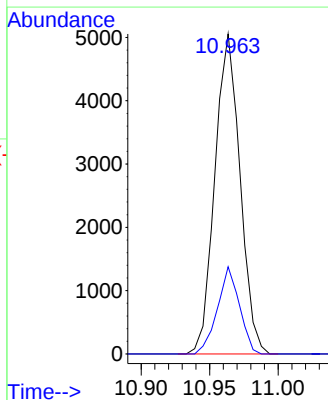
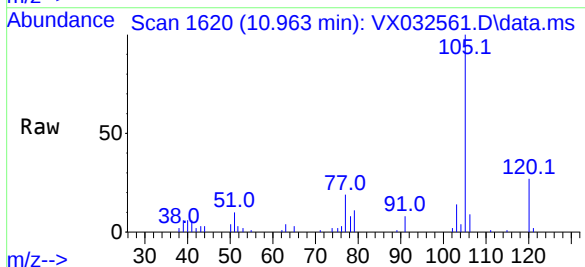




#76
1,2,3-Trichloropropane
Concen: 25.992 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24




Instrument :
MSVOA_X
ClientSampleId :
TRE-1674


Tgt Ion: 75 Resp: 56894
Ion Ratio Lower Upper
75 100
77 1.1 20.0 60.0#

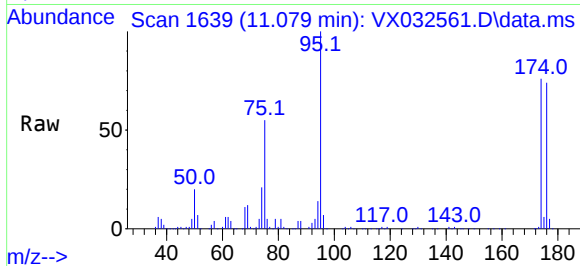

#78
n-propylbenzene
Concen: 1.861 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion: 91 Resp: 16719
Ion Ratio Lower Upper
91 100
120 23.8 11.6 34.8


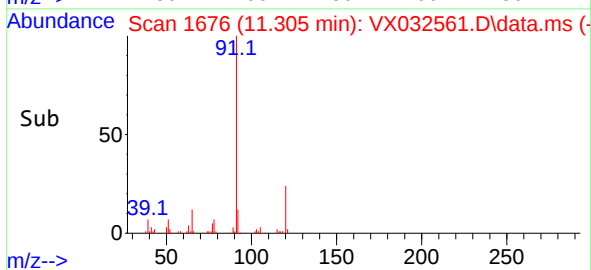

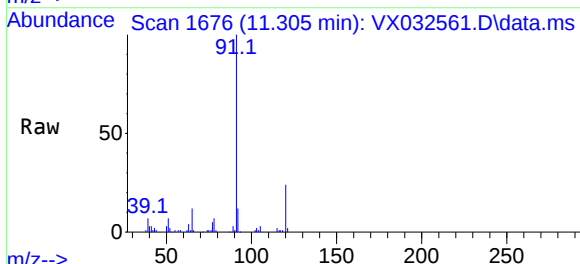




#79
2-Chlorotoluene
Concen: 1.796 ug/l
RT: 11.378 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24




Instrument :
MSVOA_X
ClientSampleId :
TRE-1674


Tgt Ion: 91 Resp: 9664
Ion Ratio Lower Upper
91 100
126 0.0 17.1 51.2#

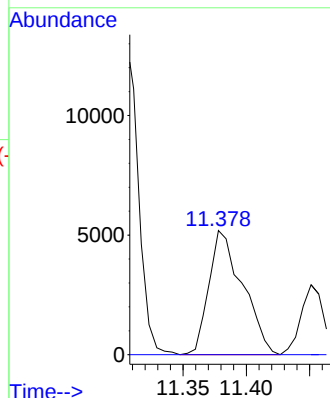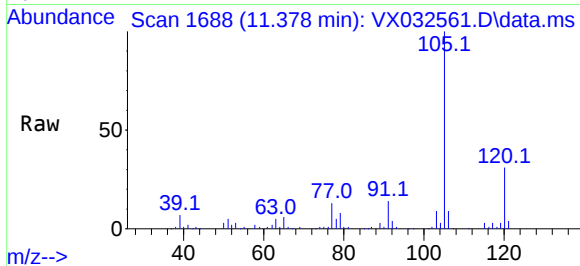

#80
1,3,5-Trimethylbenzene
Concen: 4.830 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion: 105 Resp: 32186
Ion Ratio Lower Upper
105 100
120 46.7 23.6 71.0



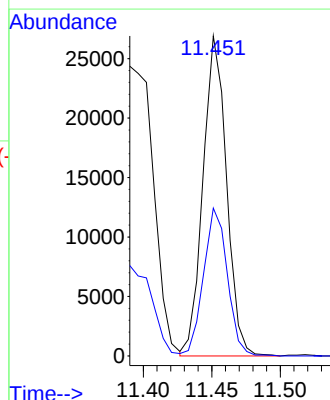
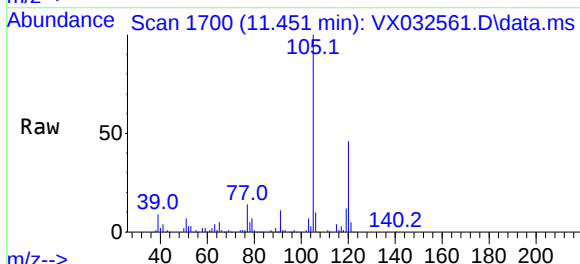




#81
trans-1,4-Dichloro-2-butene
Concen: 82.708 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24




Instrument :
MSVOA_X
ClientSampleId :
TRE-1674


Tgt Ion: 75 Resp: 56894
Ion Ratio Lower Upper
75 100
53 0.0 86.9 130.3#
89 0.0 38.3 57.5#

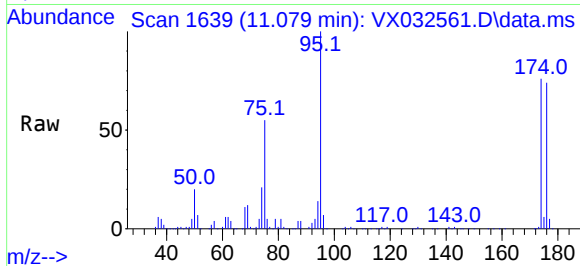

#82
4-Chlorotoluene
Concen: 0.595 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion: 91 Resp: 3747
Ion Ratio Lower Upper
91 100
126 0.0 14.8 44.4#


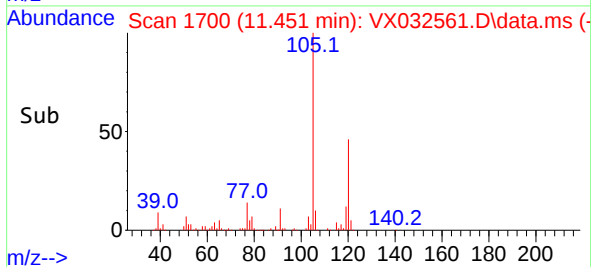

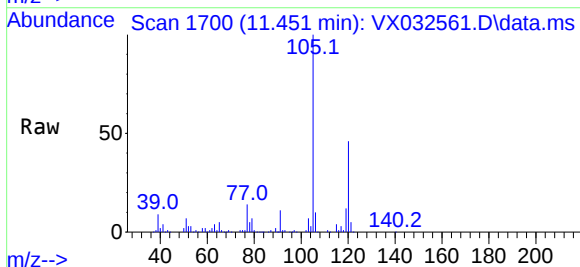




#83
tert-Butylbenzene
Concen: 1.127 ug/l
RT: 11.756 min Scan# 11
Delta R.T. 0.043 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24




Instrument :
MSVOA_X
ClientSampleId :
TRE-1674


Tgt Ion:119 Resp: 7495
Ion Ratio Lower Upper
119 100
91 94.1 29.4 88.2#
134 0.0 11.0 33.0#

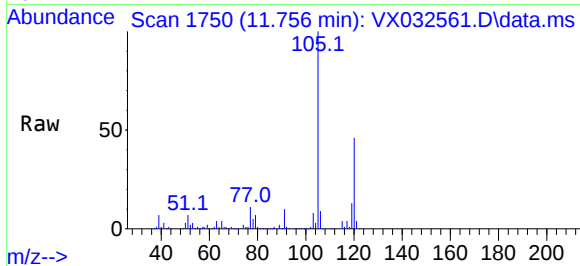

#84
1,2,4-Trimethylbenzene
Concen: 9.317 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion:105 Resp: 61745
Ion Ratio Lower Upper
105 100
120 44.4 21.9 65.5


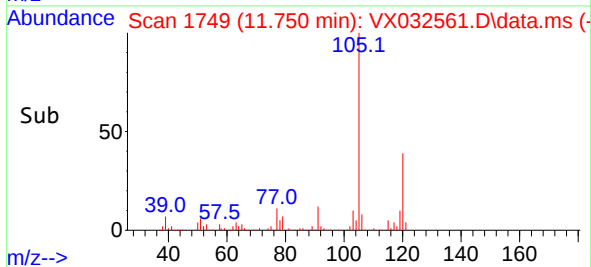

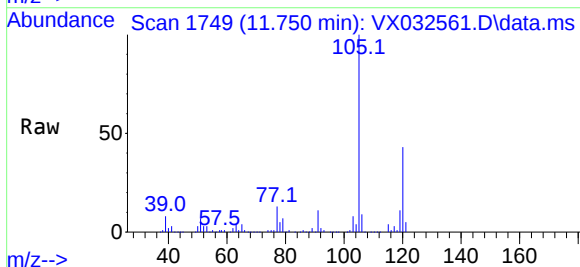




#85
sec-Butylbenzene
Concen: 1.148 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. -0.000 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24




Instrument :
MSVOA_X
ClientSampleId :
TRE-1674


Tgt Ion:105 Resp: 9190
Ion Ratio Lower Upper
105 100
134 24.8 9.9 29.7

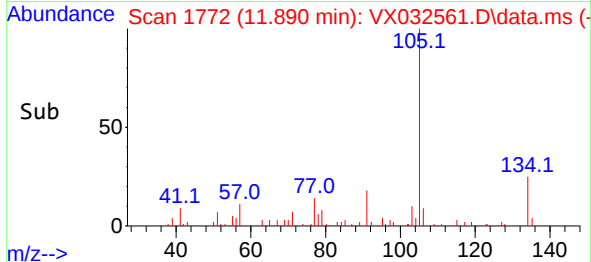

#86
p-Isopropyltoluene
Concen: 1.066 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. 0.000 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion:119 Resp: 7241
Ion Ratio Lower Upper
119 100
134 28.2 12.9 38.7
91 28.2 12.5 37.5

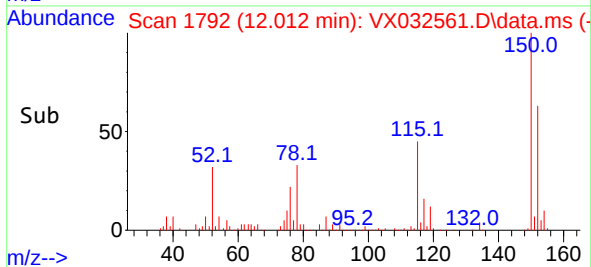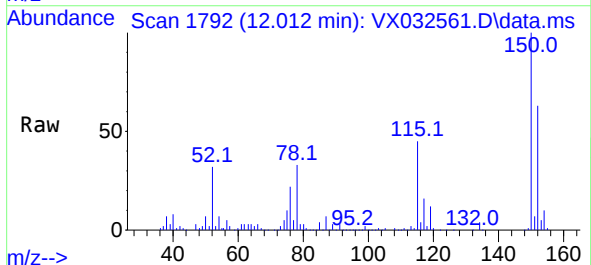



#89

n-Butylbenzene

Concen: 4.276 ug/l

RT: 12.329 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX032561.D

Acq: 03 Nov 2022 17:24

Instrument :

MSVOA_X

ClientSampleId :

TRE-1674





Tgt Ion: 91 Resp: 25269

Ion Ratio Lower Upper

91 100

92 32.6 26.2 78.6

134 94.9 12.9 38.6#

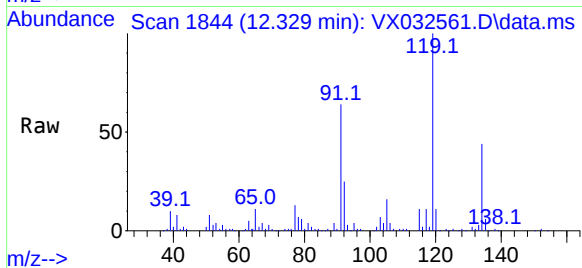

#90

Hexachloroethane

Concen: 2.694 ug/l

RT: 12.555 min Scan# 1881

Delta R.T. 0.012 min

Lab File: VX032561.D




Acq: 03 Nov 2022 17:24


Tgt Ion: 117 Resp: 2989

Ion Ratio Lower Upper

117 100

201 0.0 37.6 112.9#



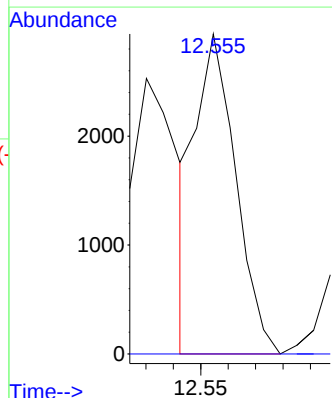
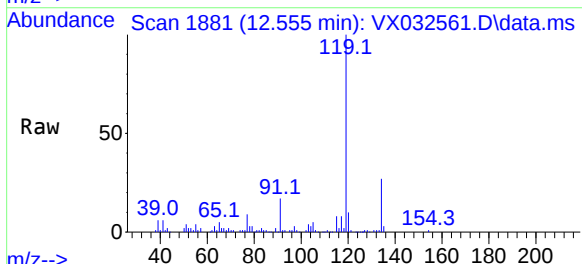




#92
1,2-Dibromo-3-Chloropropane
Concen: 1.237 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.018 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Instrument :
MSVOA_X
ClientSampleId :
TRE-1674

Tgt Ion: 75 Resp: 679
Ion Ratio Lower Upper
75 100
155 0.0 41.6 124.8#
157 0.0 54.1 162.4#

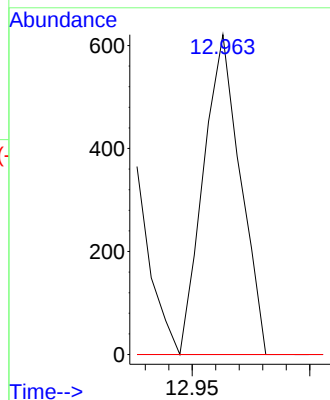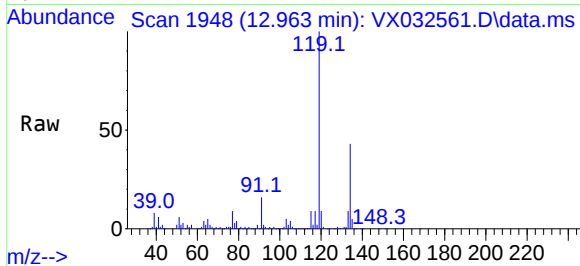

#95
Naphthalene
Concen: 2.307 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.006 min
Lab File: VX032561.D
Acq: 03 Nov 2022 17:24

Tgt Ion: 128 Resp: 17817
Ion Ratio Lower Upper
128 100
127 15.6 10.2 15.4#
129 18.9 8.9 13.3#

