

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110325\
 Data File : VX048466.D
 Acq On : 03 Nov 2025 18:25
 Operator : JC/MD
 Sample : Q3521-03 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TANK-2025

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102925W.M
 Title : SW846 8260

Signal : TIC: VX048466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.373	692	703	720	rBV2	68451	220336	26.82%	4.901%
2	5.538	720	730	750	rVB	137282	424338	51.65%	9.438%
3	5.946	787	797	820	rBV	83706	250860	30.53%	5.580%
4	6.745	919	928	949	rBV	225423	597019	72.66%	13.279%
5	8.635	1229	1238	1264	rBV	480916	821609	100.00%	18.275%
6	10.037	1462	1468	1485	rBV	508683	736824	89.68%	16.389%
7	11.061	1631	1636	1653	rBV	417415	577826	70.33%	12.853%
8	12.006	1785	1791	1799	rBV	525220	703663	85.64%	15.651%
9	13.402	2017	2020	2029	rVB4	8457	12171	1.48%	0.271%
10	13.683	2059	2066	2068	rBV6	4843	9311	1.13%	0.207%
11	13.817	2084	2088	2094	rVB6	4738	9622	1.17%	0.214%
12	14.018	2116	2121	2124	rBV	12523	13211	1.61%	0.294%
13	14.207	2144	2152	2158	rVB5	12232	22552	2.74%	0.502%
14	14.390	2178	2182	2184	rBV5	6647	8986	1.09%	0.200%
15	14.457	2189	2193	2196	rBV4	9829	14633	1.78%	0.325%
16	14.542	2203	2207	2212	rBV7	5774	9512	1.16%	0.212%
17	14.597	2212	2216	2222	rBV5	11138	19412	2.36%	0.432%
18	14.737	2236	2239	2242	rVB	12056	12833	1.56%	0.285%
19	14.823	2250	2253	2260	rVB8	6501	10488	1.28%	0.233%
20	15.390	2343	2346	2353	rVB7	5902	9177	1.12%	0.204%
21	15.463	2353	2358	2362	rBV8	5688	11438	1.39%	0.254%




Sum of corrected areas: 4495821

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110325\
Data File : VX048466.D
Acq On : 03 Nov 2025 18:25
Operator : JC/MD
Sample : Q3521-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TANK-2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102925W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

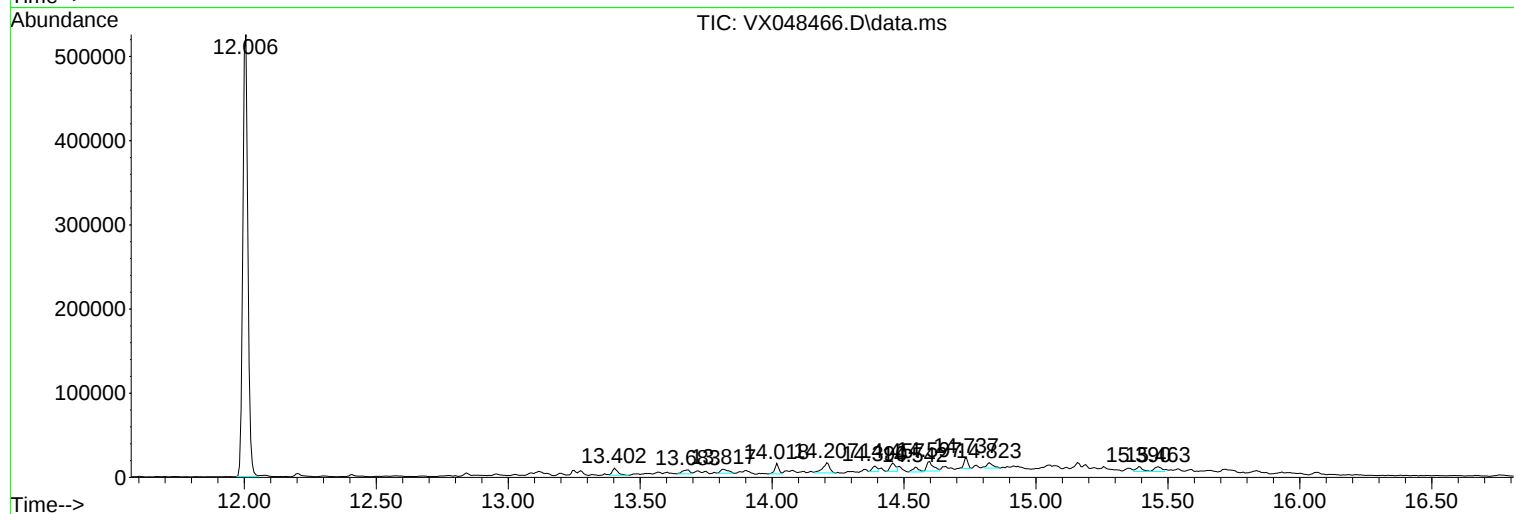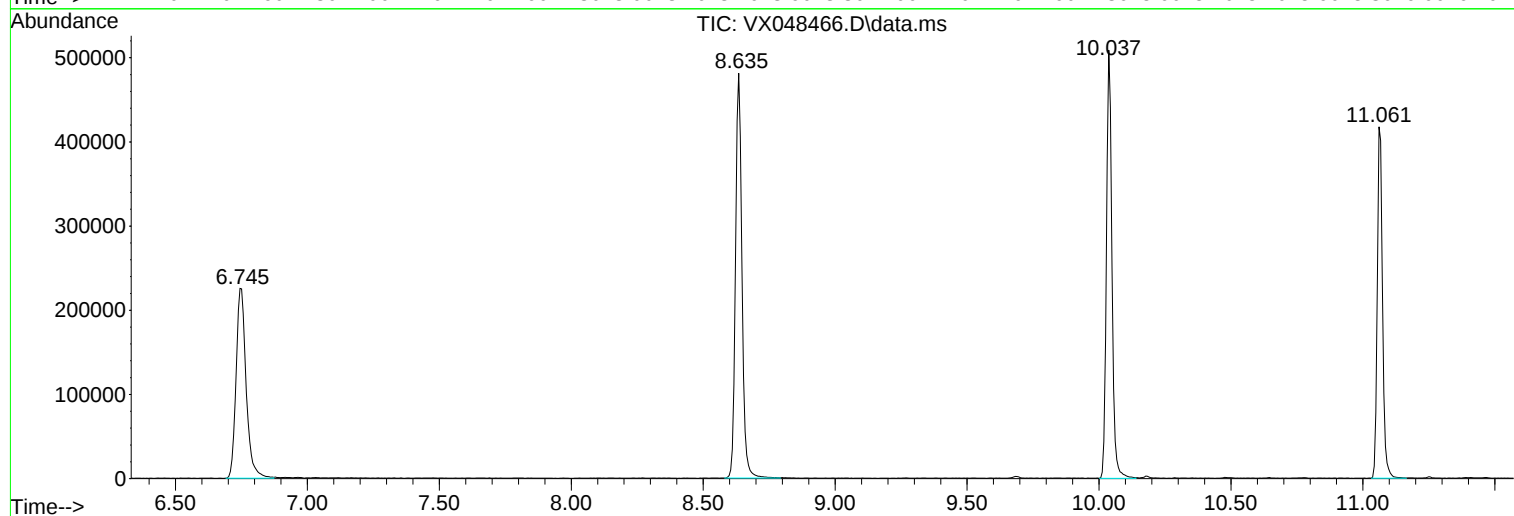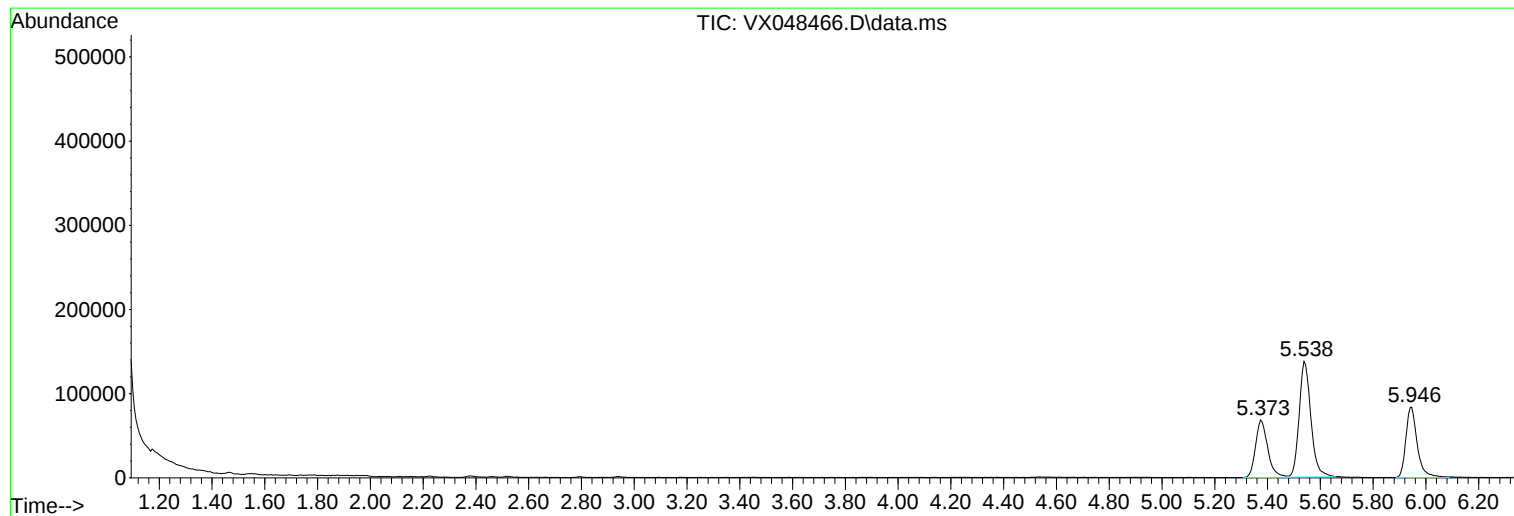

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110325\
Data File : VX048466.D
Acq On : 03 Nov 2025 18:25
Operator : JC/MD
Sample : Q3521-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TANK-2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102925W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110325\
Data File : VX048466.D
Acq On : 03 Nov 2025 18:25
Operator : JC/MD
Sample : Q3521-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TANK-2025

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102925W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------