


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110419\
Data File : VX013318.D
Acq On : 04 Nov 2019 09:23
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Title : SW846 8260
Last Update : Sat Nov 02 07:06:38 2019

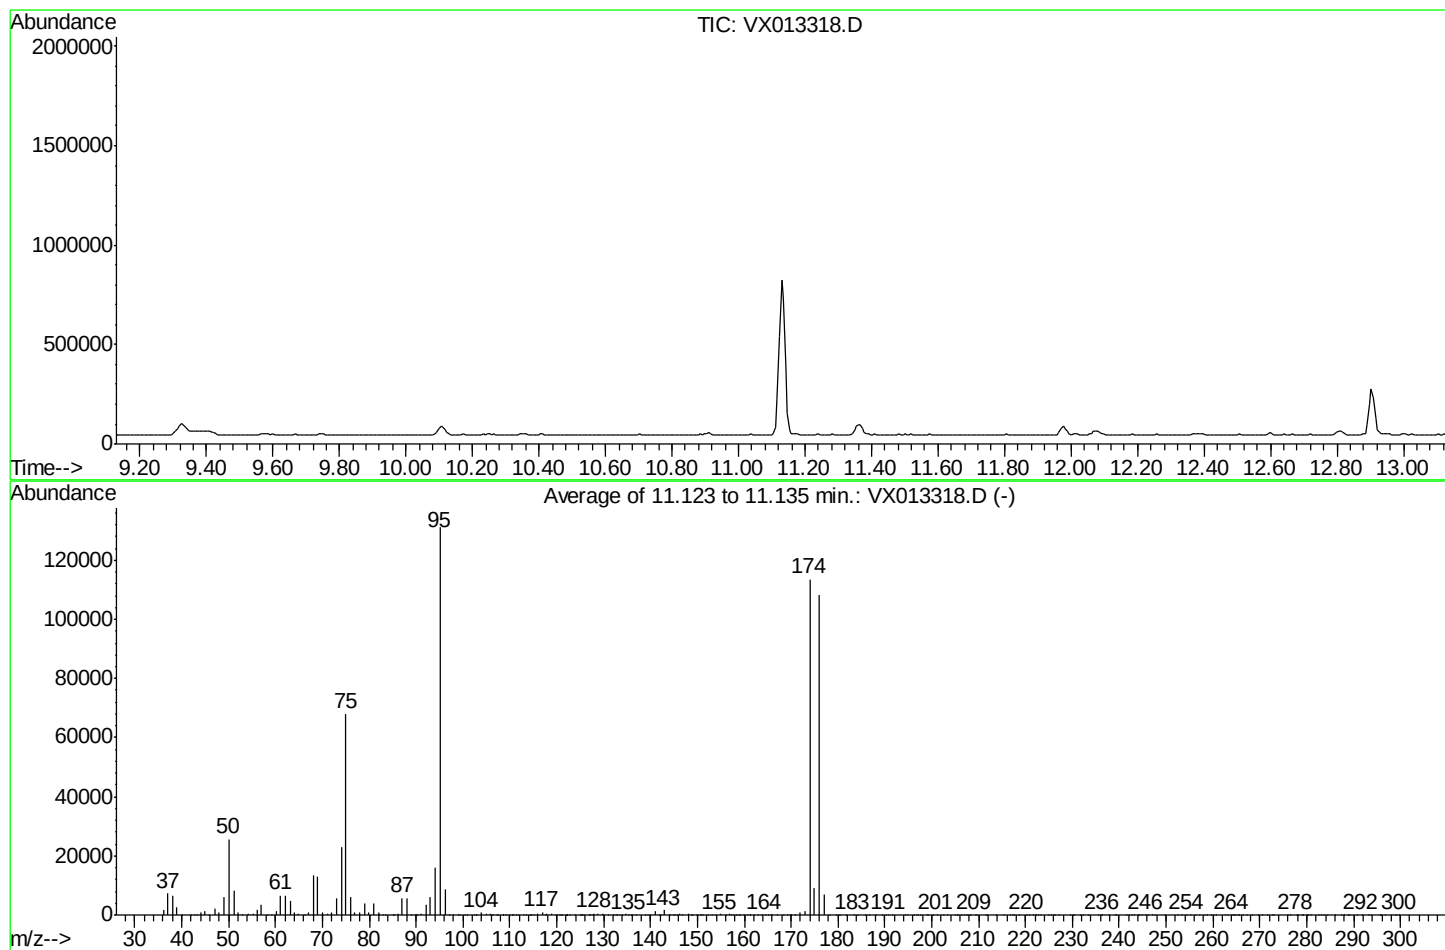

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	25612	PASS
75	95	30	60	51.9	68037	PASS
95	95	100	100	100.0	131105	PASS
96	95	5	9	6.6	8676	PASS
173	174	0.00	2	1.3	1464	PASS
174	95	50	100	86.6	113585	PASS
175	174	5	9	7.9	8962	PASS
176	174	95	101	95.3	108205	PASS
177	176	5	9	6.5	7054	PASS