


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX110420\
Data File : VX019234.D
Acq On : 03 Nov 2020 15:23
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102720W.M
Title : SW846 8260
Last Update : Tue Oct 27 13:55:07 2020

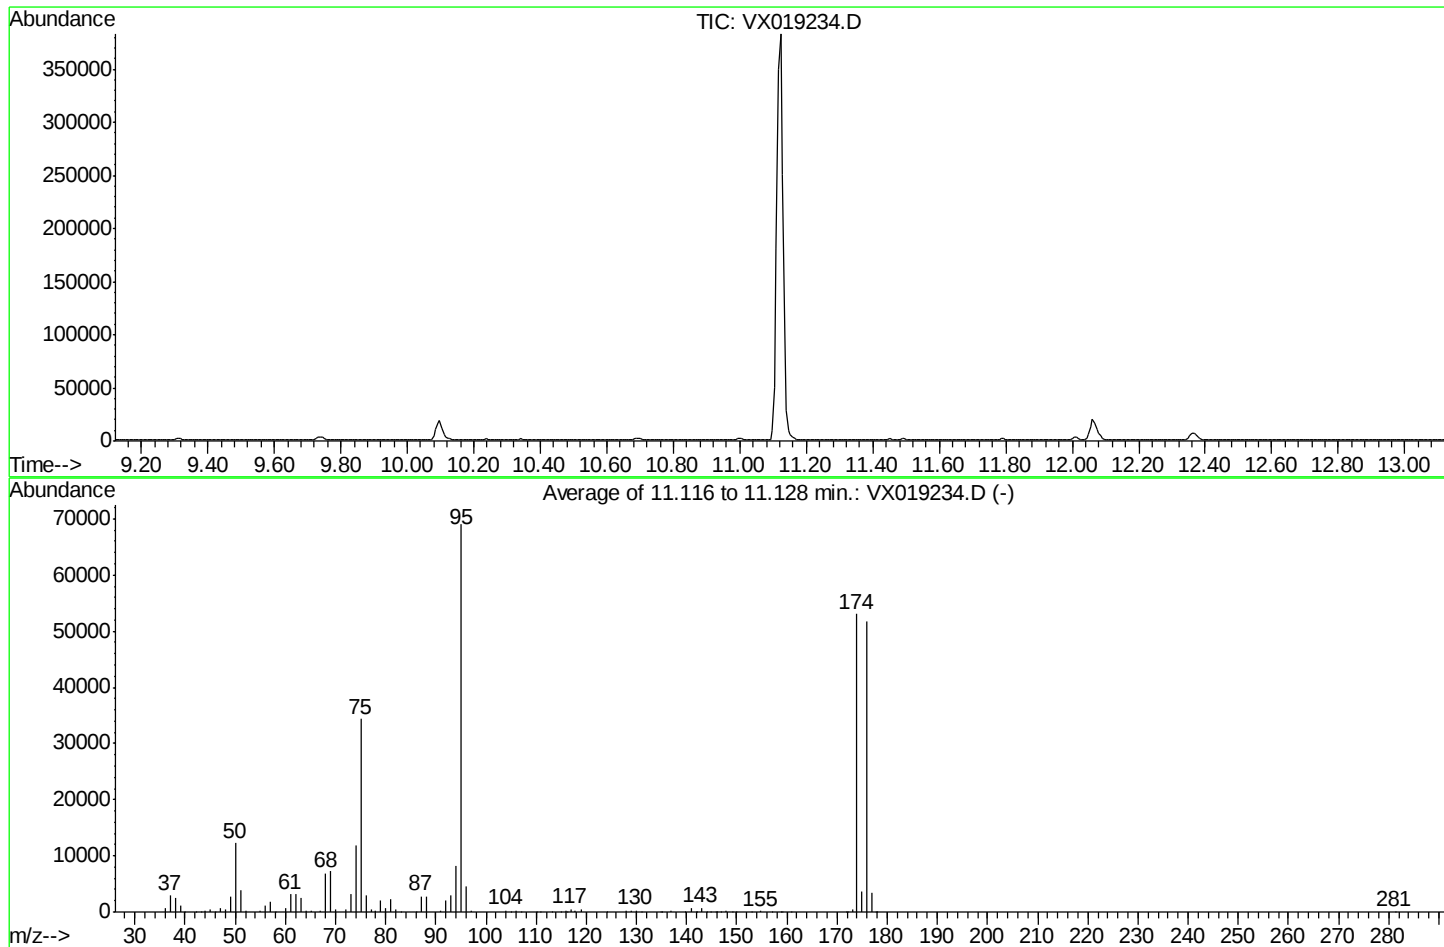

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	12232	PASS
75	95	30	60	49.7	34312	PASS
95	95	100	100	100.0	69026	PASS
96	95	5	9	6.8	4665	PASS
173	174	0.00	2	0.8	445	PASS
174	95	50	100	76.9	53058	PASS
175	174	5	9	7.0	3693	PASS
176	174	95	101	97.7	51821	PASS
177	176	5	9	6.5	3390	PASS