


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110421\
 Data File : VX025069.D
 Acq On : 04 Nov 2021 11:02
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X110421W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Nov 03 23:52:56 2021

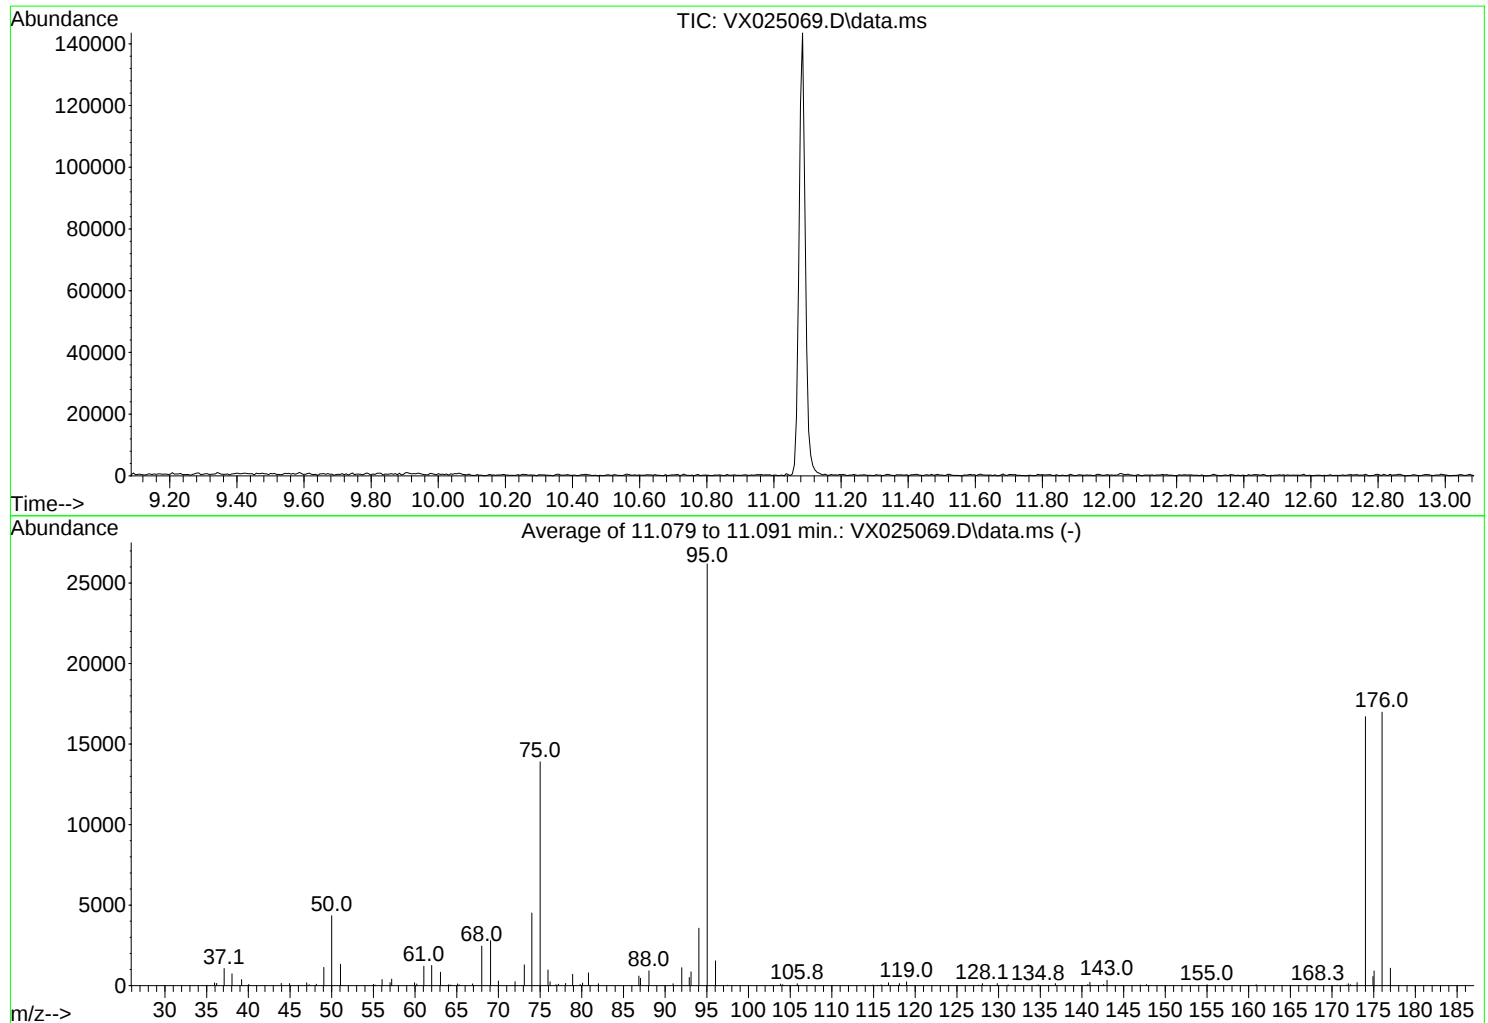

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	4340	PASS
75	95	30	60	53.1	13906	PASS
95	95	100	100	100.0	26195	PASS
96	95	5	9	5.9	1541	PASS
173	174	0.00	2	1.1	191	PASS
174	95	50	100	63.8	16701	PASS
175	174	5	9	5.5	919	PASS
176	174	95	101	101.7	16984	FAIL*
177	176	5	9	6.4	1083	PASS