

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX110518\
 Data File : VX005779.D
 Acq On : 05 Nov 2018 15:37
 Operator : JC/MD
 Sample : J5794-08
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 06 00:45:05 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103118W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 31 18:23:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	137153	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	228376	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	207648	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	90020	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	103970	51.85	ug/l	0.00
Spiked Amount			Recovery	=	103.70%	
35) Dibromofluoromethane	5.50	113	79981	50.58	ug/l	0.00
Spiked Amount			Recovery	=	101.16%	
50) Toluene-d8	8.71	98	286947	51.74	ug/l	0.00
Spiked Amount			Recovery	=	103.48%	
62) 4-Bromofluorobenzene	11.14	95	90609	44.27	ug/l	0.00
Spiked Amount			Recovery	=	88.54%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Chloroethane	1.71	64	46	Below Cal	#	42
8) Diethyl Ether	2.19	74	457	0.407	ug/l	75
10) Methyl Iodide	2.51	142	81	1.993	ug/l #	68
11) Tert butyl alcohol	3.03	59	588	1.080	ug/l #	80
13) Acrolein	2.29	56	74	12.364	ug/l #	1
16) Acetone	2.44	43	7678	Below Cal		99
18) Methyl Acetate	2.78	43	3568	1.240	ug/l	92
20) Methylene Chloride	2.85	84	42171	24.388	ug/l	98
25) 2-Butanone	4.70	43	1300	0.769	ug/l #	88
29) Tetrahydrofuran	5.16	42	585	0.567	ug/l #	66
30) Chloroform	5.21	83	1573	0.502	ug/l	85
31) Cyclohexane	5.65	56	3375	1.260	ug/l #	1
36) 1,1-Dichloropropene	5.67	75	11583	4.760	ug/l #	49
38) Carbon Tetrachloride	5.66	117	13559	6.168	ug/l #	15
40) Benzene	6.14	78	1777	0.245	ug/l #	75
43) Isopropyl Acetate	6.46	43	104757	23.251	ug/l	99
47) Bromodichloromethane	7.90	83	643	0.289	ug/l #	89
48) Methyl methacrylate	7.68	41	3888	1.783	ug/l #	28
51) 4-Methyl-2-Pentanone	8.62	43	1580	0.514	ug/l #	38
56) Ethyl methacrylate	9.04	69	85	2.499	ug/l #	1
59) 2-Hexanone	9.54	43	5370	2.148	ug/l	65
76) 1,2,3-Trichloropropane	11.14	75	47579	21.221	ug/l #	36
81) trans-1,4-Dichloro-2-buten	11.14	75	47579	68.564	ug/l #	9
84) 1,2,4-Trimethylbenzene	11.80	105	1383	0.272	ug/l	100
95) Naphthalene	13.83	128	20686	3.295	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX110518\
Data File : VX005779.D
Acq On : 05 Nov 2018 15:37
Operator : JC/MD
Sample : J5794-08
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 06 00:45:05 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X103118W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 31 18:23:06 2018
Response via : Initial Calibration

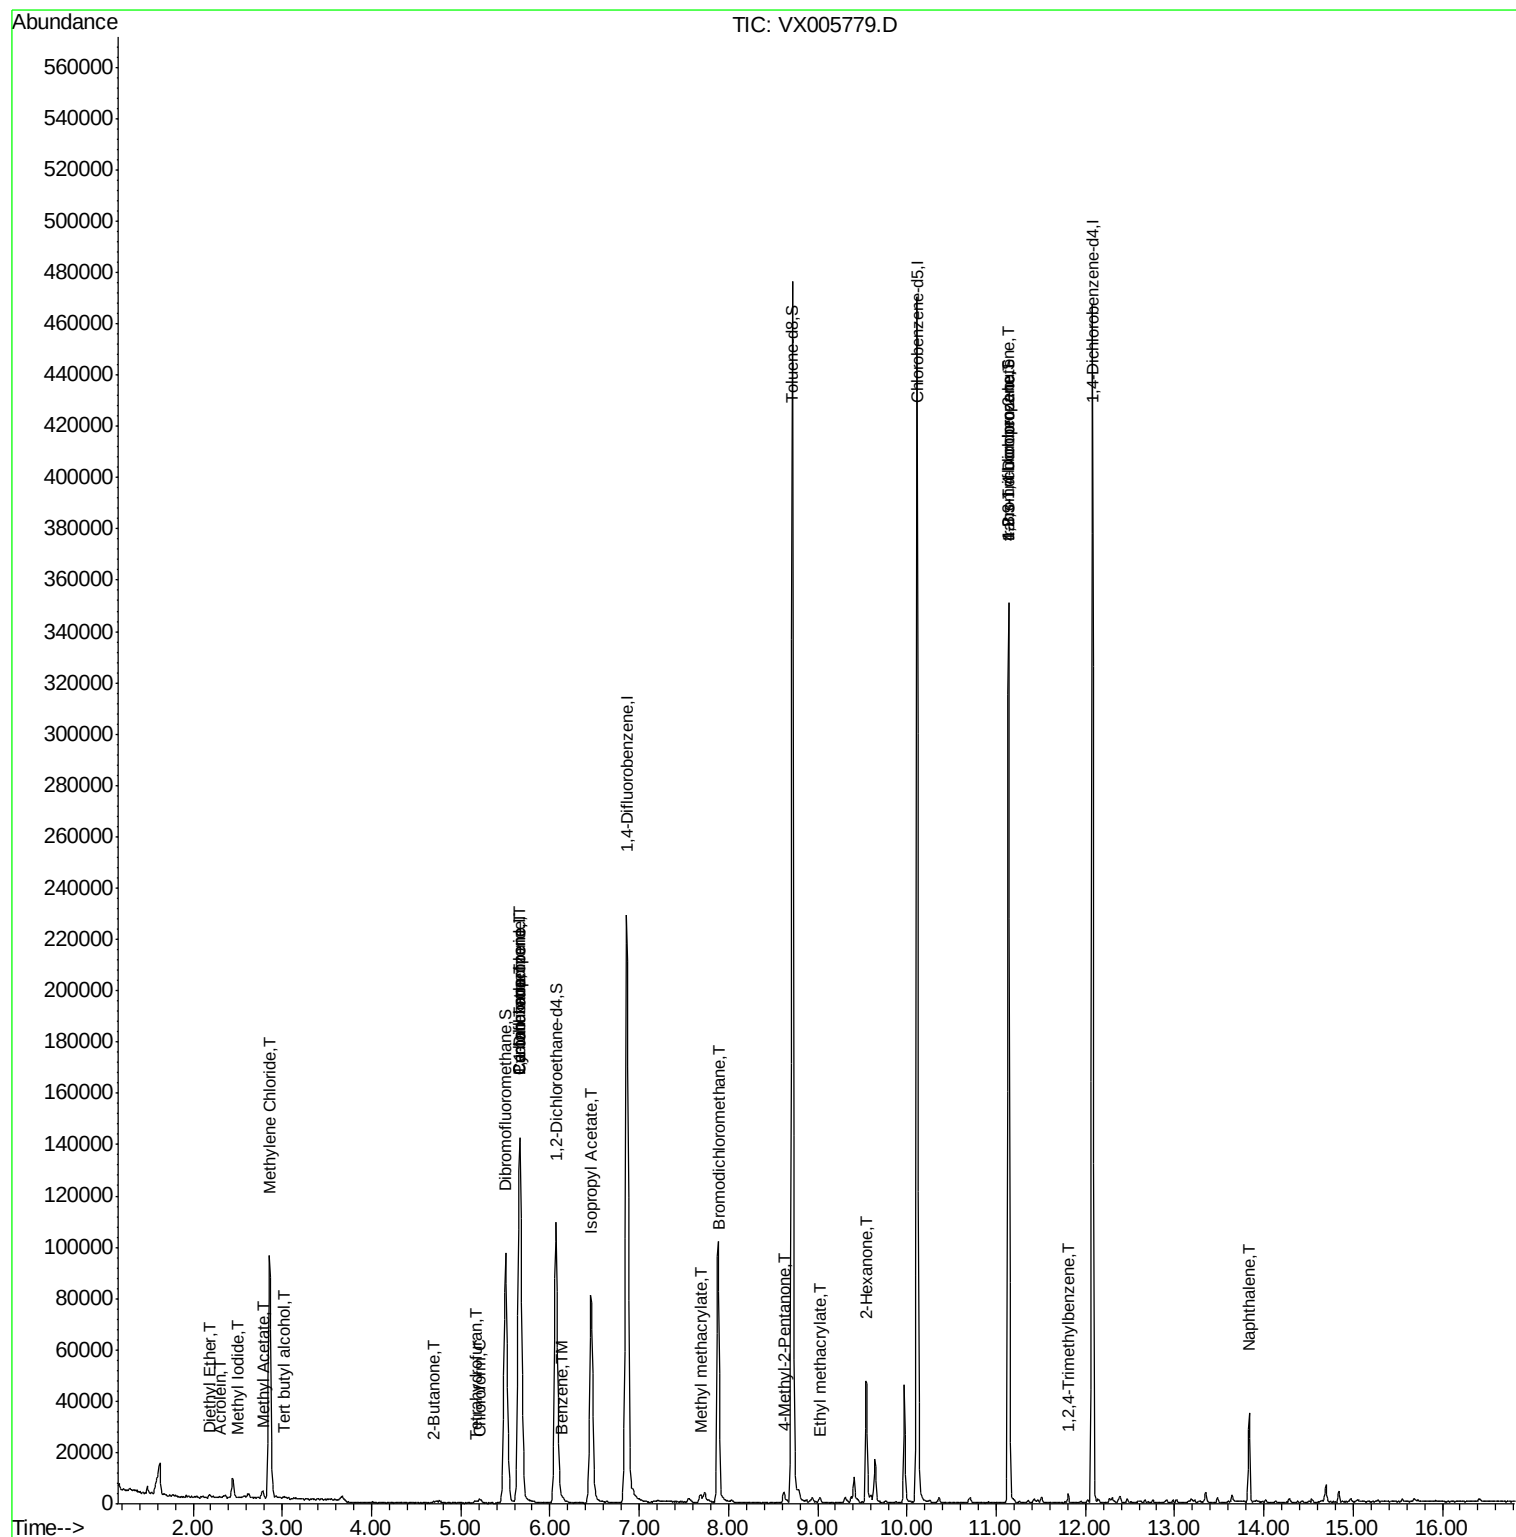



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. 0.00 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37

Instrument :

MSVOA_X


ClientSampled :

Tot Ion:168 Resp: 137153

Ion Ratio Lower Upper

168 100

99 57.2 40.7 61.1

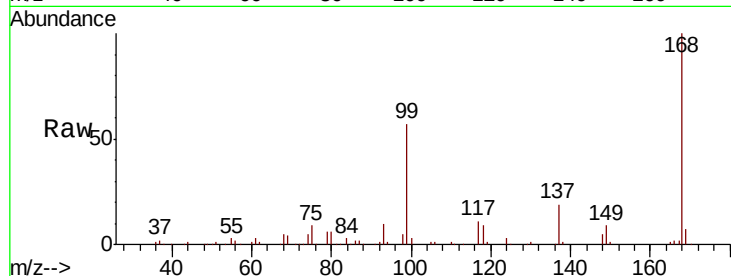

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

40000



30000

20000

10000

0

Time--> 5.50 5.60 5.70 5.80



#6

Chloroethane

Concen: Below Cal

RT: 1.71 min Scan# 91

Delta R.T. -0.01 min

Lab File: VX005779.D


Acq: 05 Nov 2018 15:37

Tgt Ion: 64 Resp: 46

Ion Ratio Lower Upper

64 100

66 0.0 25.8 38.6#



Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

1.71


60


40

20

0

Time--> 1.70 1.71 1.72 1.73



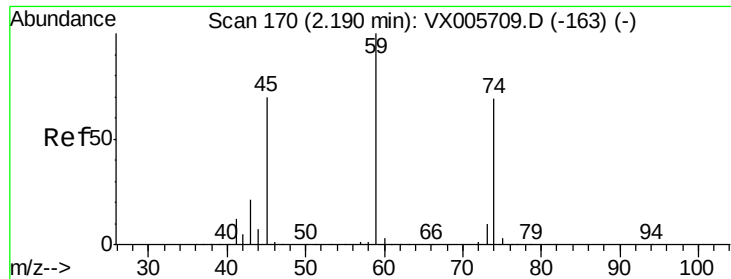

#8

Diethyl Ether

Concen: 0.407 ug/l

RT: 2.19 min Scan# 170

Delta R.T. 0.00 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 74 Resp: 457

Ion Ratio Lower Upper

74 100

45 82.1 54.1 162.3

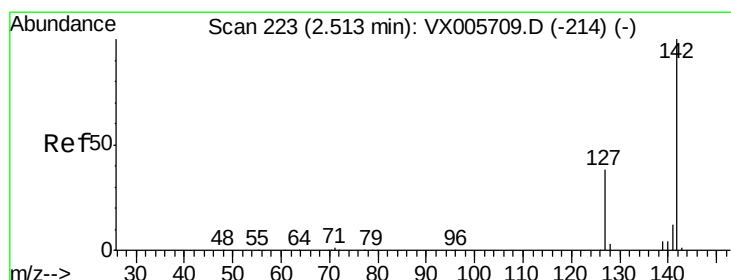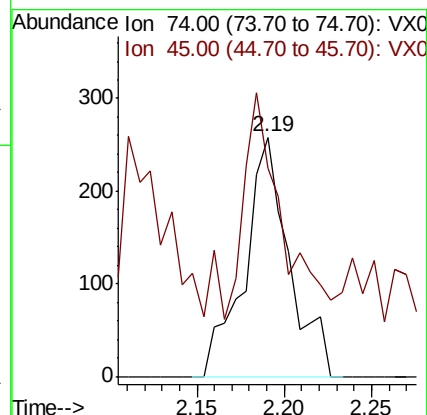

#10

Methyl Iodide

Concen: 1.993 ug/l

RT: 2.51 min Scan# 223

Delta R.T. 0.00 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37




Tgt Ion: 142 Resp: 81


Ion Ratio Lower Upper

142 100

127 24.7 36.0 54.0#

141 0.0 11.7 17.5#

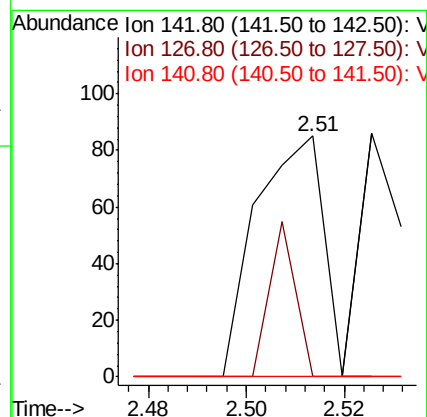




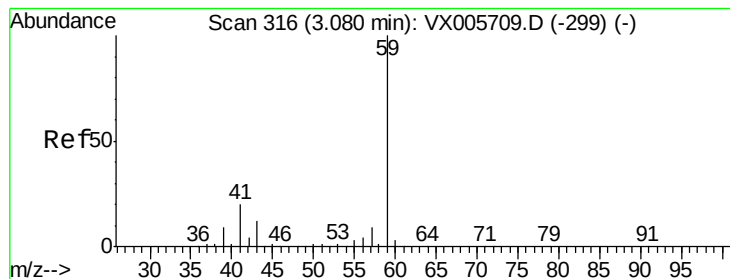


#11

Tert butyl alcohol
 Concen: 1.080 ug/l
 RT: 3.03 min Scan# 307
 Delta R.T. -0.05 min
 Lab File: VX005779.D
 Acq: 05 Nov 2018 15:37

Instrument :
 MSVOA_X
 ClientSampled :




Tot Ion: 59 Resp: 588
 Ion Ratio Lower Upper
 59 100
 57 3.2 8.5 12.7#

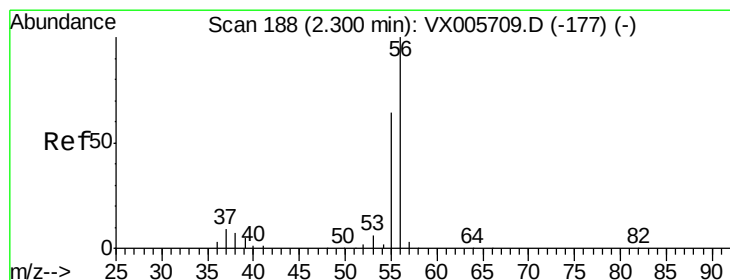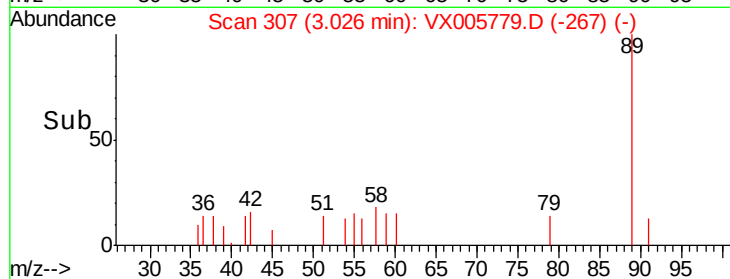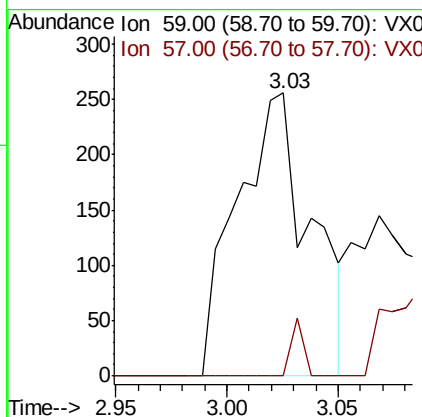


#13

Acrolein
 Concen: 12.364 ug/l
 RT: 2.29 min Scan# 187
 Delta R.T. -0.01 min
 Lab File: VX005779.D
 Acq: 05 Nov 2018 15:37

Tgt Ion: 56 Resp: 74
 Ion Ratio Lower Upper
 56 100
 55 225.7 57.3 85.9#

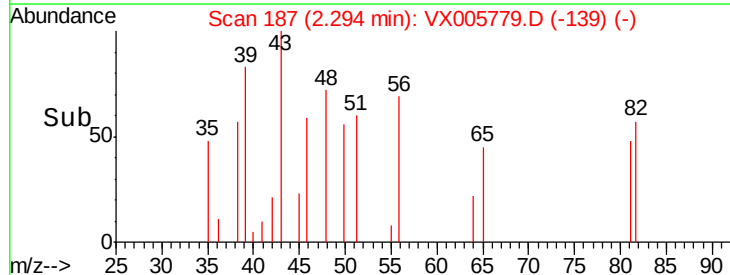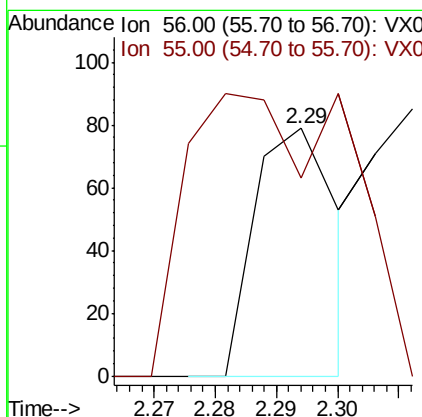

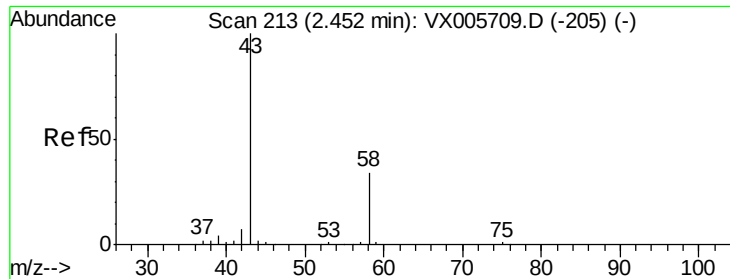

#16

Acetone

Concen: Below Cal

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37

Instrument :

MSVOA_X


ClientSampled :

Tot Ion: 43 Resp: 7678

Ion Ratio Lower Upper

43 100

58 30.1 23.8 35.6



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.44

5000

4000

3000



2000

1000

0

2.40 2.45 2.50 2.55

Time-->

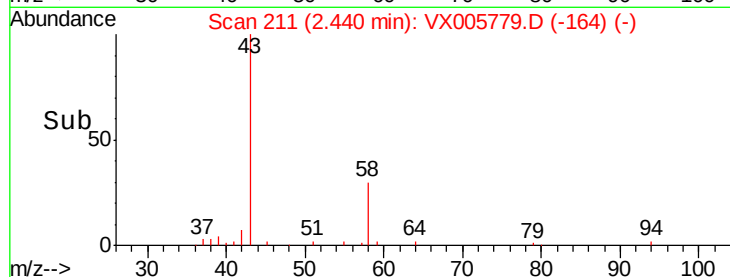

#18

Methyl Acetate

Concen: 1.240 ug/l

RT: 2.78 min Scan# 267

Delta R.T. 0.00 min

Lab File: VX005779.D


Acq: 05 Nov 2018 15:37

Tgt Ion: 43 Resp: 3568

Ion Ratio Lower Upper

43 100

74 24.7 16.8 25.2



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0

2.78

2000

1500


1000


500

0

2.70 2.75 2.80 2.85

Time-->

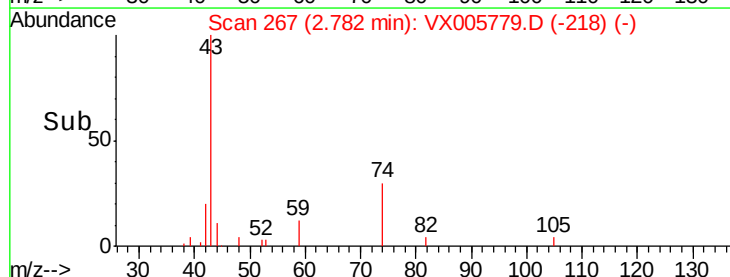


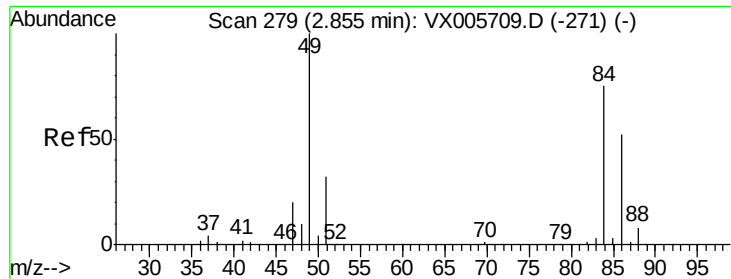




#20
Methvlene Chloride
Concen: 24.388 ug/l
RT: 2.85 min Scan# 279
Delta R.T. 0.00 min
Lab File: VX005779.D
Acq: 05 Nov 2018 15:37

Instrument :
MSVOA_X
ClientSampled :

Tot Ion: 84 Resp: 42171
Ion Ratio Lower Upper
84 100
49 137.9 109.5 164.3
51 45.1 33.3 49.9
86 64.3 52.7 79.1

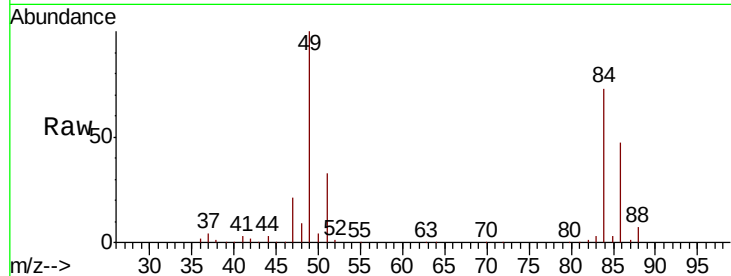


Abundance Ion 83.90 (83.60 to 84.60): VX0
Ion 48.90 (48.60 to 49.60): VX0
Ion 50.90 (50.60 to 51.60): VX0
Ion 85.90 (85.60 to 86.60): VX0

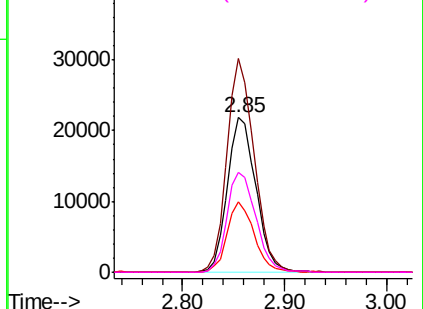




#25
2-Butanone
Concen: 0.769 ug/l
RT: 4.70 min Scan# 581
Delta R.T. -0.01 min
Lab File: VX005779.D
Acq: 05 Nov 2018 15:37

Tgt Ion: 43 Resp: 1300
Ion Ratio Lower Upper
43 100
72 30.0 19.2 28.8#

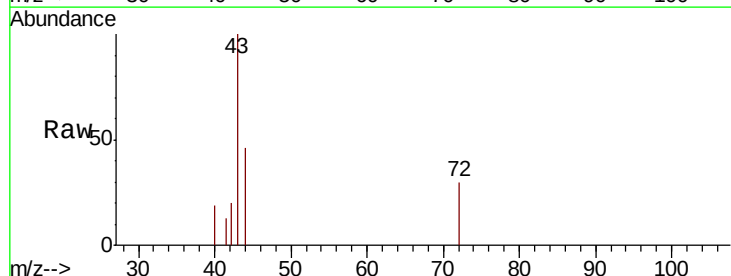

Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 72.00 (71.70 to 72.70): VX0

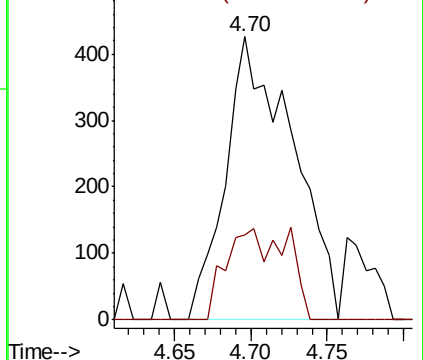

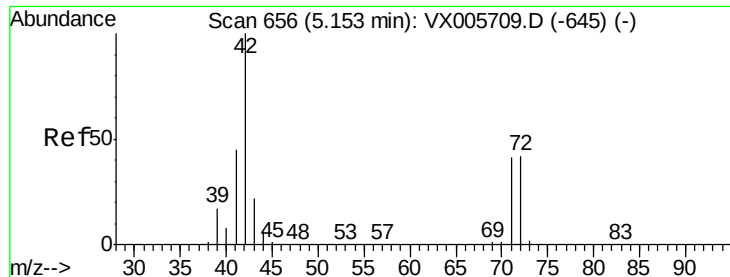

#29

Tetrahydrofuran

Concen: 0.567 ug/l

RT: 5.16 min Scan# 657

Delta R.T. 0.01 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 42 Resp: 585

Ion Ratio Lower Upper

42 100

72 19.0 32.0 48.0#




71 17.4 29.8 44.8#



Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

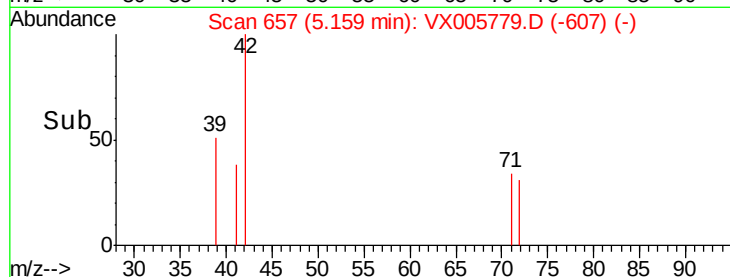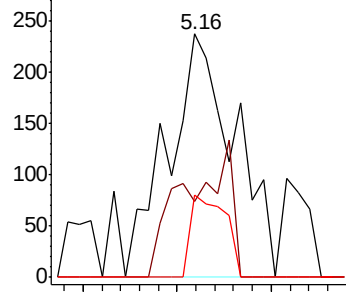

#30

Chloroform

Concen: 0.502 ug/l

RT: 5.21 min Scan# 666

Delta R.T. 0.00 min

Lab File: VX005779.D


Acq: 05 Nov 2018 15:37

Tgt Ion: 83 Resp: 1573

Ion Ratio Lower Upper



83 100


85 75.0 50.6 76.0



Abundance Ion 82.90 (82.60 to 83.60): VX0

Ion 84.90 (84.60 to 85.60): VX0

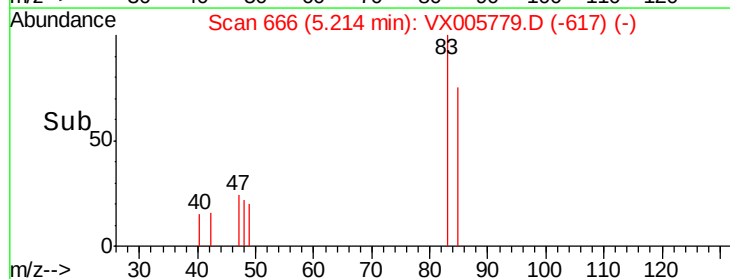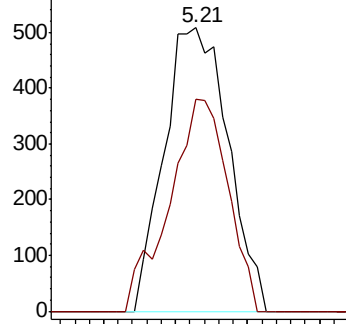

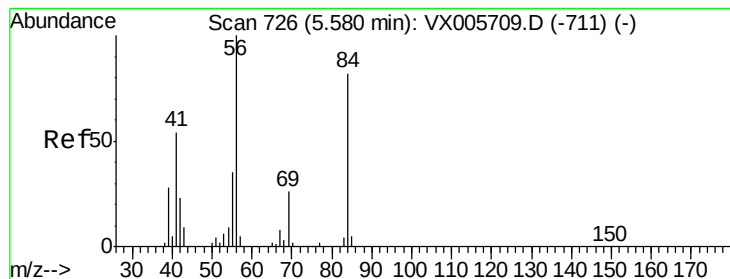

#31

Cyclohexane

Concen: 1.260 ug/l

RT: 5.65 min Scan# 738

Delta R.T. 0.07 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37

Instrument :

MSVOA_X

ClientSampled :


Tot Ion: 56 Resp: 3375

Ion Ratio Lower Upper

56 100

69 175.3 22.6 34.0#




84 120.2 62.7 94.1#



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

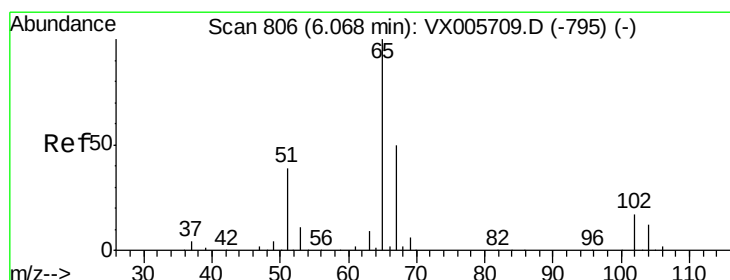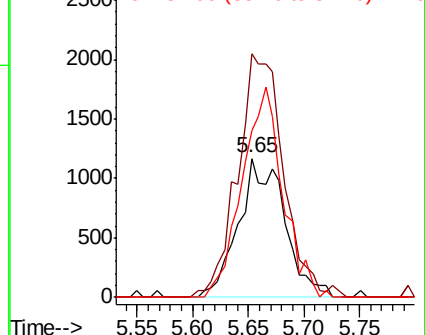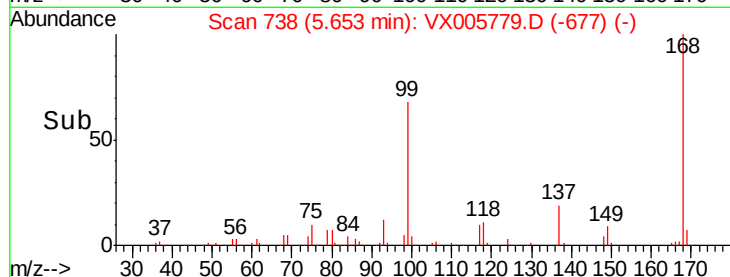

#33

1,2-Dichloroethane-d4

Concen: 51.850 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX005779.D


Acq: 05 Nov 2018 15:37

Tgt Ion: 65 Resp: 103970

Ion Ratio Lower Upper



65 100


67 53.6 0.0 105.0



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

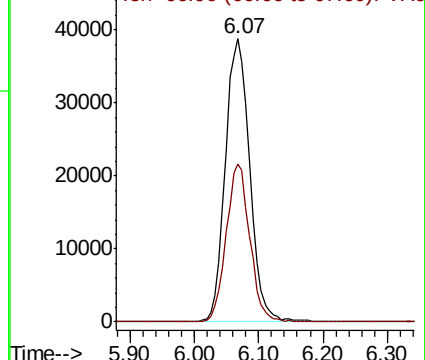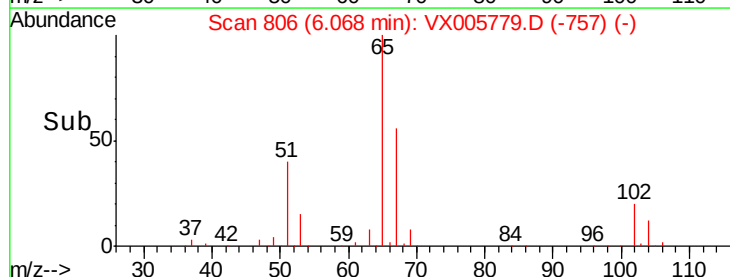

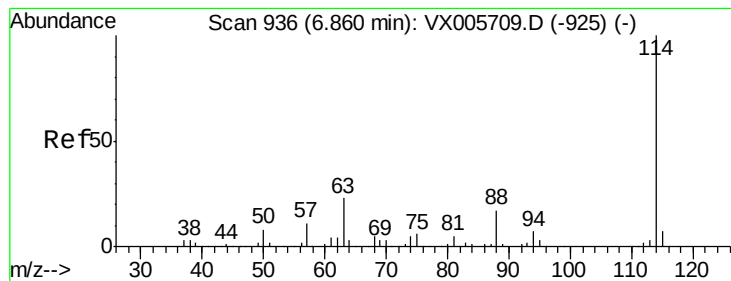

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 935

Delta R.T. -0.01 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:114 Resp: 228376

Ion Ratio Lower Upper

114 100

63 22.7 0.0 42.8




88 17.6 0.0 31.2



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

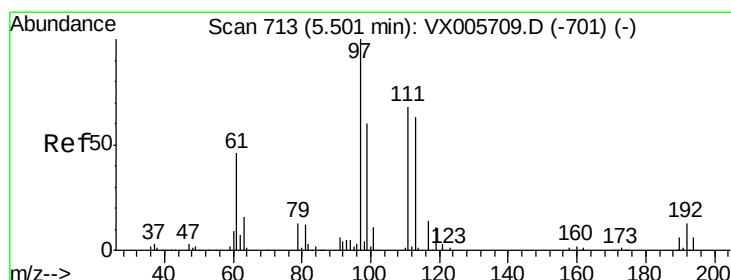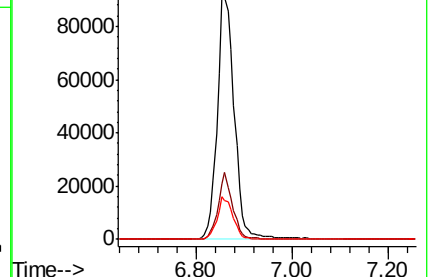

#35

Dibromofluoromethane

Concen: 50.579 ug/l

RT: 5.50 min Scan# 713

Delta R.T. 0.00 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37


Tgt Ion:113 Resp: 79981

Ion Ratio Lower Upper

113 100

111 98.5 82.3 123.5



192 20.5 17.9 26.9




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

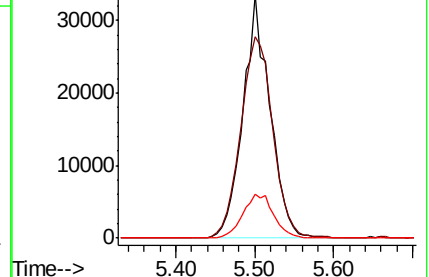


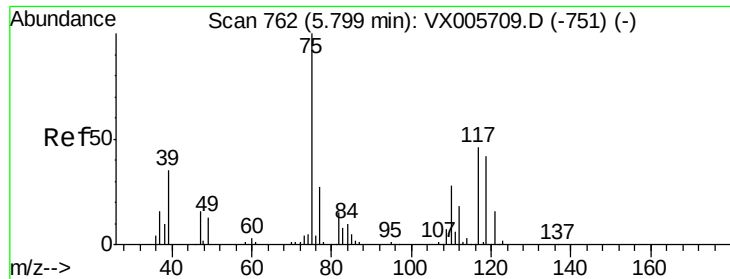




#36
 1,1-Dichloropropene
 Concen: 4.760 ug/l
 RT: 5.67 min Scan# 740
 Delta R.T. -0.13 min
 Lab File: VX005779.D
 Acq: 05 Nov 2018 15:37

Instrument :
 MSVOA_X
 ClientSampleId :

Tot Ion: 75 Resp: 11583
 Ion Ratio Lower Upper
 75 100
 110 8.9 17.4 52.2#
 77 0.0 25.8 38.6#

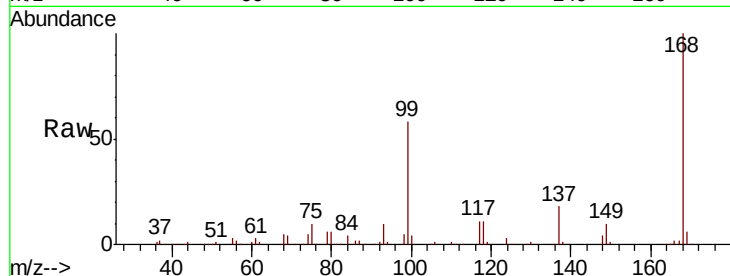


Abundance Ion 74.90 (74.60 to 75.60): VX0
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.90 (76.60 to 77.60): VX0

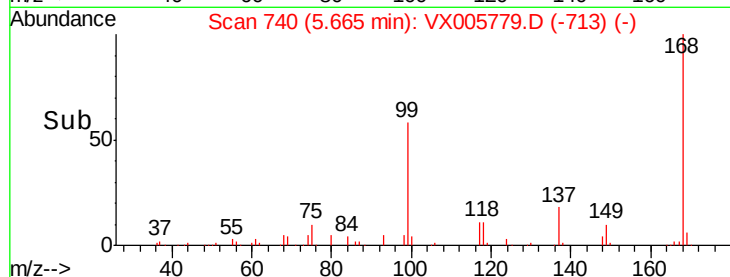
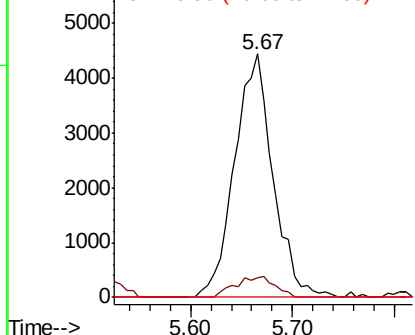



#38
 Carbon Tetrachloride
 Concen: 6.168 ug/l
 RT: 5.66 min Scan# 739
 Delta R.T. -0.13 min
 Lab File: VX005779.D
 Acq: 05 Nov 2018 15:37

Tgt Ion: 117 Resp: 13559
 Ion Ratio Lower Upper
 117 100
 119 5.4 78.1 117.1#
 121 0.0 24.6 36.8#



Abundance Ion 116.80 (116.50 to 117.50): V
 Ion 118.80 (118.50 to 119.50): V
 Ion 120.80 (120.50 to 121.50): V

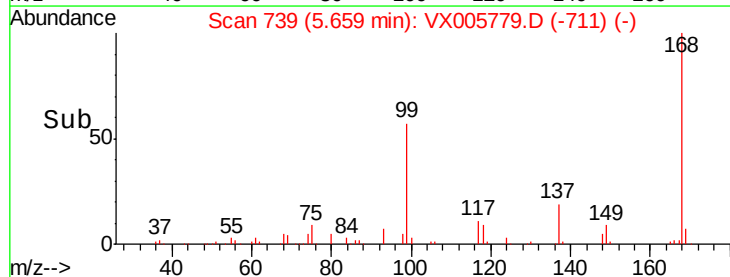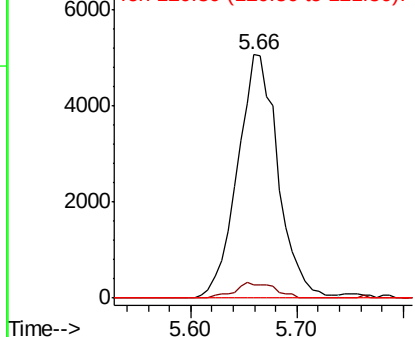



#40

Benzene

Concen: 0.245 ug/l

RT: 6.14 min Scan# 818

Delta R.T. 0.00 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37

Instrument :

MSVOA_X





ClientSampleId :

Tot Ion: 78 Resp: 1777

Ion Ratio Lower Upper

78 100

77 35.1 18.4 27.6#

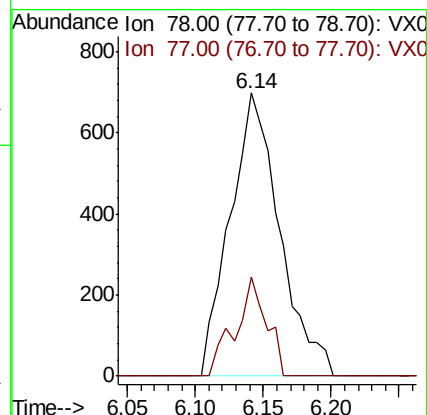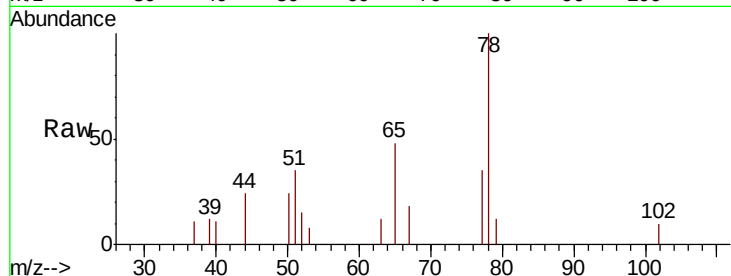

#43

Isopropyl Acetate

Concen: 23.251 ug/l

RT: 6.46 min Scan# 870

Delta R.T. 0.00 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37




Tgt Ion: 43 Resp: 104757


Ion Ratio Lower Upper

43 100

61 18.7 14.6 22.0

87 12.3 9.6 14.4

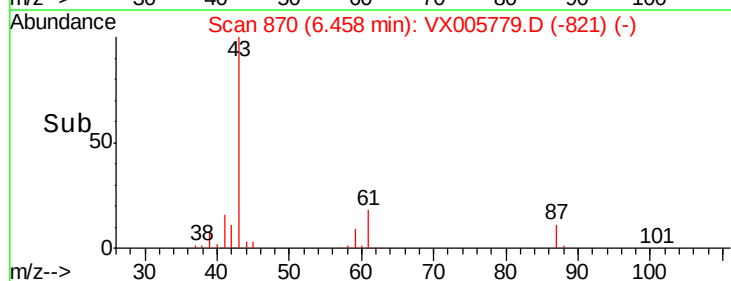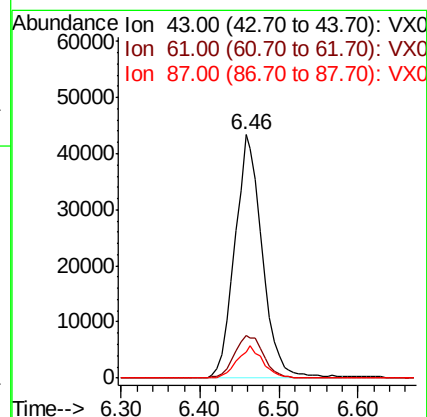

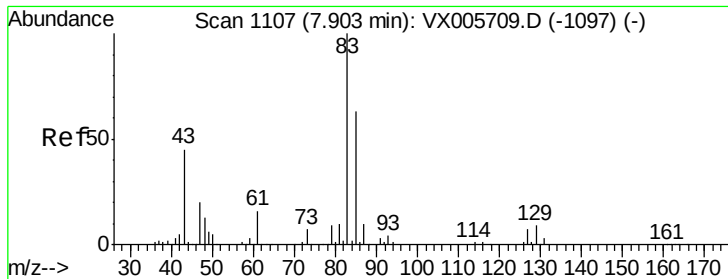

#47

Bromodichloromethane

Concen: 0.289 ug/l

RT: 7.90 min Scan# 1106

Delta R.T. -0.01 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37

Instrument :
MSVOA_X
ClientSampled :


Tot Ion: 83 Resp: 643

Ion Ratio Lower Upper




83 100

85 55.9 50.2 75.4

127 0.0 6.9 10.3#

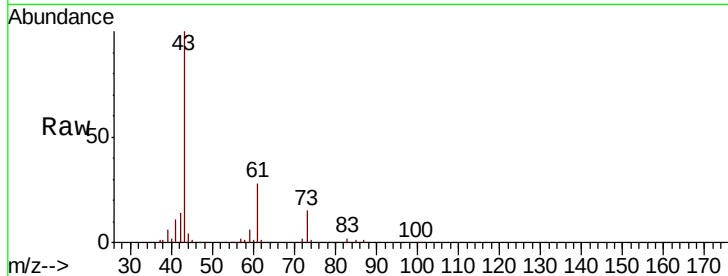

Abundance Ion 82.90 (82.60 to 83.60): VX0
Ion 84.90 (84.60 to 85.60): VX0
Ion 126.80 (126.50 to 127.50): V

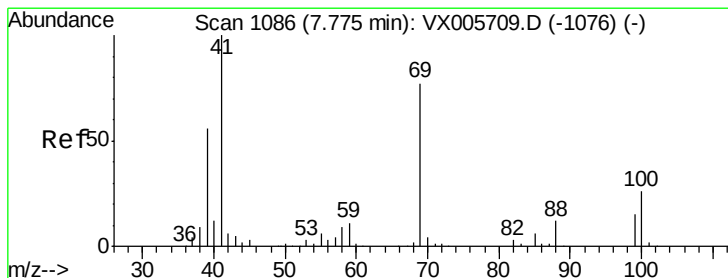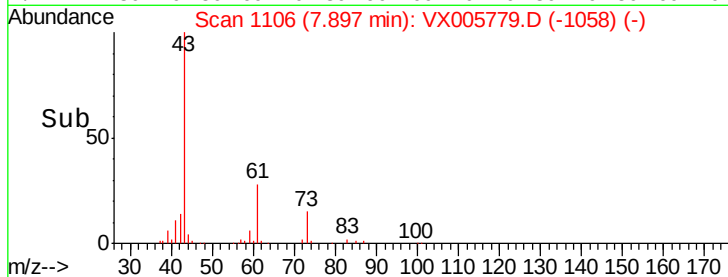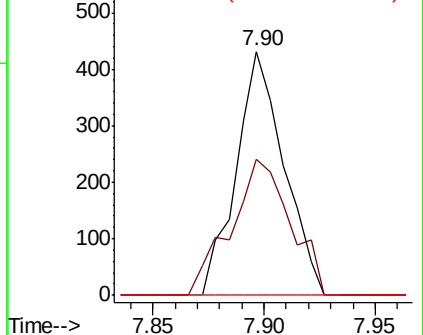

#48

Methyl methacrylate

Concen: 1.783 ug/l

RT: 7.68 min Scan# 1071

Delta R.T. -0.09 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37


Tgt Ion: 41 Resp: 3888

Ion Ratio Lower Upper



41 100


69 0.0 63.2 94.8#

39 20.3 42.2 63.2#

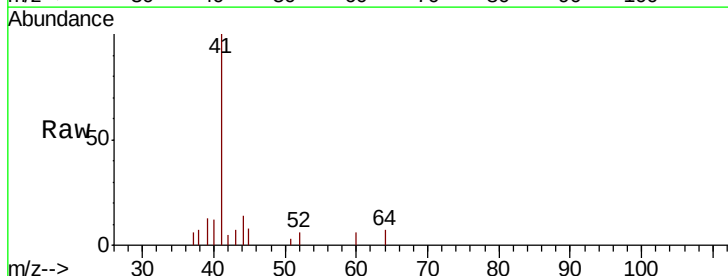

Abundance Ion 41.00 (40.70 to 41.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 39.00 (38.70 to 39.70): VX0

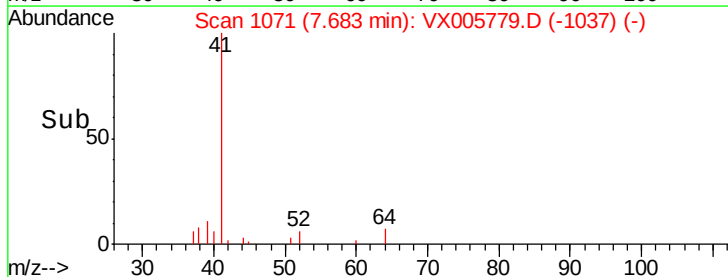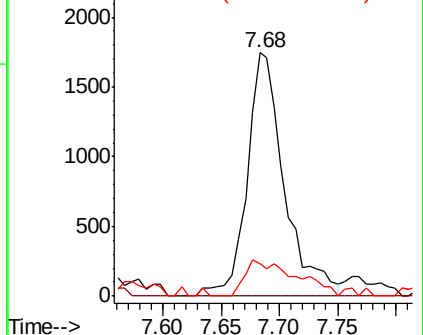



#50

Toluene-d8

Concen: 51.738 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 98 Resp: 286947

Ion Ratio Lower Upper

98 100

100 61.5 51.3 76.9



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

8.71

200000



150000

100000

50000

0

Time-->



#51

4-Methyl-2-Pentanone

Concen: 0.514 ug/l

RT: 8.62 min Scan# 1224

Delta R.T. -0.03 min

Lab File: VX005779.D


Acq: 05 Nov 2018 15:37

Tgt Ion: 43 Resp: 1580

Ion Ratio Lower Upper

43 100

58 0.0 29.7 44.5#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

8.62

1000

800


600


400

200

0

Time-->





#56

Ethyl methacrylate

Concen: 2.499 ug/l

RT: 9.04 min Scan# 1293

Delta R.T. -0.15 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion: 69 Resp: 85

Ion Ratio Lower Upper

69 100

41 429.4 57.0 85.6#




39 0.0 28.3 42.5#

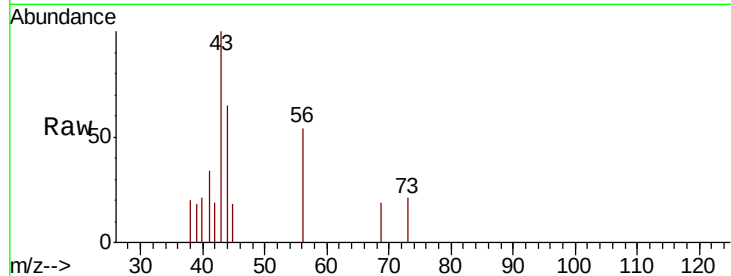

Abundance Ion 69.00 (68.70 to 69.70): VX0

Ion 41.00 (40.70 to 41.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

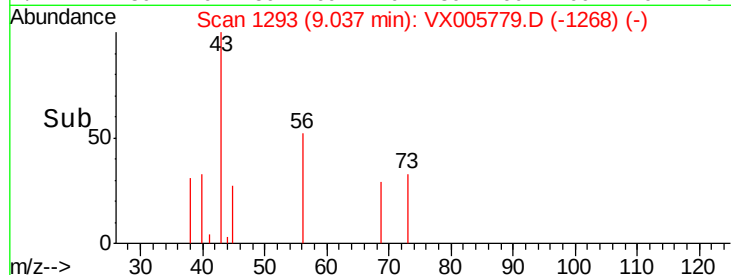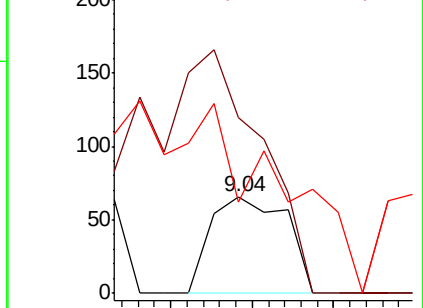

#59

2-Hexanone

Concen: 2.148 ug/l

RT: 9.54 min Scan# 1376

Delta R.T. 0.04 min

Lab File: VX005779.D


Acq: 05 Nov 2018 15:37

Tgt Ion: 43 Resp: 5370

Ion Ratio Lower Upper



43 100


58 27.4 25.9 77.8

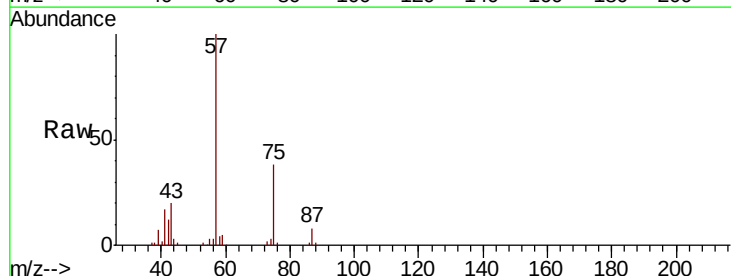

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

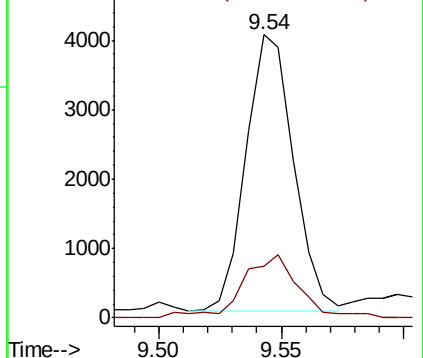


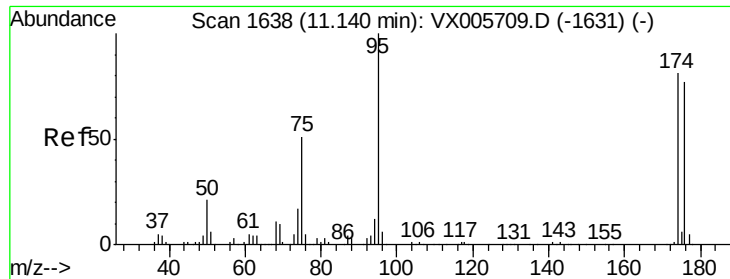




#62
4-Bromofluorobenzene
Concen: 44.266 ug/l
RT: 11.14 min Scan# 1638
Delta R.T. 0.00 min
Lab File: VX005779.D
Acq: 05 Nov 2018 15:37

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion: 95 Resp: 90609
Ion Ratio Lower Upper
95 100
174 80.2 0.0 184.4
176 77.8 0.0 177.4

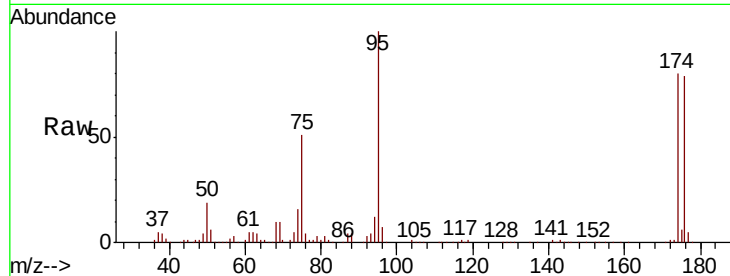


Abundance Ion 94.90 (94.60 to 95.60): VX0
Ion 173.80 (173.50 to 174.50): V
Ion 175.80 (175.50 to 176.50): V

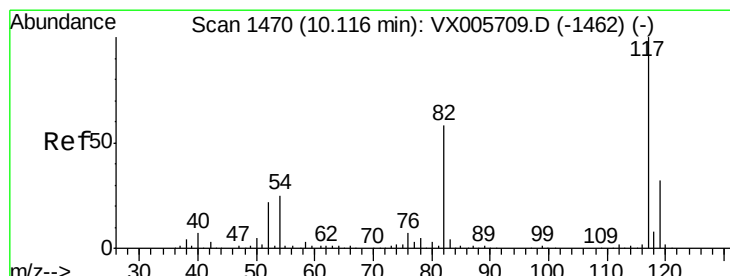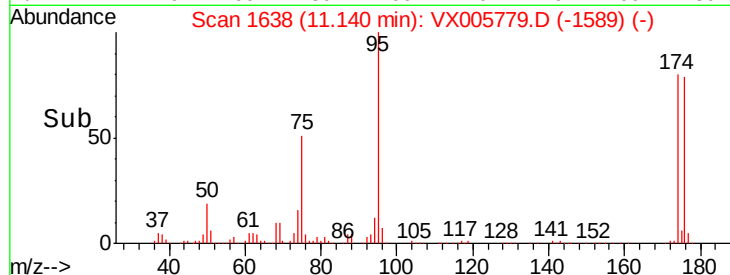
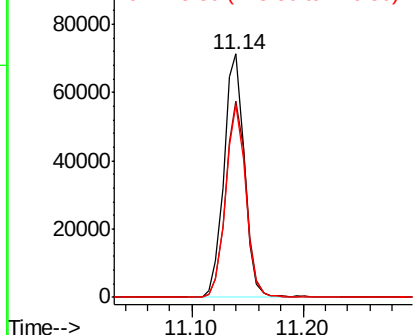



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. 0.00 min
Lab File: VX005779.D
Acq: 05 Nov 2018 15:37

Tgt Ion: 117 Resp: 207648
Ion Ratio Lower Upper
117 100
82 58.5 44.1 66.1
119 32.1 26.2 39.2

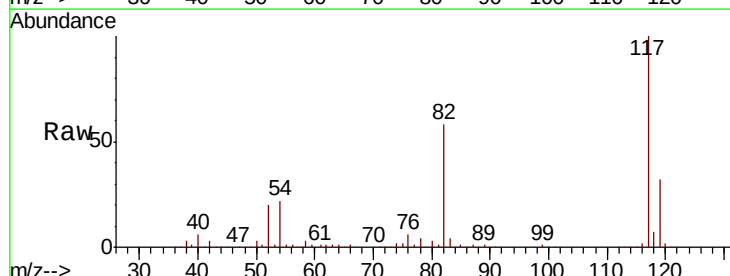

Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

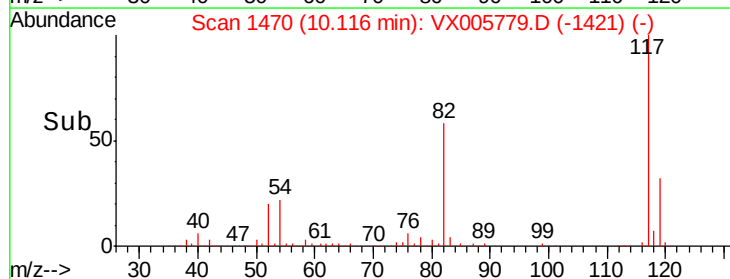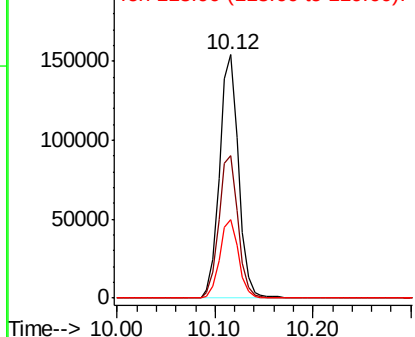

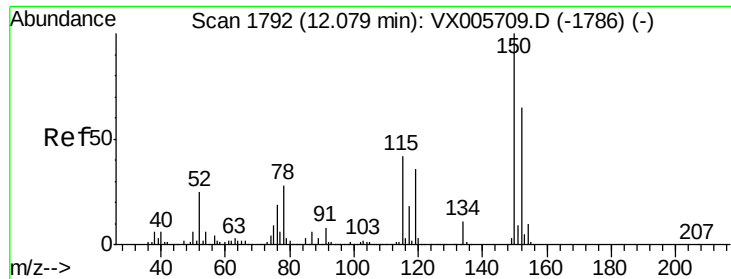

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX005779.D

Acq: 05 Nov 2018 15:37

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:152 Resp: 90020

Ion Ratio Lower Upper

152 100

115 59.5 39.4 118.1




150 157.0 0.0 346.4

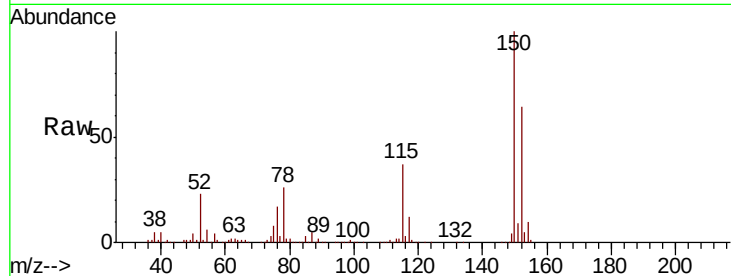

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

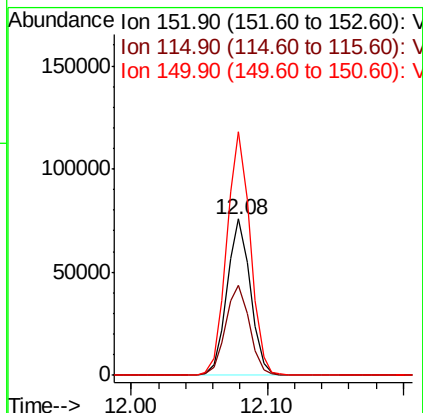

#76

1,2,3-Trichloropropane

Concen: 21.221 ug/l

RT: 11.14 min Scan# 1638

Delta R.T. -0.16 min

Lab File: VX005779.D


Acq: 05 Nov 2018 15:37

Tgt Ion: 75 Resp: 47579

Ion Ratio Lower Upper



75 100


77 1.2 20.5 61.6#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

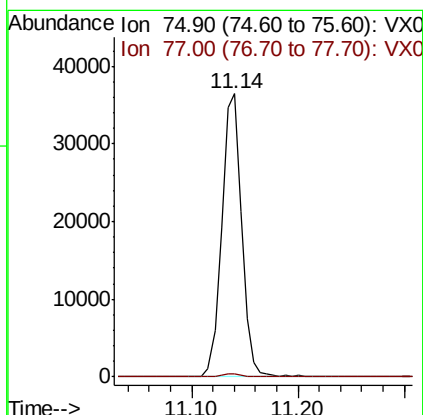


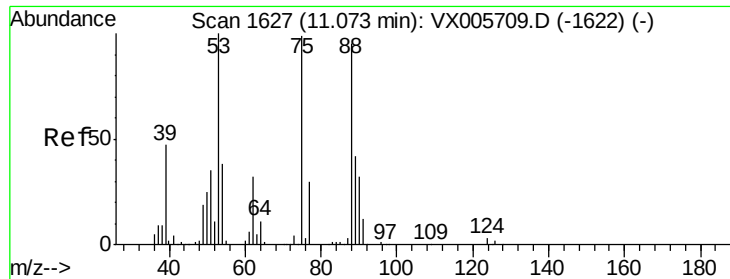




#81
trans-1,4-Dichloro-2-butene
Concen: 68.564 ug/l
RT: 11.14 min Scan# 1638
Delta R.T. 0.07 min
Lab File: VX005779.D
Acq: 05 Nov 2018 15:37

Instrument :
MSVOA_X
ClientSampled :

Tot Ion: 75 Resp: 47579
Ion Ratio Lower Upper
75 100
53 0.3 80.2 120.2#
89 0.0 39.8 59.8#

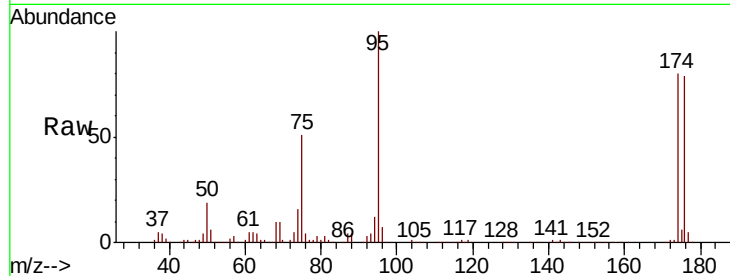


Abundance Ion 74.90 (74.60 to 75.60): VX0
Ion 53.00 (52.70 to 53.70): VX0
Ion 88.90 (88.60 to 89.60): VX0

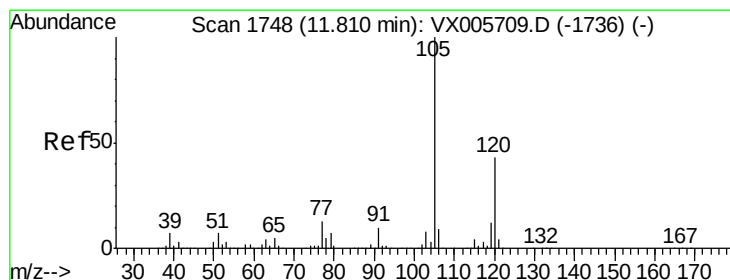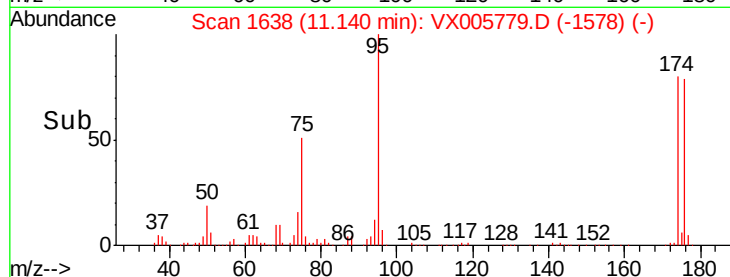
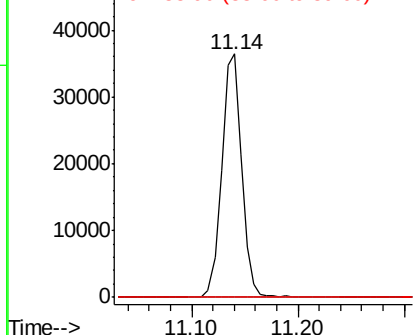



#84
1,2,4-Trimethylbenzene
Concen: 0.272 ug/l
RT: 11.80 min Scan# 1747
Delta R.T. -0.01 min
Lab File: VX005779.D
Acq: 05 Nov 2018 15:37

Tgt Ion: 105 Resp: 1383
Ion Ratio Lower Upper
105 100
120 44.6 22.4 67.0



Abundance Ion 105.00 (104.70 to 105.70): V
Ion 120.00 (119.70 to 120.70): V

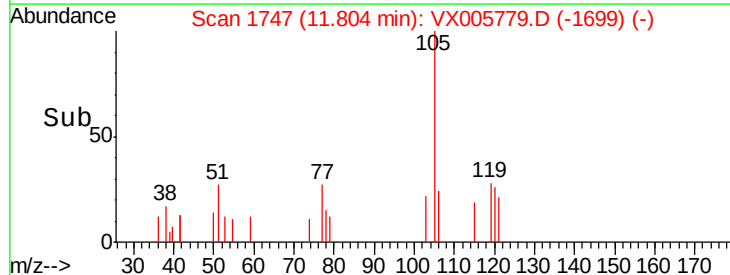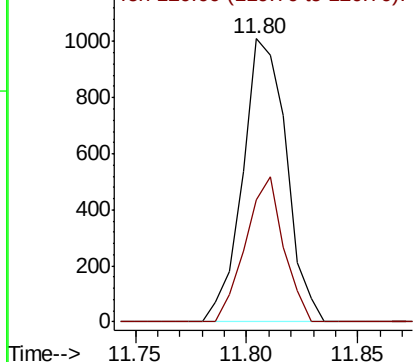

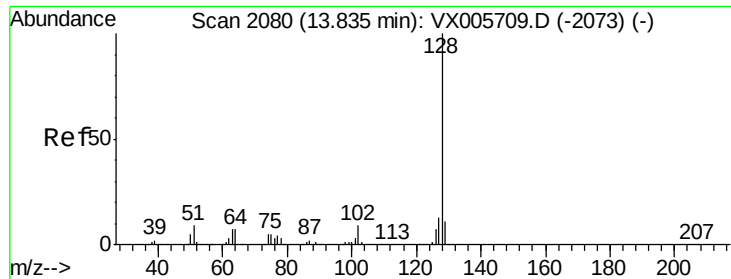

#95
Naphthalene
Concen: 3.295 ug/l
RT: 13.83 min Scan# 2080
Delta R.T. 0.00 min
Lab File: VX005779.D
Acq: 05 Nov 2018 15:37

Instrument :
MSVOA_X
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
128	100		
127	13.9	10.4	15.6
129	11.0	8.7	13.1

