


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX110520\
 Data File : VX019262.D
 Acq On : 04 Nov 2020 08:51
 Operator : JC/MD
 Sample : BFB66
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB66

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXLM110220WMA.M
 Title : VOC Analysis
 Last Update : Thu Nov 05 15:29:53 2020

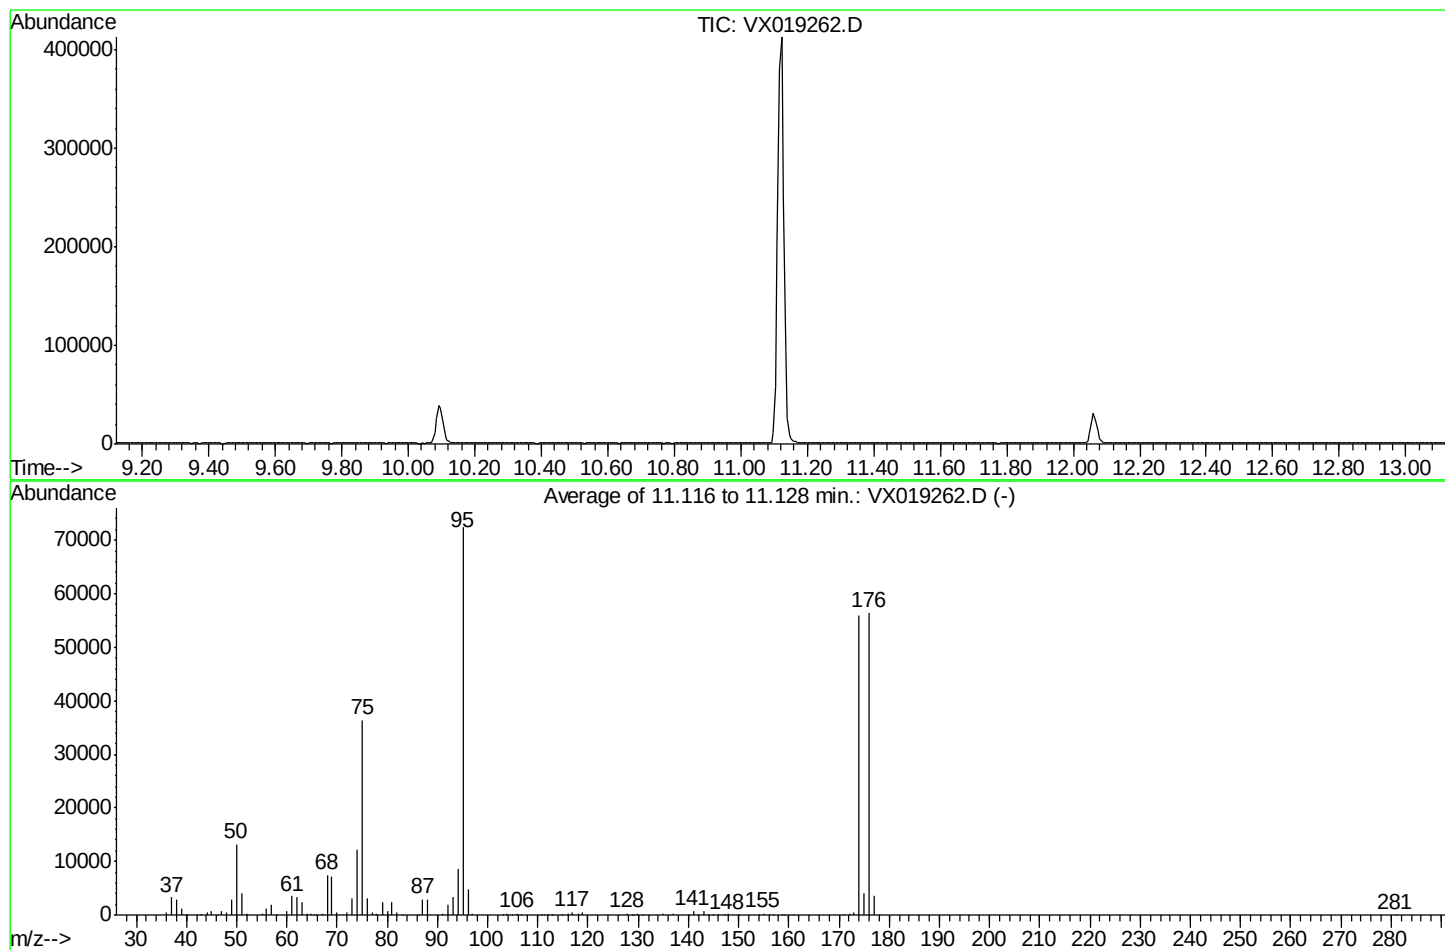

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	13148	PASS
75	95	30	80	50.3	36381	PASS
95	95	100	100	100.0	72381	PASS
96	95	5	9	6.6	4809	PASS
173	174	0.00	2	0.9	518	PASS
174	95	50	120	77.3	55965	PASS
175	174	5	9	7.2	4017	PASS
176	174	95	101	100.9	56448	PASS
177	176	5	9	6.2	3517	PASS

m/z	Abundance
36.00	239.0
37.10	1964.0
38.00	1732.0
39.10	662.0
40.00	204.0
42.10	50.0
43.10	134.0
44.00	864.0
45.10	412.0
46.10	51.0
47.00	435.0
48.00	228.0
49.00	1621.0
50.00	8067.0
51.00	2540.0
52.10	101.0
55.00	140.0
56.00	679.0
57.00	1335.0
57.90	115.0
60.10	476.0
61.00	2343.0
62.10	2216.0
63.10	1636.0
64.10	208.0
65.20	251.0
67.20	176.0
68.00	4855.0
69.10	4712.0
70.00	315.0
72.00	215.0
73.00	2073.0
74.00	8025.0
75.00	23736.0
76.10	1997.0
77.00	228.0
77.90	240.0
78.90	1484.0
80.00	589.0
81.00	1731.0
81.90	377.0
86.10	127.0
87.00	2065.0
88.00	1885.0
91.00	242.0
92.00	1402.0
93.00	2325.0
94.00	6069.0
95.10	49312.0
96.00	2824.0
97.10	133.0
103.80	240.0
104.90	63.0
105.90	309.0
111.10	65.0
116.00	219.0
117.00	394.0
117.90	199.0
118.90	320.0
127.90	244.0
128.80	98.0
130.00	191.0
131.00	126.0
135.00	88.0
137.00	118.0
140.90	629.0
143.10	621.0
144.90	80.0
145.80	119.0
147.90	112.0
155.10	205.0
156.90	83.0
159.20	75.0
160.80	63.0
172.10	243.0
173.00	502.0
174.00	46368.0
175.10	3222.0
176.00	47056.0
177.00	2678.0
178.00	76.0
207.10	53.0
281.00	57.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

m/z	Abundance
36.10	722.0
37.10	3950.0
38.00	3314.0
39.10	1519.0
40.10	229.0
43.00	77.0
44.10	930.0
44.90	715.0
46.30	87.0
47.00	881.0
48.00	511.0
49.00	3334.0
50.00	15426.0
51.00	4712.0
52.00	299.0
55.10	208.0
56.00	1277.0
57.00	2240.0
57.90	109.0
60.00	893.0
61.00	4101.0
62.00	3931.0
63.10	2639.0
64.00	244.0
64.90	216.0
67.00	267.0
68.00	8713.0
69.00	8896.0
70.00	736.0
71.90	576.0
73.00	3717.0
74.00	14291.0
75.10	42904.0
76.10	3590.0
77.00	546.0
77.90	286.0
79.00	2813.0
80.00	927.0
80.90	2978.0
82.00	693.0
83.00	74.0
86.10	102.0
87.00	3316.0
88.00	3360.0
90.90	351.0
92.10	2342.0
93.00	3959.0
94.00	10242.0
95.10	86552.0
96.10	5825.0
97.00	208.0
103.00	57.0
104.00	428.0
104.90	180.0
105.90	384.0
110.80	111.0
111.90	76.0
112.70	80.0
113.00	64.0
114.80	119.0
115.90	366.0
116.90	566.0
118.00	388.0
118.90	440.0
127.90	348.0
129.00	214.0
130.00	285.0
130.90	110.0
134.90	203.0
137.00	211.0
140.10	50.0
140.90	1159.0
141.80	129.0
143.00	956.0
145.00	148.0
145.90	142.0
147.10	68.0
147.90	231.0
149.90	88.0
154.00	65.0
155.00	330.0
156.10	55.0
156.90	156.0
158.70	110.0
160.90	125.0
172.00	310.0
173.00	578.0
174.00	65472.0
175.10	4649.0
176.00	67976.0
177.00	4443.0
178.00	146.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

207.1087.0

281.0068.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

m/z	Abundance
36.00	709.0
37.00	4040.0
38.00	3350.0
39.10	1365.0
39.90	200.0
43.10	62.0
44.00	1325.0
45.10	775.0
47.10	1030.0
47.90	574.0
49.10	3492.0
50.00	15952.0
51.00	4753.0
52.10	221.0
55.00	346.0
56.00	1320.0
57.00	2135.0
58.10	101.0
60.00	666.0
61.00	4052.0
62.00	4101.0
63.10	3116.0
64.00	352.0
64.90	204.0
65.80	51.0
67.10	214.0
68.00	8682.0
69.00	8259.0
70.00	692.0
72.00	433.0
73.00	3896.0
74.00	13926.0
75.10	42504.0
76.10	3957.0
77.00	519.0
77.90	363.0
79.00	2874.0
80.00	756.0
81.00	2798.0
81.90	547.0
83.10	68.0
87.00	3407.0
88.00	3175.0
90.90	296.0
92.00	2264.0
93.00	3473.0
94.10	9849.0
95.10	81280.0
96.00	5780.0
97.00	175.0
103.00	63.0
103.90	346.0
104.80	76.0
105.90	409.0
106.70	63.0
109.90	65.0
110.80	105.0
111.90	104.0
112.80	65.0
114.90	76.0
116.00	309.0
116.90	540.0
118.00	274.0
119.00	417.0
127.90	353.0
128.70	78.0
129.10	69.0
129.90	283.0
131.00	84.0
134.90	216.0
137.00	138.0
140.10	53.0
141.00	720.0
141.90	107.0
143.00	886.0
143.90	55.0
144.90	96.0
145.90	110.0
147.10	64.0
147.90	168.0
150.10	159.0
154.90	229.0
156.80	107.0
159.10	72.0
171.00	57.0
172.10	324.0
173.10	475.0
174.00	56056.0
175.00	4182.0
176.00	54312.0
177.00	3432.0
178.00	97.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

207.10

76.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66

Scan 1639 (11.079 min): VX019262.D
BFB66

m/z	Abundance
40.10	123.0
42.90	58.0
44.10	533.0
207.20	173.0

Instrument :
MSVOA_X
ClientSampleId :
BFB66