

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043712.D
 Acq On : 05 Nov 2024 13:40
 Operator : JC/MD
 Sample : P4621-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 06 02:03:10 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 06 01:38:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	252840	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	232120	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	106819	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	65567	48.677	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	97.360%		
7) Chloroethane-d5	1.642	69	22368	38.633	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	77.260%		
11) 1,1-Dichloroethene-d2	2.294	65	27808	44.721	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.440%		
21) 2-Butanone-d5	4.465	46	99789	113.148	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	113.150%		
24) Chloroform-d	5.050	84	131792	45.387	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.780%		
26) 1,2-Dichloroethane-d4	5.952	65	87660	47.521	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.040%		
32) Benzene-d6	5.970	84	277535	46.246	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.500%		
36) 1,2-Dichloropropane-d6	7.306	67	86604	47.434	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.860%		
41) Toluene-d8	8.647	98	247158	45.337	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.680%		
43) trans-1,3-Dichloroprop...	8.952	79	37989	43.508	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.020%		
47) 2-Hexanone-d5	9.384	63	77273	106.943	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	106.940%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	121615	51.914	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	103.820%		
66) 1,2-Dichlorobenzene-d4	12.317	152	94395	51.003	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.000%		
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	12.018	75	12264	5.915	ug/L	# 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043712.D
Acq On : 05 Nov 2024 13:40
Operator : JC/MD
Sample : P4621-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Nov 06 02:03:10 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 06 01:38:34 2024
Response via : Initial Calibration

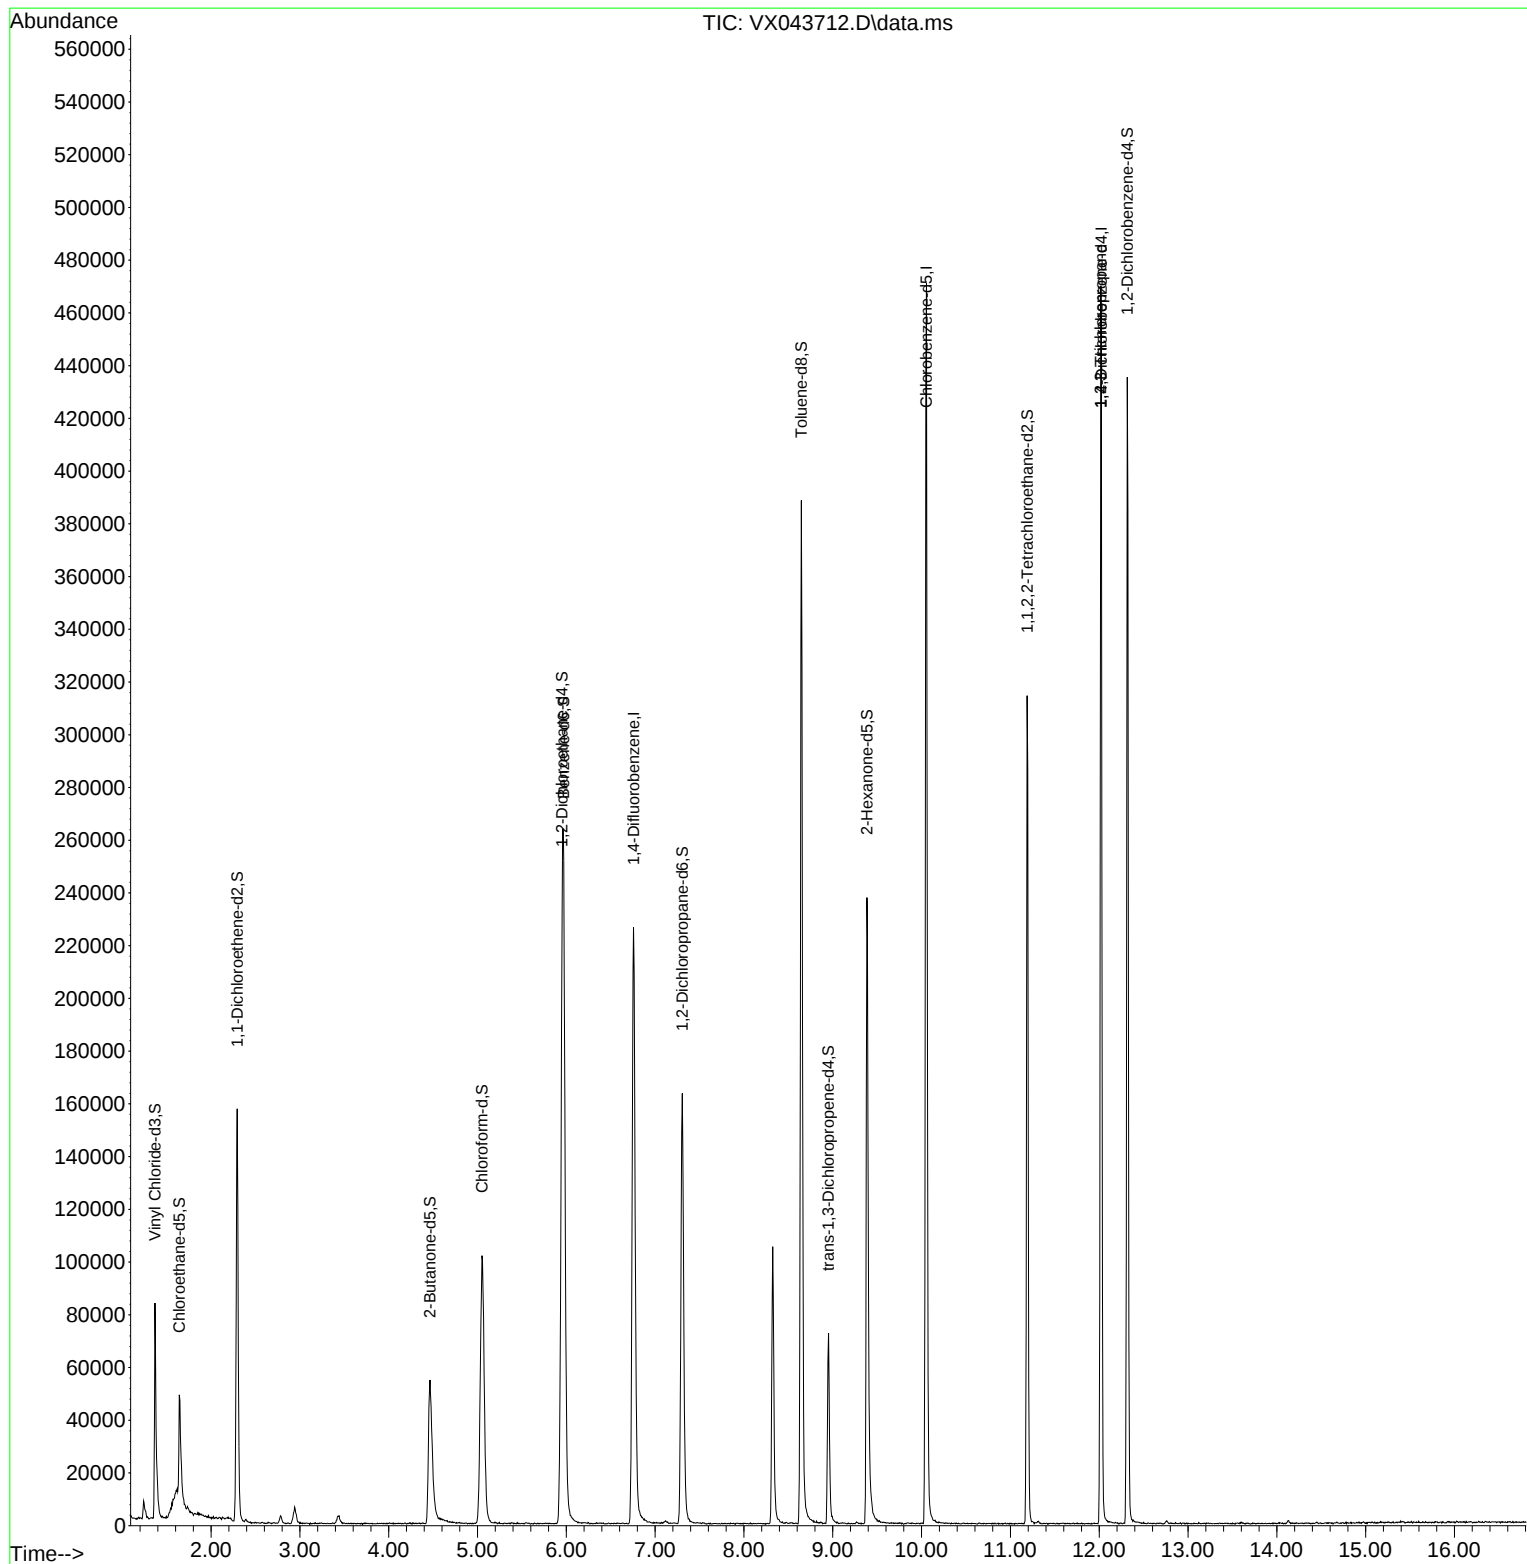

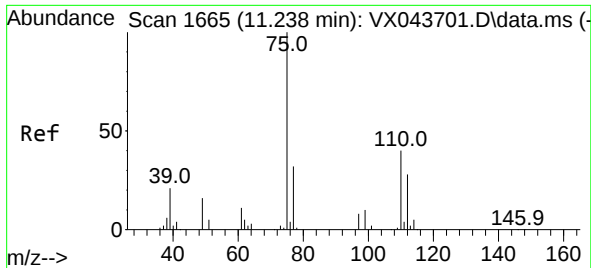

#61
 1,2,3-Trichloropropane
 Concen: 5.915 ug/L
 RT: 12.018 min Scan# 11
 Delta R.T. 0.780 min
 Lab File: VX043712.D
 Acq: 05 Nov 2024 13:40

Instrument :
 MSVOA_X
 ClientSampleId :

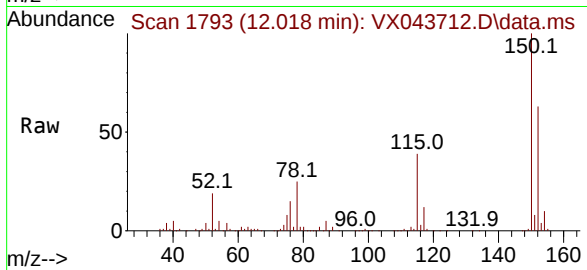

Tgt Ion: 75 Resp: 12264
 Ion Ratio Lower Upper
 75 100
 77 31.5 25.4 38.0
 110 3.4 33.6 50.4#

