

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043713.D
 Acq On : 05 Nov 2024 14:04
 Operator : JC/MD
 Sample : P4621-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 06 02:03:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 06 01:38:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	216812	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	201072	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	86743	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	68951	59.696	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 119.400%			
7) Chloroethane-d5	1.648	69	38312	77.167	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 154.340%#			
11) 1,1-Dichloroethene-d2	2.294	65	28322	53.117	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 106.240%			
21) 2-Butanone-d5	4.465	46	102074	134.972	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 134.970%#			
24) Chloroform-d	5.050	84	144996	58.232	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 116.460%			
26) 1,2-Dichloroethane-d4	5.952	65	91620	57.921	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 115.840%			
32) Benzene-d6	5.971	84	304235	58.523	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 117.040%			
36) 1,2-Dichloropropane-d6	7.306	67	94866	59.982	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 119.960%			
41) Toluene-d8	8.647	98	268505	56.858	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 113.720%			
43) trans-1,3-Dichloroprop...	8.952	79	39094	51.687	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 103.380%			
47) 2-Hexanone-d5	9.385	63	73659	117.682	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 117.680%			
56) 1,1,2,2-Tetrachloroeth...	11.189	84	119915	59.093	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 118.180%			
66) 1,2-Dichlorobenzene-d4	12.317	152	98810	65.745	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 131.500%#			
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	12.018	75	9318	5.534	ug/L	# 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043713.D
Acq On : 05 Nov 2024 14:04
Operator : JC/MD
Sample : P4621-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Nov 06 02:03:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 06 01:38:34 2024
Response via : Initial Calibration

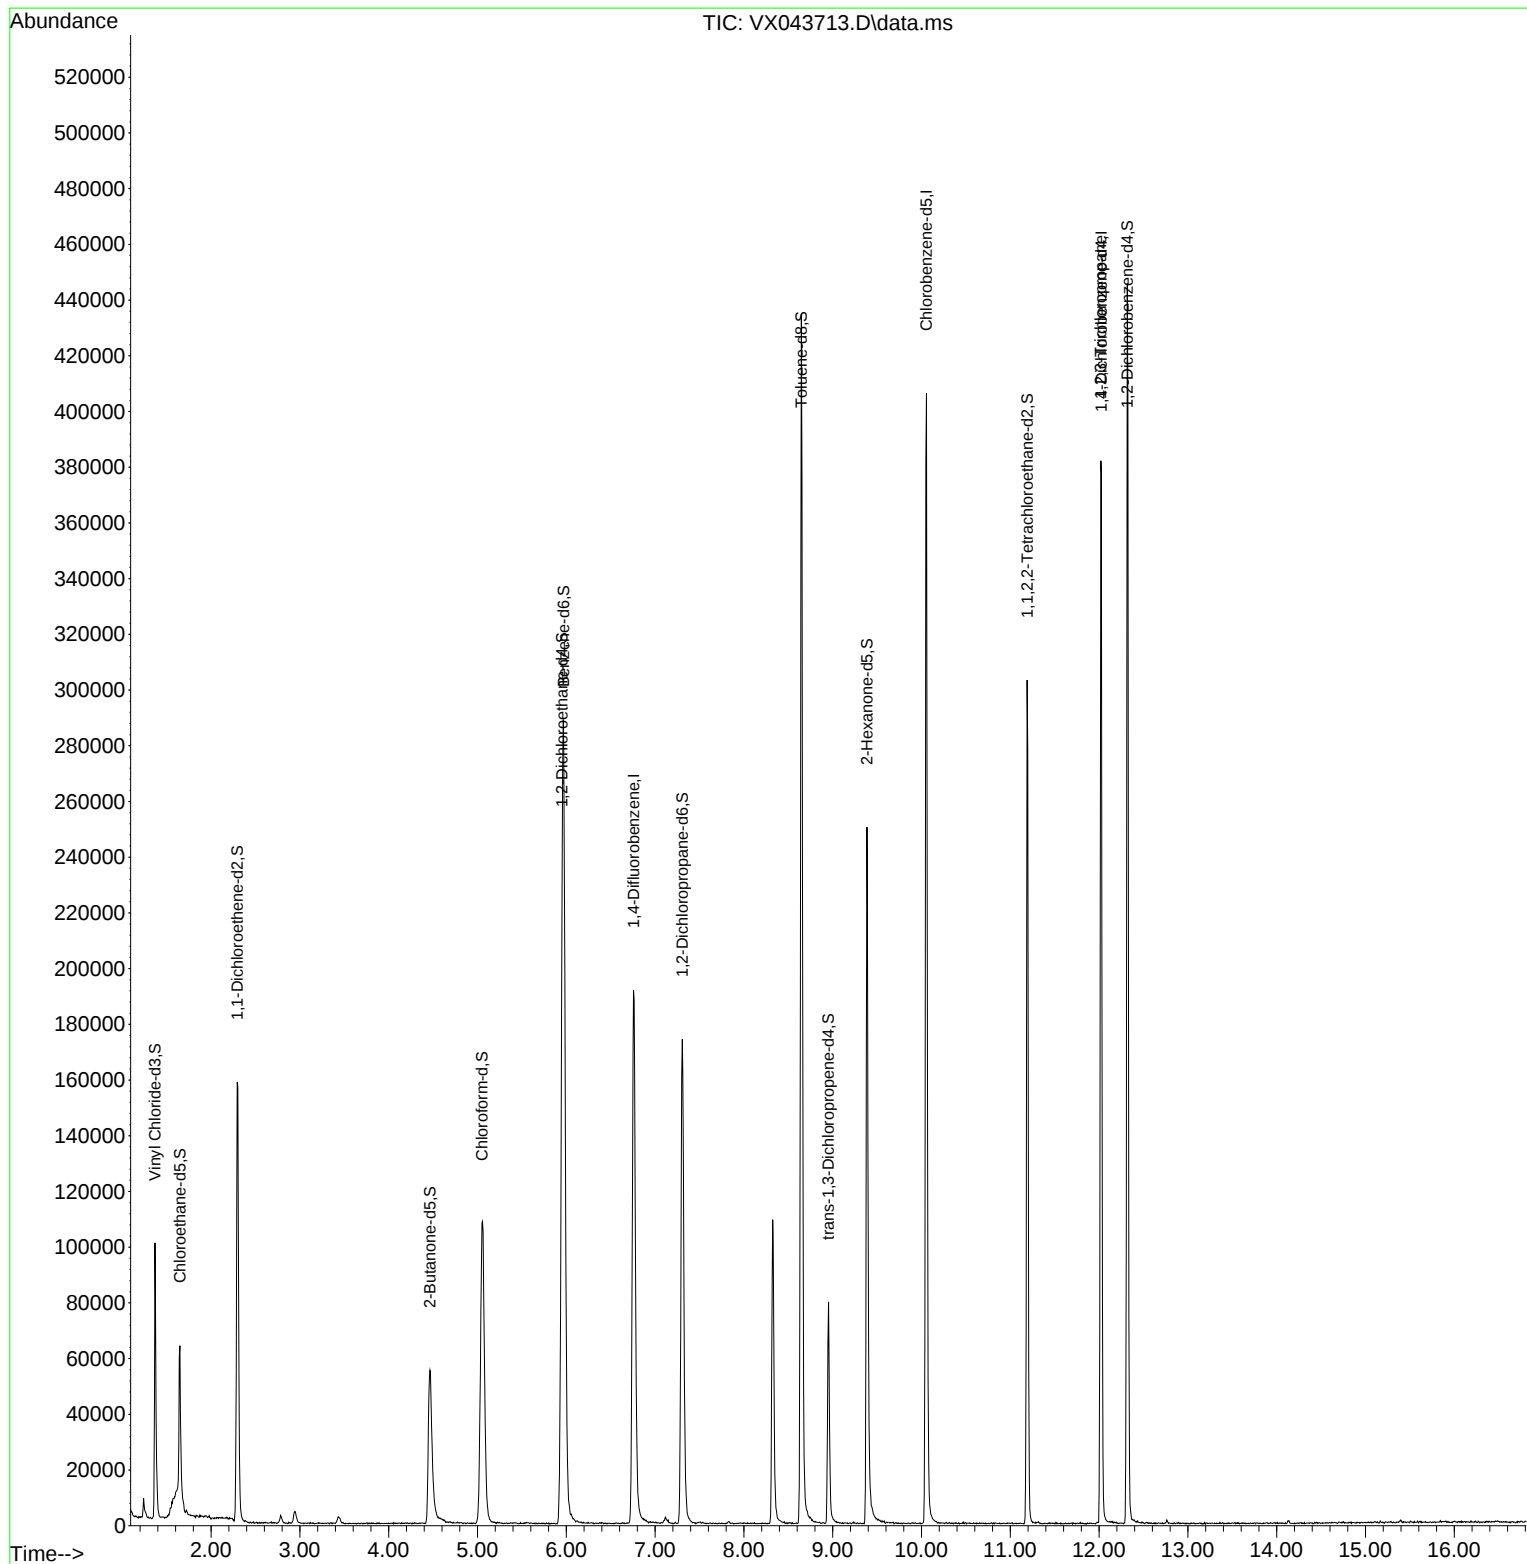

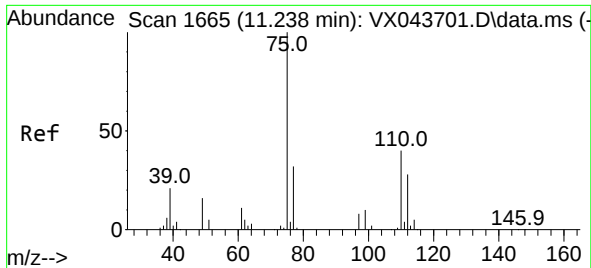

#61
 1,2,3-Trichloropropane
 Concen: 5.534 ug/L
 RT: 12.018 min Scan# 11
 Delta R.T. 0.781 min
 Lab File: VX043713.D
 Acq: 05 Nov 2024 14:04

Instrument :
 MSVOA_X
 ClientSampleId :

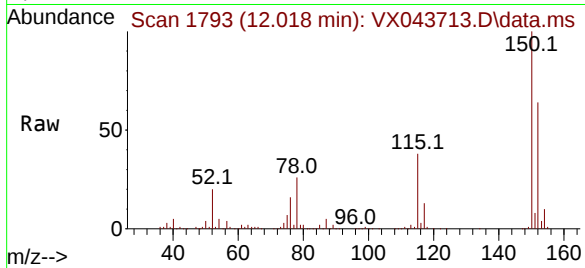

Tgt Ion: 75 Resp: 9318
 Ion Ratio Lower Upper
 75 100
 77 37.0 25.4 38.0
 110 3.8 33.6 50.4#

