

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043719.D
 Acq On : 05 Nov 2024 16:22
 Operator : JC/MD
 Sample : P4621-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 06 02:04:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 06 01:38:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	201509	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	188116	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	78845	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	48918	45.568	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.140%		
7) Chloroethane-d5	1.648	69	25796	55.903	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	111.800%		
11) 1,1-Dichloroethene-d2	2.294	65	19373	39.092	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.180%		
21) 2-Butanone-d5	4.465	46	88157	125.422	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	125.420%		
24) Chloroform-d	5.056	84	109520	47.325	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.640%		
26) 1,2-Dichloroethane-d4	5.952	65	75769	51.538	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	103.080%		
32) Benzene-d6	5.970	84	227896	46.858	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.720%		
36) 1,2-Dichloropropane-d6	7.306	67	74755	50.521	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	101.040%		
41) Toluene-d8	8.647	98	196704	44.522	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.040%		
43) trans-1,3-Dichloroprop...	8.952	79	31510	44.529	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.060%		
47) 2-Hexanone-d5	9.384	63	61276	104.641	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	104.640%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	98667	51.971	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	103.940%		
66) 1,2-Dichlorobenzene-d4	12.317	152	73769	54.000	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.000%		
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	12.018	75	8832	5.771	ug/L	# 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043719.D
Acq On : 05 Nov 2024 16:22
Operator : JC/MD
Sample : P4621-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 06 02:04:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 06 01:38:34 2024
Response via : Initial Calibration

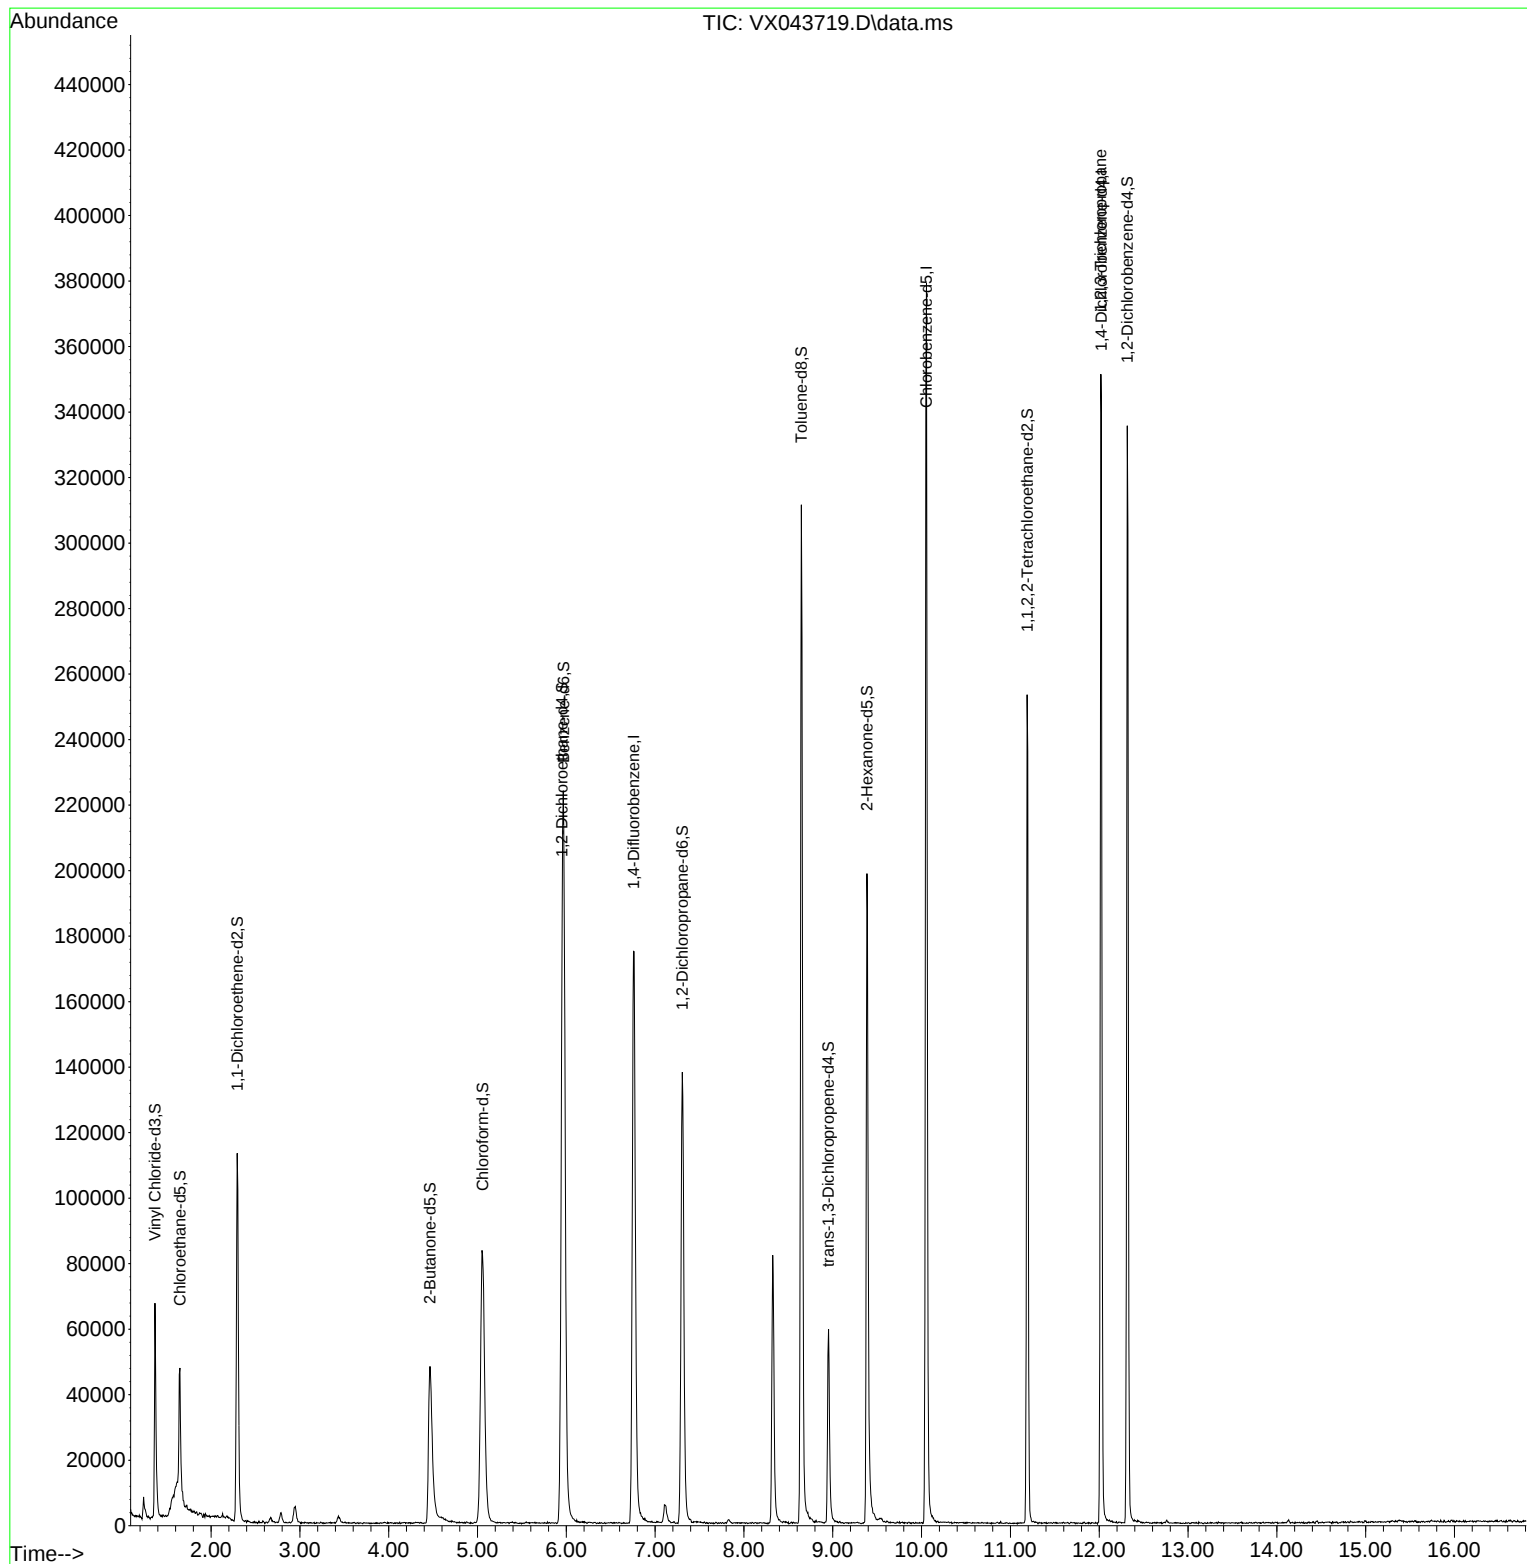

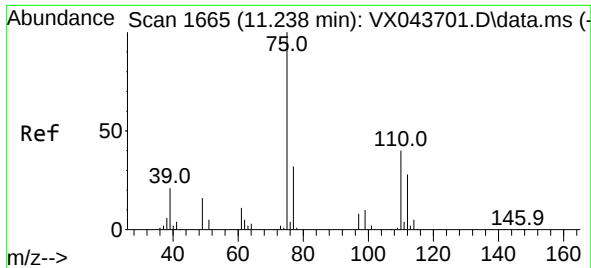

#61
1,2,3-Trichloropropane
Concen: 5.771 ug/L
RT: 12.018 min Scan# 11
Delta R.T. 0.780 min
Lab File: VX043719.D
Acq: 05 Nov 2024 16:22

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 75 Resp: 8832
Ion Ratio Lower Upper
75 100
77 31.1 25.4 38.0
110 3.2 33.6 50.4#

