

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043720.D
 Acq On : 05 Nov 2024 16:46
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 06 02:04:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 06 01:38:34 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	178586	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	165342	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	71856	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	48509	50.987	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 101.980%		
7) Chloroethane-d5	1.648	69	32072	78.426	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 156.860%#		
11) 1,1-Dichloroethene-d2	2.300	65	20778	47.309	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 94.620%		
21) 2-Butanone-d5	4.465	46	78922	126.696	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 126.700%		
24) Chloroform-d	5.050	84	102660	50.054	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 100.100%		
26) 1,2-Dichloroethane-d4	5.952	65	68752	52.768	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 105.540%		
32) Benzene-d6	5.970	84	216266	50.591	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 101.180%		
36) 1,2-Dichloropropane-d6	7.306	67	68593	52.742	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 105.480%		
41) Toluene-d8	8.647	98	187428	48.266	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 96.540%		
43) trans-1,3-Dichloroprop...	8.952	79	27542	44.282	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 88.560%		
47) 2-Hexanone-d5	9.384	63	57010	110.765	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 110.770%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	92228	55.270	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 110.540%		
66) 1,2-Dichlorobenzene-d4	12.317	152	69505	55.828	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 111.660%		
Target Compounds						
61) 1,2,3-Trichloropropane	12.018	75	7860	5.635	ug/L #	Qvalue 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043720.D
Acq On : 05 Nov 2024 16:46
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Nov 06 02:04:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 06 01:38:34 2024
Response via : Initial Calibration

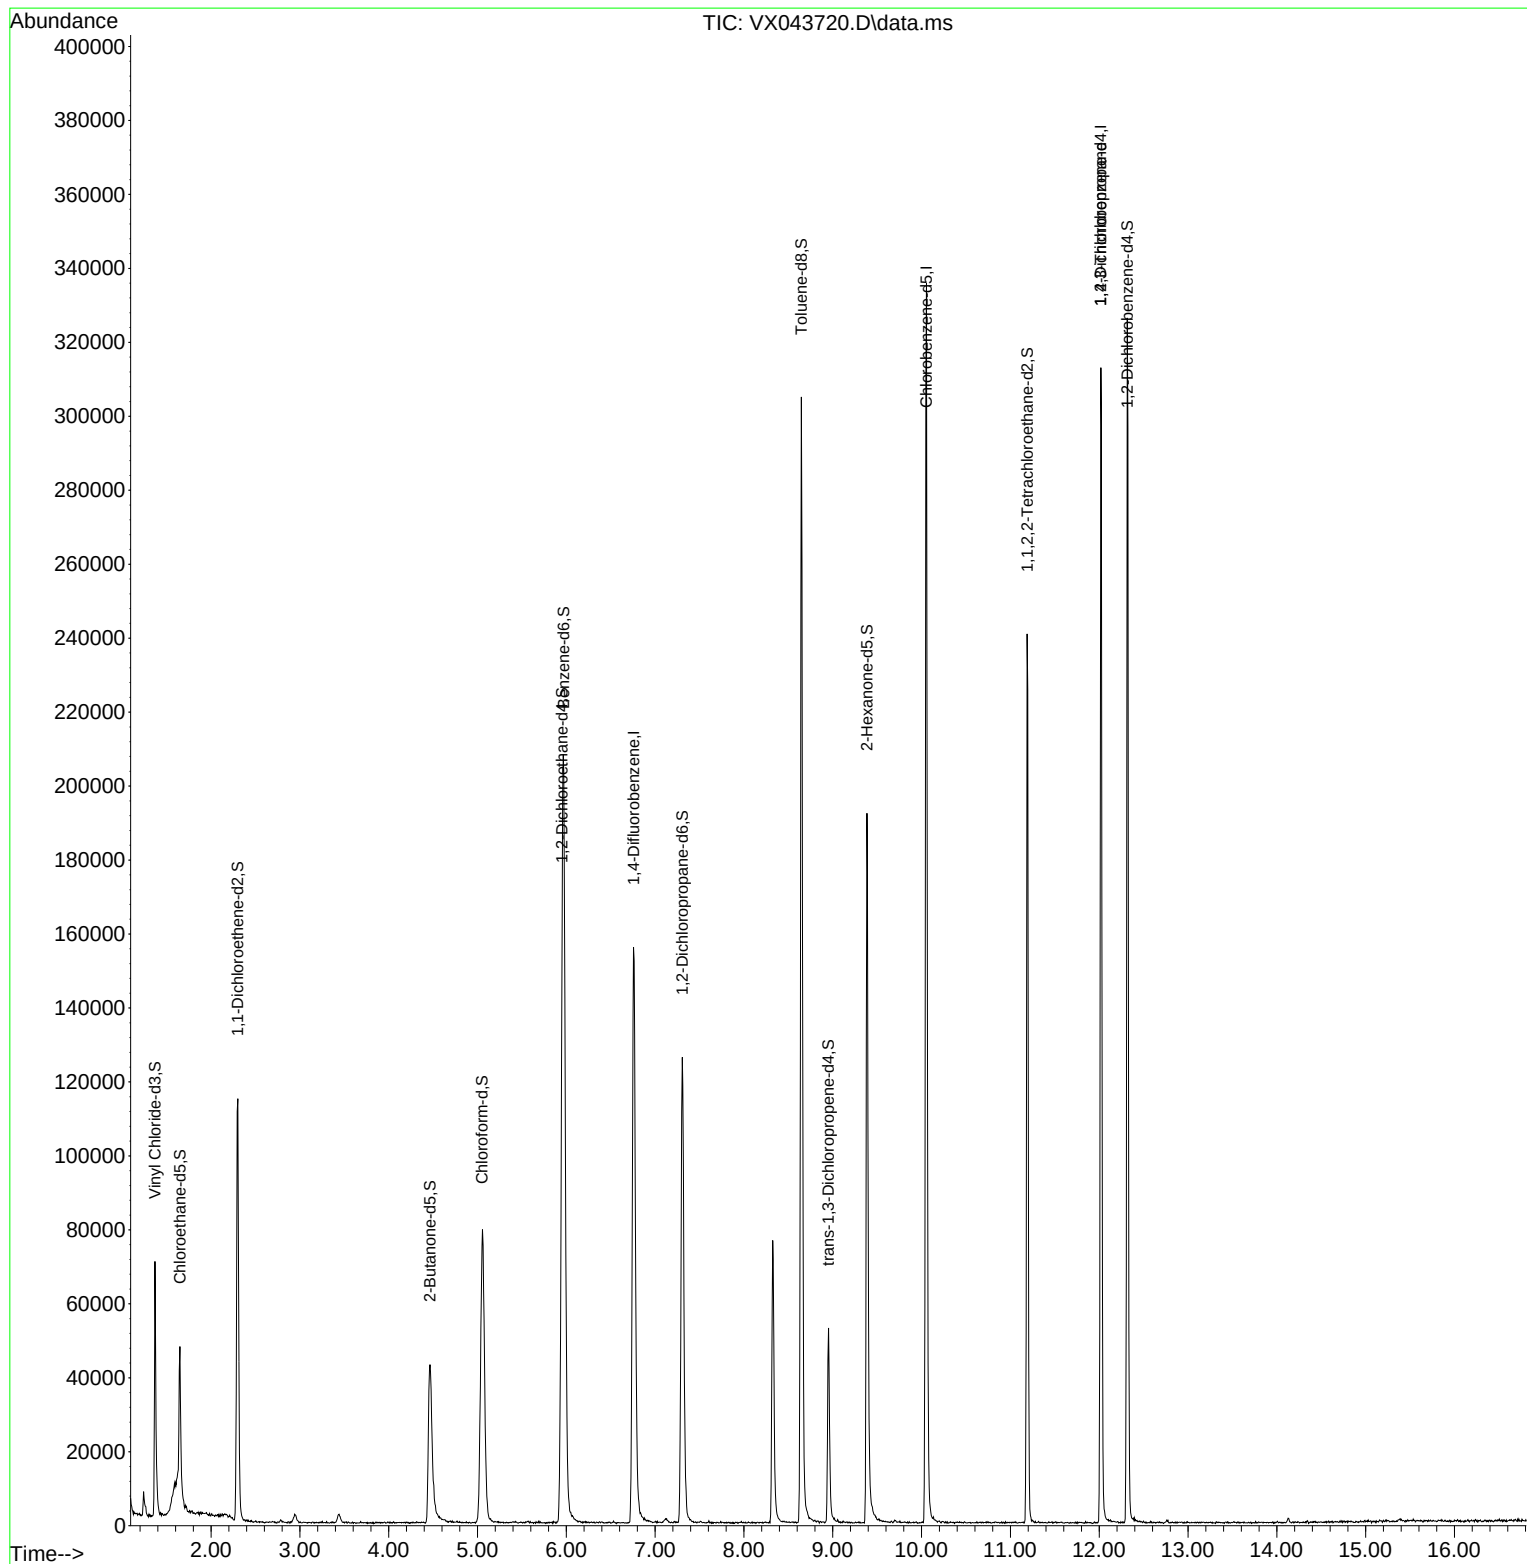

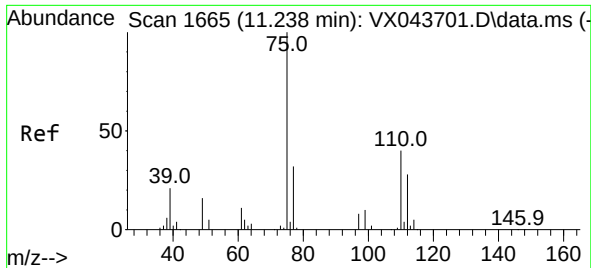

#61
1,2,3-Trichloropropane
Concen: 5.635 ug/L
RT: 12.018 min Scan# 11
Delta R.T. 0.780 min
Lab File: VX043720.D
Acq: 05 Nov 2024 16:46

Instrument :
MSVOA_X
ClientSampleId :

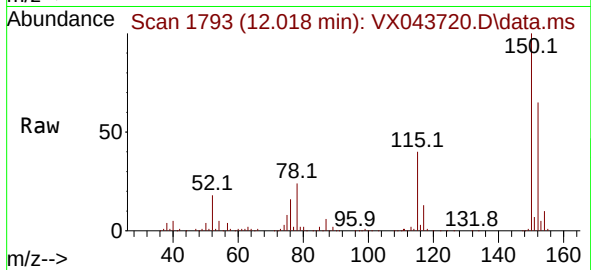

Tgt Ion: 75 Resp: 7860
Ion Ratio Lower Upper
75 100
77 32.4 25.4 38.0
110 3.1 33.6 50.4#

