

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043722.D
 Acq On : 05 Nov 2024 17:32
 Operator : JC/MD
 Sample : P4670-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 06 02:05:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 06 01:38:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	171839	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	158031	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	64889	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	37475	40.936	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.880%
7) Chloroethane-d5	1.648	69	20901	53.116	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.240%
11) 1,1-Dichloroethene-d2	2.300	65	15703	37.158	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.320%
21) 2-Butanone-d5	4.464	46	55262	92.197	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.200%
24) Chloroform-d	5.056	84	83471	42.296	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.600%
26) 1,2-Dichloroethane-d4	5.958	65	52207	41.642	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.280%
32) Benzene-d6	5.970	84	170869	41.821	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.640%
36) 1,2-Dichloropropane-d6	7.305	67	53724	43.220	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.440%
41) Toluene-d8	8.647	98	150432	40.531	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.060%
43) trans-1,3-Dichloroprop...	8.951	79	20325	34.191	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.380%
47) 2-Hexanone-d5	9.384	63	42359	86.107	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.110%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	67314	42.206	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.420%
66) 1,2-Dichlorobenzene-d4	12.317	152	53534	47.616	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.240%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	12.018	75	7188	5.707	ug/L	# 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043722.D
Acq On : 05 Nov 2024 17:32
Operator : JC/MD
Sample : P4670-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 06 02:05:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 06 01:38:34 2024
Response via : Initial Calibration

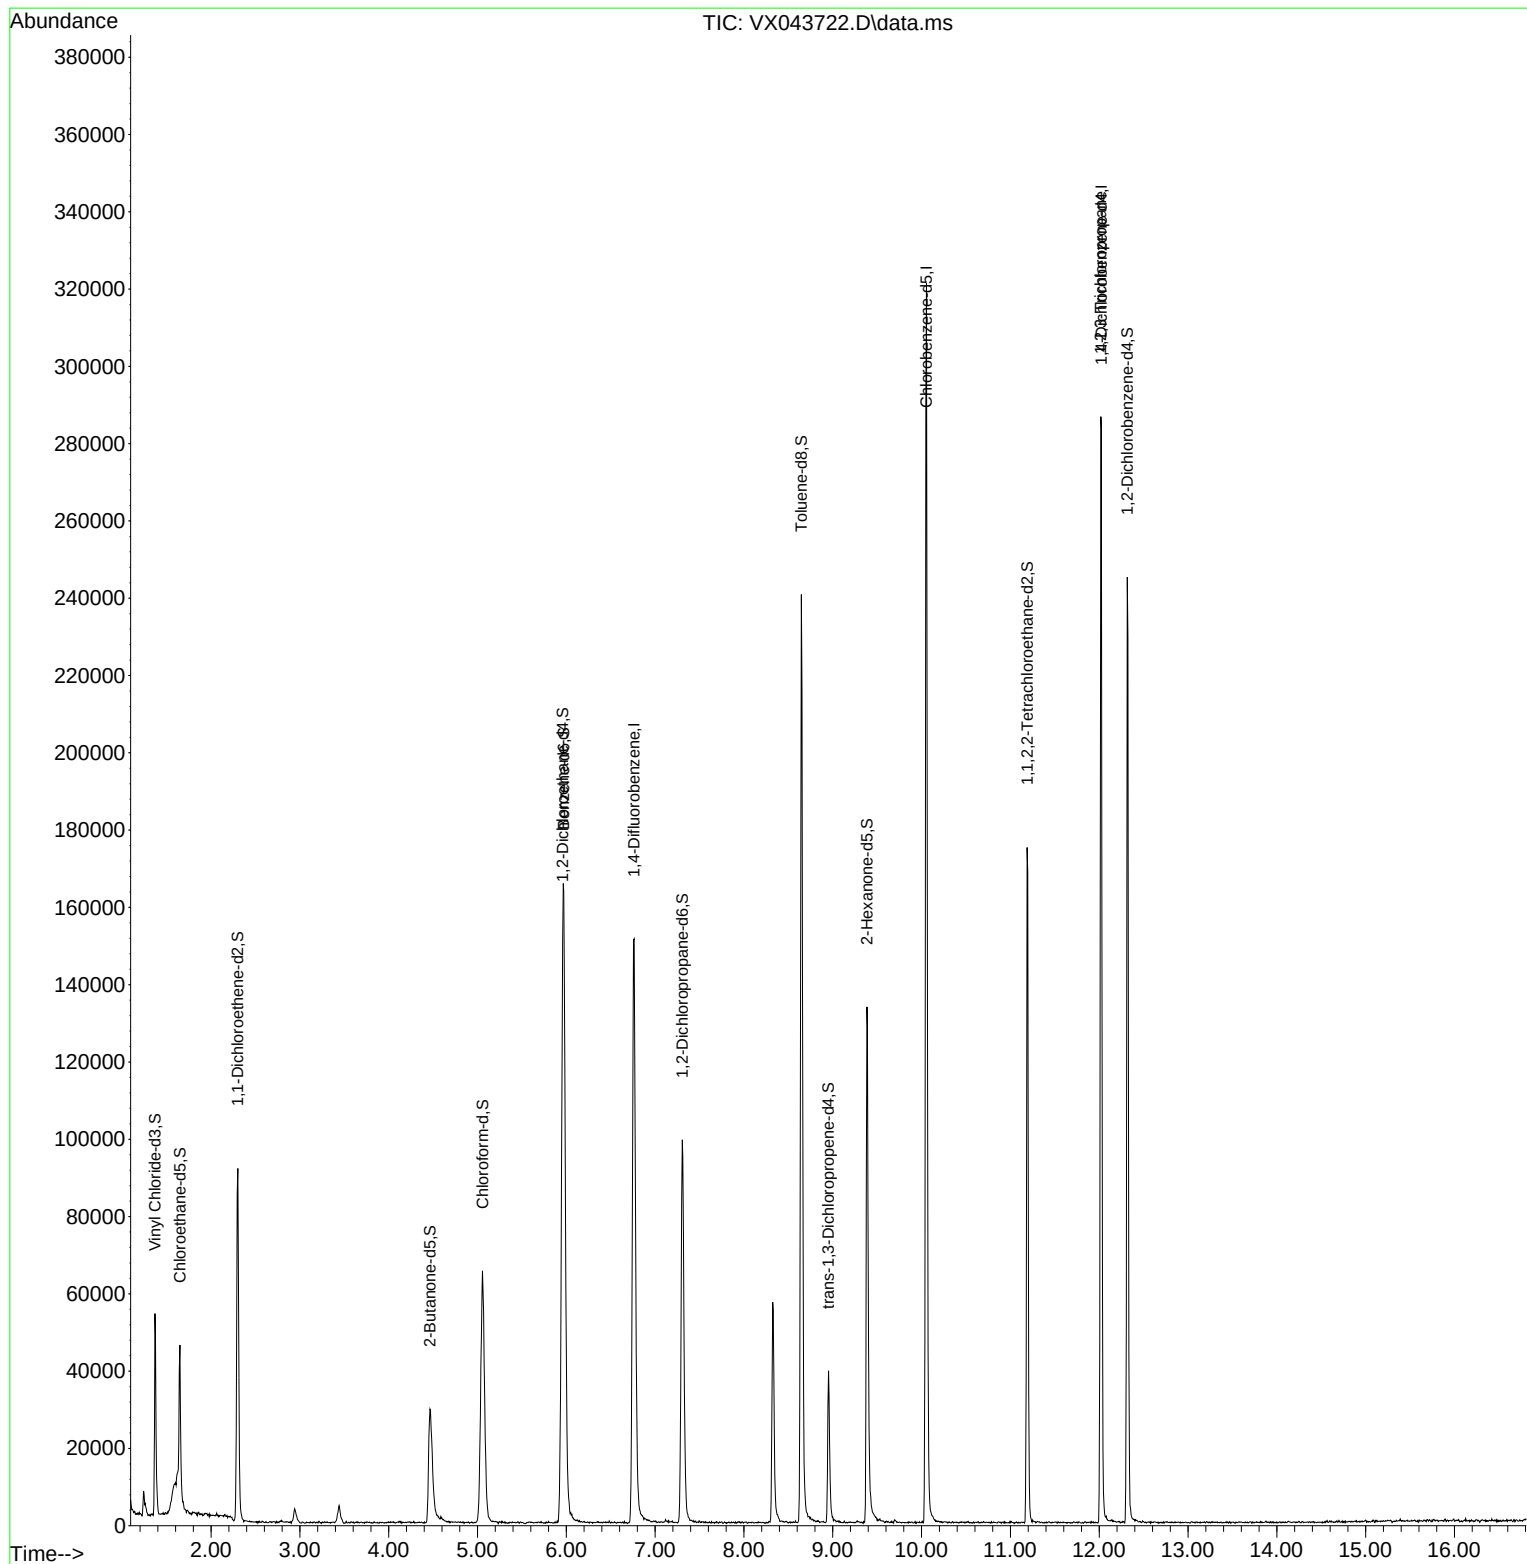

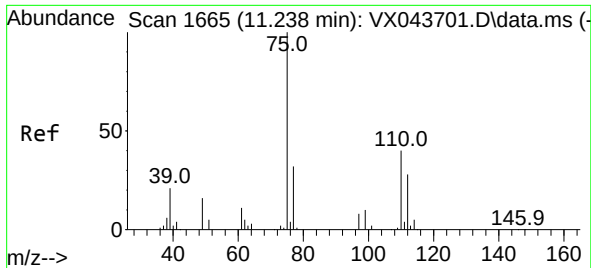

#61

1,2,3-Trichloropropane

Concen: 5.707 ug/L

RT: 12.018 min Scan# 11

Delta R.T. 0.780 min


Lab File: VX043722.D

Acq: 05 Nov 2024 17:32

Instrument :

MSVOA_X

ClientSampleId :

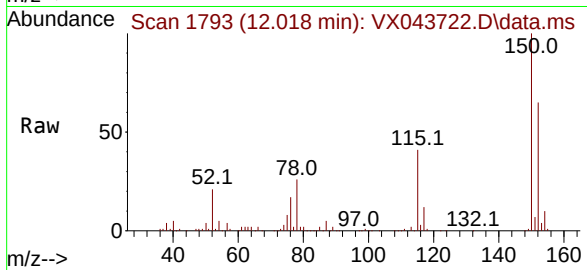

Tgt Ion: 75 Resp: 7188

Ion Ratio Lower Upper

75 100

77 32.7 25.4 38.0

110 1.4 33.6 50.4#

