

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043723.D
 Acq On : 05 Nov 2024 17:55
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 06 02:05:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 06 01:38:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	163966	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	155376	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	64727	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	33082	37.873	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.740%
7) Chloroethane-d5	1.648	69	20123	53.594	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	107.180%
11) 1,1-Dichloroethene-d2	2.300	65	14175	35.153	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.300%
21) 2-Butanone-d5	4.458	46	51431	89.925	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.930%
24) Chloroform-d	5.056	84	76100	40.413	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.820%
26) 1,2-Dichloroethane-d4	5.958	65	48129	40.233	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.460%
32) Benzene-d6	5.970	84	157741	39.267	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.540%
36) 1,2-Dichloropropane-d6	7.312	67	50142	41.028	ug/L	0.01
Spiked Amount	50.000	Range	70 - 120	Recovery	=	82.060%
41) Toluene-d8	8.647	98	137733	37.744	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	75.480%#
43) trans-1,3-Dichloroprop...	8.952	79	18662	31.930	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.860%
47) 2-Hexanone-d5	9.384	63	39638	81.953	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.950%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	65224	41.595	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.180%
66) 1,2-Dichlorobenzene-d4	12.317	152	50080	44.656	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.320%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	12.018	75	7280	5.794	ug/L	# 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043723.D
Acq On : 05 Nov 2024 17:55
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Nov 06 02:05:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 06 01:38:34 2024
Response via : Initial Calibration

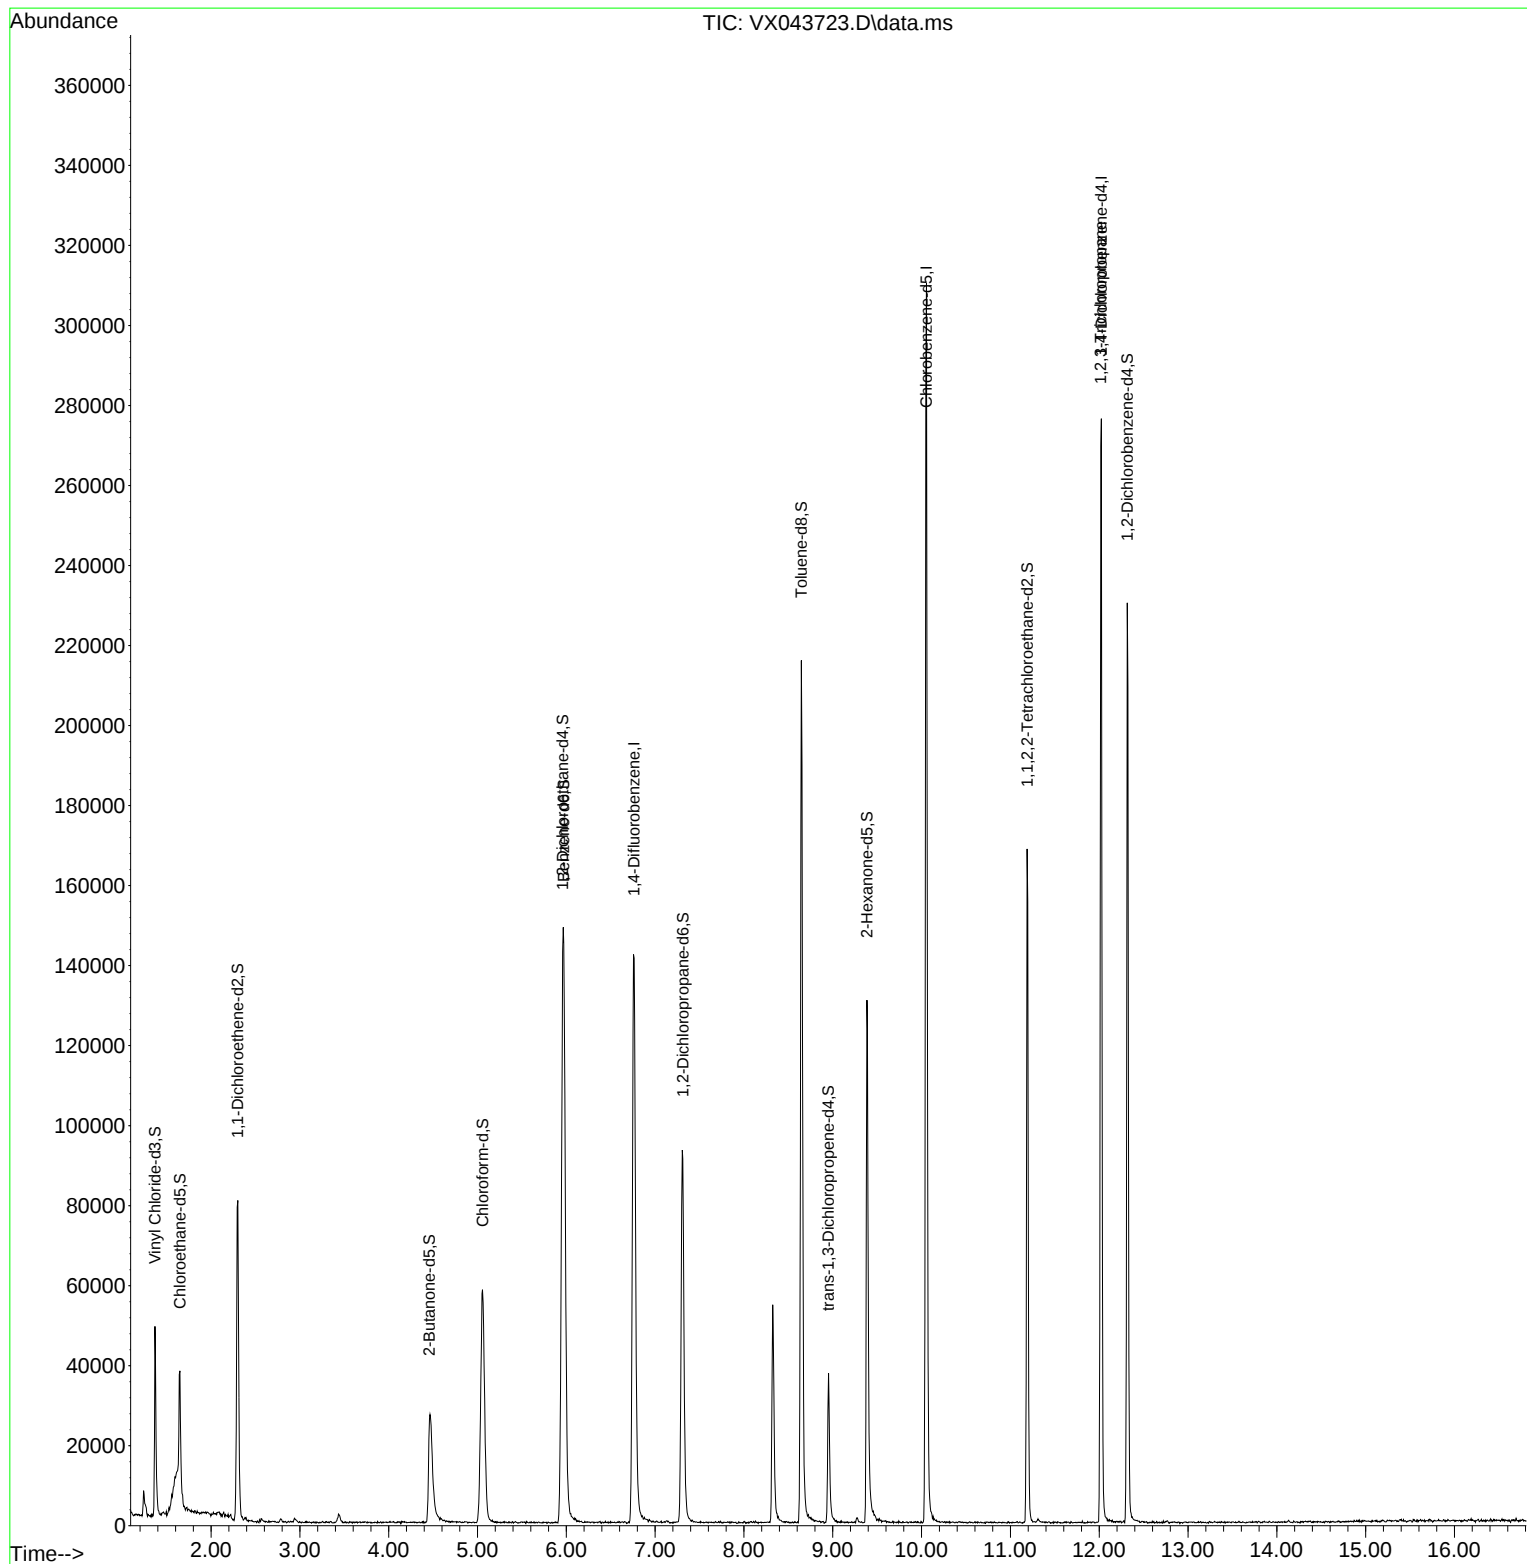

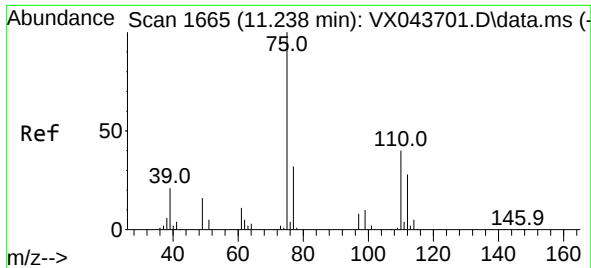

#61
1,2,3-Trichloropropane
Concen: 5.794 ug/L
RT: 12.018 min Scan# 11
Delta R.T. 0.780 min
Lab File: VX043723.D
Acq: 05 Nov 2024 17:55

Instrument :
MSVOA_X
ClientSampleId :

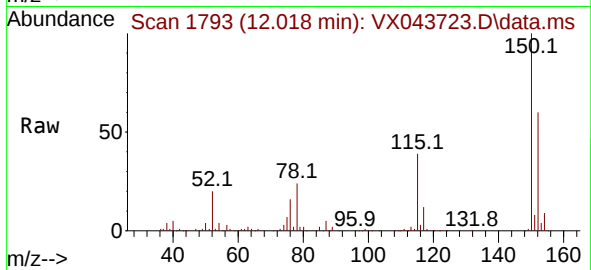

Tgt Ion: 75	Resp:	7280
Ion	Ratio	Lower Upper
75	100	
77	27.4	25.4 38.0
110	1.9	33.6 50.4#

