

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043715.D
 Acq On : 05 Nov 2024 14:50
 Operator : JC/MD
 Sample : P4621-07RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N3RE

Quant Time: Nov 06 02:03:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 06 01:38:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	159429	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	145446	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	62347	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	28806	33.916	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	67.840%		
7) Chloroethane-d5	1.648	69	17205	47.127	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	94.260%		
11) 1,1-Dichloroethene-d2	2.300	65	11287	28.787	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	57.580%#		
21) 2-Butanone-d5	4.465	46	44399	79.839	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	79.840%		
24) Chloroform-d	5.056	84	60437	33.008	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	66.020%#		
26) 1,2-Dichloroethane-d4	5.958	65	40767	35.049	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	70.100%		
32) Benzene-d6	5.971	84	125878	33.475	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	66.940%#		
36) 1,2-Dichloropropane-d6	7.306	67	39360	34.404	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	68.800%#		
41) Toluene-d8	8.647	98	106846	31.278	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	62.560%#		
43) trans-1,3-Dichloroprop...	8.958	79	16445	30.057	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	60.120%		
47) 2-Hexanone-d5	9.385	63	27400	60.518	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	60.520%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	51325	34.966	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	69.940%		
66) 1,2-Dichlorobenzene-d4	12.323	152	40256	37.266	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	74.540%#		
Target Compounds					Qvalue	
13) Acetone	2.386	43	7746	14.976	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043715.D
Acq On : 05 Nov 2024 14:50
Operator : JC/MD
Sample : P4621-07RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N3RE


Quant Time: Nov 06 02:03:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 06 01:38:34 2024
Response via : Initial Calibration

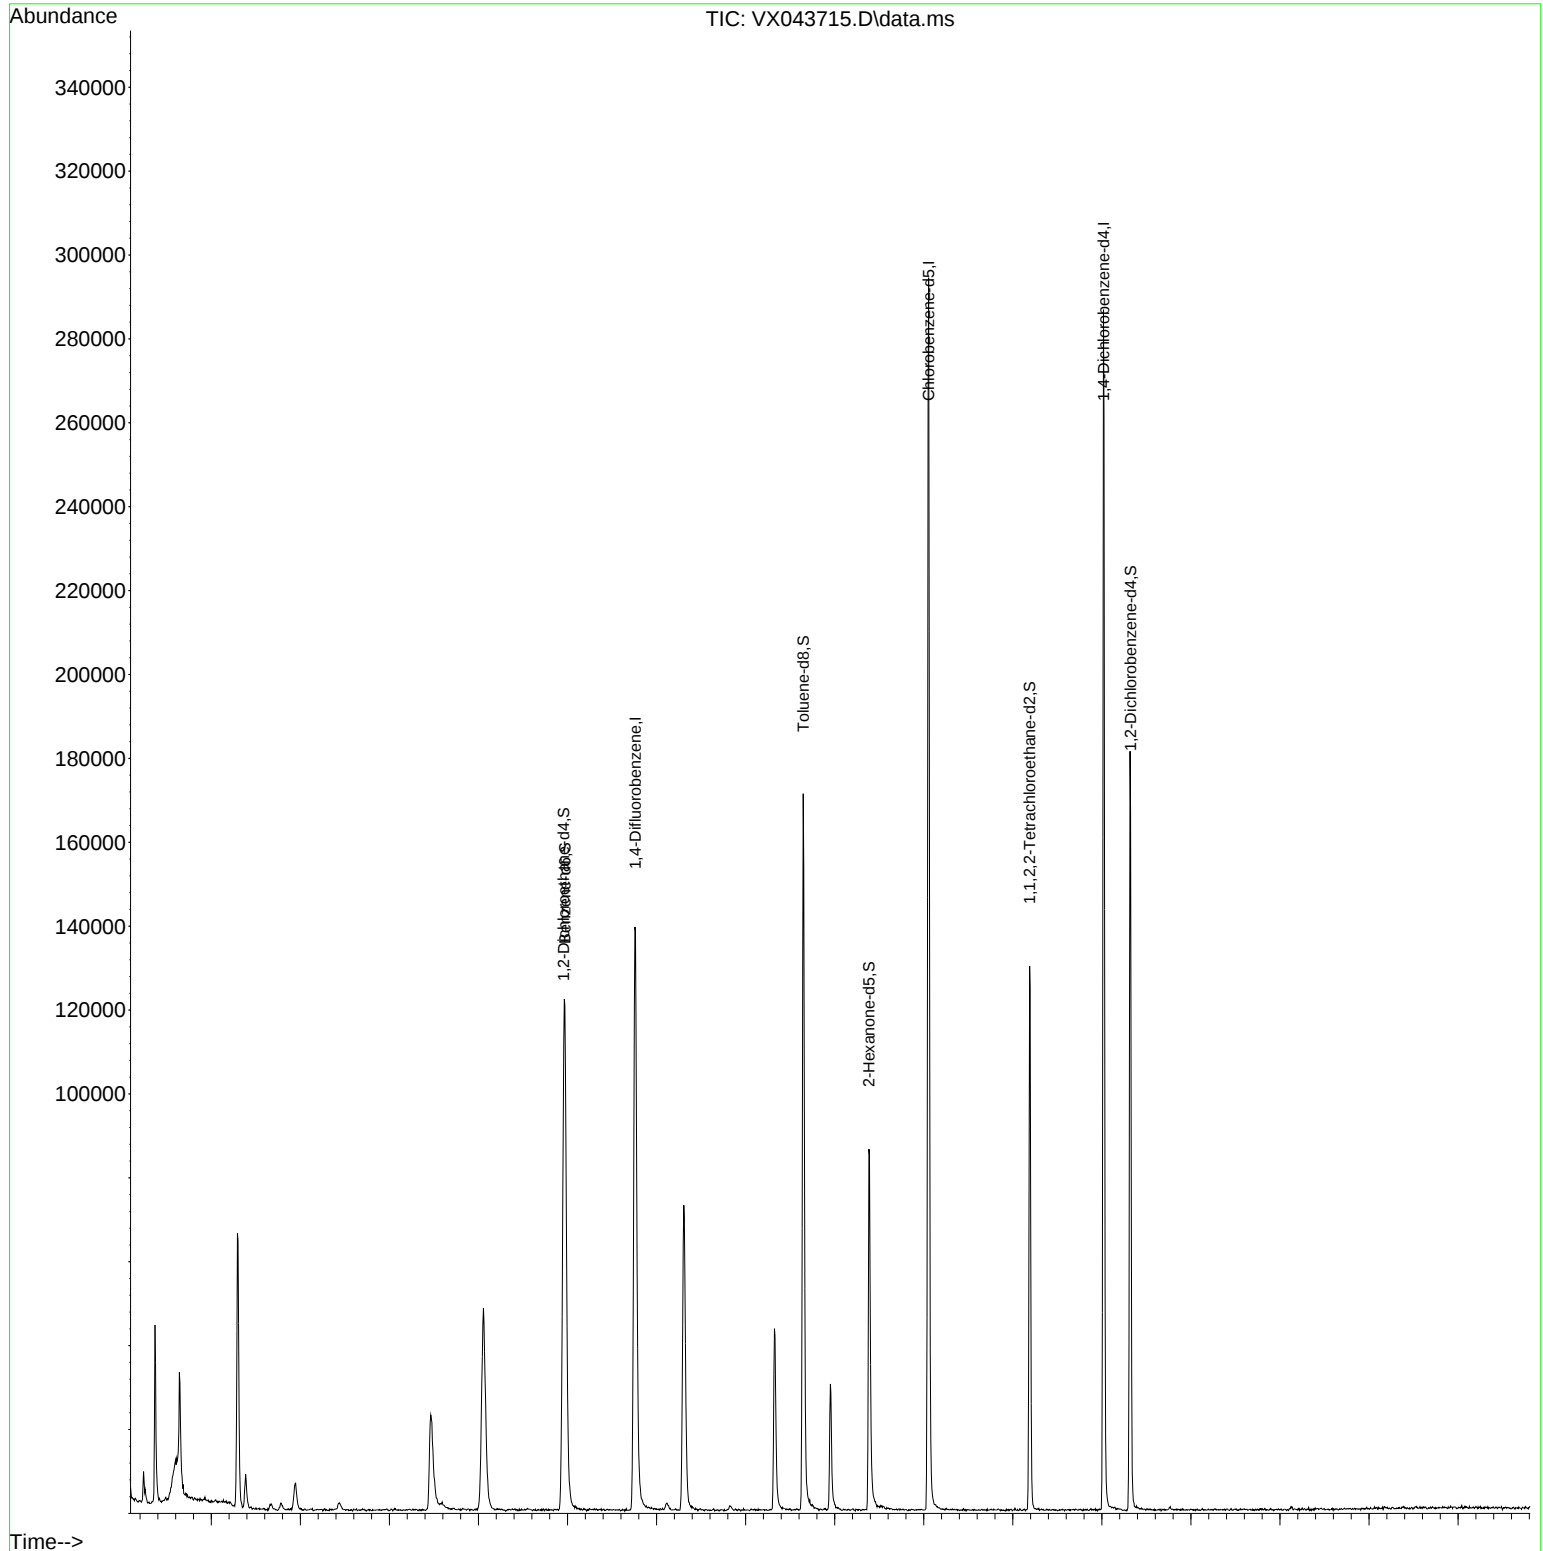

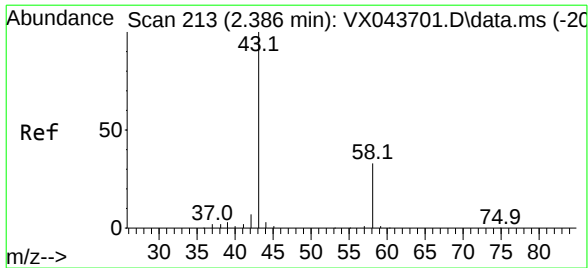

#13
 Acetone
 Concen: 14.976 ug/L
 RT: 2.386 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX043715.D
 Acq: 05 Nov 2024 14:50

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N3RE

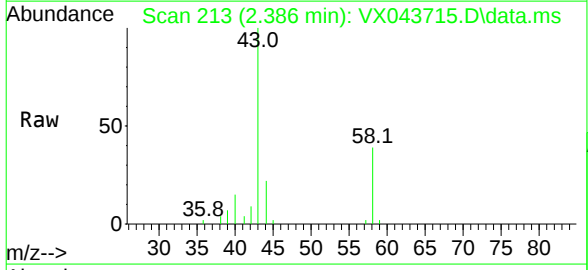

Tgt Ion: 43 Resp: 7746

Ion	Ratio	Lower	Upper
43	100		
58	34.2	0.0	63.6

